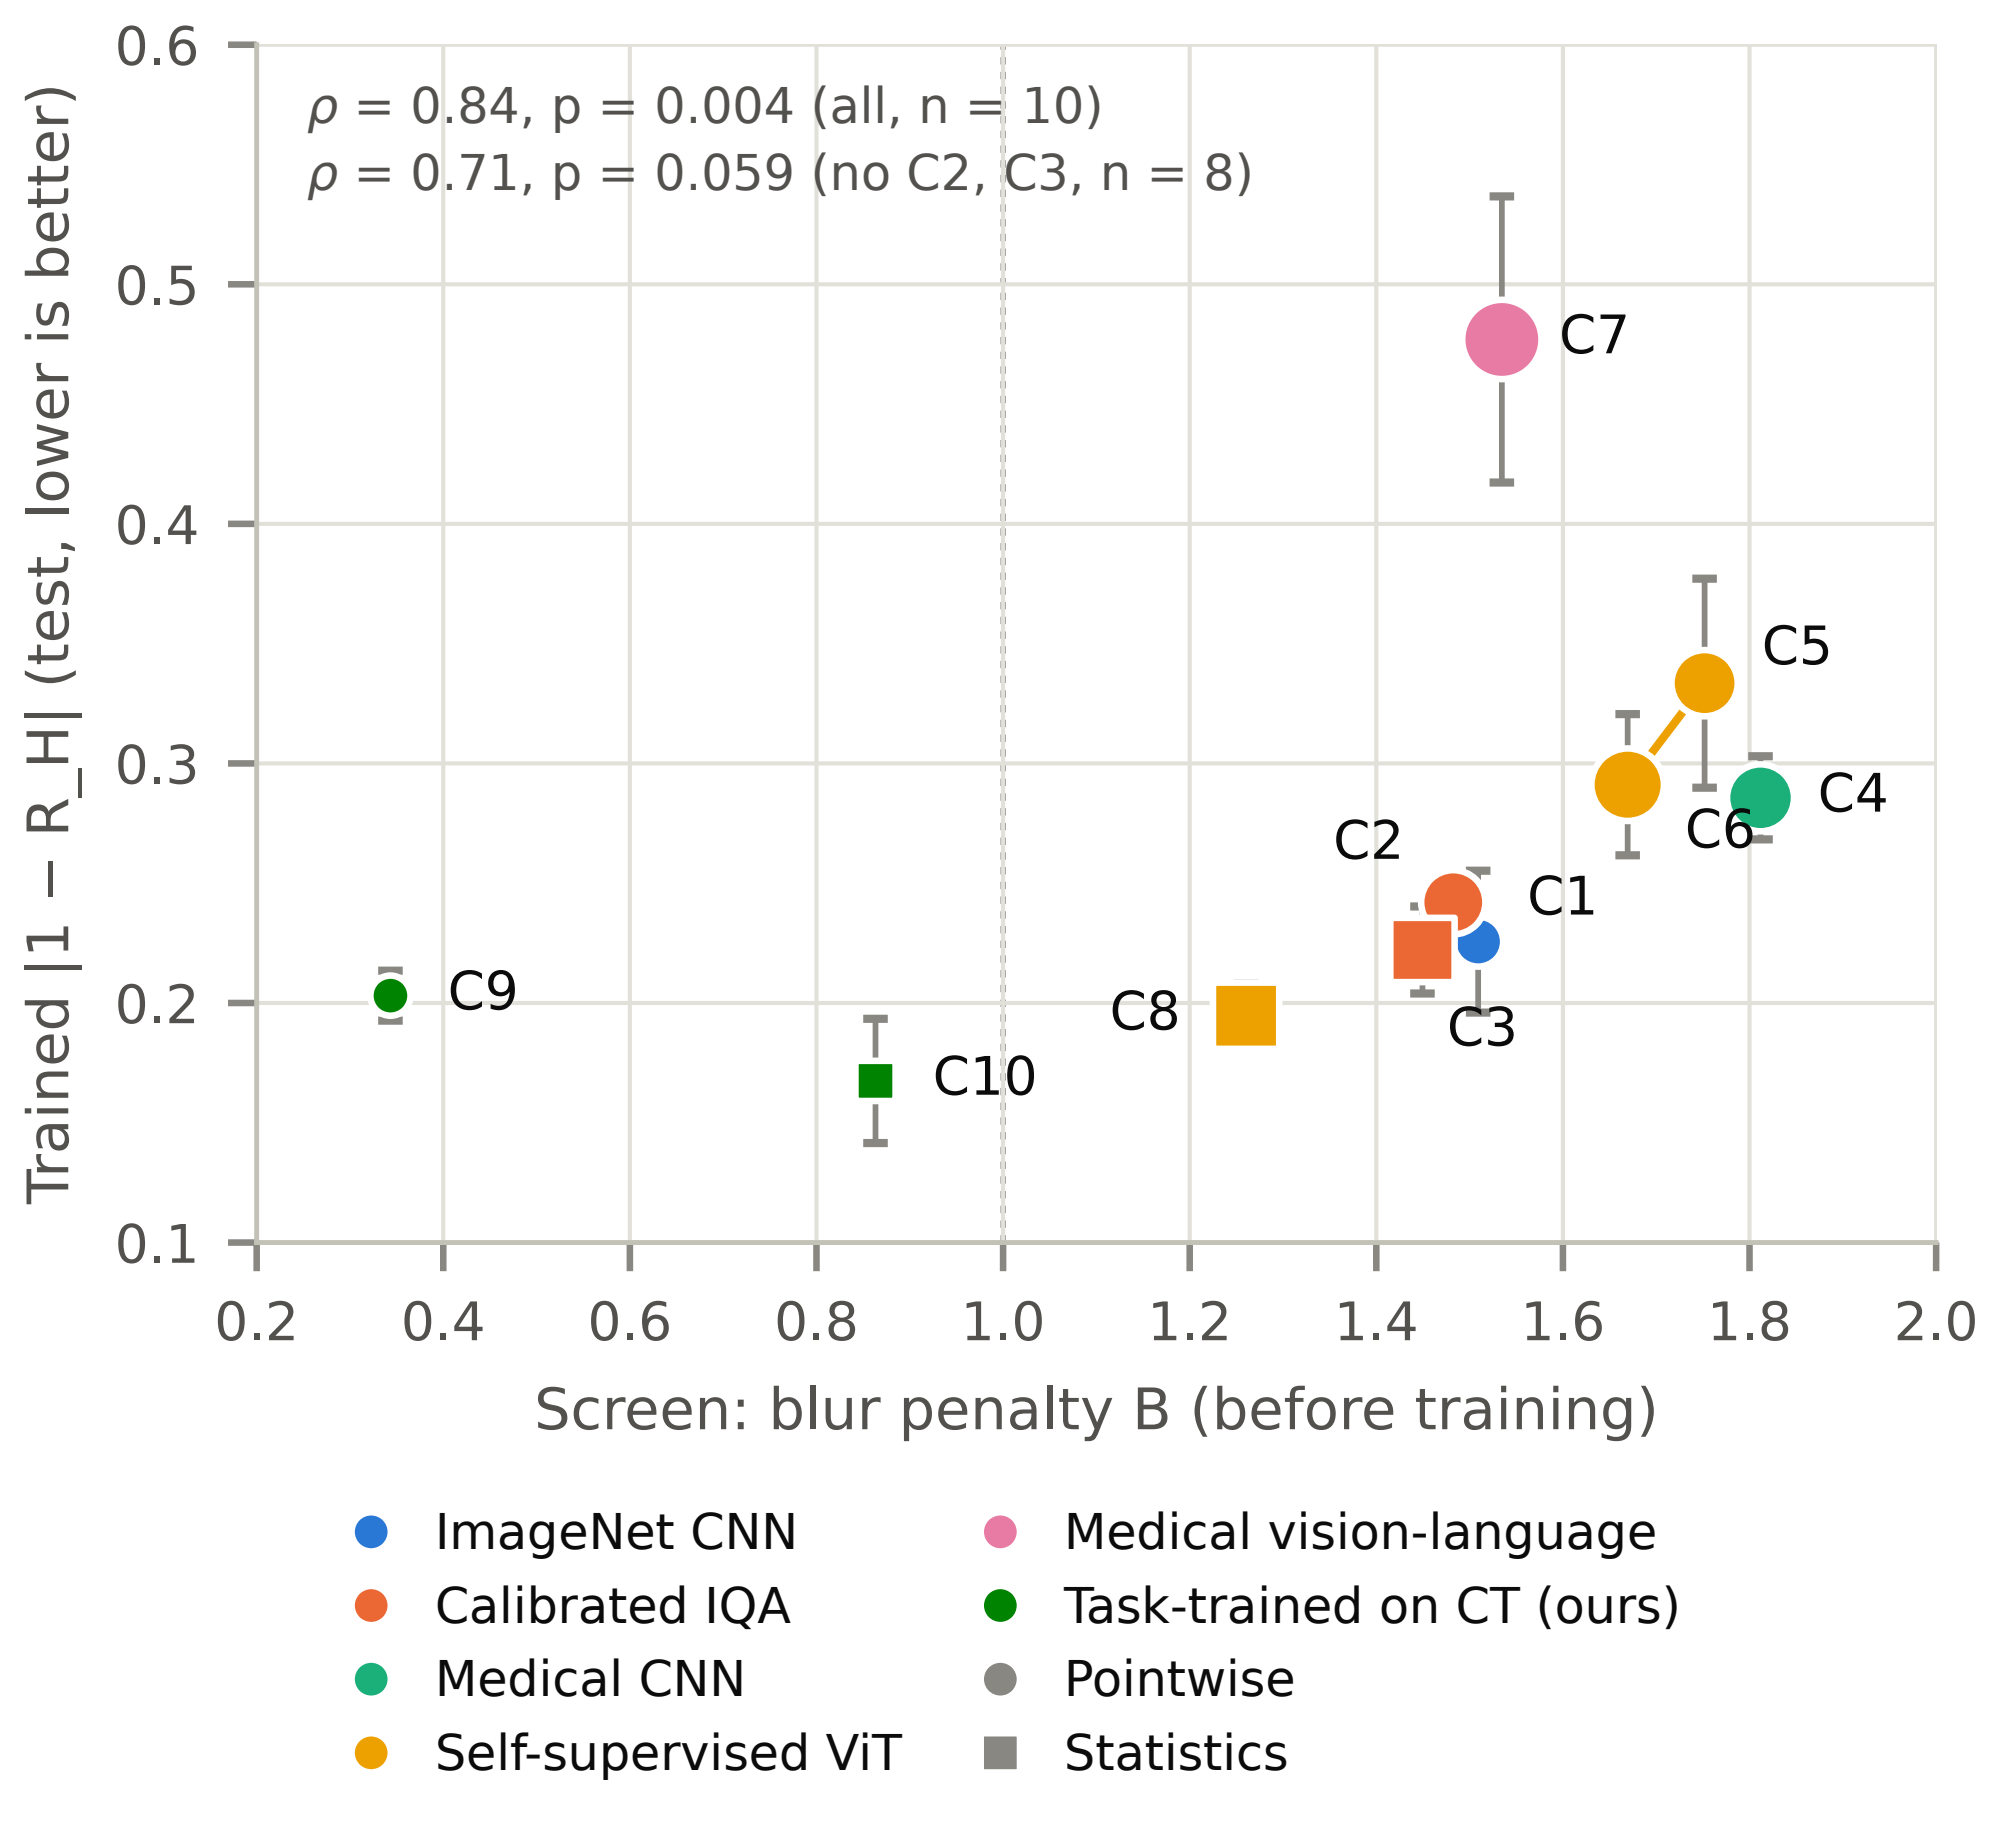
ρ = 0.84, p = 0.004 (all, n = 10)
ρ = 0.71, p = 0.059 (no C2, C3, n = 8)
Trained |1 − R_H| (test, lower is better)
Screen: blur penalty B (before training)
0.6
0.5
0.4
0.3
0.2
0.1
0.2
0.4
0.6
0.8
1.0
1.2
1.4
1.6
1.8
2.0
C7
C5
C4
C6
C2
C1
C3
C8
C9
C10
ImageNet CNN
Calibrated IQA
Medical CNN
Self-supervised ViT
Medical vision-language
Task-trained on CT (ours)
Pointwise
Statistics