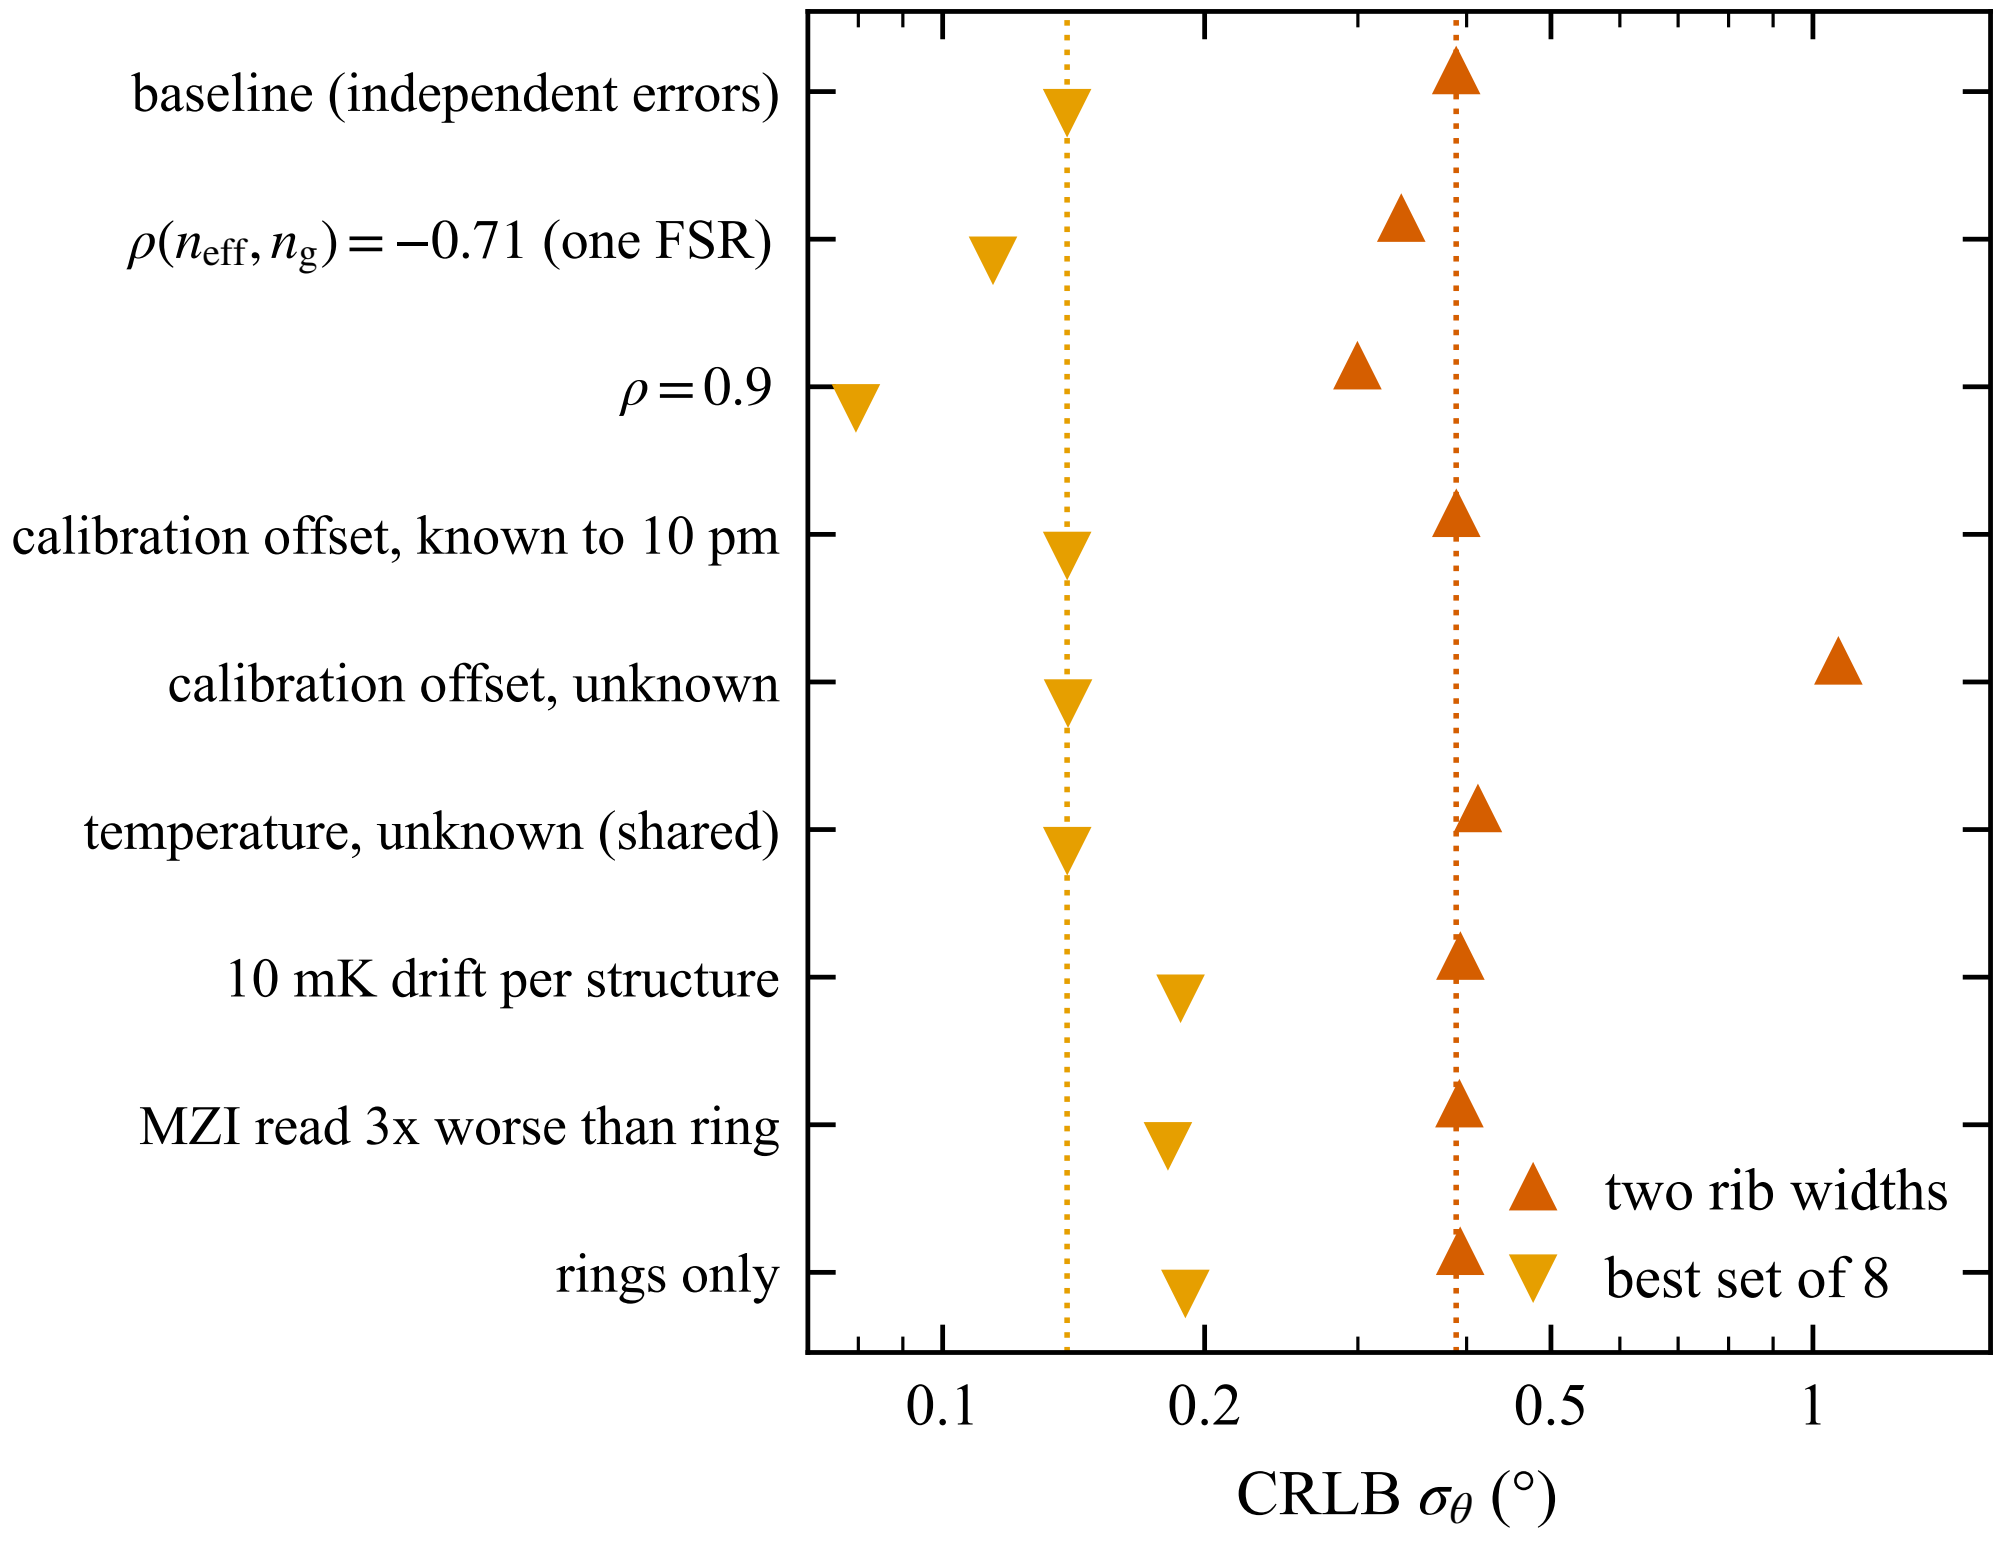
baseline (independent errors)
$\rho(n_{\mathrm{eff}}, n_{\mathrm{g}}) = -0.71$ (one FSR)
$\rho = 0.9$
calibration offset, known to 10 pm
calibration offset, unknown
temperature, unknown (shared)
10 mK drift per structure
MZI read 3x worse than ring
rings only
two rib widths
best set of 8
0.1
0.2
0.5
1
CRLB σ_θ (°)