

Case summary

Incident ID: 23-06788
Patient ID: 2023030813142100-LP1547545197
Patient Name: Ford

Patient ID:	<u>2023030813142100-LP1547545197</u>	Birth Date:	
Incident ID:	<u>23-06788</u>	Device ID:	<u>MICU 66</u>
Age at Incident:	<u>57 Years</u>	Case Start Date:	<u>3/8/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>1:14:22 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Case Summary:

Total Analyses: 0
Total Shocks: 2
Total 12-Leads: 0
Total Time Paced: 00:00:00

Notes:

Demos
1:05 pulse check
Updated at 4/8/2023 9:10:11 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)3

 CPR report (by CPR period)3


CPR report



Device Type: LIFEPAK® 15
 Power On: 3/8/2023 1:14:22 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RO40200UR
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.


Duration: 00:59:01
 Incident ID: 23-06788
 Statistical Parameters: 1000-0300-3000-05

Compression ratio
(/total time)




26:31 / 30:25 = 87 %

Compression rate




153/minute

Ventilations/minute




7/minute

Initial Rhythm

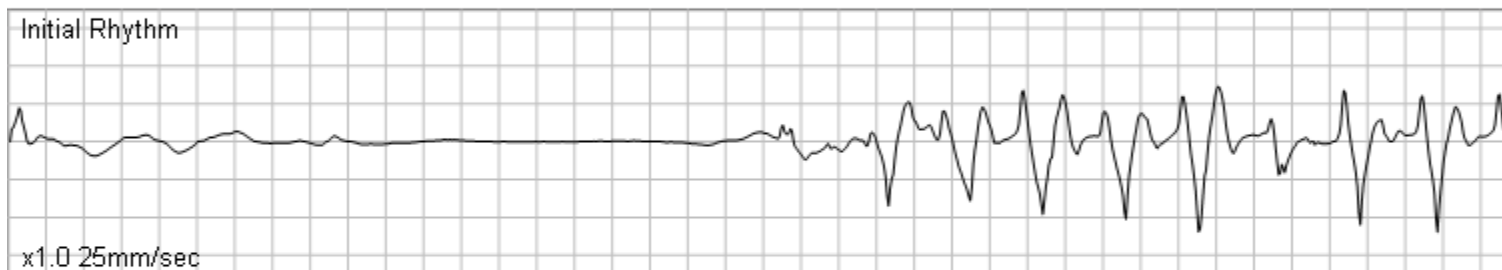

CO2 (mmHg)

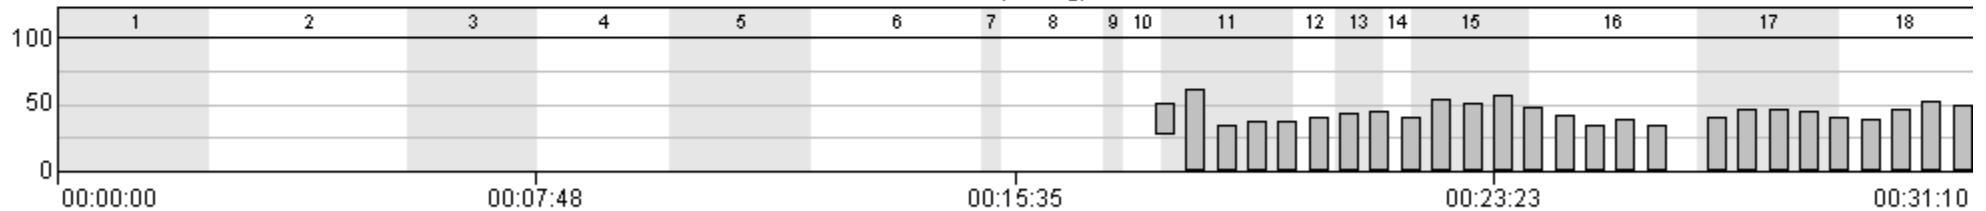

CPR report



Device Type: LIFEPAK® 15
Power On: 3/8/2023 1:14:22 PM
CPR Annotations Edited: Yes
Device Configuration: 2L355RO40200UR
*Non-paddles lead intervals are included in the reported CPR Ratio
*Times have been adjusted by the system.

Duration: 00:59:01
Incident ID: 23-06788
Statistical Parameters: 1000-0300-3000-05

Summary

CPR needed	= 31:10	CPR done	= 26:56
CPR not done	= 4:14	Compression count	= 3944
Longest compression pause	= 1:05	Pauses over 10 sec	= 9
Comment	Avg compression rate 153. Long pre-shock pauses. Precharge monitor. Tighten up 2 minute cycles.		

CPR report



Device Type: LIFEPAK® 15
 Power On: 3/8/2023 1:14:22 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RO40200UR
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 00:59:01
 Incident ID: 23-06788
 Statistical Parameters: 1000-0300-3000-05

Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:02:20	00:02:20	00:00:08	Pulse/rhythm check		92	143	--
2		00:02:28	00:05:28	00:02:59	00:00:13	Pulse/rhythm check		93	148	--
3		00:05:40	00:07:35	00:01:54	00:00:14	Pulse/rhythm check		99	151	--
4		00:07:48	00:09:50	00:02:02	00:00:08	Pulse/rhythm check		94	146	--
5		00:09:58	00:11:49	00:01:52	00:00:26	Pulse/rhythm check		90	157	--
6		00:12:16	00:14:48	00:02:33	00:00:14	Pulse/rhythm check		88	147	--
7		00:15:02	00:15:07	00:00:05	00:00:15	Defibrillation	Long pre pause	29	159	--
8		00:15:22	00:15:57	00:00:35	00:01:05	Unknown		35	162	--
9		00:17:02	00:17:09	00:00:07	00:00:12	Unknown		38	150	--
10		00:17:21	00:17:53	00:00:32	00:00:04	Unknown		84	160	--
11		00:17:57	00:19:50	00:01:53	00:00:16	Pulse/rhythm check		87	157	8
12		00:20:06	00:20:38	00:00:31	00:00:10	Unknown		77	158	7
13		00:20:48	00:21:25	00:00:37	00:00:10	Unknown		89	160	6
14		00:21:35	00:21:57	00:00:22	00:00:04	Unknown		87	166	--
15		00:22:02	00:23:49	00:01:47	00:00:09	Pulse/rhythm check		93	153	7
16		00:23:58	00:26:26	00:02:28	00:00:15	Defibrillation	Long pre pause	86	156	7
17		00:26:41	00:28:49	00:02:08	00:00:11	Pulse/rhythm check		92	172	5
18		00:29:00	00:31:10	00:02:10	00:00:00	Termination/Transfer of Care		100	154	6

Ventilation

Chest compression

AED-prompted CPR period

AED Analysis

Shock

ROSC (user annotated)


CPR report



Device Type: LIFEPAK® 15
 Power On: 3/8/2023 1:14:22 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R040200UR
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 00:59:01
 Incident ID: 23-06788
 Statistical Parameters: 1000-0300-3000-05

CPR QUIK-VIEW

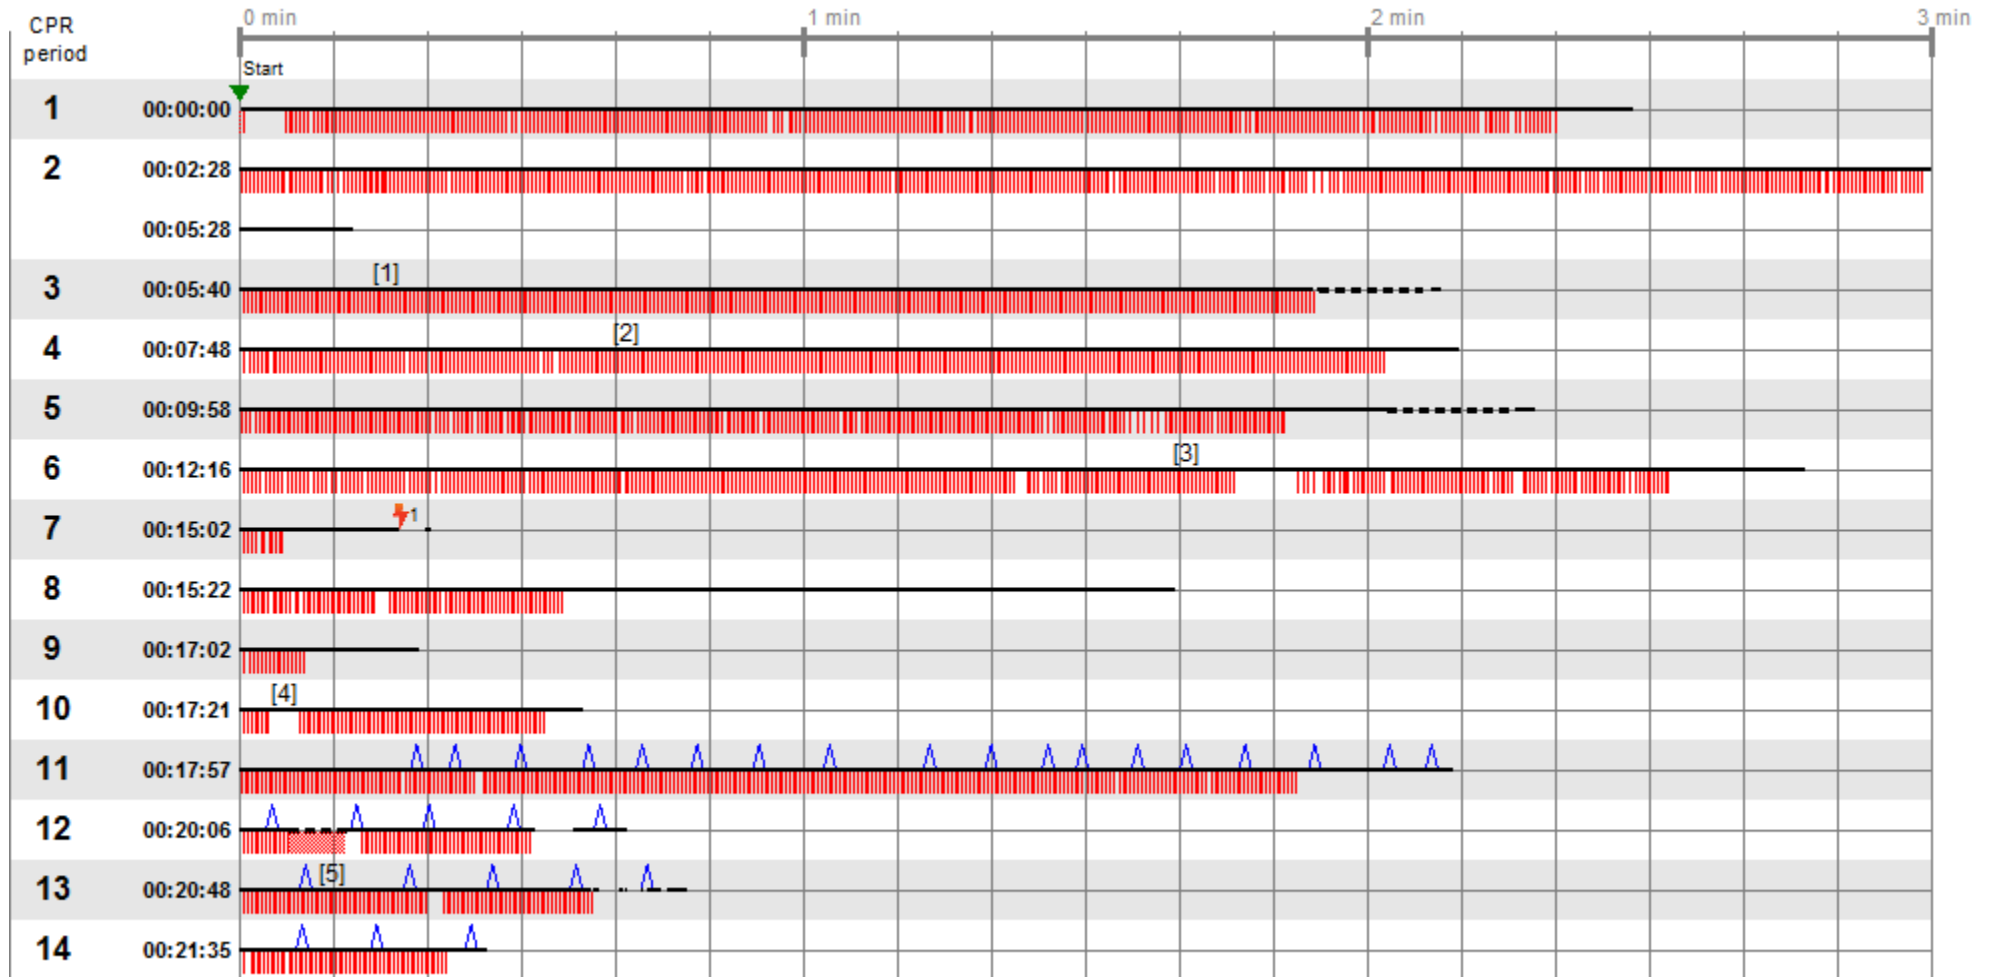


CPR report



Device Type: LIFEPAK® 15
 Power On: 3/8/2023 1:14:22 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R040200UR
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 00:59:01
 Incident ID: 23-06788
 Statistical Parameters: 1000-0300-3000-05

CPR QUIK-VIEW

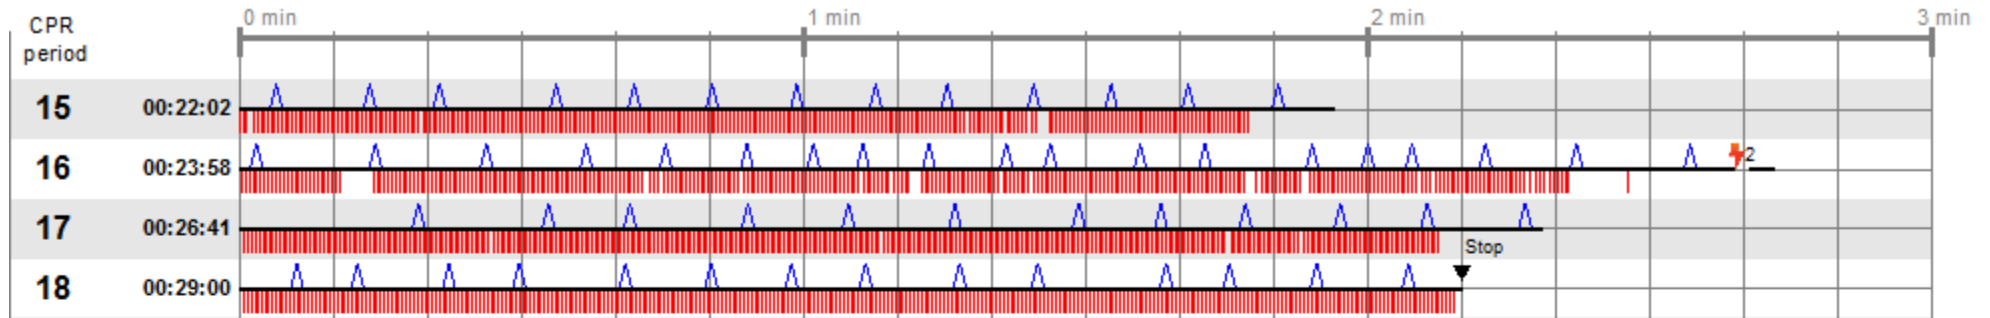

[1] EPINEPHRINE 10, [2] EPINEPHRINE 10, [3] EPINEPHRINE 10, [4] EPINEPHRINE 10, [5] EPINEPHRINE 10

Shock	Time	Energy	Pre-shock CPR pause	Post-shock CPR pause
⚡1	15:19	360 J	0:12	0:03
⚡2	26:37	360 J	0:11	0:04