

Case summary

Incident ID: 23-04554
Patient ID: 2023021413591100-LP1547559024
Patient Name: Bailey

| | | | |
|------------------|--------------------------------------|------------------|-----------------------------|
| Patient ID: | <u>2023021413591100-LP1547559024</u> | Birth Date: | |
| Incident ID: | <u>23-04554</u> | Device ID: | <u>MICU103</u> |
| Age at Incident: | <u>78 Years</u> | Case Start Date: | <u>2/14/2023</u> |
| Sex: | <u>Female</u> | Case Start Time: | <u>1:59:09 PM</u> |
| Race: | <u>Unspecified</u> | Time Adjustment: | <u>System Adjusted Time</u> |

Notes:

*** 167 rate, impressive
Updated at 3/13/2023 1:17:55 AM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)3

 CPR report (by CPR period)3

CPR report




Device Type: LIFEPAK® 15
Power On: 2/14/2023 1:59:09 PM
CPR Annotations Edited: Yes
Device Configuration: 2L355R0402000R

Duration: 18:00:52
Incident ID: 23-04554
Statistical Parameters: 1000-0300-3000-05


*Times have been adjusted by the system.

Compression ratio
(/total time)




29:16 / 33:57 = 86 %

Compression rate





167/minute

Ventilations/minute



5/minute

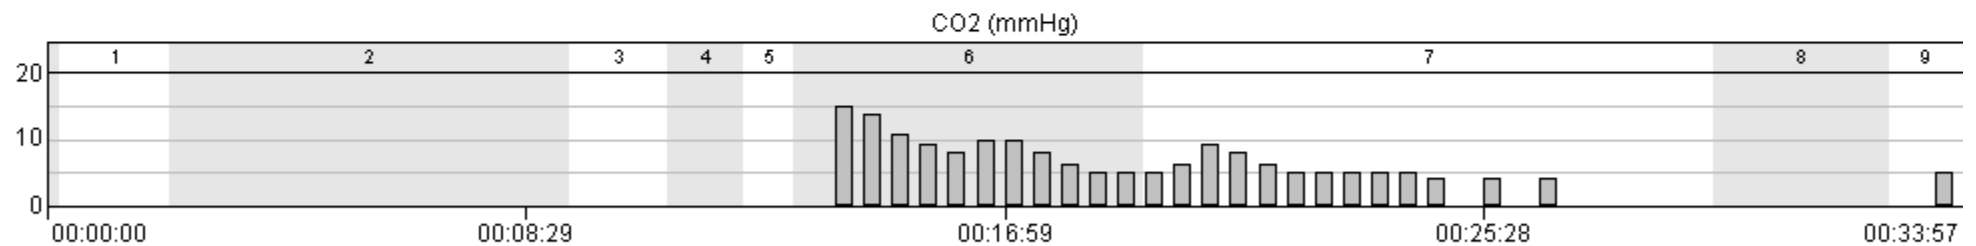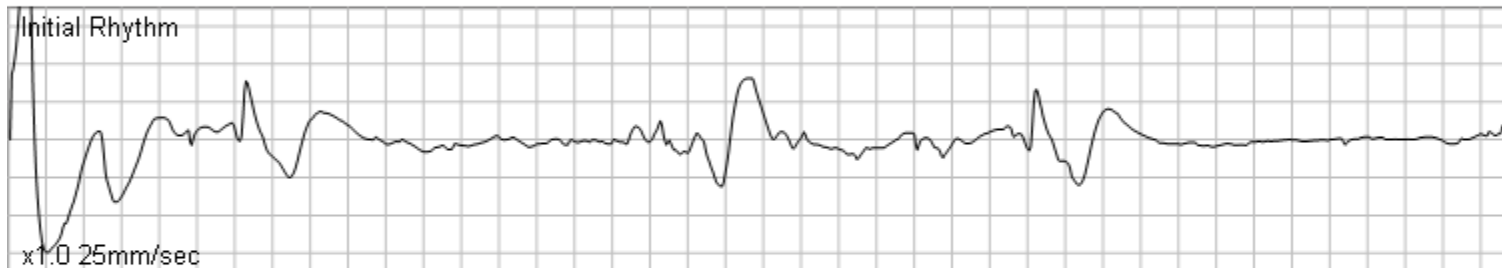

CPR report



Device Type: LIFEPAK® 15
 Power On: 2/14/2023 1:59:09 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R0402000R

Duration: 18:00:52
 Incident ID: 23-04554
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Summary

| | | | |
|---------------------------|---------|--------------------|---------|
| CPR needed | = 33:57 | CPR done | = 30:44 |
| CPR not done | = 3:13 | Compression count | = 4614 |
| Longest compression pause | = 0:59 | Pauses over 10 sec | = 8 |

Comment

Interval Statistics

| CPR period | Responsible for CPR | CPR started | CPR stopped | CPR duration | Pause duration | Reason CPR stopped | Comments | Compr. ratio, % | Compr. rate | Vent. /min |
|------------|---------------------|-------------|-------------|--------------|----------------|--------------------|----------|-----------------|-------------|------------|
| 1 | | 00:00:12 | 00:02:00 | 00:01:47 | 00:00:10 | | | 88 | 171 | -- |
| 2 | | 00:02:10 | 00:09:04 | 00:06:55 | 00:00:10 | | | 95 | 180 | -- |
| 3 | | 00:09:14 | 00:10:00 | 00:00:45 | 00:00:59 | | | 43 | 163 | -- |
| 4 | | 00:10:59 | 00:11:51 | 00:00:53 | 00:00:29 | | | 61 | 148 | -- |
| 5 | | 00:12:20 | 00:12:59 | 00:00:39 | 00:00:14 | | | 74 | 143 | -- |
| 6 | | 00:13:13 | 00:19:06 | 00:05:53 | 00:00:19 | | | 83 | 155 | 5 |
| 7 | | 00:19:25 | 00:29:22 | 00:09:58 | 00:00:09 | | | 96 | 165 | 1 |
| 8 | | 00:29:32 | 00:32:10 | 00:02:38 | 00:00:30 | | | 77 | 168 | -- |
| 9 | | 00:32:40 | 00:33:57 | 00:01:17 | 00:00:00 | | | 99 | 159 | -- |



Ventilation



Chest compression

AED-prompted CPR period



AED Analysis



Shock



ROSC (user annotated)

CPR report




Device Type: LIFEPAK® 15
 Power On: 2/14/2023 1:59:09 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R0402000R

Duration: 18:00:52
 Incident ID: 23-04554
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

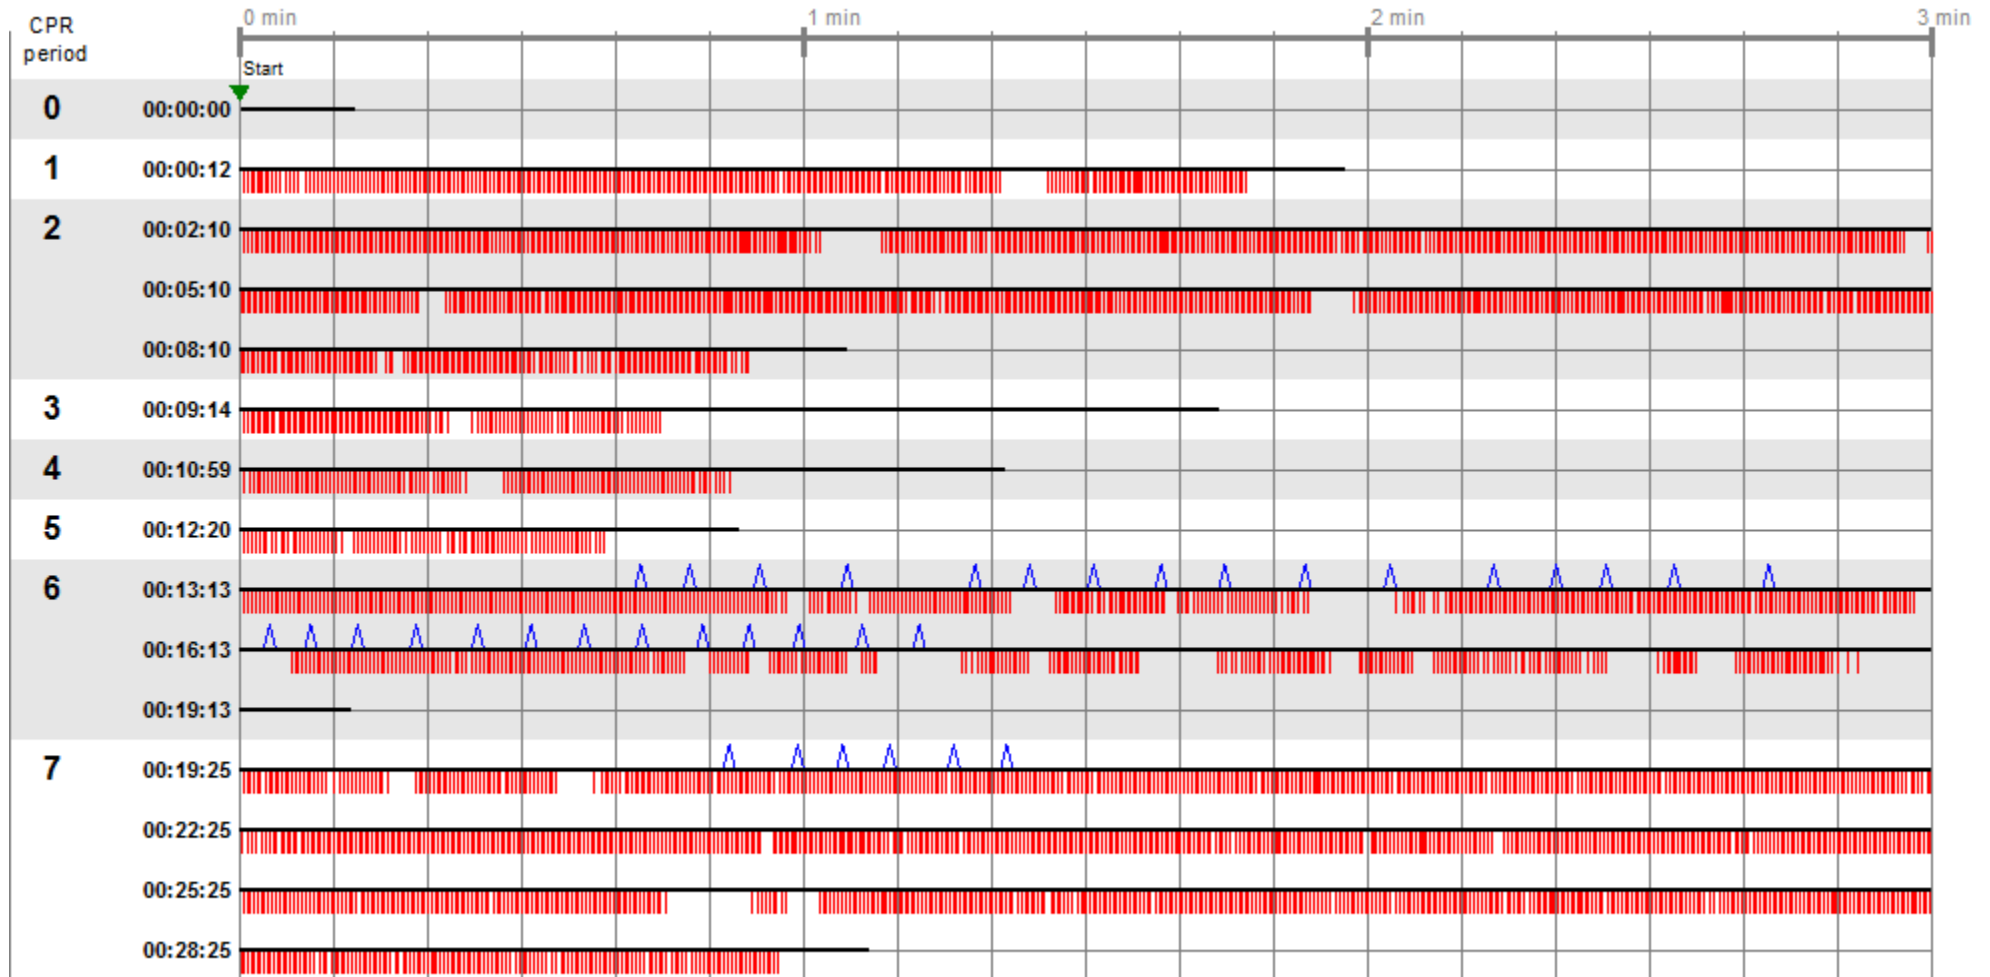

CPR report

| | | | | |
|--|--|----------------------|-------------------------|-------------------|
|  | Device Type: | LIFEPAK® 15 | Duration: | 18:00:52 |
| | Power On: | 2/14/2023 1:59:09 PM | Incident ID: | 23-04554 |
| | CPR Annotations Edited: | Yes | Statistical Parameters: | 1000-0300-3000-05 |
| | Device Configuration: | 2L355R0402000R | | |
| | *Times have been adjusted by the system. | | | |

