

Case summary

Incident ID: 23-06652
Patient ID: 2023030721264000-LP1547545197
Patient Name: Jones

Patient ID:	<u>2023030721264000-LP1547545197</u>	Birth Date:	
Incident ID:	<u>23-06652</u>	Device ID:	<u>MICU 66</u>
Age at Incident:	<u>72 Years</u>	Case Start Date:	<u>3/7/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>9:26:40 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Notes:

Demos

Updated at 4/8/2023 9:04:52 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)3

 CPR report (by CPR period)3

CPR report




Device Type: LIFEPAK® 15
 Power On: 3/7/2023 9:26:40 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R040200UR

Duration: 00:18:47
 Incident ID: 23-06652
 Statistical Parameters: 1000-0300-3000-05


*Times have been adjusted by the system.

Compression ratio
 (/total time)




15:35 / 16:42 = 93 %

Compression rate




113/minute


Ventilations/minute



4/minute

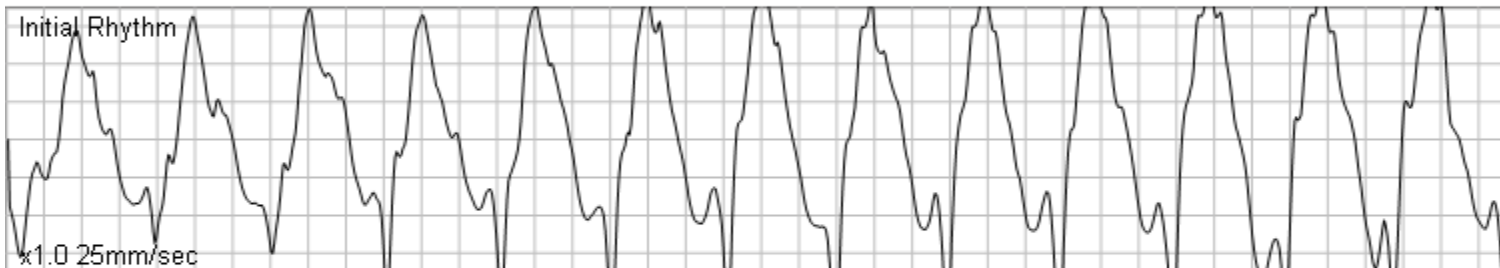

CO2 (mmHg)

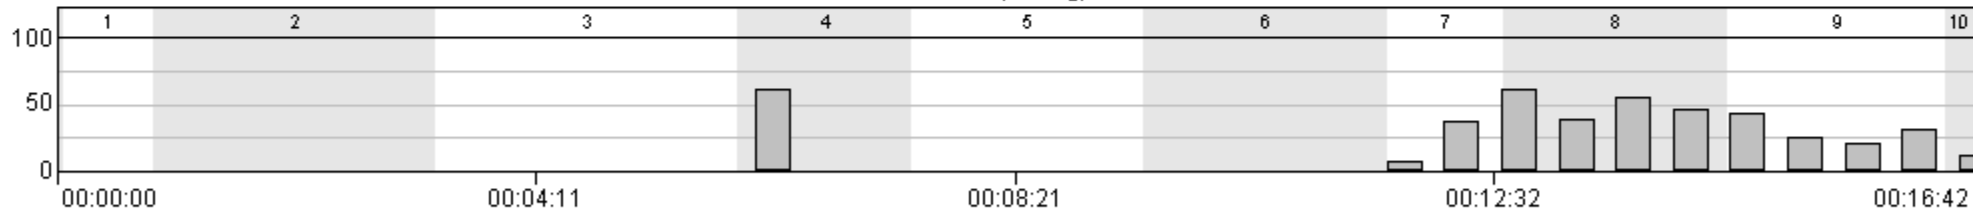

CPR report



Device Type: LIFEPAK® 15
 Power On: 3/7/2023 9:26:40 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RO40200UR

Duration: 00:18:47
 Incident ID: 23-06652
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Summary

CPR needed	= 16:42	CPR done	= 15:31
CPR not done	= 1:11	Compression count	= 1751
Longest compression pause	= 0:17	Pauses over 10 sec	= 3

Comment: Good overall, couple of longer pauses and 2 minute cycles could be better.

Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:00:47	00:00:47	00:00:03	Pulse/rhythm check		96	102	--
2		00:00:50	00:03:15	00:02:25	00:00:02	Pulse/rhythm check		100	109	--
3		00:03:17	00:05:43	00:02:26	00:00:13	Pulse/rhythm check		90	115	--
4		00:05:56	00:07:25	00:01:29	00:00:01	Pulse/rhythm check		100	137	1
5		00:07:27	00:09:11	00:01:45	00:00:17	Pulse/rhythm check		86	117	--
6		00:09:28	00:11:27	00:01:59	00:00:09	Pulse/rhythm check		94	106	--
7		00:11:36	00:12:24	00:00:49	00:00:12	Unknown		80	112	3
8		00:12:36	00:14:28	00:01:52	00:00:06	Pulse/rhythm check		96	112	9
9		00:14:33	00:16:20	00:01:47	00:00:08	Pulse/rhythm check		94	116	8
10		00:16:28	00:16:42	00:00:13	00:00:00			96	125	--

Ventilation

Chest compression

AED-prompted CPR period

AED Analysis

Shock

ROSC (user annotated)

CPR report




Device Type: LIFEPAK® 15
 Power On: 3/7/2023 9:26:40 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R040200UR

Duration: 00:18:47
 Incident ID: 23-06652
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

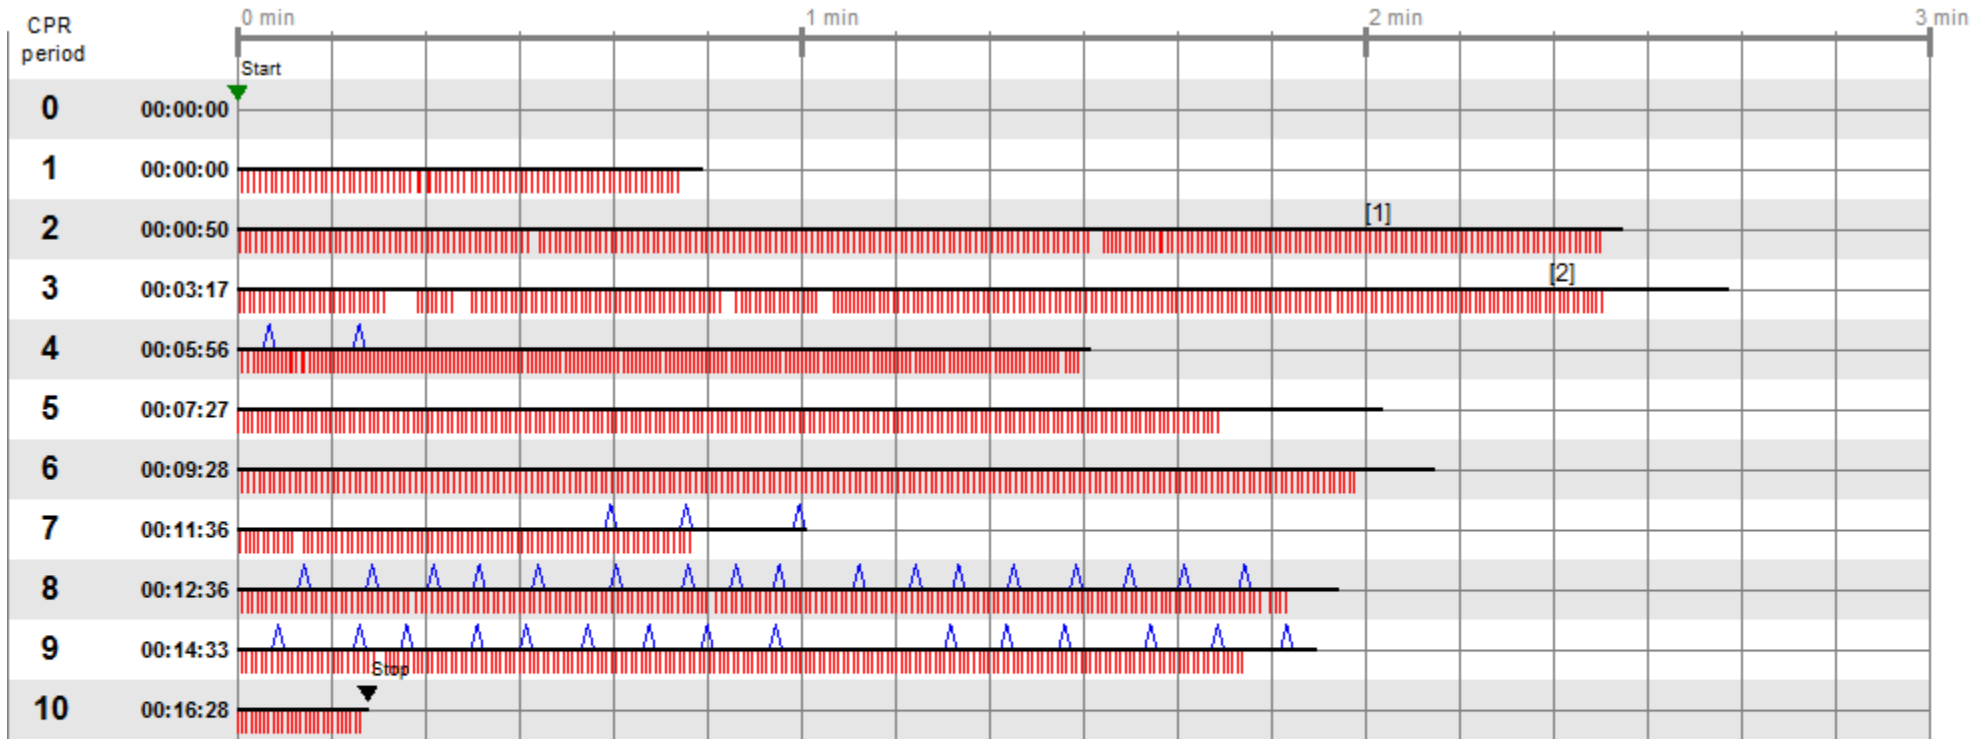

[1] EPINEPHRINE 10, [2] EPINEPHRINE 10