

## Case summary

Incident ID: 23-07690  
Patient ID: 2023031712100700-LP1547542357  
Patient Name: Twyman

Patient ID:	<u>2023031712100700-LP1547542357</u>	Birth Date:	
Incident ID:	<u>23-07690</u>	Device ID:	<u>LP152357</u>
Age at Incident:	<u>29 Years</u>	Case Start Date:	<u>3/17/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>12:10:07 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

### Notes:

Demos

Updated at 4/8/2023 9:41:44 PM by zphillips (Zach Phillips).

### Comments:

# Table of Contents

CPR reports (by CPR period) .....3

    CPR report (by CPR period) .....3

## CPR report




Device Type: LIFEPAK® 15  
Power On: 3/17/2023 12:10:07 PM  
CPR Annotations Edited: Yes  
Device Configuration: 2L355RRB0200UR

Duration: 00:24:28  
Incident ID: 23-07690  
Statistical Parameters: 1000-0300-3000-05


\*Times have been adjusted by the system.

Compression ratio  
(/total time)




20:16 / 22:46 = 89 %

Compression rate




126/minute

Ventilations/minute




5/minute

Initial Rhythm

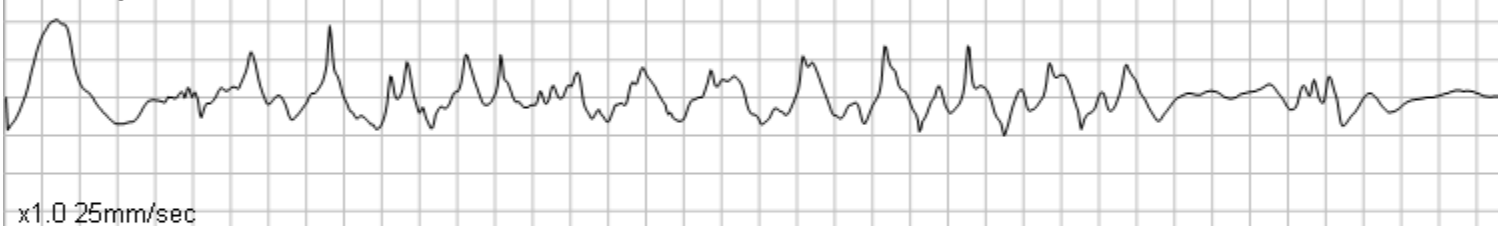

CO2 (mmHg)

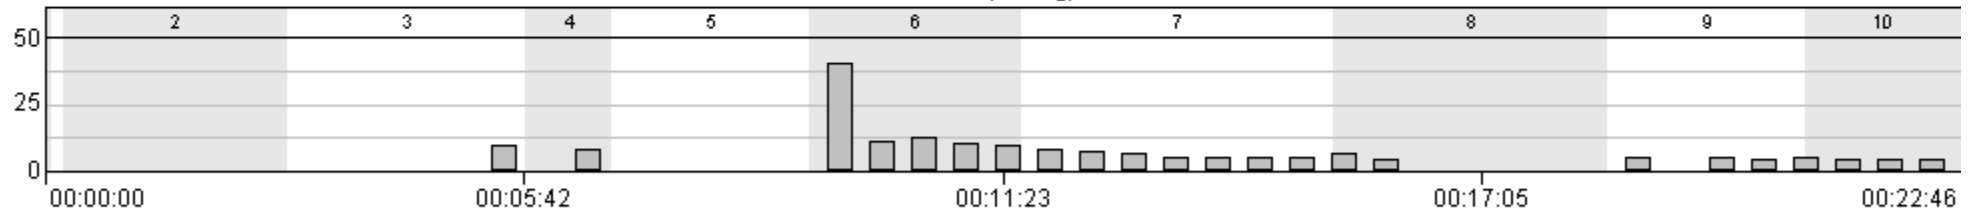

## CPR report



Device Type: LIFEPAK® 15  
 Power On: 3/17/2023 12:10:07 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2L355RRB0200UR

Duration: 00:24:28  
 Incident ID: 23-07690  
 Statistical Parameters: 1000-0300-3000-05

\*Times have been adjusted by the system.

### Summary

CPR needed	= 22:46	CPR done	= 20:15
CPR not done	= 2:31	Compression count	= 2450
Longest compression pause	= 0:52	Pauses over 10 sec	= 5

Comment: 2 possible VF not shocked. Long pauses for pulse checks. Work on 2 minute cycles.

### Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:02	00:00:06	00:00:04	00:00:06	Pulse/rhythm check		45	134	--
2		00:00:12	00:02:38	00:02:26	00:00:14	Pulse/rhythm check		92	139	--
3		00:02:52	00:04:50	00:01:58	00:00:52	Pulse/rhythm check		69	141	1
4		00:05:42	00:06:27	00:00:45	00:00:16	Unknown		73	104	1
5		00:06:43	00:08:38	00:01:55	00:00:26	Pulse/rhythm check		82	104	--
6		00:09:04	00:11:27	00:02:22	00:00:09	Pulse/rhythm check		94	103	11
7		00:11:36	00:15:10	00:03:34	00:00:08	Pulse/rhythm check		97	126	--
8		00:15:18	00:18:27	00:03:09	00:00:07	Pulse/rhythm check		96	115	--
9		00:18:34	00:20:45	00:02:11	00:00:10	Pulse/rhythm check		93	134	--
10		00:20:55	00:22:46	00:01:51	00:00:00	Termination/Transfer of Care		100	134	--

Ventilation

Chest compression

AED-prompted CPR period

AED Analysis

Shock

ROSC (user annotated)

# CPR report




Device Type: LIFEPAK® 15  
 Power On: 3/17/2023 12:10:07 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2L355RRB0200UR

Duration: 00:24:28  
 Incident ID: 23-07690  
 Statistical Parameters: 1000-0300-3000-05

\*Times have been adjusted by the system.

## CPR QUIK-VIEW

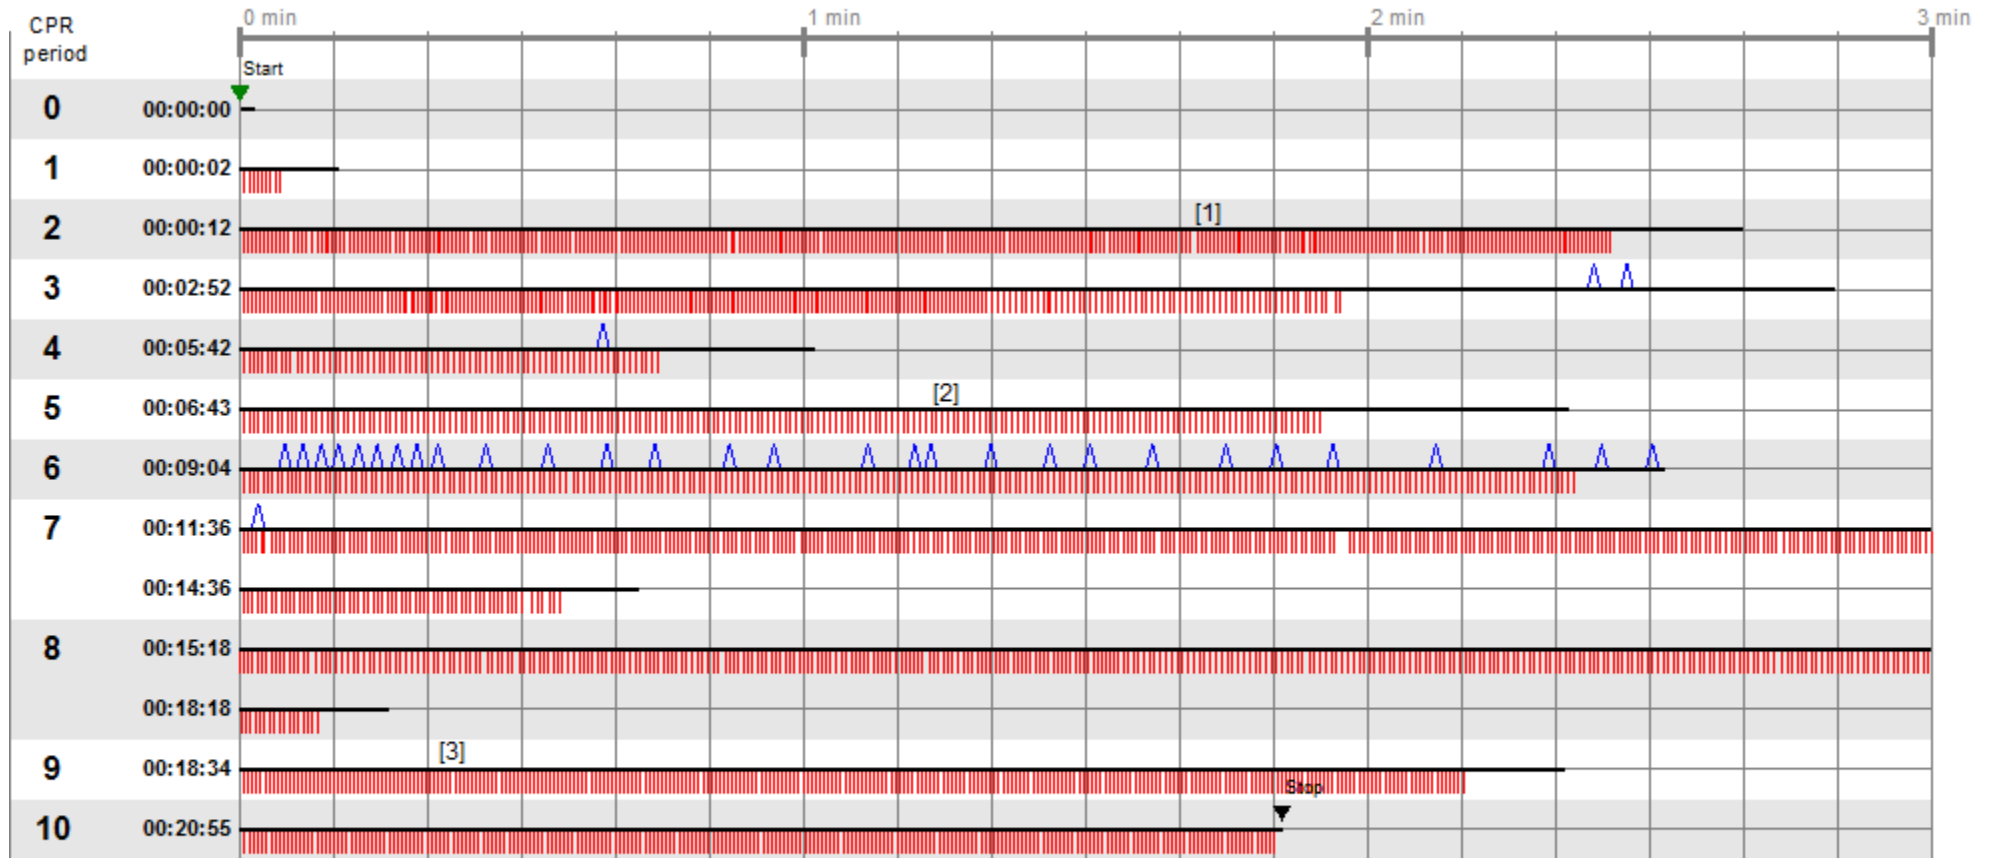

[1] Epinephrine, [2] Epinephrine, [3] Epinephrine, [4] Generic