

Case summary

Incident ID: 23-05481
Patient ID: 2023022322094600-LP1547542357
Patient Name: Heavens

Patient ID:	<u>2023022322094600-LP1547542357</u>	Birth Date:	
Incident ID:	<u>23-05481</u>	Device ID:	<u>LP152357</u>
Age at Incident:	<u>62 Years</u>	Case Start Date:	<u>2/23/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>10:09:47 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Notes:

Summary complete.
Demos only
Updated at 3/13/2023 1:48:10 AM by zphillips (Zach Phillips).
Updated at 3/29/2023 4:45:00 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)	3
CPR report (by CPR period)	3

CPR report




Device Type: LIFEPAK® 15
Power On: 2/23/2023 10:09:47 PM
CPR Annotations Edited: Yes
Device Configuration: 2L355RRB0200UR

Duration: 00:21:44
Incident ID: 23-05481
Statistical Parameters: 1000-0300-3000-05


*Times have been adjusted by the system.

Compression ratio
(/total time)




17:00 / 18:52 = 90 %

Compression rate





125/minute

Ventilations/minute



9/minute

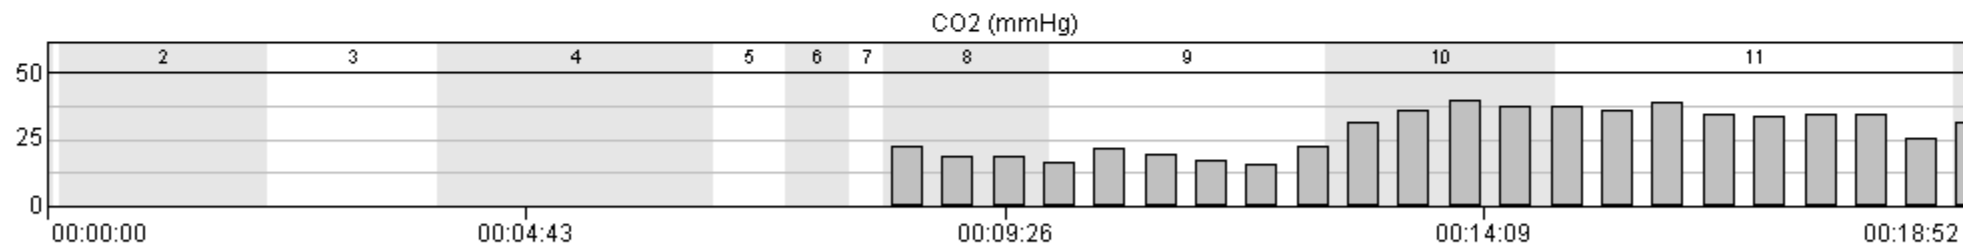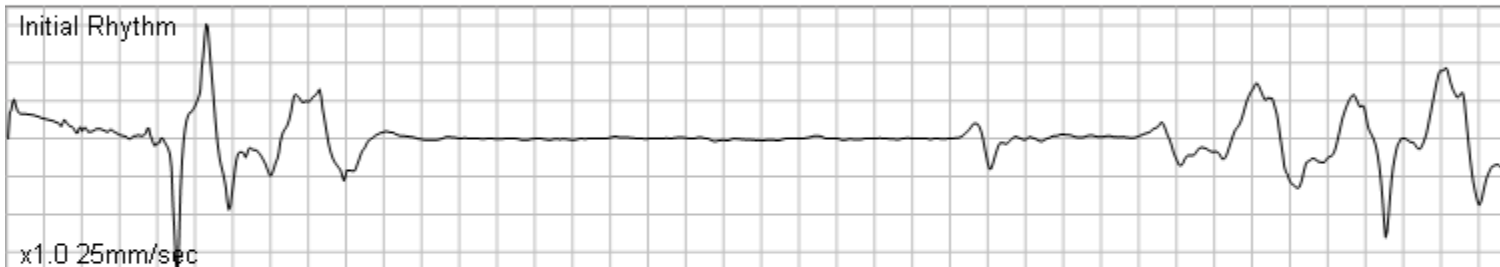

CPR report



Device Type: LIFEPAK® 15
 Power On: 2/23/2023 10:09:47 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RRB0200UR

Duration: 00:21:44
 Incident ID: 23-05481
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Summary

CPR needed	= 18:52	CPR done	= 16:55
CPR not done	= 1:56	Compression count	= 2061
Longest compression pause	= 0:25	Pauses over 10 sec	= 4

Comment: Compression rate slightly fast.

Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:00:02	00:00:02	00:00:05	Pulse/rhythm check	Initial check	35	--	--
2		00:00:07	00:02:07	00:02:00	00:00:02	Pulse/rhythm check		100	122	--
3		00:02:09	00:03:41	00:01:32	00:00:09	Pulse/rhythm check	Aim for 2 min	91	140	--
4		00:03:50	00:06:20	00:02:30	00:00:12	Pulse/rhythm check	Aim for 2 min	92	127	--
5		00:06:33	00:07:02	00:00:29	00:00:14	Pulse/rhythm check	Not sure why not continuous	67	132	--
6		00:07:16	00:07:37	00:00:21	00:00:17	Pulse/rhythm check	Not sure why not continuous	55	131	--
7		00:07:53	00:08:05	00:00:12	00:00:08	Pulse/rhythm check		61	132	--
8		00:08:13	00:09:48	00:01:35	00:00:04	Pulse/rhythm check		97	129	9
9		00:09:52	00:12:25	00:02:34	00:00:10	Pulse/rhythm check	Rhythm change	94	108	10
10		00:12:35	00:14:42	00:02:07	00:00:10	Pulse/rhythm check		93	125	9
11		00:14:51	00:18:21	00:03:30	00:00:25	Pulse/rhythm check	Long change	89	122	8
12		00:18:46	00:18:51	00:00:05	00:00:00	Termination/Transfer of Care		90	125	--

Ventilation

Chest compression

AED-prompted CPR period

AED Analysis

Shock

ROSC (user annotated)

CPR report




Device Type: LIFEPAK® 15
 Power On: 2/23/2023 10:09:47 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RRB0200UR

Duration: 00:21:44
 Incident ID: 23-05481
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

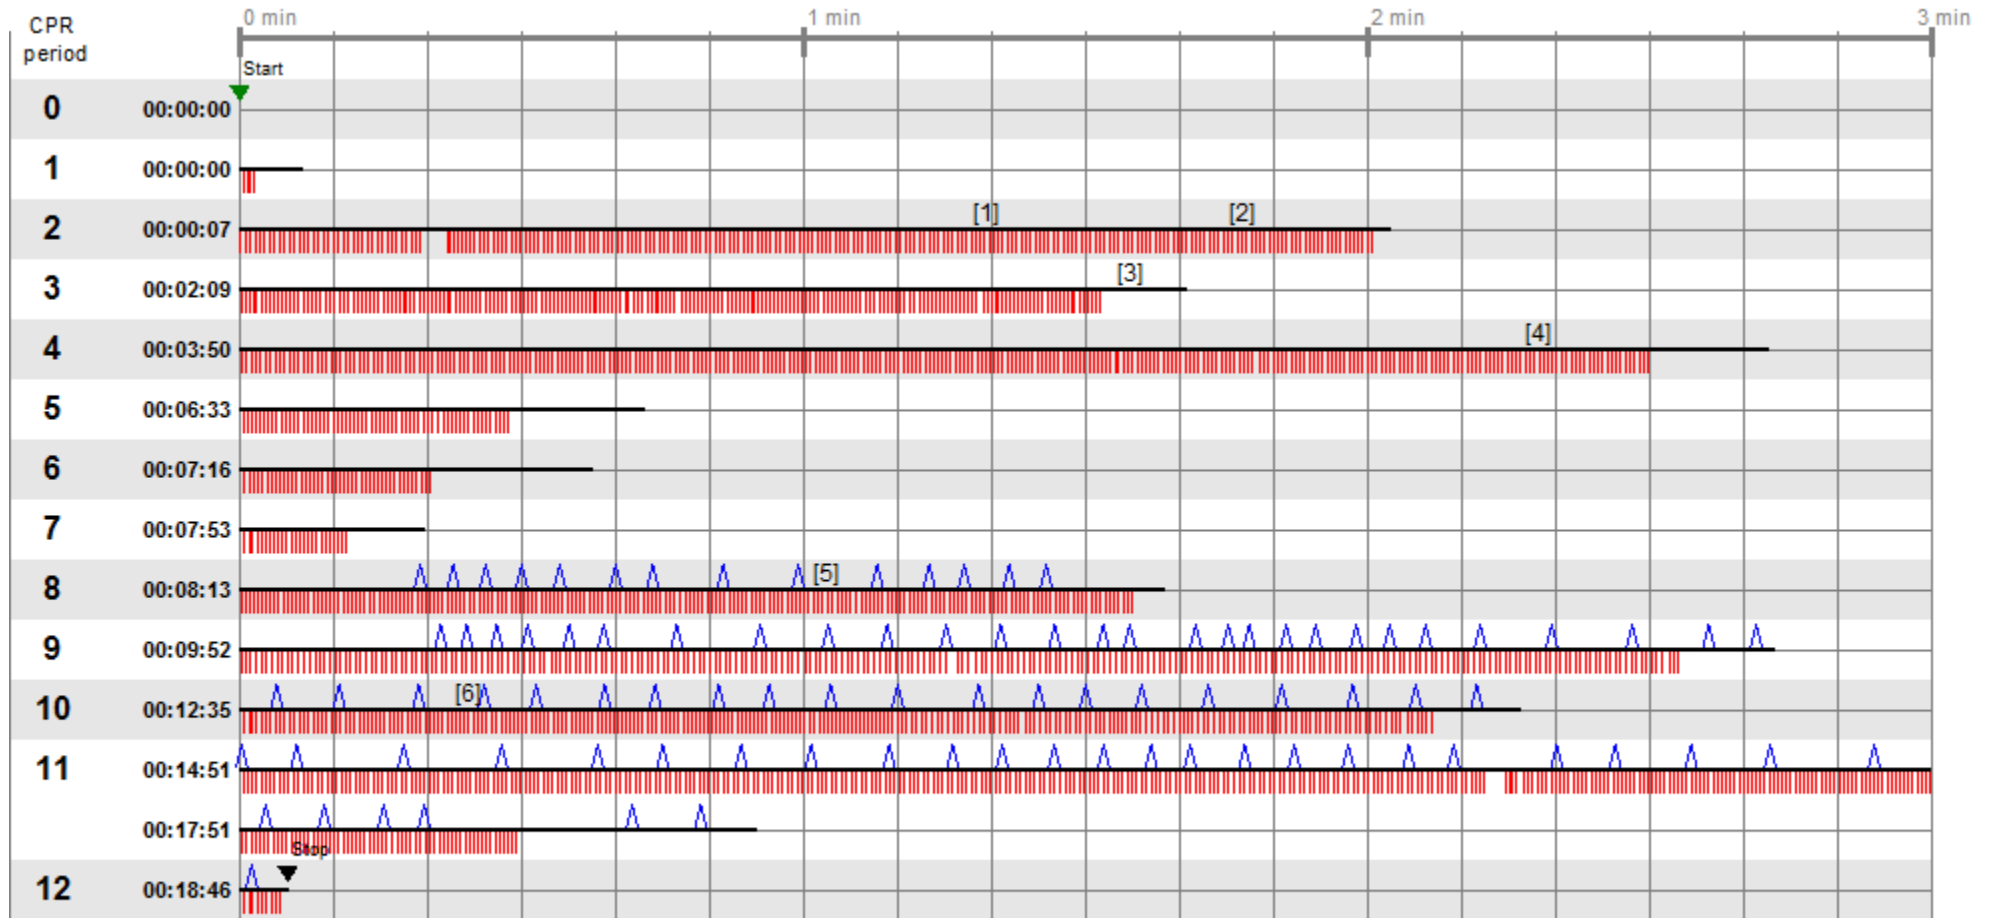

[1] IV Access, [2] Epinephrine, [3] Epinephrine, [4] Epinephrine, [5] Bicarb, [6] Epinephrine