

Case summary

Incident ID: 23-01676
Patient ID: 2023011605064000-LP1547547705
Patient Name: Gniewosz

Patient ID:	<u>2023011605064000-LP1547547705</u>	Birth Date:	
Incident ID:	<u>23-01676</u>	Device ID:	<u>DCMH1</u>
Age at Incident:	<u>60 Years</u>	Case Start Date:	<u>1/16/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>5:06:40 AM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Notes:

A lot of early pausing compressions. Need to shorten pulse checks. Long pauses in compressions due to preparing for and transporting to ambulance and ED. Med Command denied termination.

Comments:

Table of Contents

CPR reports (by CPR period)3

 CPR report (by CPR period)3

CPR report




Device Type: LIFEPAK® 15
Power On: 1/16/2023 5:06:40 AM
CPR Annotations Edited: Yes
Device Configuration: 2D355RO40200UR

Duration: 00:54:22
Incident ID: 23-01676
Statistical Parameters: 1000-0300-3000-05


*Times have been adjusted by the system.

Compression ratio
(/total time)




37:20 / 44:38 = 84 %

Compression rate





136/minute

Ventilations/minute



--

Initial Rhythm

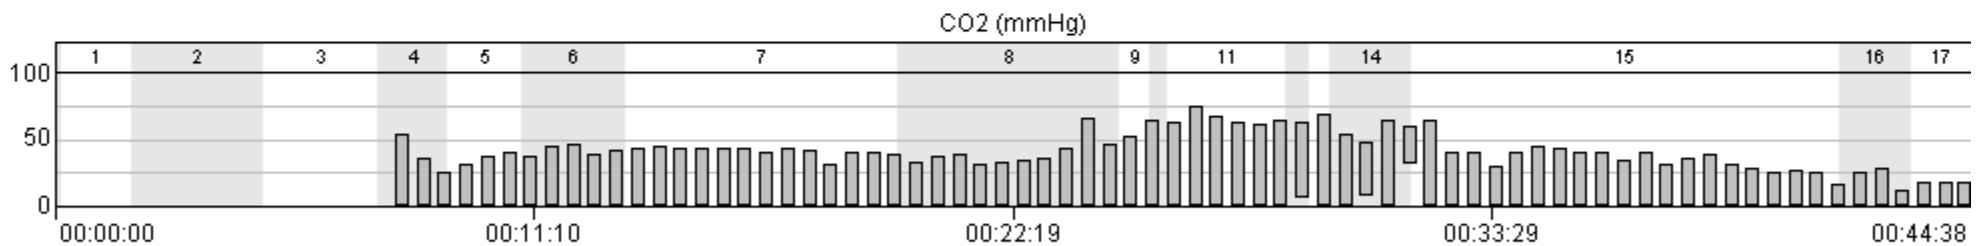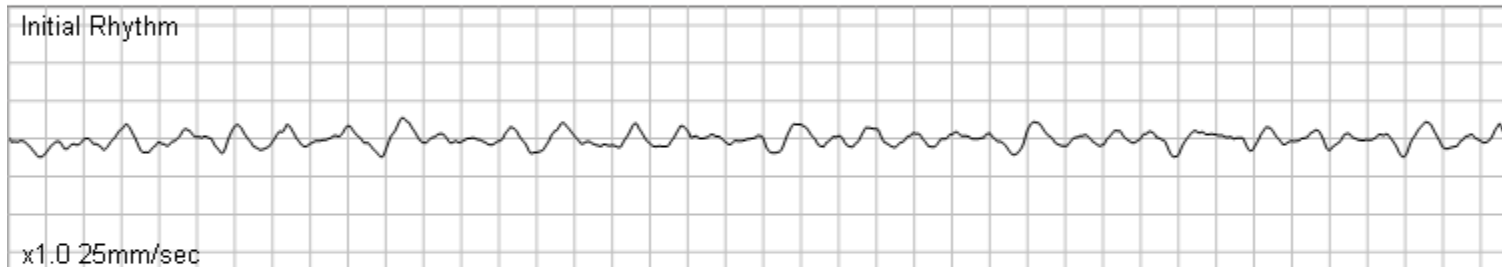

CPR report



Device Type: LIFEPAK® 15
Power On: 1/16/2023 5:06:40 AM
CPR Annotations Edited: Yes
Device Configuration: 2D355RO40200UR

Duration: 00:54:22
Incident ID: 23-01676
Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Summary

CPR needed	= 44:38	CPR done	= 38:51
CPR not done	= 5:47	Compression count	= 4827
Longest compression pause	= 0:47	Pauses over 10 sec	= 13

Comment

CPR report



Device Type: LIFEPAK® 15
 Power On: 1/16/2023 5:06:40 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2D355RO40200UR

Duration: 00:54:22
 Incident ID: 23-01676
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:01:35	00:01:35	00:00:11			73	140	--
2		00:01:46	00:04:34	00:02:48	00:00:15			88	131	--
3		00:04:49	00:07:21	00:02:32	00:00:10			92	131	--
4		00:07:31	00:08:53	00:01:22	00:00:13			86	117	--
5		00:09:06	00:10:41	00:01:35	00:00:09			91	141	--
6		00:10:50	00:13:07	00:02:16	00:00:11			93	143	--
7		00:13:17	00:19:22	00:06:05	00:00:15			93	134	--
8		00:19:36	00:24:02	00:04:25	00:00:47			83	132	--
9		00:24:48	00:25:11	00:00:23	00:00:18			56	139	--
10		00:25:29	00:25:41	00:00:13	00:00:14			47	142	--
11		00:25:55	00:28:13	00:02:18	00:00:28			83	139	--
12		00:28:41	00:28:54	00:00:13	00:00:19			40	74	--
13		00:29:13	00:29:33	00:00:19	00:00:09			67	134	--
14		00:29:42	00:30:52	00:01:10	00:00:45			43	126	--
15		00:31:37	00:40:59	00:09:22	00:00:37			90	136	--
16		00:41:36	00:42:29	00:00:53	00:00:47			53	153	--
17		00:43:16	00:44:38	00:01:22	00:00:01			99	144	--

Ventilation

Chest compression

AED-prompted CPR period

AED Analysis

Shock

ROSC (user annotated)

CPR report




Device Type: LIFEPAK® 15
 Power On: 1/16/2023 5:06:40 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2D355R040200UR

Duration: 00:54:22
 Incident ID: 23-01676
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

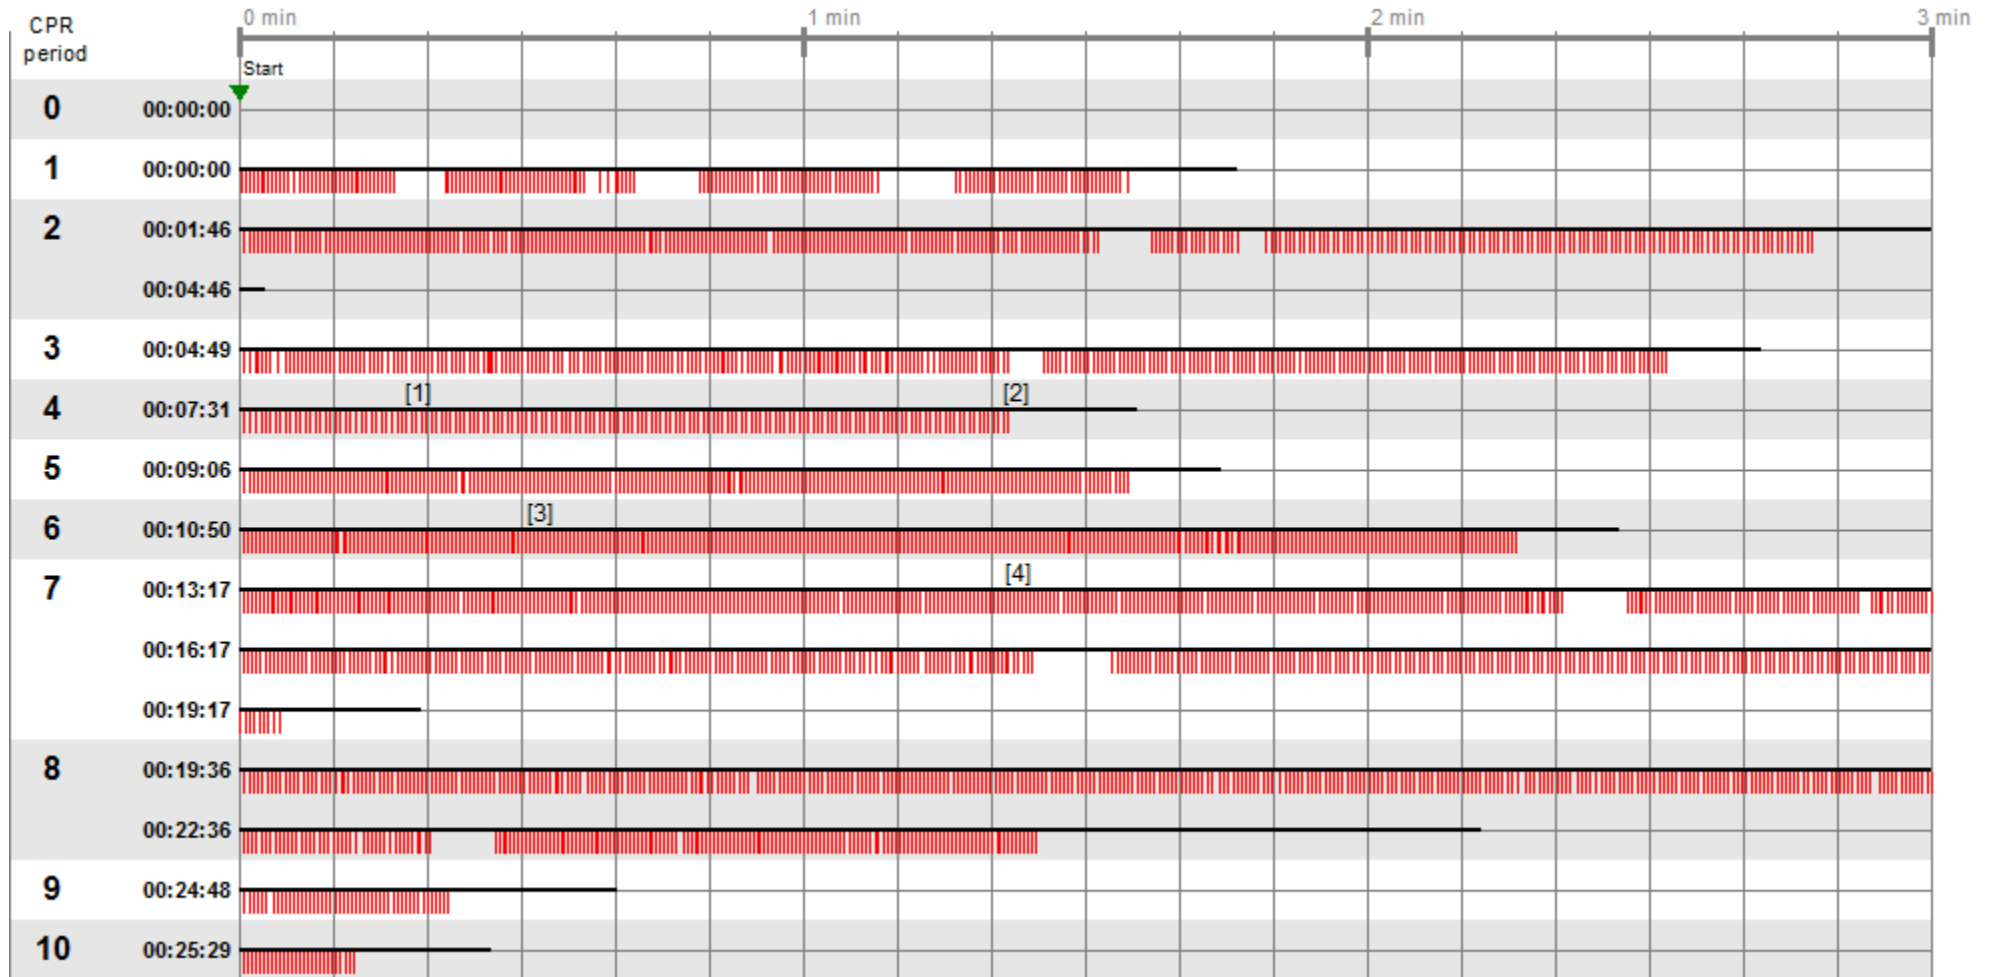

CPR report




Device Type: LIFEPAK® 15
 Power On: 1/16/2023 5:06:40 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2D355RO40200UR

Duration: 00:54:22
 Incident ID: 23-01676
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

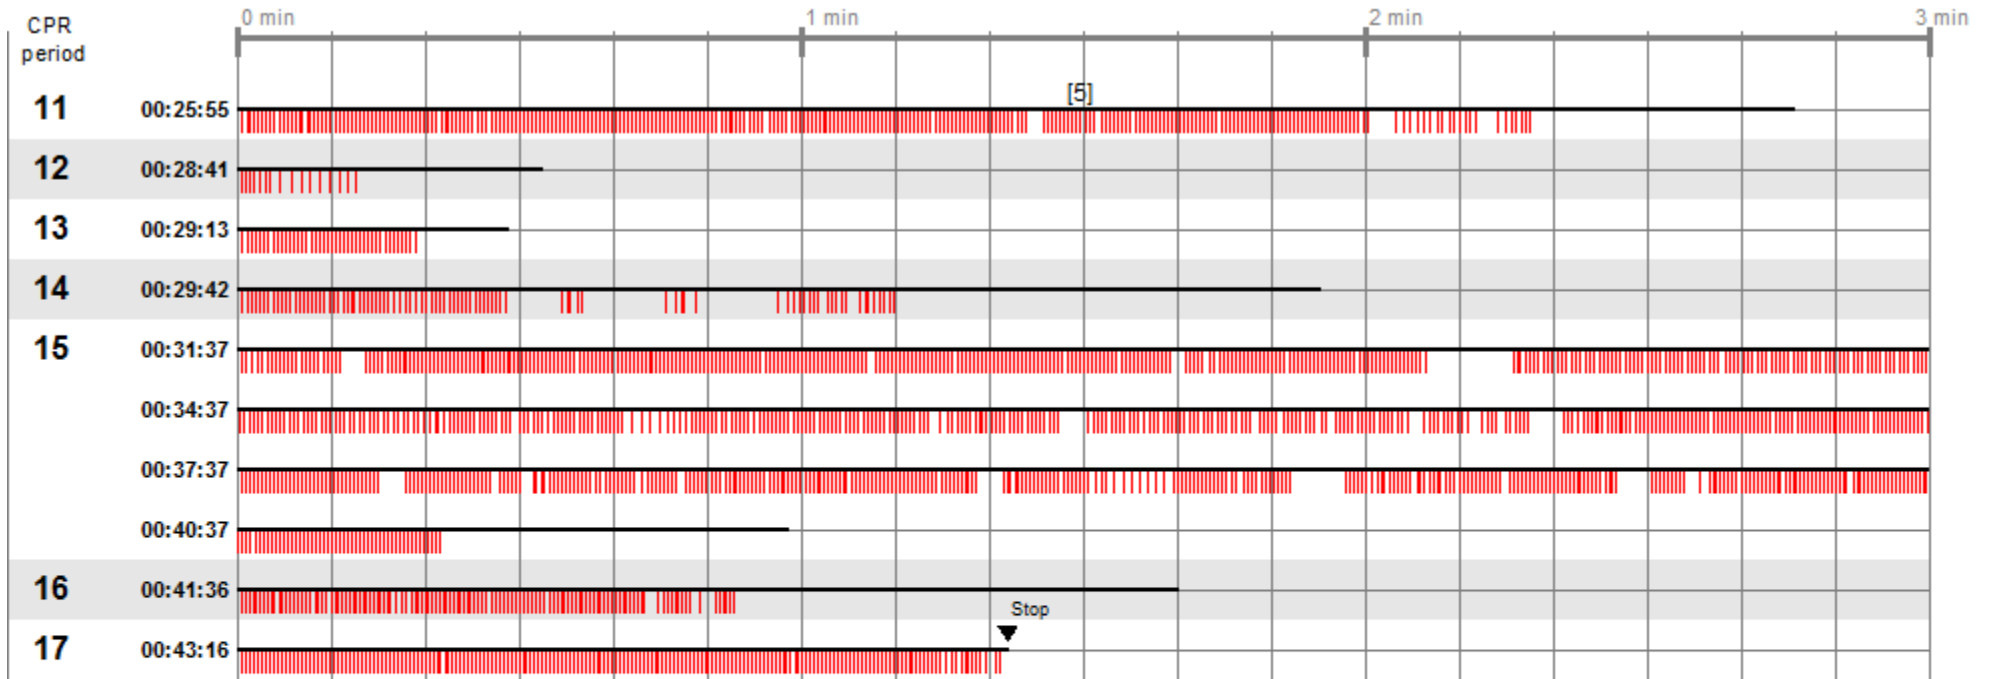

[1] Generic, [2] Epinephrine, [3] Epinephrine, [4] Epinephrine, [5] Epinephrine