

Case summary

Incident ID: 23-06109
Patient ID: 2023030209125400-LP1547545108
Patient Name: Spiller

Patient ID:	<u>2023030209125400- LP1547545108</u>	Birth Date:	
Incident ID:	<u>23-06109</u>	Device ID:	<u>MICU 103A</u>
Age at Incident:	<u>75 Years</u>	Case Start Date:	<u>3/2/2023</u>
Sex:	<u>Female</u>	Case Start Time:	<u>9:12:54 AM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Notes:

Summary complete.
Updated at 3/29/2023 8:13:34 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)	3
CPR report (by CPR period)	3


CPR report



Device Type: LIFEPAK® 15
 Power On: 3/2/2023 9:12:54 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RO402000R
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.


Duration: 00:26:07
 Incident ID: 23-06109
 Statistical Parameters: 1000-0300-3000-05

Compression ratio
(/total time)




21:40 / 23:06 = 94 %

Compression rate




127/minute

Ventilations/minute




9/minute

Initial Rhythm

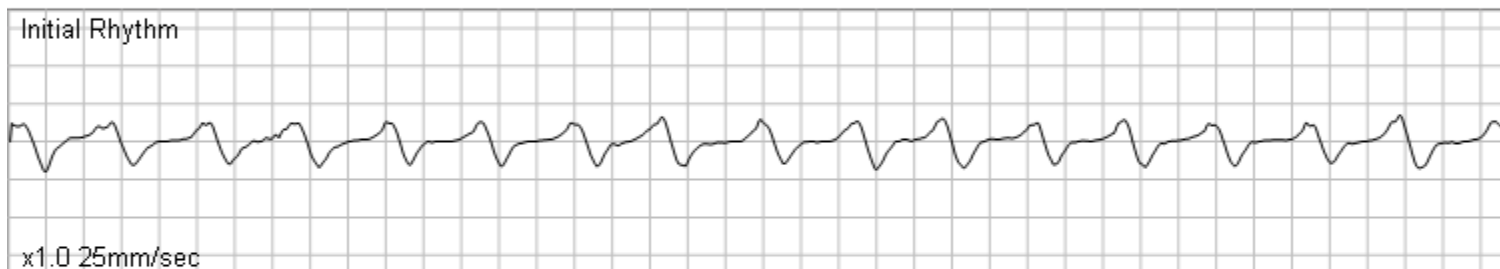

CO2 (mmHg)

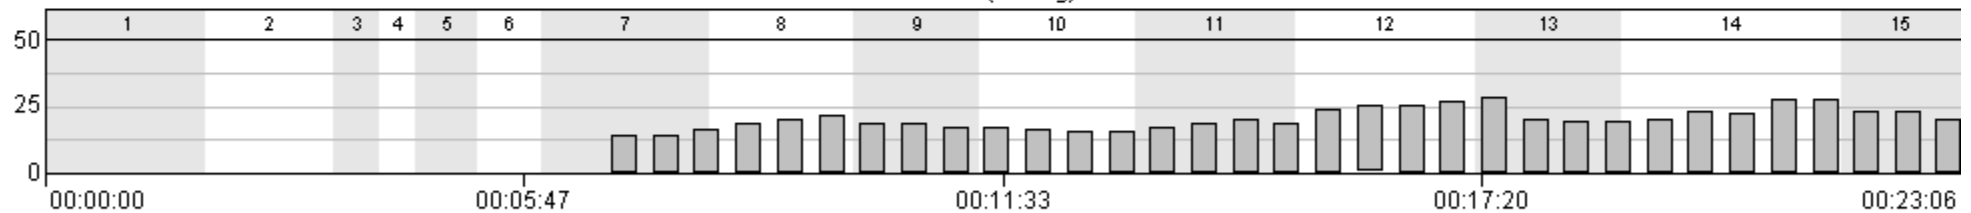

CPR report



Device Type: LIFEPAK® 15
 Power On: 3/2/2023 9:12:54 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RO402000R
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 00:26:07
 Incident ID: 23-06109
 Statistical Parameters: 1000-0300-3000-05

Summary

CPR needed	= 23:06	CPR done	= 21:31
CPR not done	= 1:35	Compression count	= 2720
Longest compression pause	= 0:17	Pauses over 10 sec	= 3

Comment: Try to aim for 2 minutes between pulse checks and to minimize interruptions between pulse checks.

Interval Statistics


CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:01:49	00:01:49	00:00:06	Pulse/rhythm check	Initial rhythm check	95	121	--
2		00:01:55	00:03:23	00:01:28	00:00:05	Pulse/rhythm check	Aim for 2 minutes between pulse checks	95	135	--
3		00:03:28	00:04:00	00:00:32	00:00:01	Unknown	Try to minimize interruptions	100	144	--
4		00:04:02	00:04:25	00:00:24	00:00:03	Unknown	Try to minimize interruptions	92	150	--
5		00:04:28	00:05:05	00:00:38	00:00:06	Unknown	Try to minimize interruptions	87	128	--
6		00:05:12	00:05:56	00:00:44	00:00:02	Unknown	Try to minimize interruptions	100	126	--
7		00:05:58	00:07:47	00:01:49	00:00:13	Pulse/rhythm check		90	118	1
8		00:08:00	00:09:42	00:01:42	00:00:03	Pulse/rhythm check		100	117	11
9		00:09:44	00:11:13	00:01:28	00:00:03	Pulse/rhythm check	Try for 2 minutes between pulse checks.	98	131	11
10		00:11:15	00:13:00	00:01:45	00:00:09	Pulse/rhythm check		93	126	10
11		00:13:09	00:14:55	00:01:46	00:00:10	Pulse/rhythm check		91	123	8
12		00:15:05	00:17:01	00:01:56	00:00:14	Pulse/rhythm check		89	126	8
13		00:17:15	00:18:56	00:01:41	00:00:04	Pulse/rhythm check		97	124	9
14		00:19:00	00:21:24	00:02:24	00:00:17	Pulse/rhythm check		89	136	8
15		00:21:41	00:23:06	00:01:25	00:00:01	Termination/Transfer of Care		99	138	8

CPR report




Device Type: LIFEPAK® 15
 Power On: 3/2/2023 9:12:54 AM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355R0402000R
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 00:26:07
 Incident ID: 23-06109
 Statistical Parameters: 1000-0300-3000-05



CPR QUIK-VIEW

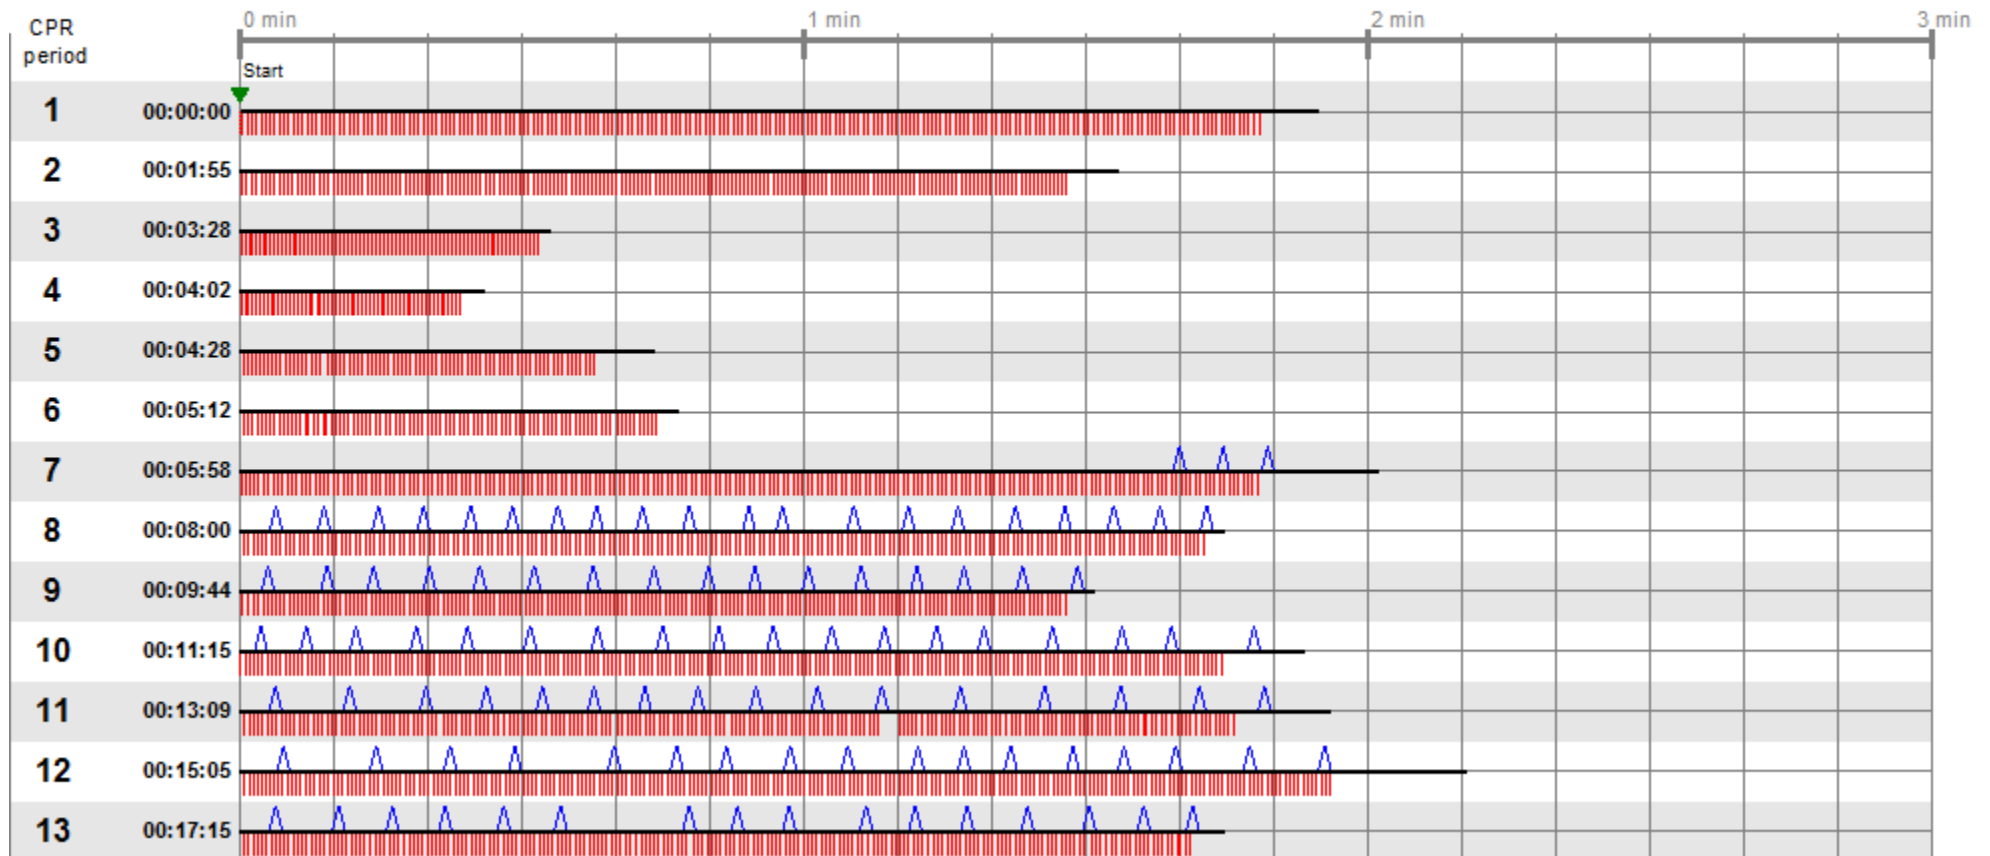

CPR report



Device Type: LIFEPAK® 15
Power On: 3/2/2023 9:12:54 AM
CPR Annotations Edited: Yes
Device Configuration: 2L355RO402000R
*Non-paddles lead intervals are included in the reported CPR Ratio
*Times have been adjusted by the system.

Duration: 00:26:07
Incident ID: 23-06109
Statistical Parameters: 1000-0300-3000-05

CPR QUIK-VIEW

