

Case summary

Incident ID: 23-01961
Patient ID: 2023012016204200-LP1547542228
Patient Name: Grieff

| | | | |
|------------------|--------------------------------------|------------------|-----------------------------|
| Patient ID: | <u>2023012016204200-LP1547542228</u> | Birth Date: | |
| Incident ID: | <u>23-01961</u> | Device ID: | <u>CROZER</u> |
| Age at Incident: | <u>66 Years</u> | Case Start Date: | <u>1/20/2023</u> |
| Sex: | <u>Male</u> | Case Start Time: | <u>4:20:42 PM</u> |
| Race: | <u>Unspecified</u> | Time Adjustment: | <u>System Adjusted Time</u> |

Case Summary:

Total Analyses: 0
Total Shocks: 0
Total 12-Leads: 1
Total Time Paced: 00:00:00

Notes:

Long intubation pause.
Some long PEA pauses.
Ventilation rate could use work.
Updated at 1/27/2023 11:01:21 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

- 12-Lead reports3
 - 12-Lead 13
- CPR reports (by CPR period)4
 - CPR report (by CPR period)4


*Times have been adjusted by the system.

12-Lead 1

Incident ID: 23-01961
Patient ID: 2023012016204200-LP1547542228
Patient Name: Grieff
Power On: 1/20/2023 4:20:42 PM
Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15
Device ID: CROZER
Serial Number: LP1547542228
Device Configuration: 2L355RRB0200UR
Software Version: 3313494-010

Name: 12-Lead 1 HR 42bpm Borderline ECG **Unconfirmed**
ID: 012023162042 1/20/2023 4:48:07 PM Regular supraventricular rhythm
Patient ID: PR 0.110s QRS 0.098s Prolonged QT interval
Incident ID: QT/QTc: 0.588s/0.557s Incomplete RBBB
Age: 66 Sex: M P-QRS-T Axes: -37°2°18° Widespread ST-T abnormality is nonspecific

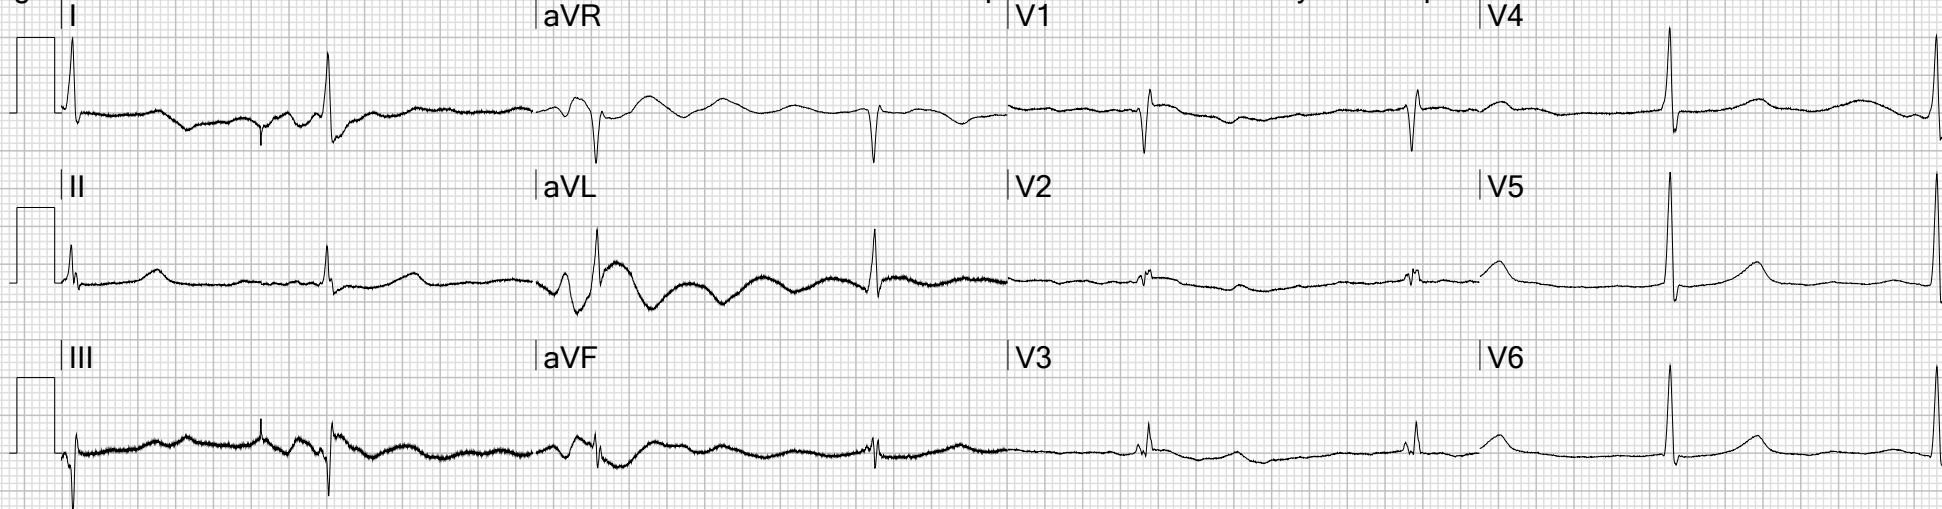

x1.0 .05-150Hz 25mm/sec

Physio-Control, Inc. Comments:

CROZER MICU 131 3313494-010 LP1547542228


CPR report



Device Type: LIFEPAK® 15
Power On: 1/20/2023 4:20:42 PM
CPR Annotations Edited: Yes
Device Configuration: 2L355RRB0200UR
*Non-paddles lead intervals are included in the reported CPR Ratio
*Times have been adjusted by the system.


Duration: 01:05:09
Incident ID: 23-01961
Statistical Parameters: 1000-0300-3000-05

Compression ratio
(/total time)




23:58 / 28:10 = 85 %

Compression rate





123/minute

Ventilations/minute



8/minute

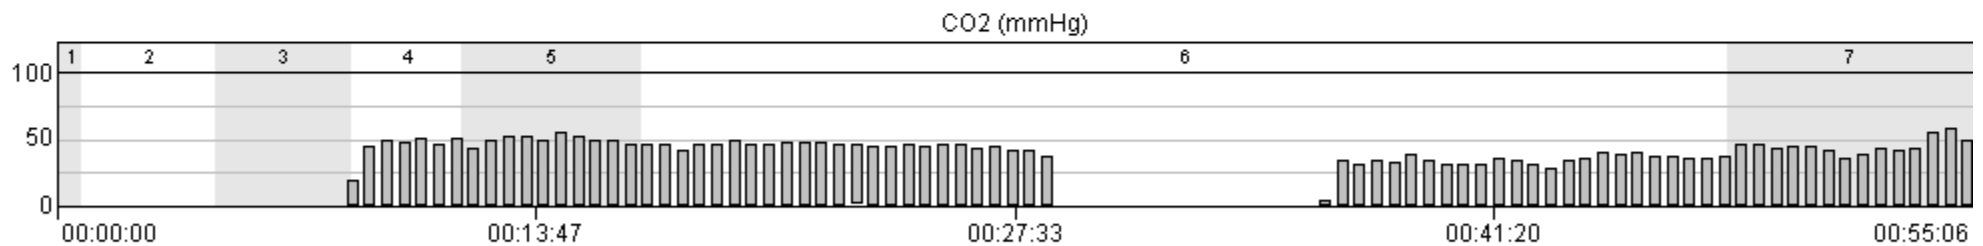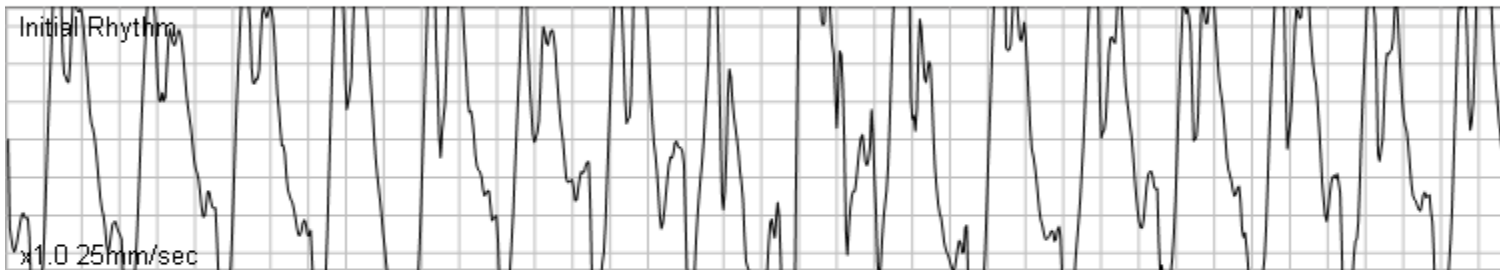


**PHYSIO
CONTROL**

Duration: 01:05:09
Incident ID: 23-01961
Statistical Parameters: 1000-0300-3000-05

| | | | |
|---------------------------|---------|--------------------|---------|
| CPR needed | = 28:10 | CPR done | = 24:55 |
| CPR not done | = 3:16 | Compression count | = 2918 |
| Longest compression pause | = 1:04 | Pauses over 10 sec | = 5 |
| Comment | | | |

| CPR period | Responsible for CPR | CPR started | CPR stopped | CPR duration | Pause duration | Reason CPR stopped | Comments | Compr. ratio, % | Compr. rate | Vent. /min |
|------------|---------------------|-------------|-------------|--------------|----------------|--------------------|----------|-----------------|-------------|------------|
| 1 | | 00:00:00 | 00:00:11 | 00:00:11 | 00:00:28 | | | 28 | 121 | -- |
| 2 | | 00:00:39 | 00:04:22 | 00:03:43 | 00:00:09 | | | 91 | 128 | -- |
| 3 | | 00:04:31 | 00:07:30 | 00:02:59 | 00:00:57 | | | 74 | 127 | 1 |
| 4 | | 00:08:27 | 00:11:23 | 00:02:56 | 00:00:12 | | | 93 | 122 | 7 |
| 5 | | 00:11:35 | 00:16:21 | 00:04:46 | 00:00:24 | | | 90 | 121 | 7 |
| 6 | | 00:16:45 | 00:20:02 | 00:03:17 | 00:28:00 | | | 75 | 116 | 8 |
| 7 | | 00:48:03 | 00:55:06 | 00:07:03 | 00:00:00 | | | 92 | 125 | 9 |

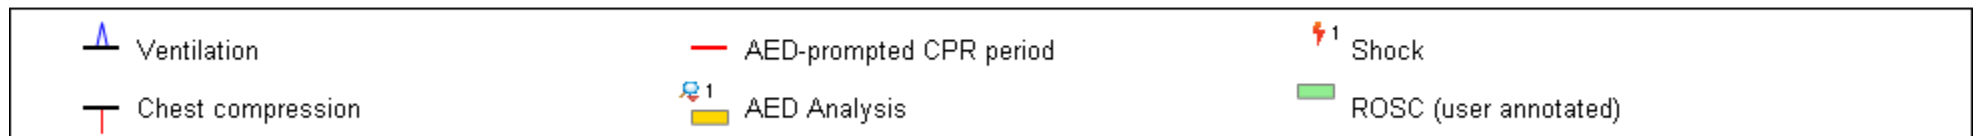


CPR report



Device Type: LIFEPAK® 15
 Power On: 1/20/2023 4:20:42 PM
 CPR Annotations Edited: Yes
 Device Configuration: 2L355RRB0200UR
 *Non-paddles lead intervals are included in the reported CPR Ratio
 *Times have been adjusted by the system.

Duration: 01:05:09
 Incident ID: 23-01961
 Statistical Parameters: 1000-0300-3000-05

CPR QUIK-VIEW

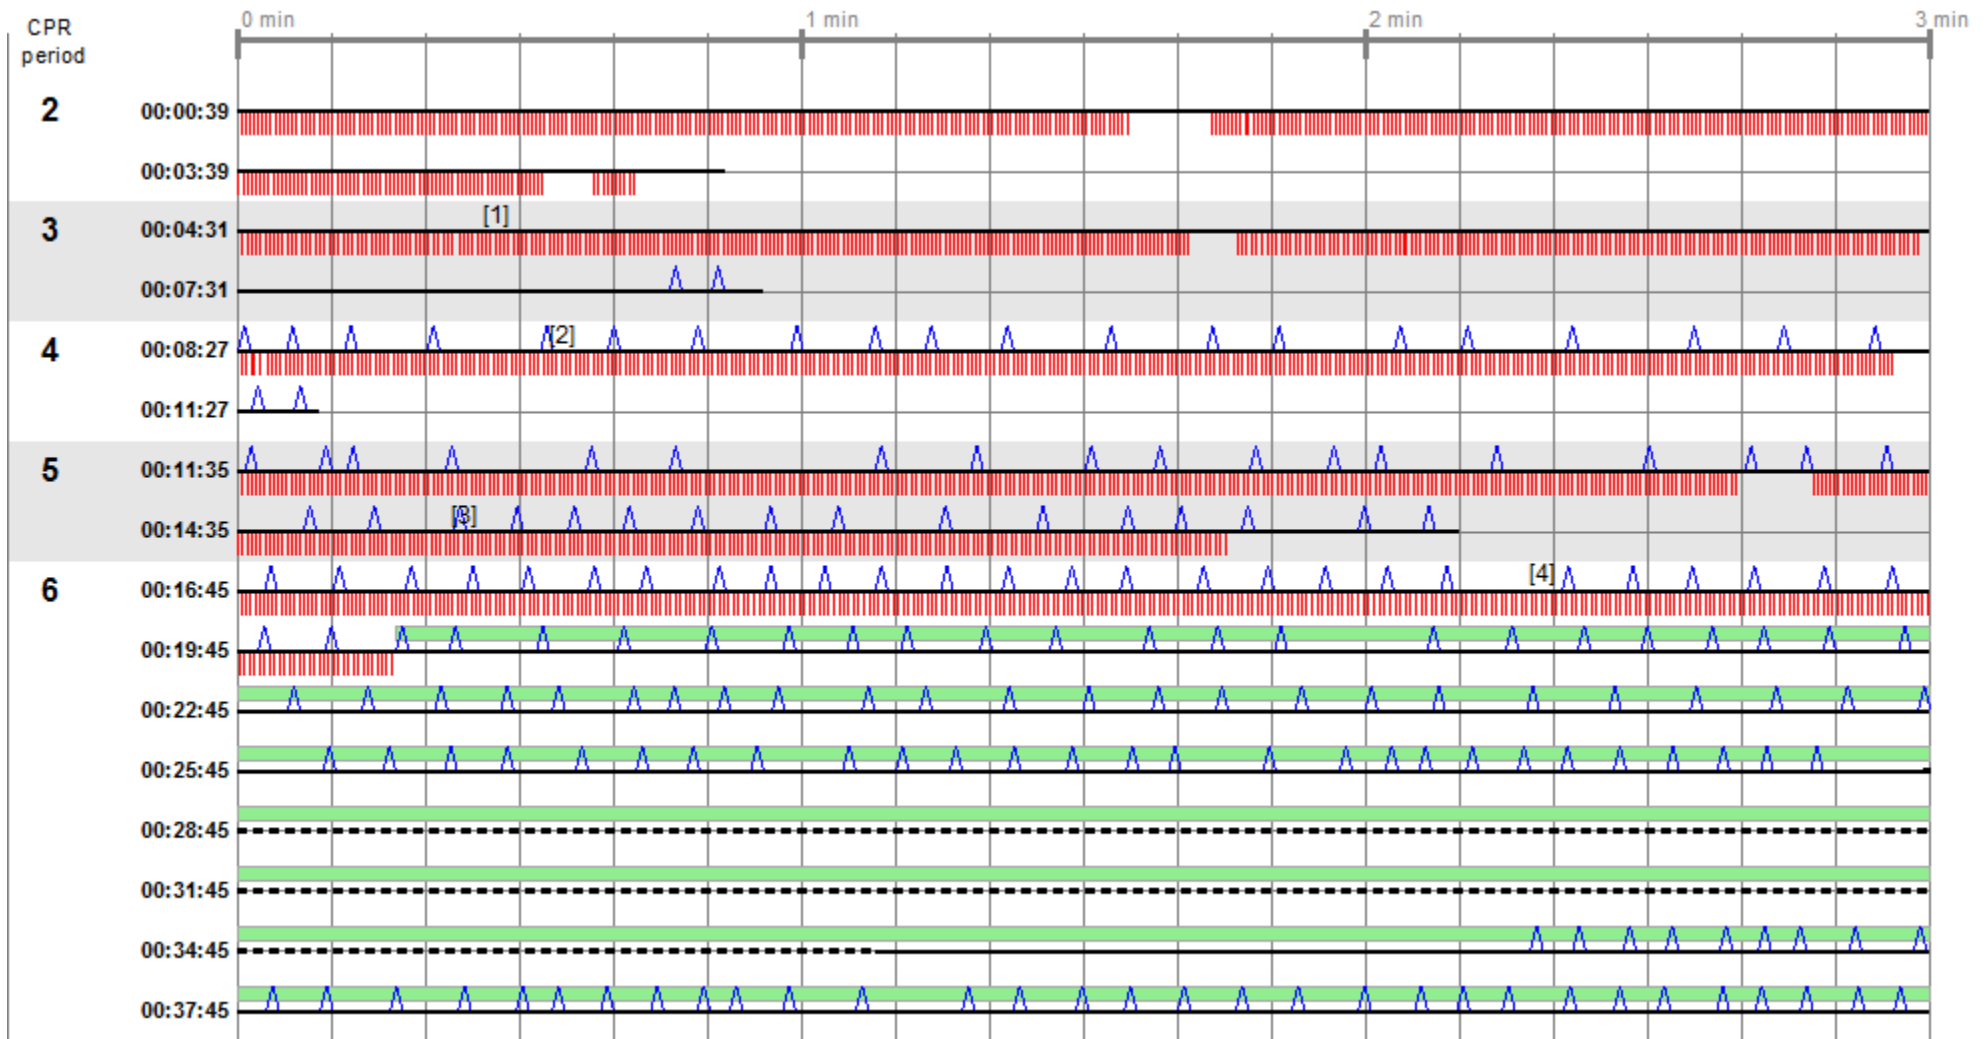


CPR report



Device Type: LIFEPAK® 15
Power On: 1/20/2023 4:20:42 PM
CPR Annotations Edited: Yes
Device Configuration: 2L355RRB0200UR
*Non-paddles lead intervals are included in the reported CPR Ratio
*Times have been adjusted by the system.

Duration: 01:05:09
Incident ID: 23-01961
Statistical Parameters: 1000-0300-3000-05

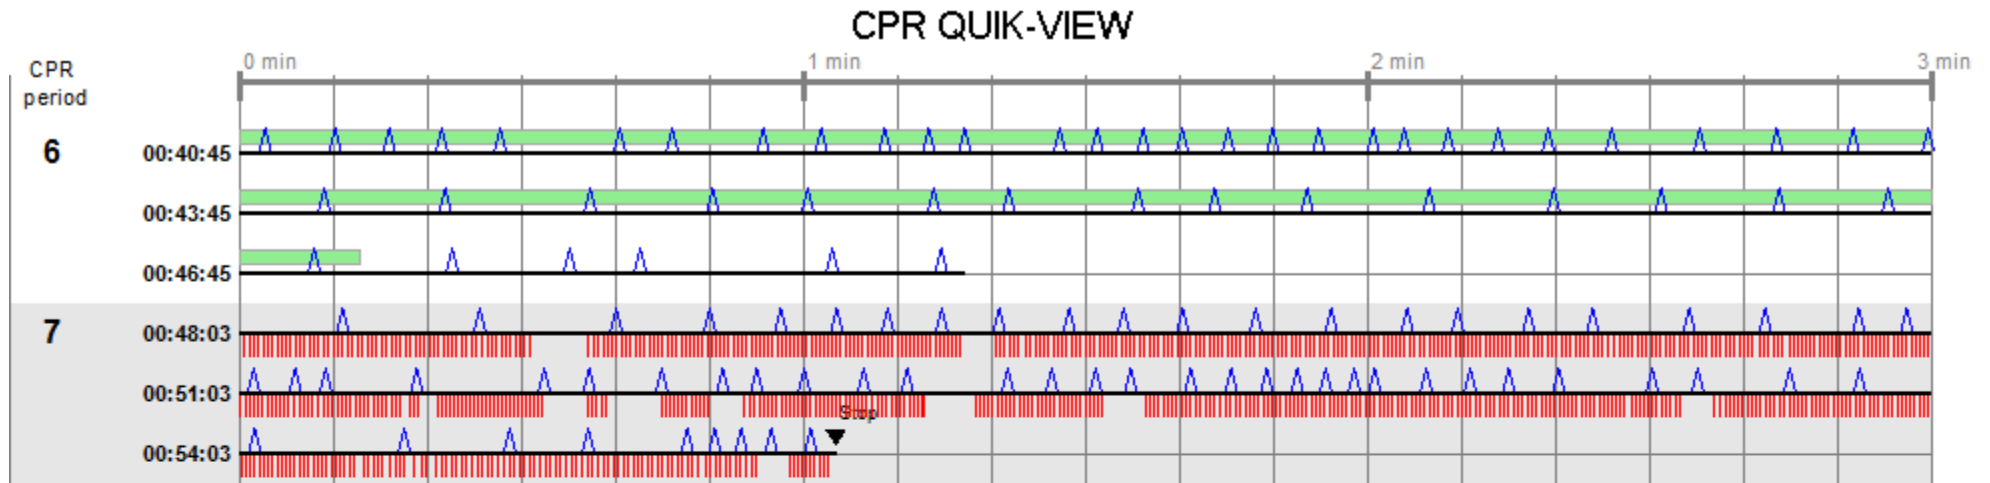

[1] Epinephrine, [2] Epinephrine, [3] Epinephrine, [4] Generic