

## Case summary

Incident ID: 23-02198  
Patient ID: 2023012305203500-LP1547547705  
Patient Name: Sharpless, Chearle

Patient ID:	<u>2023012305203500-LP1547547705</u>	Birth Date:	<u>11/5/1946</u>
Incident ID:	<u>23-02198</u>	Device ID:	<u>DCMH1</u>
Age at Incident:	<u>76 Years</u>	Case Start Date:	<u>1/23/2023</u>
Sex:	<u>Female</u>	Case Start Time:	<u>5:05:00 AM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

### Notes:

Pulse checks too far apart.  
Updated at 1/27/2023 11:32:36 PM by zphillips (Zach Phillips).

### Comments:

# Table of Contents

CPR reports (by CPR period) .....3

    CPR report (by CPR period) .....3

# CPR report




Device Type: LIFEPAK® 15  
Power On: 1/23/2023 5:20:36 AM  
CPR Annotations Edited: Yes  
Device Configuration: 2D355RO40200UR

Duration: 00:33:36  
Incident ID: 23-02198  
Statistical Parameters: 1000-0300-3000-05


\*Times have been adjusted by the system.

Compression ratio  
(/total time)




21:54 / 22:50 = 96 %

Compression rate





140/minute

Ventilations/minute



--

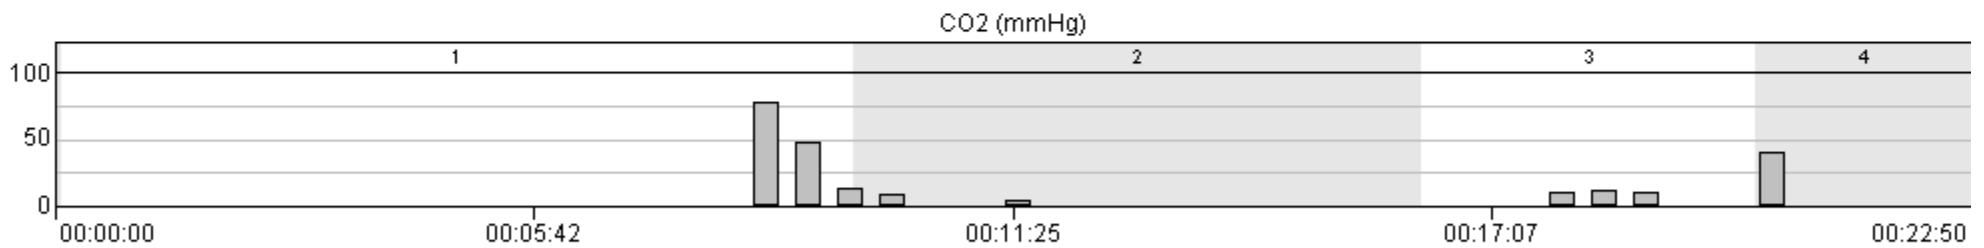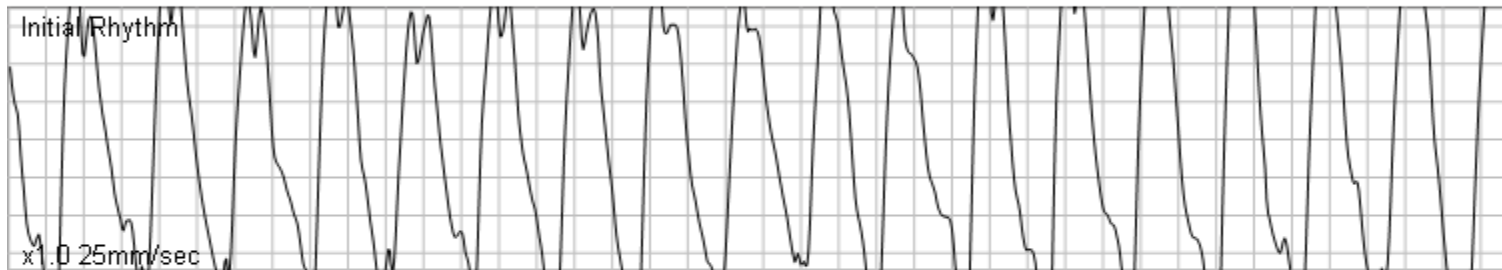

## CPR report



Device Type: LIFEPAK® 15  
 Power On: 1/23/2023 5:20:36 AM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355RO40200UR

Duration: 00:33:36  
 Incident ID: 23-02198  
 Statistical Parameters: 1000-0300-3000-05

\*Times have been adjusted by the system.

## Summary

CPR needed	= 22:50	CPR done	= 22:15
CPR not done	= 0:35	Compression count	= 3032
Longest compression pause	= 0:13	Pauses over 10 sec	= 3

Comment

## Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:09:20	00:09:20	00:00:10			96	135	--
2		00:09:30	00:16:05	00:06:35	00:00:11			95	146	--
3		00:16:16	00:20:02	00:03:46	00:00:13			94	145	--
4		00:20:15	00:22:50	00:02:34	00:00:00			100	142	--



Ventilation



Chest compression

— AED-prompted CPR period



AED Analysis



Shock



ROSC (user annotated)

# CPR report




Device Type: LIFEPAK® 15  
 Power On: 1/23/2023 5:20:36 AM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355R040200UR

Duration: 00:33:36  
 Incident ID: 23-02198  
 Statistical Parameters: 1000-0300-3000-05

\*Times have been adjusted by the system.

## CPR QUIK-VIEW

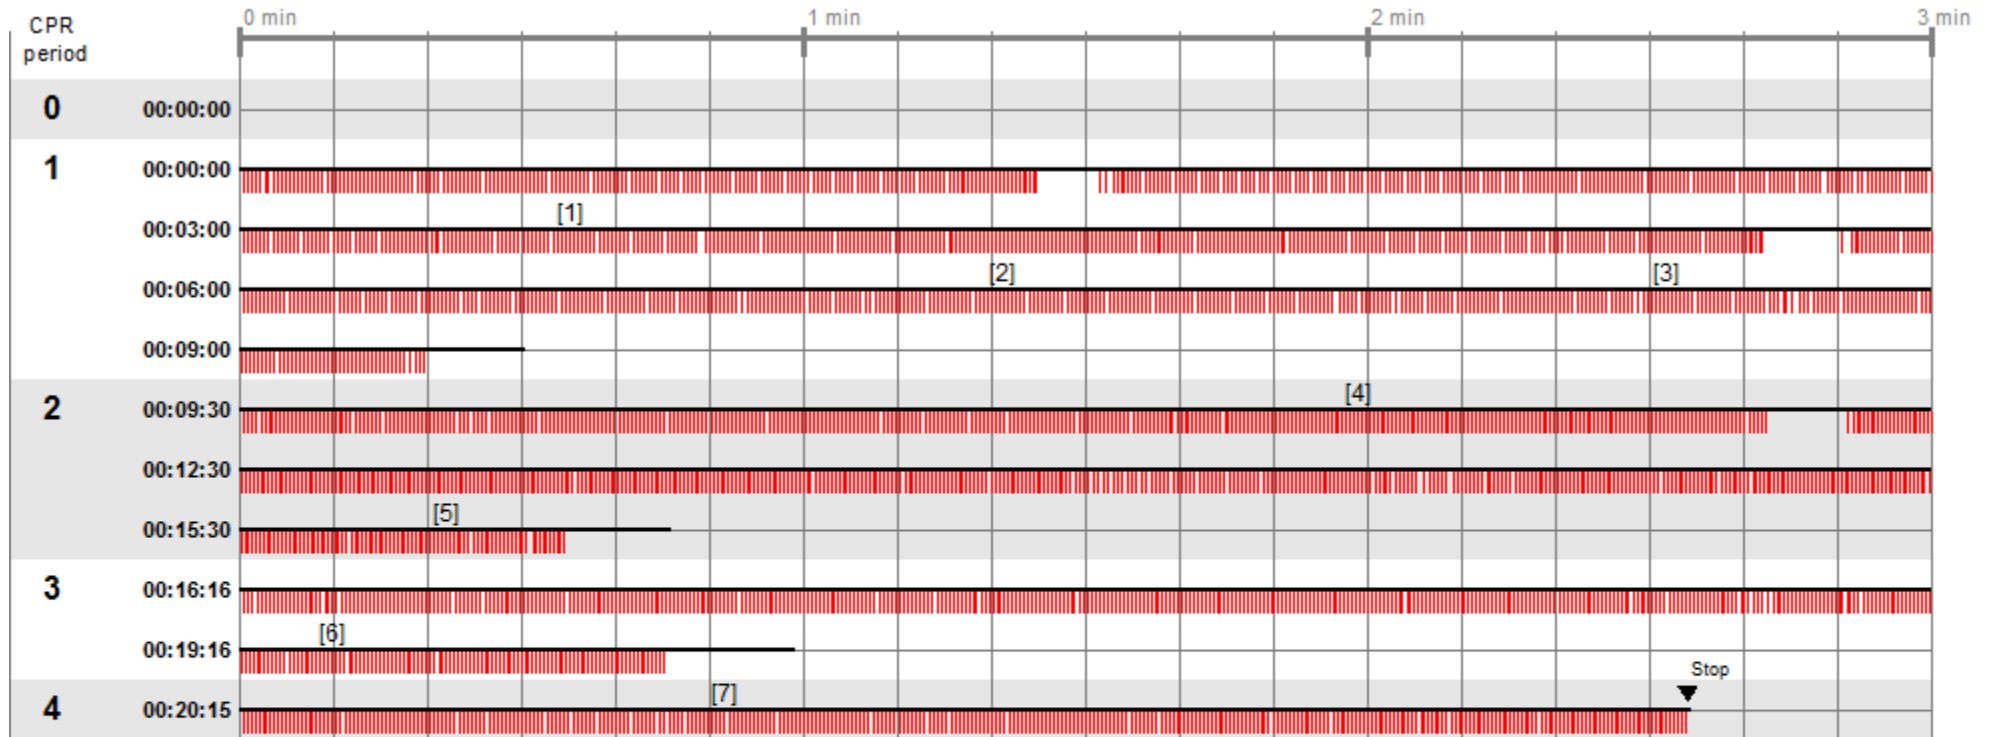

[1] Generic, [2] Epinephrine, [3] Intubation, [4] Epinephrine, [5] Epinephrine, [6] Intubation, [7] Epinephrine