

Case summary

Incident ID: 23-07233
Patient ID: 2023031223114100-LP1547542988
Patient Name: Hunter

Patient ID:	<u>2023031223114100-LP1547542988</u>	Birth Date:	
Incident ID:	<u>23-07233</u>	Device ID:	<u>CROZER EMS</u>
Age at Incident:	<u>55 Years</u>	Case Start Date:	<u>3/12/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>11:11:41 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

Notes:

Demos
Pads off for >50% of the time
Updated at 4/8/2023 9:30:40 PM by zphillips (Zach Phillips).

Comments:

Table of Contents

CPR reports (by CPR period)3

 CPR report (by CPR period)3

CPR report




Device Type: LIFEPAK® 15
Power On: 3/12/2023 11:11:41 PM
CPR Annotations Edited: No
Device Configuration: 2LB55RO40200UR

Duration: 00:26:11
Incident ID: 23-07233
Statistical Parameters: 1000-0300-3000-05


*Times have been adjusted by the system.

Compression ratio
(/total time)




7:54 / 9:08 = 86 %

Compression rate





124/minute

Ventilations/minute



4/minute

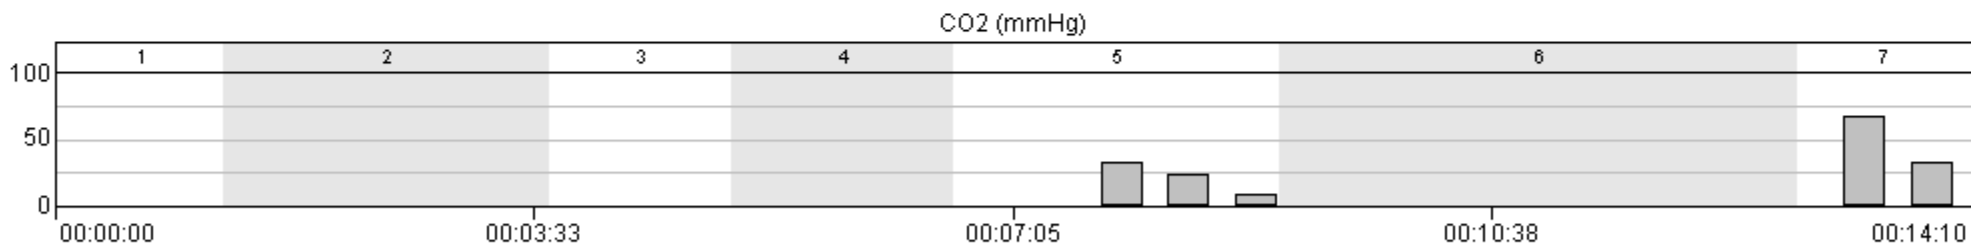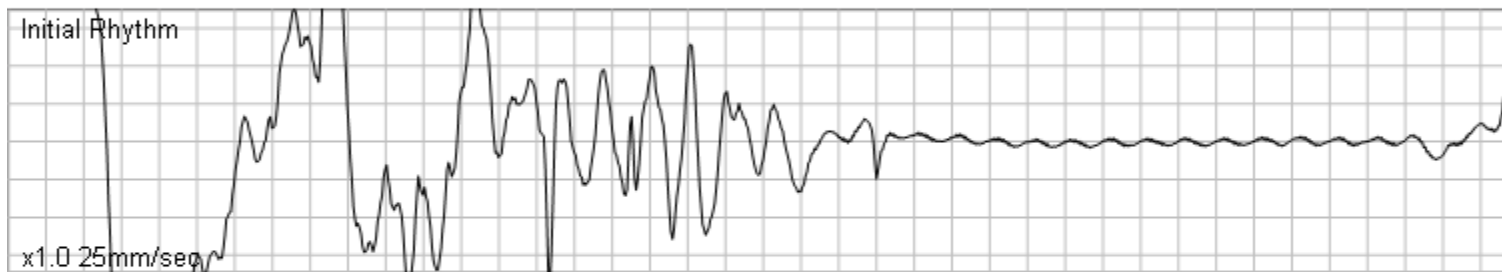

CPR report



Device Type: LIFEPAK® 15
 Power On: 3/12/2023 11:11:41 PM
 CPR Annotations Edited: No
 Device Configuration: 2LB55RO40200UR

Duration: 00:26:11
 Incident ID: 23-07233
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

Summary

CPR needed	= 9:08	CPR done	= 8:17
CPR not done	= 0:52	Compression count	= 929
Longest compression pause	= 0:09	Pauses over 10 sec	= 0

Comment: I really can't check this. The pads are off for approximately 50% of the time. DNR.

Interval Statistics

CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:00:12	00:00:12	00:01:02			55	125	--
2		00:01:15	00:01:51	00:00:37	00:01:48			94	124	--
3		00:03:39	00:04:42	00:01:02	00:00:18			81	122	--
4		00:05:00	00:06:26	00:01:26	00:00:13			96	124	--
5		00:06:39	00:08:36	00:01:58	00:00:27			95	123	2
6		00:09:03	00:10:49	00:01:45	00:02:05			80	123	--
7		00:12:53	00:14:10	00:01:16	00:00:00			80	128	10

Ventilation
 AED-prompted CPR period
 Shock

Chest compression
 AED Analysis
 ROSC (user annotated)

CPR QUIK-VIEW



CPR report




Device Type: LIFEPAK® 15
 Power On: 3/12/2023 11:11:41 PM
 CPR Annotations Edited: No
 Device Configuration: 2LB55RO40200UR

Duration: 00:26:11
 Incident ID: 23-07233
 Statistical Parameters: 1000-0300-3000-05

*Times have been adjusted by the system.

CPR QUIK-VIEW

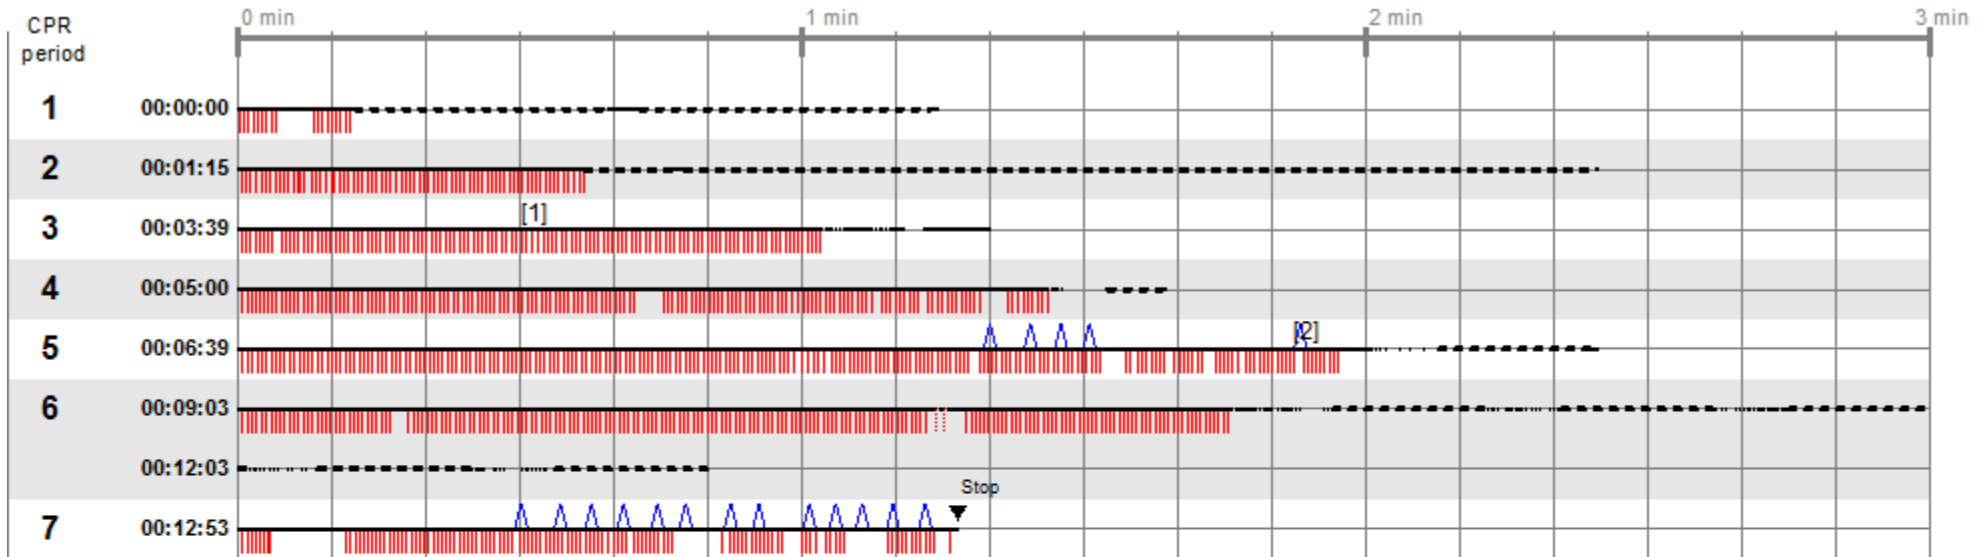

[1] Epinephrine, [2] Epinephrine, [3] Generic