

## Case summary

Incident ID: 23-08546  
Patient ID: 2023032612362700-LP1547546923  
Patient Name: Pore-Rapanan

Patient ID:	<u>2023032612362700-LP1547546923</u>	Birth Date:	
Incident ID:	<u>23-08546</u>	Device ID:	<u>CROZER EMS</u>
Age at Incident:	<u>52 Years</u>	Case Start Date:	<u>3/26/2023</u>
Sex:	<u>Male</u>	Case Start Time:	<u>12:36:27 PM</u>
Race:	<u>Unspecified</u>	Time Adjustment:	<u>System Adjusted Time</u>

### Case Summary:

Total Analyses: 0  
Total Shocks: 4  
Total 12-Leads: 5  
Total Time Paced: 00:00:00

### Notes:

LUCAS, not precharging monitor.  
Updated at 4/8/2023 10:12:55 PM by zphillips (Zach Phillips).  
Updated at 5/20/2023 1:46:10 AM by zphillips (Zach Phillips).

### Comments:


## Table of Contents

12-Lead reports .....	3
12-Lead 1 .....	3
12-Lead 2 .....	4
12-Lead 3 .....	5
12-Lead 4 .....	6
12-Lead 5 .....	7
CPR reports (by CPR period) .....	8
CPR report (by CPR period) .....	8

# 12-Lead 1

Incident ID: 23-08546  
 Patient ID: 2023032612362700-LP1547546923  
 Patient Name: Pore-Rapanan  
 Power On: 3/26/2023 12:36:27 PM  
 Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15  
 Device ID: CROZER EMS  
 Serial Number: LP1547546923  
 Device Configuration: 2D355RO40200OR  
 Software Version: 3313494-010

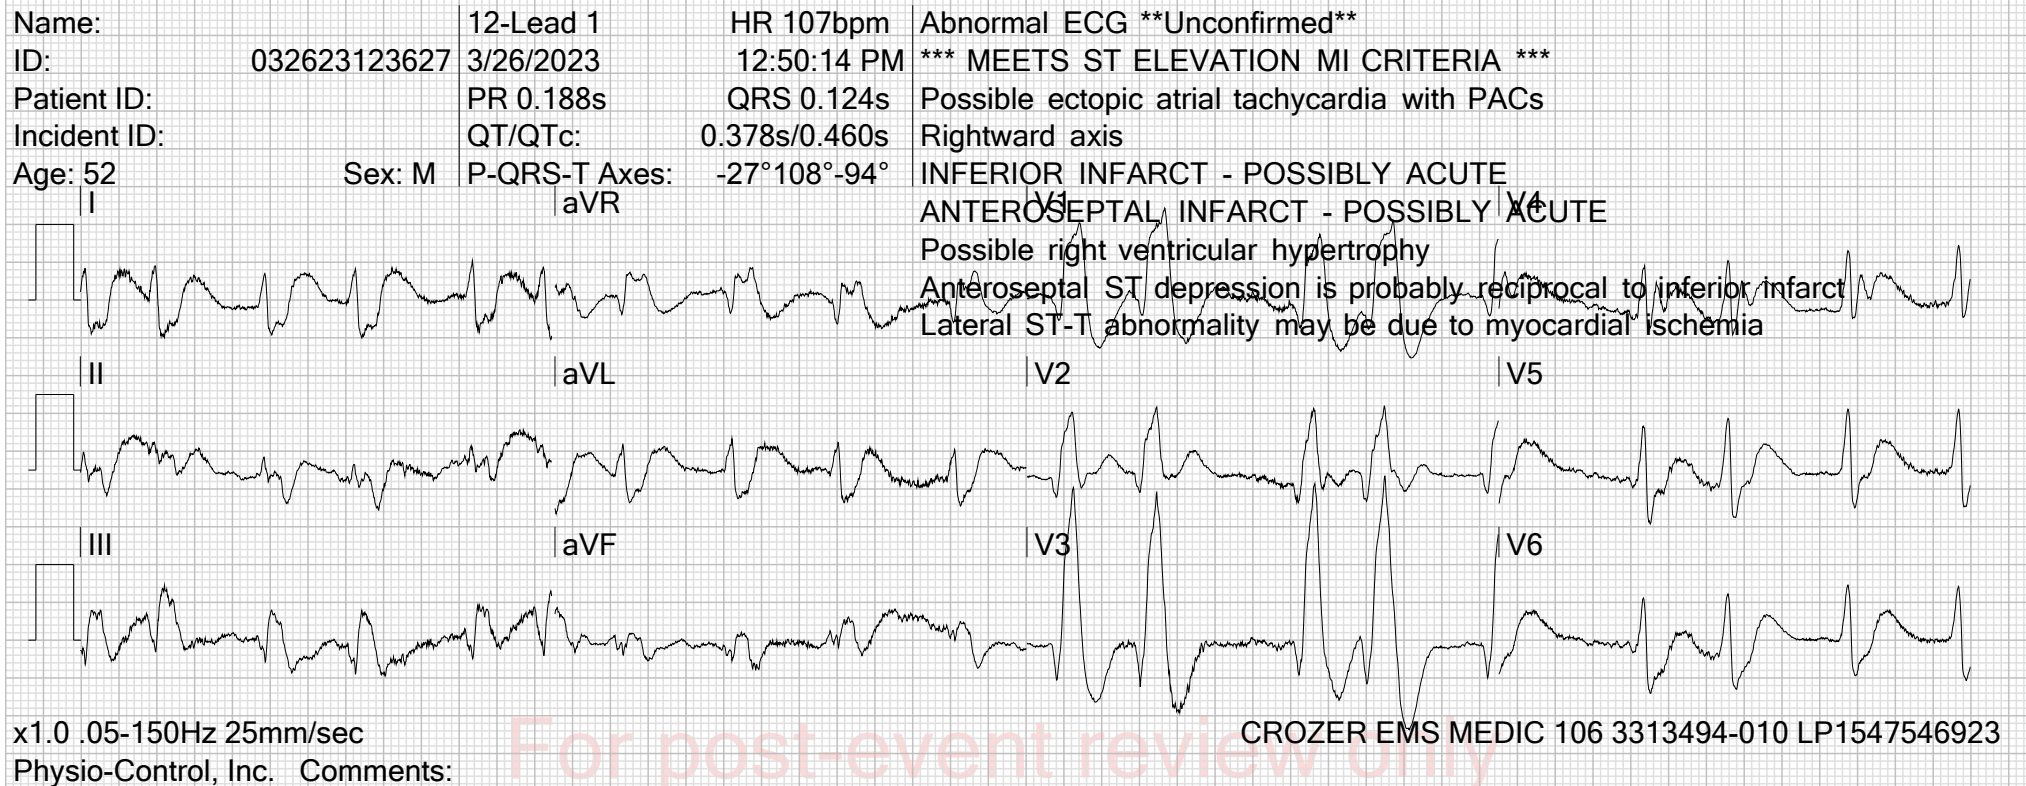


## 12-Lead 2

Incident ID: 23-08546  
 Patient ID: 2023032612362700-LP1547546923  
 Patient Name: Pore-Rapanan  
 Power On: 3/26/2023 12:36:27 PM  
 Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15  
 Device ID: CROZER EMS  
 Serial Number: LP1547546923  
 Device Configuration: 2D355RO40200OR  
 Software Version: 3313494-010

Name: 12-Lead 2 HR 37bpm Abnormal ECG \*\*Unconfirmed\*\*  
 ID: 032623123627 3/26/2023 12:55:35 PM \*\*\* MEETS ST ELEVATION MI CRITERIA \*\*\*  
 Patient ID: PR 0.156s QRS 0.184s Atrial fibrillation with slow ventricular response  
 Incident ID: QT/QTc: 0.448s/0.408s Indeterminate axis  
 Age: 52 Sex: M P-QRS-T Axes: 86°0°-12° Right bundle branch block

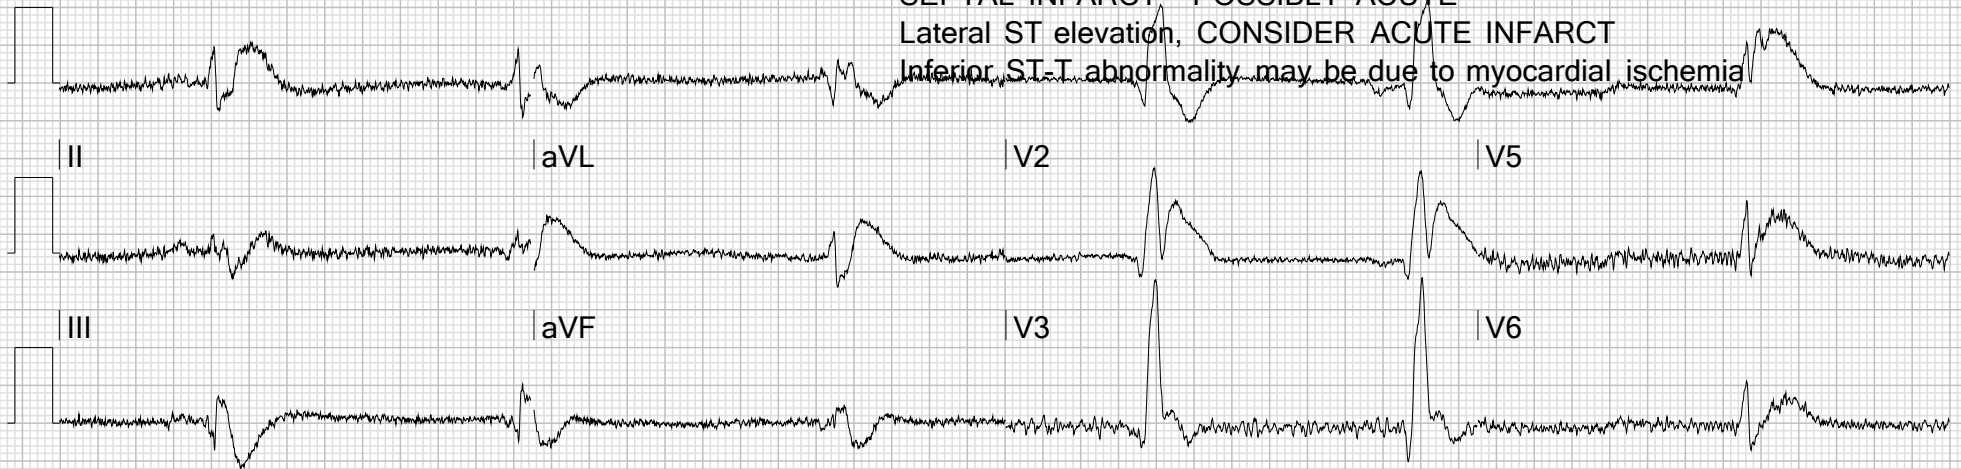

x1.0 .05-150Hz 25mm/sec

Physio-Control, Inc. Comments:

CROZER EMS MEDIC 106 3313494-010 LP1547546923


# 12-Lead 3

Incident ID: 23-08546  
 Patient ID: 2023032612362700-LP1547546923  
 Patient Name: Pore-Rapanan  
 Power On: 3/26/2023 12:36:27 PM  
 Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15  
 Device ID: CROZER EMS  
 Serial Number: LP1547546923  
 Device Configuration: 2D355RO40200OR  
 Software Version: 3313494-010

Name: 12-Lead 3 HR 25bpm Abnormal ECG **\*\*Unconfirmed\*\***  
 ID: 032623123627 3/26/2023 12:57:10 PM Atrial fibrillation with slow ventricular response  
 Patient ID: PR 0.204s QRS 0.224s Severe right axis deviation  
 Incident ID: QT/QTc: 0.528s/0.467s Right bundle branch block  
 Age: 52 Sex: M P-QRS-T Axes: -152°-177°-69° Possible septal infarct - age undetermined  
 aVR V1 Possible posterior infarct - age undetermined

Inferior ST-T abnormality suggests myocardial infarct

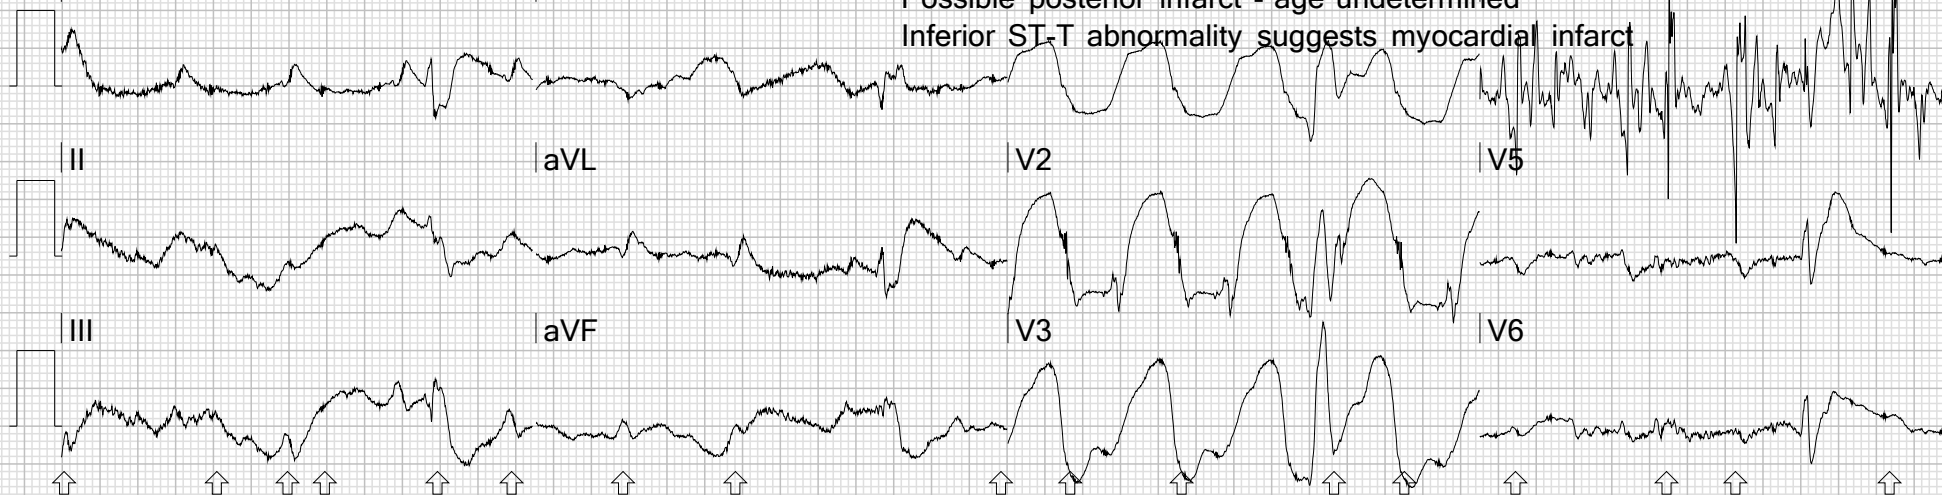

x1.0 .05-150Hz 25mm/sec


Physio-Control, Inc. Comments:

CROZER EMS MEDIC 106 3313494-010 LP1547546923

# 12-Lead 4

Incident ID: 23-08546  
 Patient ID: 2023032612362700-LP1547546923  
 Patient Name: Pore-Rapanan  
 Power On: 3/26/2023 12:36:27 PM  
 Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15  
 Device ID: CROZER EMS  
 Serial Number: LP1547546923  
 Device Configuration: 2D355RO40200OR  
 Software Version: 3313494-010

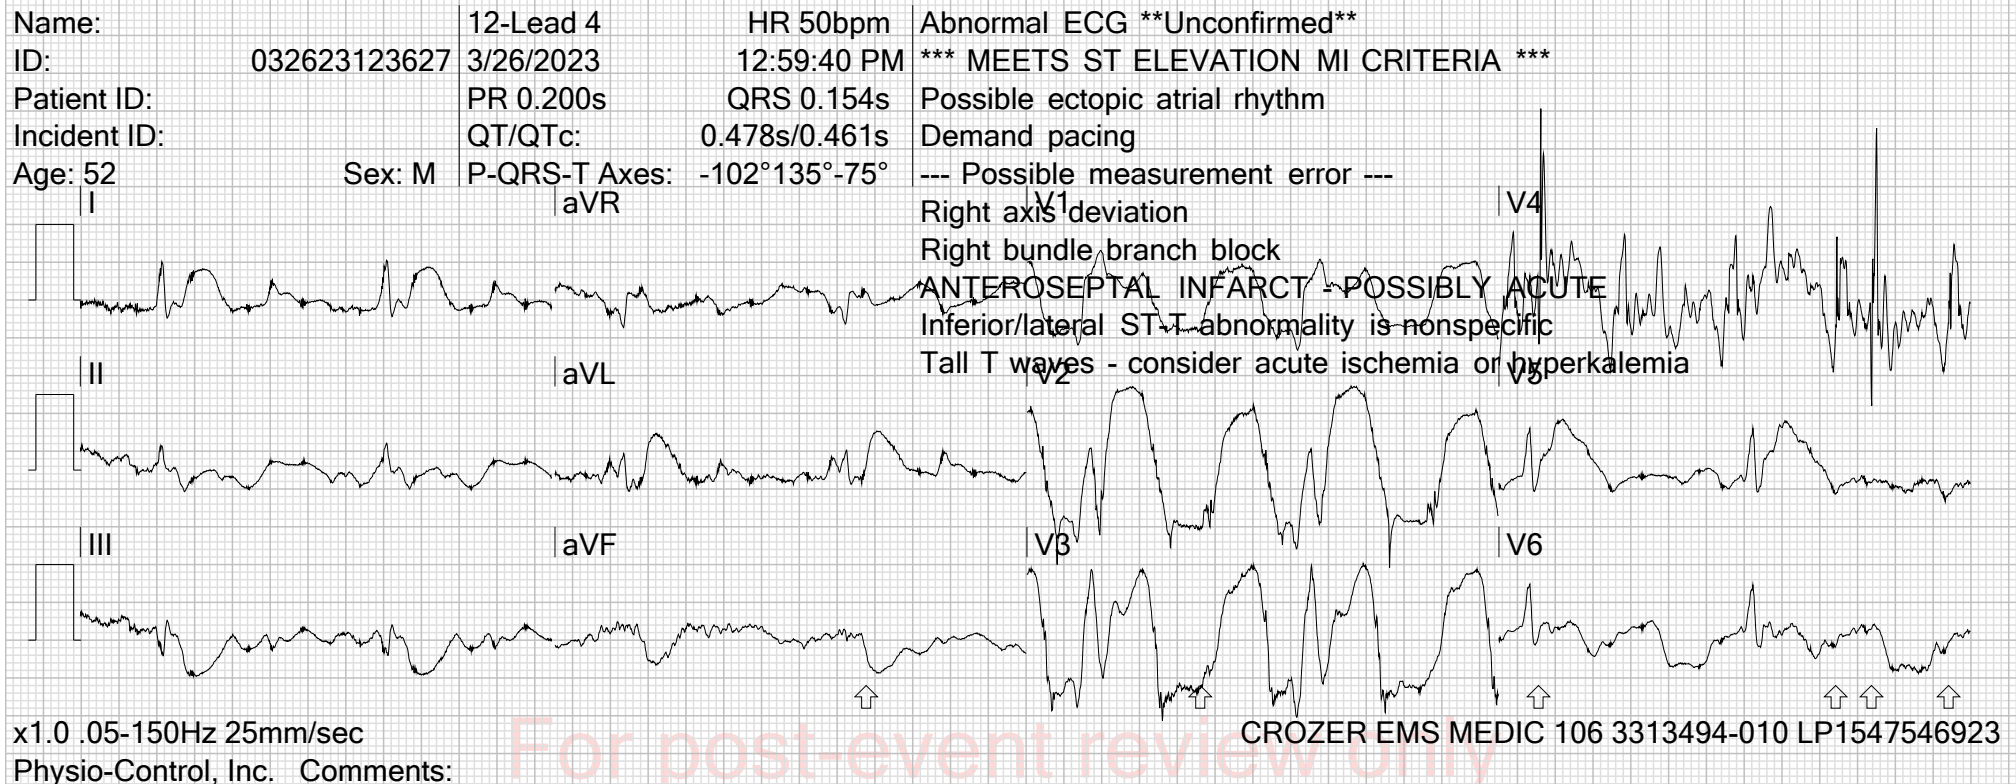


\*Times have been adjusted by the system.

## 12-Lead 5

Incident ID: 23-08546  
Patient ID: 2023032612362700-LP1547546923  
Patient Name: Pore-Rapanan  
Power On: 3/26/2023 12:36:27 PM  
Speed/Size: 25mm/sec/ x1.0

Device Type: LIFEPAK® 15  
Device ID: CROZER EMS  
Serial Number: LP1547546923  
Device Configuration: 2D355RO40200OR  
Software Version: 3313494-010

Name: 12-Lead 5 HR 50bpm Abnormal ECG \*\*Unconfirmed\*\*  
ID: 032623123627 3/26/2023 1:02:10 PM Demand pacing  
Patient ID: PR 0.318s QRS 0.194s Lead(s) unsuitable for analysis: III aVL aVF  
Incident ID: QT/QTc: 0.446s/0.429s IV conduction defect  
Age: 52 Sex: M P-QRS-T Axes: --°--°--° Anterolateral infarct - age undetermined

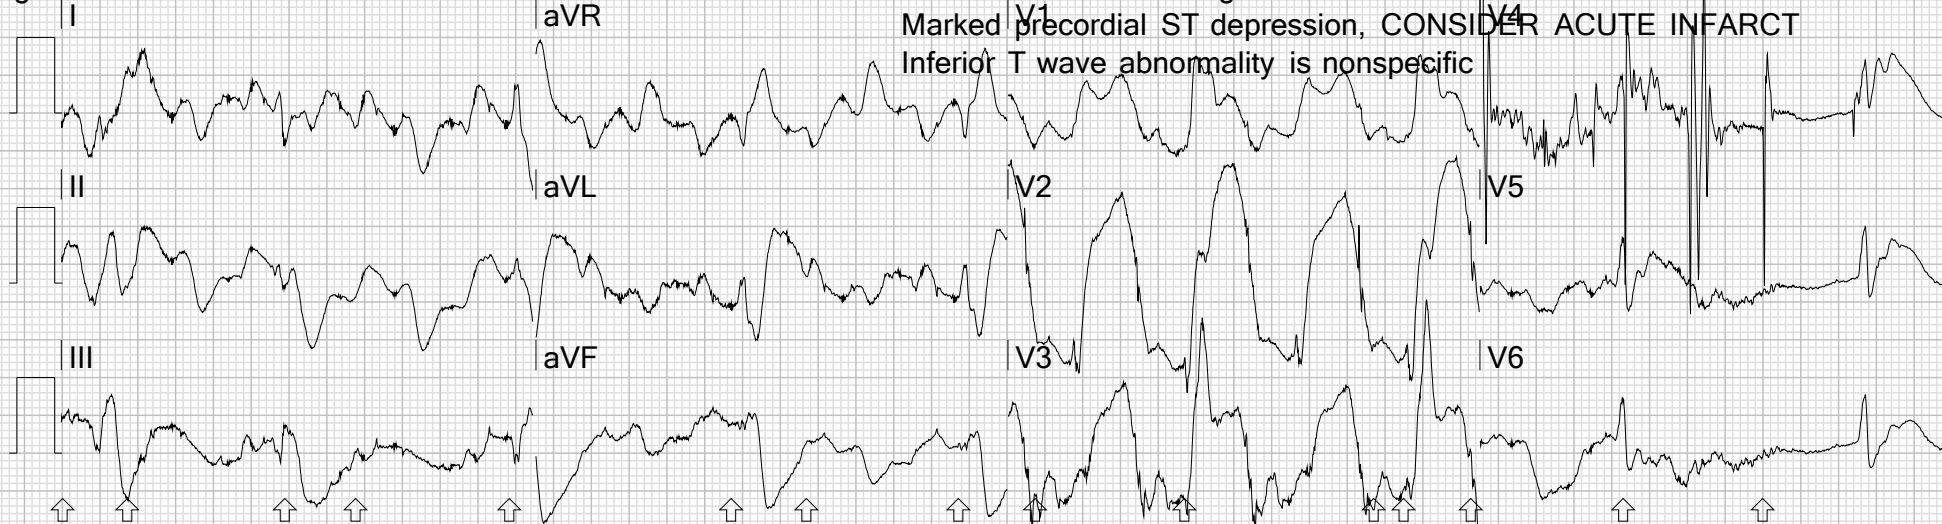

x1.0 .05-150Hz 25mm/sec

Physio-Control, Inc. Comments:

CROZER EMS MEDIC 106 3313494-010 LP1547546923


# CPR report



Device Type: LIFEPAK® 15  
 Power On: 3/26/2023 12:36:27 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355R0402000R  
 \*Non-paddles lead intervals are included in the reported CPR Ratio  
 \*Times have been adjusted by the system.


Duration: 00:41:36  
 Incident ID: 23-08546  
 Statistical Parameters: 1000-0300-3000-05

Compression ratio  
(/total time)




23:46 / 28:42 = 83 %

Compression rate




102/minute

Ventilations/minute




--

Initial Rhythm

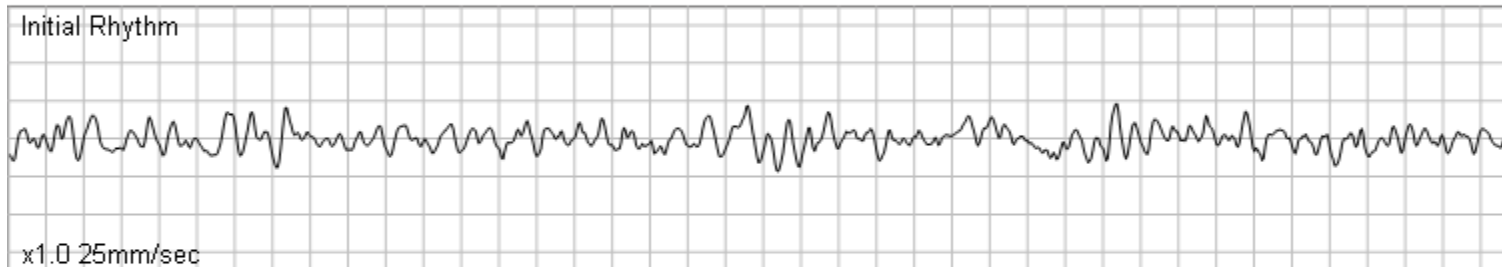

CO2 (mmHg)

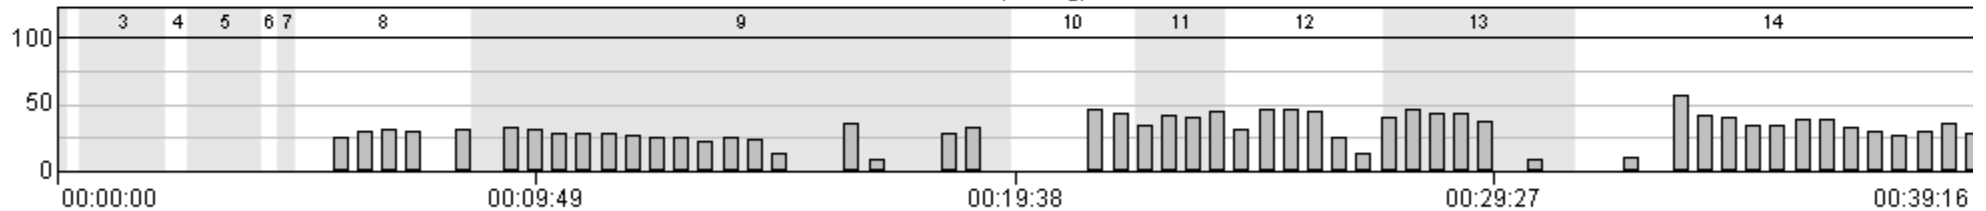



## CPR report



Device Type: LIFEPAK® 15  
 Power On: 3/26/2023 12:36:27 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355R0402000R  
 \*Non-paddles lead intervals are included in the reported CPR Ratio  
 \*Times have been adjusted by the system.

Duration: 00:41:36  
 Incident ID: 23-08546  
 Statistical Parameters: 1000-0300-3000-05

### Summary

CPR needed	=	28:51	=	CPR done	=	23:44
CPR not done	=	5:07	=	Compression count	=	2558
Longest compression pause	=	1:38	=	Pauses over 10 sec	=	8

Comment: Precharge monitor. LUCAS. Work on two minute cycles.

### Interval Statistics


CPR period	Responsible for CPR	CPR started	CPR stopped	CPR duration	Pause duration	Reason CPR stopped	Comments	Compr. ratio, %	Compr. rate	Vent. /min
1		00:00:00	00:00:02	00:00:02	00:00:10	Pulse/rhythm check		15	--	--
2		00:00:11	00:00:20	00:00:09	00:00:07	Defibrillation		71	134	--
3		00:00:27	00:02:01	00:01:34	00:00:10	Pulse/rhythm check		91	133	--
4		00:02:11	00:02:27	00:00:16	00:00:11	Defibrillation		63	141	--
5		00:02:38	00:03:58	00:01:20	00:00:12	Pulse/rhythm check		87	163	--
6		00:04:10	00:04:23	00:00:13	00:00:07	Defibrillation		83	165	--
7		00:04:30	00:04:34	00:00:04	00:00:18	Pulse/rhythm check		19	146	--
8		00:04:52	00:08:18	00:03:26	00:00:10	Pulse/rhythm check	LUCAS attached	96	102	--
9		00:08:28	00:08:47	00:00:19	00:10:45	Defibrillation	ROSC. 2 mins of CPR post shock	52	102	--
10		00:19:32	00:21:41	00:02:09	00:00:25	Pulse/rhythm check		84	102	--
11		00:22:06	00:23:41	00:01:35	00:00:16	Pulse/rhythm check		86	102	--
12		00:23:57	00:25:34	00:01:37	00:01:38	Pulse/rhythm check		50	102	--
13		00:27:12	00:30:05	00:02:53	00:01:03	Pulse/rhythm check		73	102	--
14		00:31:09	00:39:16	00:08:07	00:00:00	Termination/Transfer of Care		100	102	--

# CPR report




Device Type: LIFEPAK® 15  
 Power On: 3/26/2023 12:36:27 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355R0402000R  
 \*Non-paddles lead intervals are included in the reported CPR Ratio  
 \*Times have been adjusted by the system.

Duration: 00:41:36  
 Incident ID: 23-08546  
 Statistical Parameters: 1000-0300-3000-05



## CPR QUIK-VIEW

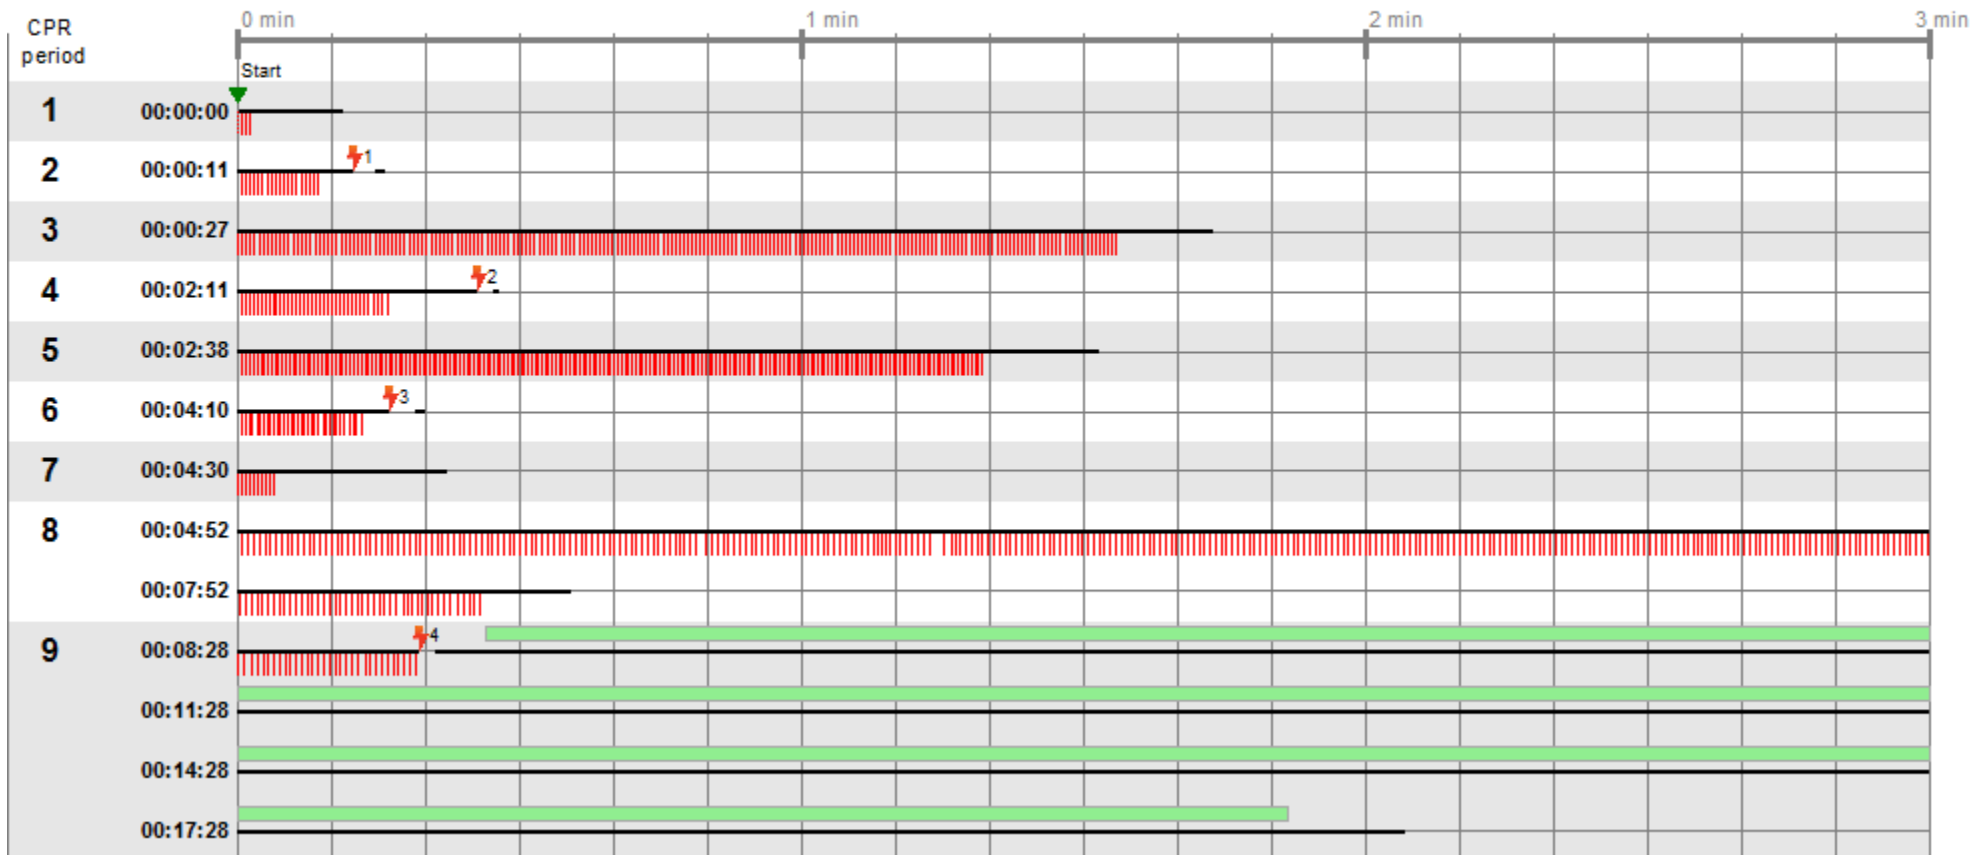


# CPR report



Device Type: LIFEPAK® 15  
 Power On: 3/26/2023 12:36:27 PM  
 CPR Annotations Edited: Yes  
 Device Configuration: 2D355R0402000R  
 \*Non-paddles lead intervals are included in the reported CPR Ratio  
 \*Times have been adjusted by the system.

Duration: 00:41:36  
 Incident ID: 23-08546  
 Statistical Parameters: 1000-0300-3000-05

## CPR QUIK-VIEW

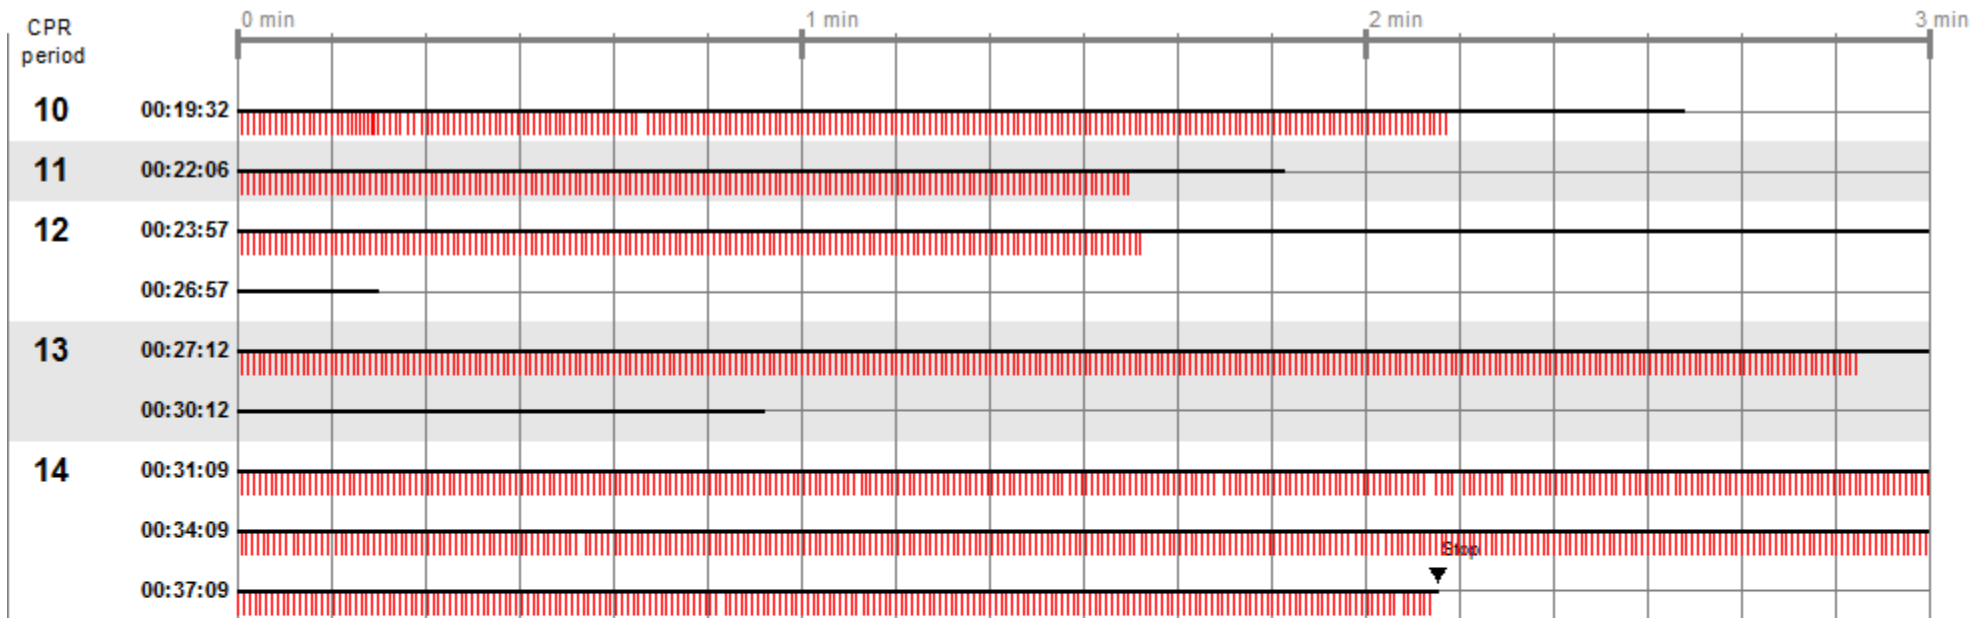

Shock	Time	Energy	Pre-shock CPR pause	Post-shock CPR pause
⚡1	0:23	200 J	0:04	0:03
⚡2	2:36	200 J	0:09	0:02
⚡3	4:26	200 J	0:03	0:04
⚡4	8:47	200 J	0:00	0:07