
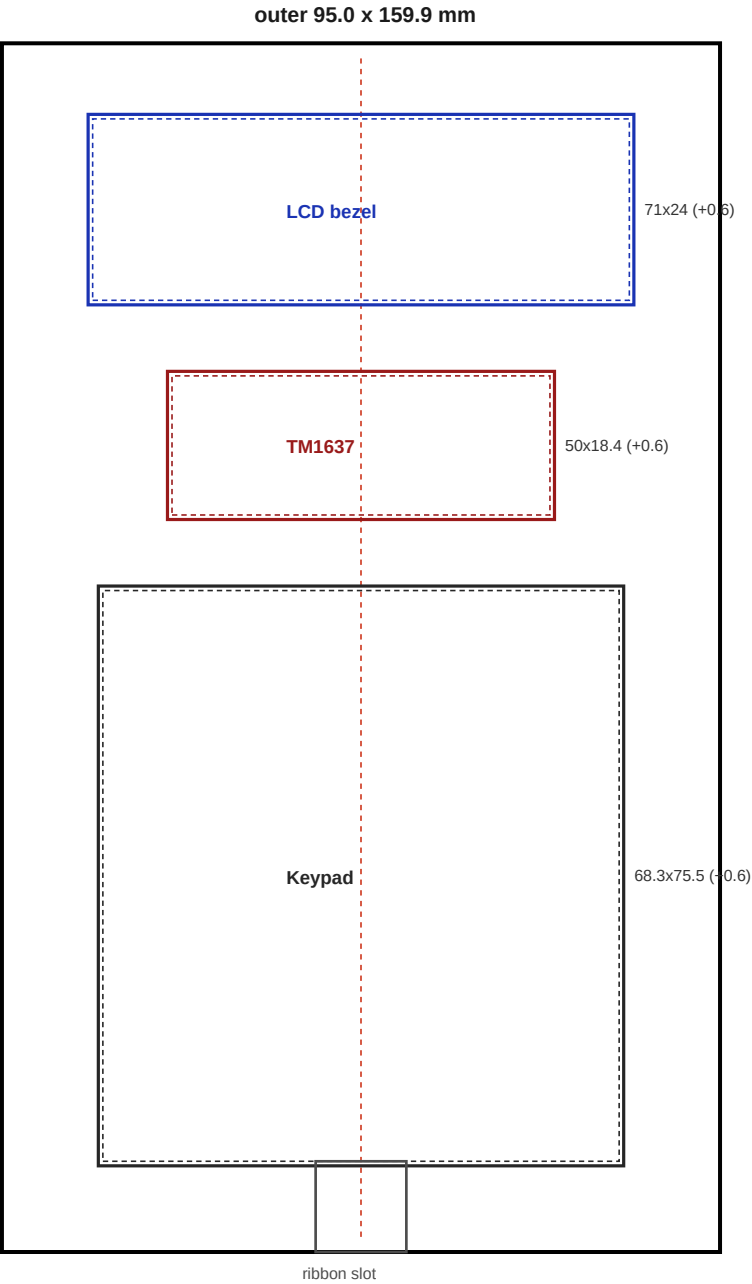


Phototherapy Timer - cardboard cut template (1:1)

PRINT AT 100% / Actual size - do NOT fit-to-page. Solid = cut. Dashed = fold/mark only.
Plate 95.0 x 159.9 mm | LCD 71x24 TM 50x18.4 Key 68.3x75.5 | gaps 10/10 mm | openings +0.6 mm clear
100 mm scale - must measure 100.0 mm on print




Instructions:

- 1) Confirm 100 mm bar. 2) Cut outer plate (heavy black). 3) Cut solid openings (LCD/TM/keypad).
- 4) Dashed inner rects = exact face size (optional mark). 5) Tape/glue parts from behind; faces flush to front.

Face outlines only - dry-fit parts (1:1)

Same sizes/gaps as cut template. PRINT 100%. Place LCD, TM1637, keypad on dashed boxes.

100 mm

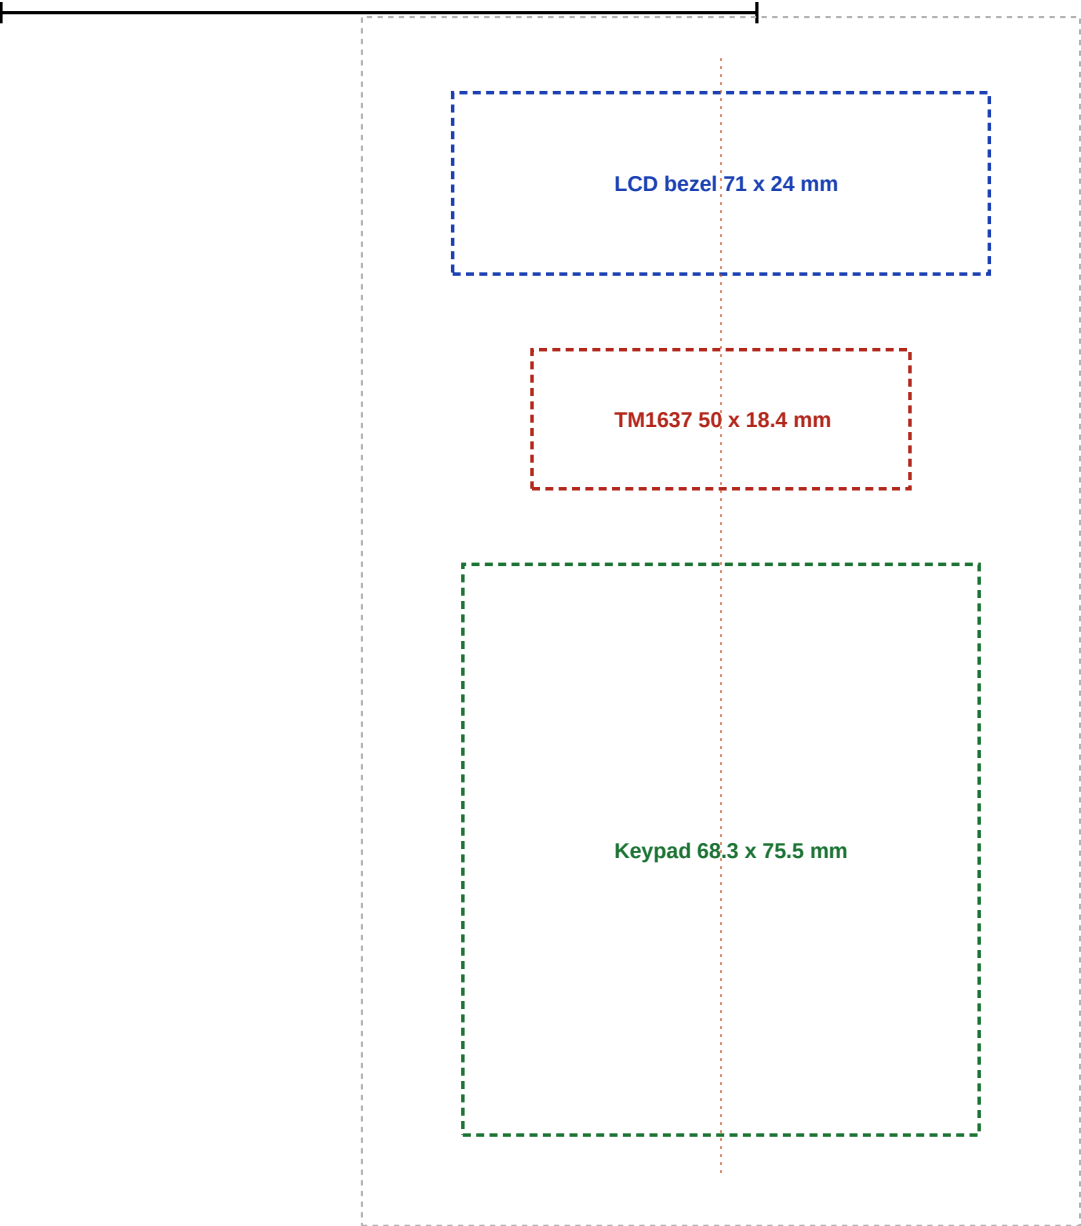

Use this page to check part placement before cutting the plate on page 1.

Gaps: LCD-TM 10 mm, TM-keypad 10 mm. Faces coplanar on finished plate.