

CERTIFICADO PATRON DE CND


TEND

NDT Reference Standard Certificate

Tubo patrón número
Reference standard #

1c442

Datos del Producto Product Information								
Diametro [mm]	60,3	Cliente Client	Ciclo Product	70932				
Espesor [mm] Wall Thickness	5,54	Tratamiento Termico	Colada _{Heat}	0				
Trazabilidad Traceability	0		Expediente Manufacturing Order					

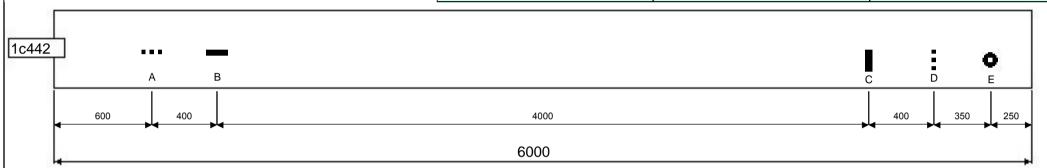

Valores Pedidos / Requested Values

Valores Medidos / Measured Values

Posicion Position	Tipo de Notch Notch Type	Ancho / Diam Max [mm] Max Width / Diam	Profundidad Nominal [%] Depth	Tolerancia [%] Tolerance	Profundidad Maxima [mm] Max Depth	Profundidad Minima [mm] Min Depth	Profundidad Nominal [mm] Nom Depth	Longitud Maxima [mm] Max Length	Longitud [mm] Length	Profundida d A [mm] Depth A	Profundida d B [mm] Depth B	Ancho / Diam [mm] Width / Diam	Responsable Responsible	Fecha Date
Α	Longitudinal Interno Longitudinal ID	0,92	5	±15	0,319	0,235	0,277	37,80	37,80	0,300	0,300	0,92	Sebastian Monteros	09/09/04
В	Longitudinal Externo longitudinal OD	0,91	5	±15	0,319	0,235	0,277	25,20	25,20	0,310	0,310	0,91	Sebastian Monteros	09/09/04
С	Transversal Externo Transverse OD	0,92	5	±15	0,319	0,235	0,277	25,80	25,80	0,310	0,300	0,92	Sebastian Monteros	09/09/04
D	Transversal Interno Transverse ID	0,93	5	±15	0,319	0,235	0,277	38,60	38,60	0,320	0,320	0,93	Sebastian Monteros	09/09/04
Е	Agujero Pasante Drilled hole	3,18	-	-	-	-	-	-	-	-	-	3,18	Sebastian Monteros	09/09/04

Instrumentos de Medicion Utilizados:

Notas:

1.-Todas las dimensiones son en milimetros excepto que se indique lo contrario.

2.-Minima Profundidad Nominal de las ranuras 0.3 mm.

CERTIFICADO CON REPLICA NO

Notes:

1.-All dimensions in milimeters unless stated.

1/2

2.-Minimum notch nominal depth 0.3 mm.

CERTIFIED WITH PLASTIC REPLICA NO