


Work Breakdown Structure — Peritoneal Dialysis Remote Patient Monitoring System

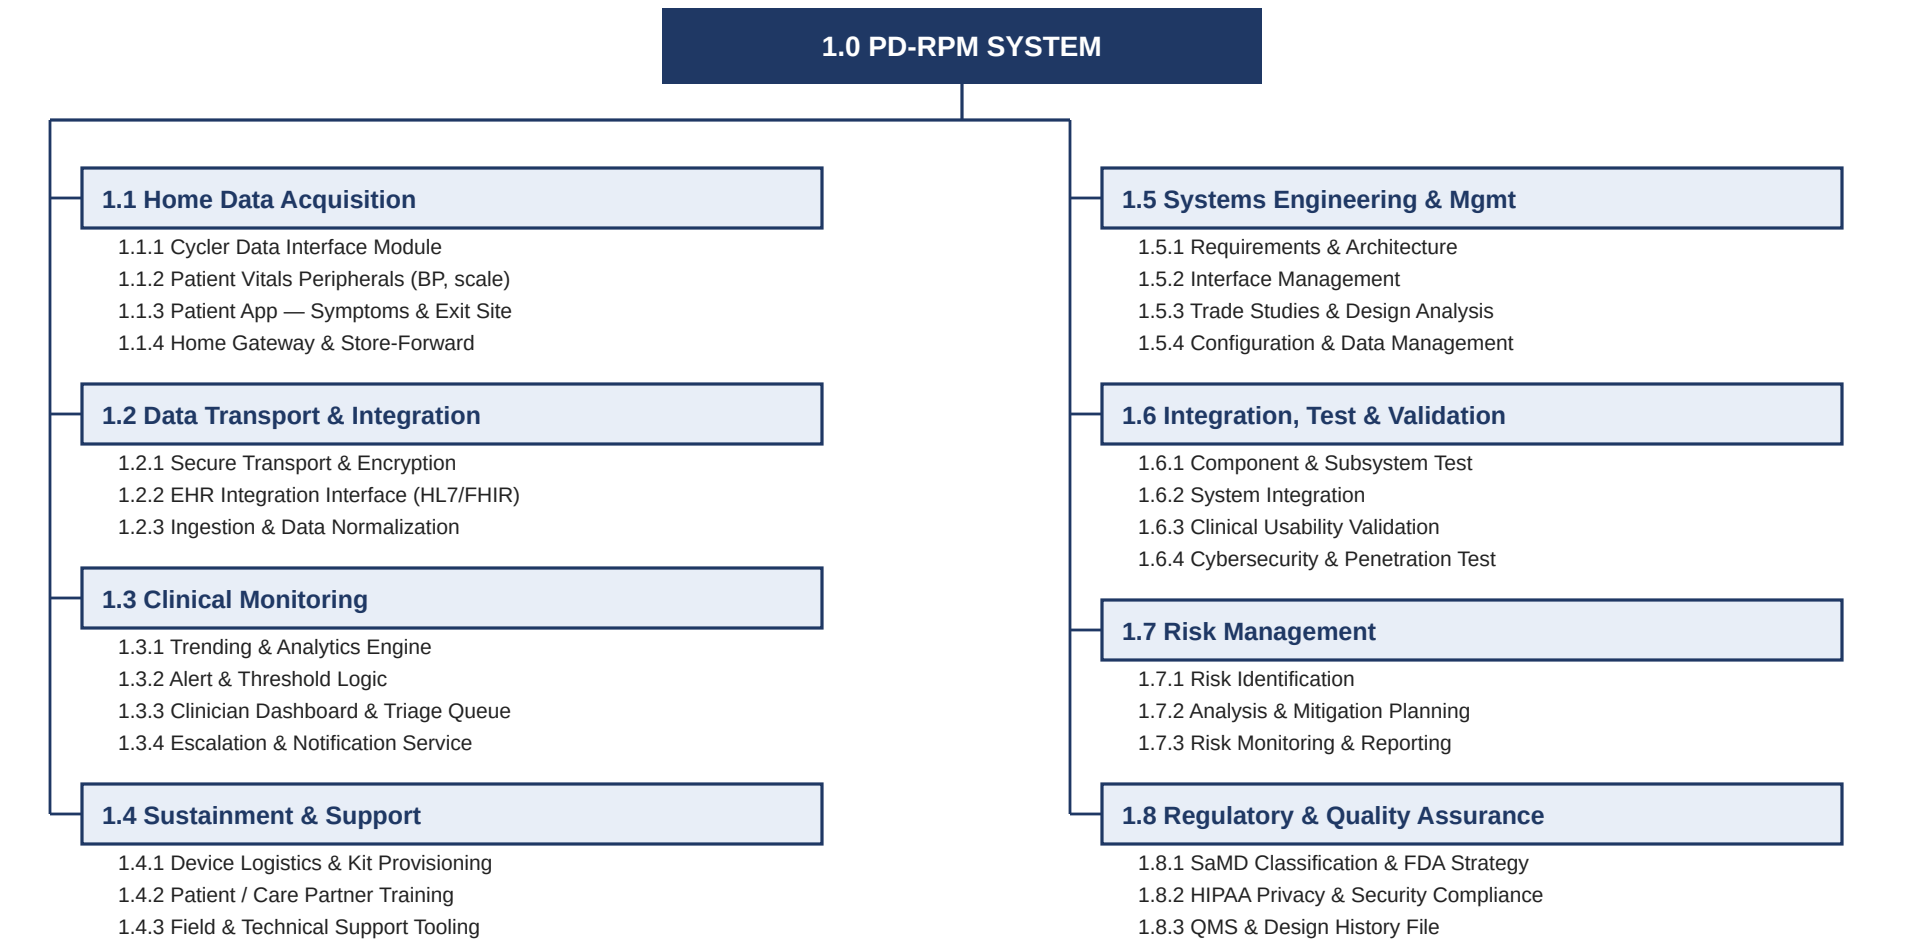

Outside the WBS — required for operation, not built by this project (interface defined instead):

- PD cyclor — manufacturer's regulated Class II device; interface defined at 1.1.1
- Broadband / cellular carrier network; interface defined at 1.2.1
- EHR platform itself; interface defined at 1.2.2
- Dialysate manufacturing & distribution; interface defined at 1.4.1

Elements 1.5–1.8 are non-deliverable work packages: they consume schedule, budget, and staff, so they are carried in the WBS even though they produce no hardware.