

NARDA Safety Test

Solutions S.r.I. Socio Unico

Sales & Support:

Via Leonardo da Vinci, 21/23 20090 Segrate (MI) - ITALY Tel: +39 02 2699871

Fax: +39 02 26998700

Manufacturing Plant:

Via Benessea, 29/B 17035 Cisano sul Neva (SV) Tel.: +39 0182 58641 Fax: +39 0182 586400



User's Manual

PMM EP600

ELECTRIC FIELD PROBE 100 kHz ÷ 9.25 GHz

PMM EP601

ELECTRIC FIELD PROBE 10 kHz ÷ 9.25 GHz

PMM EP602

ELECTRIC FIELD PROBE 5 kHz ÷ 9.25 GHz

PMM EP603

ELECTRIC FIELD PROBE 300 kHz ÷ 18 GHz

SERIAL NUMBER OF THE INSTRUMENT

You can find the Serial Number on the fiber optic holder of the instrument. The Serial Number is in the form: 000XY00000.

The first three digits and the two letters are the Serial Number prefix, the last five digits are the Serial Number suffix. The prefix is the same for identical instruments, it changes only when a configuration change is made to the instrument. The suffix is different for each instrument

Document EP60XEN-21013-2.06 - Copyright © NARDA 2009



NOTE:

® Names and Logo are registered trademarks of Narda Safety Test Solutions GmbH and L3 Communications Holdings, Inc. – Trade names are trademarks of the owners.

If the instrument is used in any other way than as described in this Users Manual, it may become unsafe

Before using this product, the related documentation must be read with great care and fully understood to familiarize with all the safety prescriptions.



To ensure the correct use and the maximum safety level, the User shall know all the instructions and recommendations contained in this document.

This product is a **Safety Class III** instrument according to IEC classification and has been designed to meet the requirements of EN61010-1 (Safety Requirements for Electrical Equipment for Measurement, Control and Laboratory Use).

In accordance with the IEC classification, the battery charger of this product meets requirements **Safety Class II** and **Installation Category II** (having double insulation and able to carry out mono-phase power supply operations)..



It complies with the requirements of **Pollution Class II** (usually only non-conductive pollution). However, occasionally it may become temporarily conductive due to condense on it.

The information contained in this document is subject to change without notice.

KEY TO THE ELECTRIC AND SAFETY SYMBOLS:



You now own a high-quality instrument that will give you many years of reliable service. Nevertheless, even this product will eventually become obsolete. When that time comes, please remember that electronic equipment must be disposed of in accordance with local regulations. This product conforms to the WEEE Directive of the European Union (2002/96/EC) and belongs to Category 9 (Monitoring and Control Instruments). You can return the instrument to us free of charge for proper environment friendly disposal. You can obtain further information from your local Narda Sales Partner or by visiting our website at www.narda-sts.it.



Warning, danger of electric shock





Read carefully the Operating Manual and its instructions, pay attention to the safety symbols.





Earth Protection



KEY TO THE SYMBOLS USED IN THIS DOCUMENT:



DANGER

The DANGER sign draws attention to a potential risk to a person's safety. All the precautions must be fully understood and applied before proceeding.



WARNING

The WARNING sign draws attention to a potential risk of damage to the apparatus or loss of data. All the precautions must be fully understood and applied before proceeding.



CAUTION

The CAUTION sign draws attention against unsafe practices for the apparatus functionality.



NOTE:

The NOTE draw attention to important information.

II Note and symbols



Contents

	Page
Safety requirements and instructions	VI
EC Conformity Certificate	VII
1 General	Page
1.1 Documentation	1-1
1.2 Diode-based isotropic electric field probes	1-1
1.3 Introduction	1-2
1.4 Specifications EP600	1-3
1.5 Typical frequency responce with correction EP600	1-4
1.6 Specifications EP601	1-5
1.7 Typical frequency responce with correction EP601	1-6
1.8 Specifications EP602	1-7
1.9 Typical frequency responce with correction EP602	1-8
	1-0
1.10 Specifications EP603	-
1.11 Typical frequency responce with correction EP603	1-10
1.12 Typical anisotropicity @ 50 MHz EP603	1-10
1.13 Battery management PMM EP600/EP601/EP602/EP603	1-11
1.14 Housing and connectors EP600/EP601/EP602/EP603	1-12
1.15 Standard accessories	1-12
1.16 Options	1-12
2 Operation	Page
2.1 Foreword	2-1
2.2 Inspection.	2-1
2.3 Ambient	2-1
2.4 Return for service.	2-1
	2-1
2.5 Cleaning.	
2.6 Probe support	2-2
2.7 Coupling between probe and conductive surfaces	2-2
2.8 Coupling between probe and operator's body	2-2
2.9 Multiple sources	2-2
2.10 Connecting EP600/EP601/EP602/EP603	2-3
2.10.1 RS232 Connection	2-3
2.10.2 USB Connection	2-5
2.10.3 Connection of fiber optic extension FO-EP600/10	2-7
2.11 EP600/EP601/EP602/EP603 Installation	2-8
2.11.1 EP600/EP601/EP602/EP603 Installation on the conical holder	2-8
2.11.1.1 EP600/EP601/EP602/EP603 removal from the conical holder.	2-10
2.11.2 EP600/EP601/EP602/EP603 installation on tripod PMM TR-02	2-11
3 Measurements	Page
3.1 Foreword	3-1
	3-1
3.2 Preliminary	
3.2.1 Spurious signals	3-1
3.3 General requirements	3-2
3.3.1 Probes	3-2
3.3.2 Connections	3-2
3.3.3 Metering equipment	3-2
3.4 Basic functional checks	3-2
3.5 Measurement procedures	3-2
3.6 Preventing measurement errors	3-3
3.7	3-3
3.8	3-3
3.9 PMM EP600/EP601/EP602/EP603 operation	3-4
3.10 Applications	3-6
3.10.1 EMC	3-6
	3-8
3.10.2	
3.11 Operating EP600/EP601/EP602/EP603 with 8053B	3-9
3.12 Operating EP600/EP601/EP602/EP603 with PMM SB10 (Option).	3-10



4 Battery cha		Pa
		4-
	er	4-
4.2.1 AC maii	ns plug	4-
	HARGER	4-
4.3.1 Specific	ationsCHARGER components	4-: 4-:
	PMM EP600/EP601/EP602/EP603on EP600 CHARGER	4-
4.4 mstalling	FININI EF000/EF001/EF002/EF003011 EF000 CHARGER	4-
5 WinFP600	Operating instructions	Pa
5.1 Foreword		5-
5.2 PC minim	um requirements	5-
5.3 Installatio	n	5-
	settings with 8053-OC	5-
5.4.1 WinEP6	600 COM port settings	5-
5.4.2 SetAddl	EP600 COM port settings	5-
5.5 COM port	settings with adapter USB-RS232	5-
5.5.1 WinEP6	500 COM port settings	5-
	EP600 COM port settings	5-
	VinEP600	5- 5-
	low contents	5- 5-
	ndow displayed measurements	5- 5-
	ncy correction setting	5-
5.7.4 Reading	Rate setting	5-
	OT	5-
	RUN	5-
		5-
5.7.8 Setting	menu	5-
	gs	5-
	rence	5-
	0)	5-
	SetAddEP600	5-
5.9 Main wind	dow	5- 5-
	rlata	5- 5-
	dress	5- 5-
		5-
	ling WinEP600 and SetAddEP600	5-
	ling the driver of RS232-USB adapter	5-
	ation protocol	Pa
	r	6-
6.2 Protocol		6-
DII Euroti	ion reference guide	ъ.
	gege	Pa 7-
.1 0 Earigua 7 1 1 PMM (CreateProbe()	7-
	RemoveProbe()	7-
	irmware()	7-
	ProbeName()	7-
	Model()	7-
	CalibrationDate()	7-
	ReadBattery()	7-
1.1.8 PMM_R	ReadTemperature()	7-
	SerialNumber()	7-
	SetFrequency()	7-
	SetFilter()	7- 7
.1.12 PMM_	SetTimeout()	7- 7
	SetAutoOffTime()	7- 7
	ReadTotalField()ReadAxisField	7- 7-
, . i . i ⊍ Fiviivi_ 7 2 ∖/isııal Ra	sic	7- 7-
	de	7-
	Ī	•
IV	Contents	



8 Accessories	Page
8.1 Foreword	8-1
8.2 Inspection	8-1
8.3 Ambient	8-1
8.4 Return for service	8-1
8.5 Cleaning	8-1
8.6 8053-OC Optical Serial converter	8-3
8.7 8053-OC-PS Power Supply	8-5
8.8 TR-02A Tripod	8-7
8.9 TT-01 Telescopic extension	8-11
8.10 SB-10 Switching Control Box	8-13



Figures

Figure		Page
1-1	EP600/EP601/EP602/EP603	1-2
1-2	Typical frequency responce with correction EP600	1-4
1-3	Typical frequency responce with correction EP601	1-6
1-4	Typical frequency responce with correction EP602	1-8
1-5	Typical frequency responce with correction EP603	1-10
1-6	Typical anisotropicity @ 50 MHz EP603	1-10
1-7	Plastic housing	1-12
1-8	Optical connectors	1-12
2-1	RS232 connection of EP600/EP601/EP602/EP603 with FO-EP600/10	
	extension	2-4
2-2	USB connection of EP600/EP601/EP602/EP603 with FO-EP600/10	
	extension	2-6
2-3	EP600/EP601/EP602/EP603 mounted on conical holder	2-9
2-4	EP600/EP601/EP602/EP603 on TR-02A	2-11
2-5	EP600/EP601/EP602/EP603 on TR-02A with PMM 8053-SN	2-11
3-1	EP600/EP601/EP602/EP603 in open site	3-6
3-2	EP600/EP601/EP602/EP603 in TEM cell	3-7
3-3	EP600/EP601/EP602/EP603 in Anechoic Chamber	3-7
3-4	EP600/EP601/EP602/EP603 with 8053B	3-9
3-5	EP600/EP601/EP602/EP603 with one SB-10	3-10
3-6	EP600/EP601/EP602/EP603 with five SB-10	3-10
3-7	EP600/EP601/EP602/EP603 with SB-10 in open site	3-10
4-1	AC Adapter	4-1
4-2	EP600 CHARGER	4-1
4-3	EP600 CHARGER components	4-3
4-4	EP600/EP601/EP602/EP603 on EP600 CHARGER	4-5
8-1	8053-OC Panels	8-3
8-2	8053-OC-PS	8-5
8-3	TR02A	8-8
8-4	Adjustable swivel	8-9
8-5	TT-01 Fiberglass telescopic extension with PMM EP600/EP601/EP602/EP603	
	installed on the top	8-11

Tables

Table		Page
1-1	Specifications of the electric field probe EP600	1-3
1-2	Specifications of the electric field probe EP601	1-5
1-3	Specifications of the electric field probe EP602	1-7
1-4	Specifications of the electric field probe EP603	1-9
1-5	Battery management PMM EP600/EP601/EP602/EP603	1-11
4-1	Characteristics and specifications of the battery charger EP600 CHARGER	4-2
4-2	EP600 CHARGER Led status – Start up phase	4-5
4-3	EP600 CHARGER Led status – Charge phase	4-5
6-1	Query Commands	6-3
6-2	Setting Commands	6-4
6-3	Operative Commands	6-5
7-1	Status code	7-1
8-1	Specifications of PMM 8053-OC	8-3
8-2	Specifications of 8053-OC-PS Power Supply	8-5
8-3	Characteristics of PMM TR-02A	8-7
8-4	Characteristics of TT-01	8-11





SAFETY RECOMMENDATIONS AND INSTRUCTIONS

This product has been designed, produced and tested in Italy, and it left the factory in conditions fully complying with the current safety standards. To maintain it in safe conditions and ensure correct use, these general instructions must be fully understood and applied before the product is used.

- When the device must be connected permanently, first provide effective grounding;
- If the device must be connected to other equipment or accessories, make sure they are all safely grounded;
- In case of devices permanently connected to the power supply, and lacking any fuses or other devices of mains protection, the power line must be equipped with adequate protection commensurate to the consumption of all the devices connected to it;
- In case of connection of the device to the power mains, make sure before connection that the
 voltage selected on the voltage switch and the fuses are adequate for the voltage of the actual
 mains;
- Devices in Safety Class I, equipped with connection to the power mains by means of cord and plug, can only be plugged into a socket equipped with a ground wire;
- Any interruption or loosening of the ground wire or of a connecting power cable, inside or outside the device, will cause a potential risk for the safety of the personnel;
- Ground connections must not be interrupted intentionally;
- To prevent the possible danger of electrocution, do not remove any covers, panels or guards installed on the device, and refer only to NARDA Service Centers if maintenance should be necessary;
- To maintain adequate protection from fire hazards, replace fuses only with others of the same type and rating:
- Follow the safety regulations and any additional instructions in this manual to prevent accidents and damages.



EC Conformity Certificate

(in accordance with the Directives: EMC 89/336/EEC and Low Voltage 73/23/EEC)

This is to certify that the product: EP600 Electric field Probe

Produced by: NARDA Safety Test Solutions

Via Benessea 29/B

17035 Cisano sul Neva (SV) - ITALY

complies with the following European Standards:

Safety: CEI EN 61010-1 (2001) EMC: EN 61326-1 (2007)

This product complies with the requirements of the Low Voltage Directive 73/23/EEC, amended by 93/68/EEC, and with the EMC Directive EMC 89/336/EEC amended by 92/31/EEC, 93/68/EEC, 93/97/EEC.

NARDA Safety Test Solutions

EC Conformity Certificate

(in accordance with the Directives: EMC 89/336/EEC and Low Voltage 73/23/EEC)

This is to certify that the product: EP601 Electric field Probe

Produced by: NARDA Safety Test Solutions

Via Benessea 29/B

17035 Cisano sul Neva (SV) - ITALY

complies with the following European Standards:

Safety: CEI EN 61010-1 (2001) EMC: EN 61326-1 (2007)

This product complies with the requirements of the Low Voltage Directive 73/23/EEC, amended by 93/68/EEC, and with the EMC Directive EMC 89/336/EEC amended by 92/31/EEC, 93/68/EEC, 93/97/EEC.

NARDA Safety Test Solutions

EC Conformity Certificate

(in accordance with the Directives: EMC 89/336/EEC and Low Voltage 73/23/EEC)

This is to certify that the product: EP602 Electric field Probe

Produced by: NARDA Safety Test Solutions

Via Benessea 29/B

17035 Cisano sul Neva (SV) - ITALY

complies with the following European Standards:

Safety: CEI EN 61010-1 (2001) EMC: EN 61326-1 (2007)

This product complies with the requirements of the Low Voltage Directive 73/23/EEC, amended by 93/68/EEC, and with the EMC Directive EMC 89/336/EEC amended by 92/31/EEC, 93/68/EEC, 93/97/EEC.

NARDA Safety Test Solutions



EC Conformity Certificate

(in accordance with the Directives: EMC 89/336/EEC and Low Voltage 73/23/EEC)

This is to certify that the product: EP603 Electric field Probe

Produced by: NARDA Safety Test Solutions Via Benessea 29/B

17035 Cisano sul Neva (SV) - ITALY

complies with the following European Standards:

Safety: CEI EN 61010-1 (2001) EMC: EN 61326-1 (2007)

This product complies with the requirements of the Low Voltage Directive 73/23/EEC, amended by 93/68/EEC, and with the EMC Directive EMC 89/336/EEC amended by 92/31/EEC, 93/68/EEC, 93/97/EEC.

NARDA Safety Test Solutions



This page has been left blank intentionally



1 - General

1.1 Documentation

This Manual includes:

- Questionnaire to resend together with the instrument to service.
- Check list of supplied accessories.
- 1.2 Diode-based isotropic electric field probes

This type of probes are made by small antennas terminated on multiple diodes. To ensure optimal isotropy, the antenna elements are configured orthogonally in order to add all of the electromagnetic wave components. They measure the field independently from field polarization and direction.

The diodes feature linear and quadratic responses to level variations. At low levels of field the output voltages are proportional to the square value of the field (E^2) i.e. to the RMS value.

At higher field levels, up to the saturation, the response becomes linear, thus the output voltages are proportional to the peak value of the field. The calibration is performed in terms of RMS value in both cases, therefore modulated sources may require a proper correction factor to be taken into account.



1.3 Introduction

The EP600/EP601/EP602/EP603 is a diode-type, three-axis technology-edge isotropic sensor of electric fields: from 0.14 to 140 V/m in the frequency range 100 kHz - 9.25 GHz (EP600), from 0.5 to 500 V/m in the frequency range 10 kHz - 9.25 GHz (EP601), from 1.5 to 1500 V/m in the frequency range 5 kHz - 9.25 GHz (EP602) and from 0.17 to 170 V/m in the frequency range 300 kHz - 18 GHz (EP603).

The spherical plastic housing includes: 6 orthogonal cones (one for each monopole) that allow for an easy identification of the electric field vectors; the ON/OFF button and LED; the battery and the charger connector.

A plastic fiber optic (not removable) is fixed to the EP600/EP601/EP602/EP603 housing; at its extremity two connectors compatible with PMM devices allow for connection to PC (via optical adapter) or to the hand-held meter PMM 8053B to display the measurements and to set the proper filter for optimizing noise reduction, sampling time and battery autonomy.

The software supplied allows for storing the measurements and convert the same in text format. The recorded data can be viewed either as a graph or as a table.

The EP600/EP601/EP602/EP603 includes an E²PROM that stores serial number, calibration data, calibration factors and Firmware version.

Three Analog/Digital converters – one for each axis - read the electric field simultaneously; the sensors consist in 6 monopoles mounted orthogonally. Another Analog/Digital converter internal to the microcontroller provides the battery voltage and temperature measurements.

The EP600/EP601/EP602/EP603 is supplied by an internal rechargeable battery capable of up to 80 hours of operation.



Fig. 1-1 EP600/EP601/EP602/EP603



1.4 Specifications EP600 This condition applies to all specifications:

• The operating ambient temperature range must be -10° to 50 °C.

TABLE 1-1 Specifications of the electric field probe PMM EP600

Frequency range 100 kHz - 9.25 GHz
Level range 0.14 - 140 V/m
Overload > 300 V/m
Dynamic range 60 dB

Linearity 0.4 dB @ 50 MHz/0.3 – 100 V/m

Resolution 0.01 V/m Sensitivity 0.14 V/m

Flatness 1 – 150 MHz 0.8dB

0.5 – 6000 MHz 1.6 dB 0.3 – 7500 MHz 3.2 dB

(With frequency correction OFF)

0.3 - 7500 MHz 0.4 dB

(Typical with frequency correction ON)

Isotropicity 0.5 dB (0.3 dB typical @ 50 MHz)

Sensors Six monopoles

X/Y/Z reading Simultaneous sampling of the components

Battery reading 10 mV res.
Temperature reading 0.1 °C res.
Internal data memory Serial number
Date calibration

Calibration Factor SW release.

Battery Panasonic ML621S 3V 5mA/h rechargeable Li-Mn

Operation time 80 h @ 0.4 S/sec 28 Hz filter 60 h @ 5 S/sec 28 Hz filter

Recharge time 48h for maximum autonomy

Dimensions 17 mm sphere 17 mm sensor

53 mm overall

Weight 23g including FO weight (1m)

Operating temperature -10° - +50°
Software for PC
YES

Optical fiber connector HFBR-0500

Tripod adapter ½ - 20 UNC female



1.5 Typical frequency response with correction OFF EP600

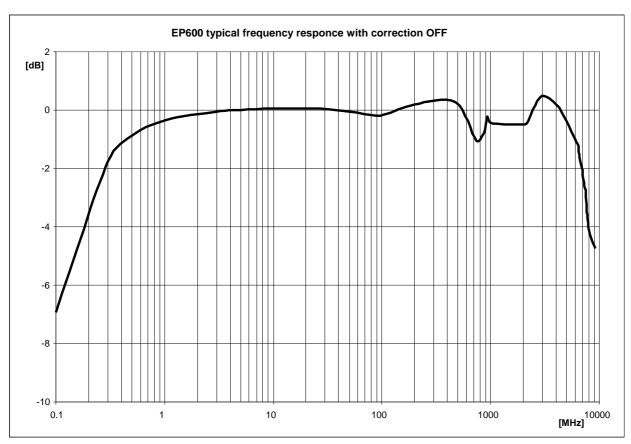


Fig. 1-2 EP600 typical frequency responce with correction OFF



1.6 Specifications EP601

This condition applies to all specifications:

• The operating ambient temperature range must be -10° to 50 °C.

TABLE 1-2 Specifications of the electric field probe PMM EP601

Frequency range 10 kHz - 9.25 GHzLevel range 0.5 - 500 V/mOverload > 1000 V/mDynamic range 60 dB

Linearity 0.4 dB @ 50 MHz/1 – 500 V/m

Resolution 0.01 V/m Sensitivity 0.5 V/m

Flatness 0.1 – 150 MHz 0.4dB

 $\begin{array}{ll} 0.05-6000~\text{MHz} & 1.6~\text{dB} \\ 0.03-7500~\text{MHz} & 3.2~\text{dB} \\ \text{(With frequency correction OFF)} \end{array}$

0.05 - 7500 MHz 0.4 dB

(Typical with frequency correction ON)

Isotropicity 0.5 dB (0.3 dB typical @ 50 MHz)

Sensors Six monopoles

X/Y/Z reading Simultaneous sampling of the components

Battery reading 10 mV res.
Temperature reading 0.1 °C res.
Internal data memory Serial number
Date calibration

Calibration Factor SW release.

Battery Panasonic ML621S 3V 5mA/h rechargeable Li-Mn

Operation time 80 h @ 0.4 S/sec 28 Hz filter 60 h @ 5 S/sec 28 Hz filter

Recharge time 48h for maximum autonomy

Dimensions 17 mm sphere 17 mm sensor

53 mm overall

Weight 23g including FO weight (1m)

Operating temperature -10° - +50°
Software for PC YES
Optical fiber connector HFBR-0500

Tripod adapter ½ - 20 UNC female



1.7 Typical frequency response with correction OFF EP601

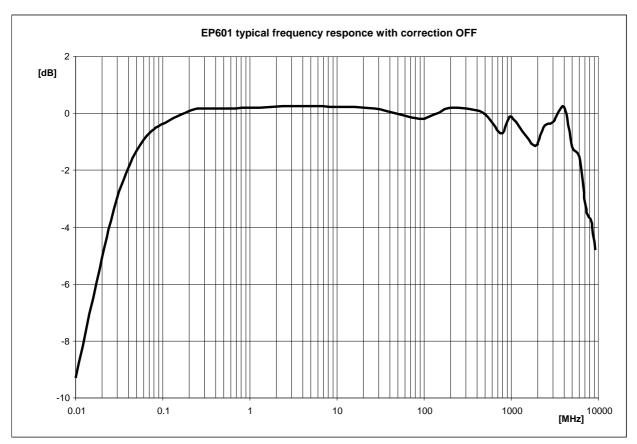


Fig. 1-3 EP601 typical frequency responce with correction OFF



1.8 Specifications EP602 This condition applies to all specifications:

• The operating ambient temperature range must be -10° to 50 °C.

TABLE 1-3 Specifications of the electric field probe PMM EP602

Frequency range 5 kHz - 9.25 GHzLevel range 1.5 - 1500 V/mOverload > 3000 V/mDynamic range 60 dB

Linearity 0.4 dB @ 50 MHz/2.5 – 1000 V/m

Resolution 0.01 V/m Sensitivity 1.5 V/m

Flatness 0.05 – 150 MHz 0.4dB

0.05 - 7500 MHz 0.4 dB

(Typical with frequency correction ON)

Isotropicity 0.5 dB (0.3 dB typical @ 50 MHz)

Sensors Six monopoles

X/Y/Z reading Simultaneous sampling of the components

Battery reading
Temperature reading
Internal data memory

Date calibration
Calibration Fact

Calibration Factor SW release.

Battery Panasonic ML621S 3V 5mA/h rechargeable Li-Mn

Operation time 80 h @ 0.4 S/sec 28 Hz filter 60 h @ 5 S/sec 28 Hz filter

Recharge time 48h for maximum autonomy

Dimensions 17 mm sphere 17 mm sensor 53 mm overall

23g including FO weight (1m)

Weight 23g includir
Operating temperature -10° - +50°
Software for PC YES

Optical fiber connector HFBR-0500

Tripod adapter ½ - 20 UNC female



1.9 Typical frequency response with correction OFF EP602

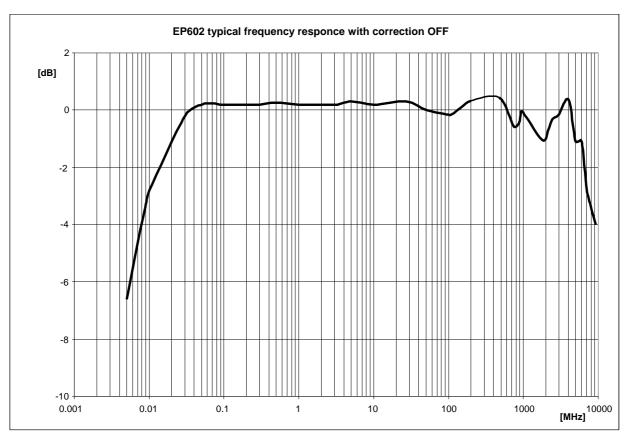


Fig. 1-4 EP602 typical frequency responce with correction OFF



1.10 Specifications EP603 This condition

This condition applies to all specifications:

• The operating ambient temperature range must be -10° to 50 °C.

TABLE 1-4 Specifications of the electric field probe PMM EP603

Frequency range 300 kHz – 18 GHz
Level range 0.17 – 170 V/m
Overload > 350 V/m
Dynamic range 60 dB

Linearity 0.4 dB @ 50 MHz/0.3 – 170 V/m

Resolution 0.01 V/m Sensitivity 0.17 V/m

Flatness 3 – 8200 MHz 1.4dB

1 – 12000 MHz 2.4 dB 0.6 – 18000 MHz 3.8 dB (With frequency correction OFF)

0.3 - 18000 MHz 0.4 dB

(Typical with frequency correction ON)

Isotropicity 0.4 dB (0.2 dB typical @ 50 MHz)

Sensors Six monopoles

X/Y/Z reading Simultaneous sampling of the components

Battery reading 10 mV res.
Temperature reading 0.1 °C res.
Internal data memory Serial number
Date calibration

Calibration Factor SW release.

Battery Panasonic ML621S 3V 5mA/h rechargeable Li-Mn

Operation time 80 h @ 0.4 S/sec 28 Hz filter 60 h @ 5 S/sec 28 Hz filter

Recharge time 48h for maximum autonomy

Dimensions 17 mm sphere 17 mm sensor 53 mm overall

Weight 23g including FO weight (1m)

Operating temperature -10° - +50°
Software for PC YES
Optical fiber connector HFBR-0500

Tripod adapter ½ - 20 UNC female



1.11 Typical frequency response with correction OFF EP603

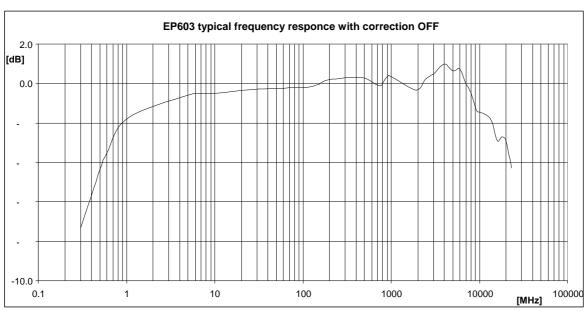


Fig. 1-5 EP603 typical frequency responce with correction OFF

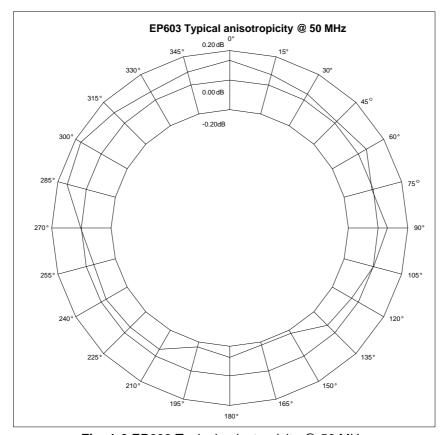


Fig. 1-6 EP603 Typical anisotropicity @ 50 MHz



1.12 Battery management EP600/EP601/EP602/ EP603

PMM EP600/EP601/EP602/EP603 has an internal Li-Mn rechargeable battery. To charge it use the provided EP600 CHARGER (see chapter 4). The EP600 CHARGER manages the battery charging taking it to full charge automatically.

Nevertheless this type of battery allows partial charge without damages expect for the ageing due to the number of cycles.

The table below shows the typical discharge values of a new battery according to the charge time.

TABLE 1-4 Battery management PMM EP600/EP601/EP602/EP603			
	Filter 28Hz Rate 0.2 sec [5 Sample/sec]	Filter 28 Hz Rate 2.5 sec [0.4 Sample/sec]	
Charge time [h]	Discharge time [h]	Discharge time [h]	
1	3	5	
2	4	8	
4	8	12	
8	13	21	
12	18	31	
24	32	56	
36	45	70	
48	60	80	



1.13 Housing and connectors





Fig. 1-7 Plastic housing



BLUE = Transmitter

1. ON-OFF Led

2. ON-OFF pushbutton

3. Battery compartment and closure

Charger connector receptacle

5. Fiber optic holder and ID label

GREY = Receiver



Fig. 1-8 Optical connectors

1.14 Standard accessories

and **PMM** Accessories documents supplied with EP600/EP601/EP602/EP603:

- Battery charger EP-600 CHARGER
- AC adapter EP-600 CHARGER
- International plugs (UK, USA)
- Italian plug;
- Fiber optic adapter, Blue
- Fiber optic adapter, Grey
- Fiber optic cable FO-EP600/10 (length: 10m)
- Optical-RS232 converter 8053-OC
- USB-RS232 converter
- Tripod mounting adapter
- Mini tripod
- Nylon adapter ¼" Withworth
- Carrying case
- Software CD-ROM
- Operating Manual
- Calibration Certificate
- Service form

1.15 Options

Options to order separately:

- PMM 8053B Hand-held metering unit
- PMM SB-10 Switching Control Box
- Fiber optic cable FO-EP600/10 (length: 10m)
- Fiber optic cable FO-EP600/20 (length: 20m)
- Fiber optic cable FO-EP600/40 (length: 40m)
- Optical-RS232 converter 8053-OC
- 8053-OC-PS Power Supply
- TR-02A tripod
- TT-01 Telescopic extension



2 - Operation


2.1 Foreword

None

2.2 Inspection

Once received the instrument, check:

- packing integrity
- instrument and accessories integrity
- contents, according to the check list attached to this manual



If anything is found damaged or missed, immediately contact your Dealer.

2.3 Ambient

Store instrument and accessories in clean, dry environment free of dust and acid vapours.

Follow requirements for temperature and humidity:

Operation:

Temperature
 Humidity
 -10° to +40° C
 90% RH

Storage:

Temperature
 Humidity
 -20° to + 70° C
 95% RH

2.4 Return for service

Every part of the instrument, included the battery, can only be replaced by NARDA, when the instrument needs repair or is malfunctioning, please contact the NARDA Support center.

When the instrument needs to be sent to NARDA for repairs please complete the questionnaire enclosed with this Operating Manual making sure you fill in all the details relative to the service requested.

In order to minimize repair time, please describe the nature of the failure. If the failure occurs only under certain conditions, please provide details on how we may recreate the same condition in order to identify the fault.

If possible, please reuse the original packaging, making sure the instrument in wrapped in heavy paper or plastic.

Alternatively, use a strong box filled with shockproof material, place enough material all around the equipment so that the unit is stable and firmly blocked inside the box.


Whilst packing, pay special care in protecting the unit's front panel.

Seal the box firmly before shipment.

Mark the box: FRAGILE HANDLE WITH CARE.

2.5 Cleaning

To clean the equipment use only dust-free, non-abrasive dry cloths.



To avoid damage never use any kind of solvent, acid, or similar to clean the instrument.



2.6 Probe support

The conical holder and the extension fiber optic FO-EP600/10 are essential for proper operation. The optional tripod PMM TR-02 is highly recommended for positioning the EP600/EP601/EP602/EP603 at the required height and distance.

2.7 Coupling between probe and conductive surfaces

Close proximity of the probe to conductive surfaces can cause direct coupling (capacitive or inductive) with the field sensing dipoles.

Additional measurement uncertainty due to coupling can be limited to 1dB by respecting these minimum distances between the probe and any conductive surface:

- 250 mm, for frequencies 100 kHz 3 MHz
- 150 mm, for frequencies 3 MHz 10 MHz
- 100 mm, for frequencies > 10 MHz

2.8 Coupling between probe and operator's body

Accuracy characteristics are referred to non-perturbed electric fields. Always use a fiber optic extension of proper length to keep the probe far away from operator's body.

2.9 Multiple sources

Measuring complex electromagnetic fields as produced by multiple RF sources of different frequencies does require isotropic and broadband field probes, as well as fiber optic connections to eliminate errors due to scattering and pick-up effects. PMM EP600/EP601/EP602/EP603 perfectly meets these requirements.



2.10 Connecting EP600/ EP601/EP602/EP603

2.10.1 RS232 Connection Requirements to connect the probe PMM EP600/EP601/EP602/EP603 to PC RS232 port:

✓ NOTE

Some PC models may not provide enough power through the DB9 connector to supply the optical/RS232 adapter 8053-OC. In such cases install the separate power adapter model 8053-OC-PS between the optical/RS232 adapter 8053-OC and the PC (see chapter "Accessories").

- Connect the 8053-OC to the first available PC RS232 port, directly or with the supplied serial extension cable





- match the colors of the EP600/EP601/EP602/EP603 fiber optic connectors with the colors of the fiber optic adapters:



- match the colors of the FO-EP600/10 extension connectors with colors of the fiber optic adapters:





- at one extremity the extension optic cable FO-EP600/10 is terminated with a shaped connector. Respect the connection sense when connecting the same into the shaped receptacle OPTIC LINK of the 8053-OC adapter.





Do not connect/disconnect the optic fibre by applying force to the fiber optic cable directly: this may damage the optical connection. Always hold the connectors with your fingers firmly to connect/disconnect the optic fibre.

Presence of dust, dirt or particles of any nature on the optical connecting surfaces must be carefully prevented.

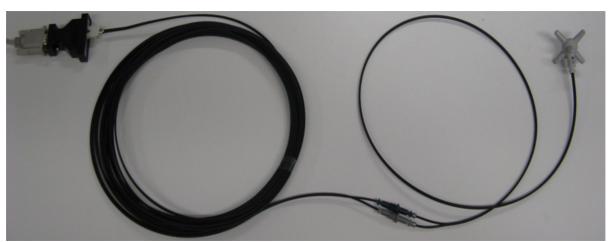


Fig. 2-1 RS232 connection of EP600/EP601/EP602/EP603 with FO-EP600/10 extension



2.10.2 USB Connection

Requirements to connect the probe PMM EP600/EP601/EP602/EP603 to PC USB:




In some cases the 8053-OC connected with an USB HUB or USB extension might not work properly. Connect the 8053-OC to an USB port of PC directly.



Install the supplied driver software before connecting the USB-RS232 adapter; the driver can also be downloaded directly from the following Web site http://www.manhattan-products.com/en-us/support/downloads/product/708-usb-to-serial-converter













- match the colors of the EP600/EP601/EP602/EP603 fiber optic connectors with the colors of the fiber optic adapters:



- match the colors of the FO-EP600/10 extension connectors with colors of the fiber optic adapters:





- at one extremity the extension optic cable FO-EP600/10 is terminated with a shaped connector. Respect the connection sense when connecting the same into the shaped receptacle OPTIC LINK of the 8053-OC adapter.





Do not connect/disconnect the optic fibre by applying force to the fiber optic cable directly: this may damage the optical connection. Always hold the connectors with your fingers firmly to connect/disconnect the optic fibre.

Presence of dust, dirt or particles of any nature on the optical connecting surfaces must be carefully prevented.



Fig. 2-2 USB connection of EP600/EP601/EP602/EP603 with FO-EP600/10 extension



2.10.3 Connection of fiber optic extension FO-EP600/10 The 10 m extension FO-EP600/10 is supplied with the PMM EP600/EP601/EP602/EP603 as standard accessory, together with the two fiber optic adapters – grey and blue (see picture below).



√ NOTE

Some PC models may not provide enough power through the DB9 connector to supply the optical/RS232 adapter 8053-OC. In such cases install the separate power adapter model 8053-OC-PS between the optical/RS232 adapter 8053-OC and the PC (see chapter "Accessories").



Do not connect/disconnect the optic fibre by applying force to the fiber optic cable directly: this may damage the optical connection. Always hold the connectors with your fingers firmly to connect/disconnect the optic fibre.

Presence of dust, dirt or particles of any nature on the optical connecting surfaces must be carefully prevented.



2.11 EP600/EP601/EP602/ EP603 installation

2.11.1 EP600/EP601/ EP602/EP603 installation on the conical holder Unexpected variations of the probe position may vary the field measurements. Make sure the probe is steadily installed by using the recommended standard or optional accessories.

Using the conical holder supplied with the PMM EP600/EP601/EP602/EP603 as support for the same is essential for correct measurements.

An inadequate support might significantly influence the measurements results; hence it is highly recommended to make use of the supplied conical holder as support for the probe.

To mount the PMM EP600/EP601/EP602/EP603 on the conical holder:

- place the conical holder vertical on a stable surface



- Apply the probe to the conical holder as shown in the picture, having the fiber optic passing through the slot of the conical holder. The picture below shows how to hold the probe between your fingers.



- Rotate the probe 45° counterclockwise:






- Pull the probe gently downwards until the probe plug is locked in the conical holder top.



- The installation is now completed.



Fig. 2-3 EP600/EP601/EP602/EP603 mounted on conical holder



As a general rule, when measuring the field from a transmitting antenna it is advisable to position the probe supporting devices perpendicular to the antenna polarization, particularly for frequencies in the range of megahertz.



2.11.1.1 EP600/EP601/ EP602/EP603

removal from the conical holder To remove the PMM EP600/EP601/EP602/EP603 correctly from the conical holder:

- Hold the probe and conical holder in vertical position
- Hold the probe as shown in the picture. Handle the probe with care.



- With the conical holder in vertical position, gently rotate the probe of 45° clockwise. The probe will be automatically released from the conical holder.



- The EP600/EP601/EP602/EP603 removal from conical holder is completed.





2.11.2 EP600/EP601/ EP602/EP603 installation on tripod PMM TR-02 It is recommended to make use of the optional tripod PMM TR-02 to position the PMM EP600/EP601/EP602/EP603 as required by the reference standards. Maintaining the same hardware configuration contributes to improbe the measurement repeatability (see chapter "Accessories").

Fix the EP600/EP601/EP602/EP603 conical holder to the tripod TR-02A by means of the screw at the top or by means of the swivel PMM 8053-SN.



Fig. 2-4 EP600/EP601/EP602/EP603 on TR-02A



Fig. 2-5 EP600/EP601/EP602/EP603 on TR-02A with PMM 8053-SN



This page has been left blank intentionally



3 - Measurements

3.1 Foreword

The following procedures and measurement methods apply to electromagnetic field sources present in industrial, medical, research, residential and telecommunication applications..

3.2 Preliminary

Before starting measuring electromagnetic fields (EMF) potentially dangerous, it's advisable to determine the known characteristics of the sources and their possible propagation characteristics.

This will allow for a better evaluation of the field distribution and for selecting the correct measuring equipments and procedures.

The source characteristics may include:

- type of generator and radiated power
- carrier frequency or frequencies (i)
- modulation
- polarization of transmitting antenna
- duty cycle, width and repetition frequency for pulsed modulations
- type of antenna and characteristics (gain, size, radiation diagram etc.)
- the number of sources, including those out of the probe bandwidth

To know for propagation evaluation:

- distance between source and point of measurement
- presence of RF absorbing or reflecting structures that may influence the field intensity.

3.2.1 Spurious signals

The operation with diode-based field sensors does require considering possible effects due to spurious signals, like:

- **Multiple sources**. Diodes feature RMS response only for low level signals. In presence of two or more strong signals the probe readings are higher than the real RMS value of the field in the corresponding bandwidth.
- **Pulse modulation**. At high levels the diode response is linear. Consequently, in presence of pulsed signals of low duty cycle the probe tends to read values higher than the real average value. This must be particularly considered for radar signals.
- **Sensitivity to light**. The Schottky diodes employed in some field probes are sensitive to light, including infrared. In such cases it's advisable to avoid direct exposition to the light sources.
- **Perturbing structures** . Metallic and in general conductive surfaces and structures can influence the field probe readings. Field probes must be operated at a proper distance from such structures.



3.3 General requirements The basic components of a field measuring equipment are:

- field probe (field sensor and transducer)
- connecting cables
- metering and data processing equipment

3.3.1 Probes

As a general rule the field probes must respect the following conditions:

- High rejection to spurious signals
- No perturbation of the field surrounding the sensors
- Such connecting cables e.g. fiber optics that do not perturb the field to measure
- Known response to the operating ambient

3.3.2 Connections

The connection between field probe and metering equipment transfer the data relevant to the measurements and the probe/converter settings without influencing the measure.

Also, unwanted couplings and noise pick-up must be avoided. Fiber optic connections do perfectly meet the requirements.

3.3.3 Metering equipment The metering/data processing equipment is designed so that the probe signals or data are properly read, displayed and stored.

3.4 Basic functional checks

Some basic functional checks are:

- check of the proper probe operation
- check for the readings not varying significantly when rotating the probe along one of its axis

3.5 Measurement procedures

The measurement procedures must minimize:

- Risks of exposure of personnel to hazardous electromagnetic fields
- Measurement errors
- Interferences
- Damages to the equipment



3.6 Preventing measurement errors

To prevent influencing the field measurements the operator, vehicles etc. should stay away of 5 meters from the field sensor; the same should not be located near metallic or conductive surfaces and objects.

From the definition of difference of potential between two points:

$$V_{21} = -\int_{r_1}^{r_2} \overline{E} \, dr$$

<--- NOTE

We obtain that, with constant difference of potential, when the distance between the two given points diminishes, the field strength increases.

Example: the field strength present between the two plates of a condenser at a distance of 0,1 m and with 100 V applied is of:

$$E = \frac{100V}{0.1m} = 1 \frac{KV}{m}$$


To remark that a voltage of 100 V applied in these conditions produces a field strength of 1000 V/m, i.e. much higher than the applied voltage.

3.7 Void

3.8 Void



3.9 PMM EP600/EP601/ EP602/EP603 operation





The PMM EP600/EP601/EP602/EP603 is supplied from an internal battery that can be recharged by the charge EP600 CHARGER supplied with.

✓ NOTE

One full charge cycle before operation is recommended to obtain the maximum autonomy.

The PMM EP600/EP601/EP602/EP603 can be switched ON by shortly pressing the pushbutton, after that the LED is sequentially turned on with **green, red and blue indications** as a test for the same; then the LED will blink **red,** this meaning the EP600/EP601/EP602/EP603 is ready for the operation.

√ NOTE

The PMM EP600/EP601/EP602/EP603 cannot be switched OFF by the pushbutton.

The PMM EP600/EP601/EP602/EP603 automatically turns OFF when:

- after 180 sec. the fiber optic has been disconnected or the communication with PC is not established; use the operative command ${\it \#00e}$ ${\it n}^*$ (see chapter 6) to set the time before the EP600/EP601/EP602/EP603 auto-switches off.



The command #00e n* is available with Firmware release 1.12 or higher

- when the battery voltage is below 2.05V (the battery voltage is displayed by the software WinEP600).
- when the Software WinEP600 is closed



Do not expose the probe to a field higher than the max. allowed. Field strengths exceeding the allowed may cause severe probe damage whether it is connected or not, either turner ON or OFF.



The fiber optic must be connected or disconnected by holding it by the connectors only. Pulling the fiber optic cable may cause severe damages to the PMM EP600/EP601/EP602/EP603 and to the fiber optic cable itself.

Dust and dirt must be prevented to be in between the optical connections.



The EP600/EP601/EP602/EP603 can be connected to the PC via fiber

optic either when ON or OFF.

When making measurements with PMM EP600/EP601/EP602/EP603

the power supply must be ALWAYS removed.

The min. battery voltage allowed for proper operation is of 2,05 V; it is **WARNING** displayed by the PC software WinEP600. Lower values do require

recharging the battery.

VARNING The max. battery autonomy is of approx. 80 hours (with Filter 28 Hz

and Rate 2.5 sec), according to the filter setting.

The internal battery can be replaced at factory only; in case of VARNING

damage or incorrect operation contact your Dealer.

It is recommended to fully recharge the battery before long-term storage of the probe; a full recharge shall be performed every 4

months since then.



3.10 Applications

The PMM EP600/EP601/EP602/EP603 field probe is connected to the user's PC via fiber optic and the optic to serial converter (see chapter Operation).

3.10.1 EMC

The wide frequency range and small size allow for using the PMM EP600/EP601/EP602/EP603 in EMC applications for monitoring the field strength during radiated immunity tests in open site, TEM/GTEM and anechoic chamber.

The optional accessory PMM SB10 allows for controlling up to 10 field probes at the same time. Up to five PMM SB10 can be connected together to control up to 50 field probes.

Examples of measuring configurations:

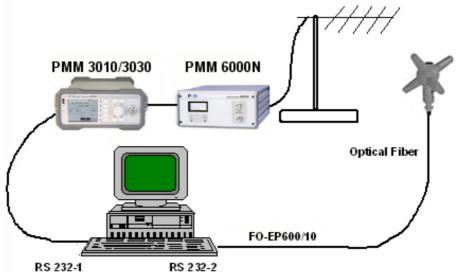


Fig. 3-1 PMM EP600/EP601/EP602/EP603 in open site

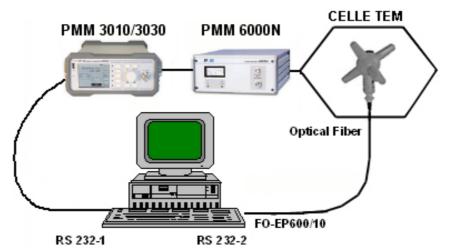


Fig. 3-2 PMM EP600/EP601/EP602/EP603 in TEM cell



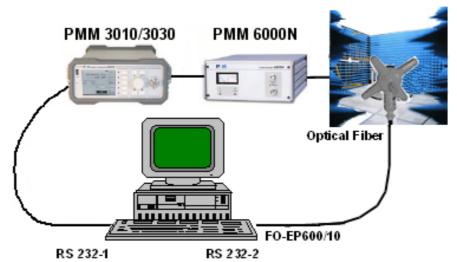


Fig. 3-3 PMM EP600/EP601/EP602/EP603 in Anechoic Chamber



3.10.2 Void

This page has been left blank intentionally




3.11 Operating PMM EP600/EP601/ EP602/EP603 with 8053B (Option) The EP600/EP601/EP602/EP603 can be connected and operated by the meter PMM 8053B.



Fig. 3-4 EP600/EP601/EP602/EP603 with 8053B

- Display of field strength in ABS/%, MIN-MAX/AVG, MIN-MAX/RMS modes.

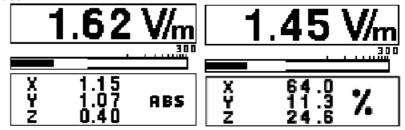

- Graph of field strength in PLOT mode.



- Field strength data recording in Data Logger mode.



√ NOTE

For further information on configuration and operation with PMM 8053B, please refer to the operation manual supplied with it.



3.12 Operating EP600/ EP601/EP602/ EP603 with PMM SB10 (Option) The optional accessory PMM SB10 allows for controlling up to 10 field probes at the same time. Up to five PMM SB10 can be connected together to control up to 50 field probes.

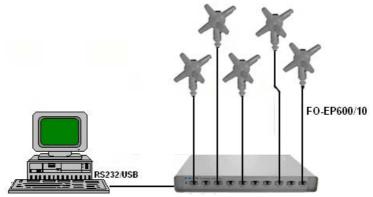


Fig. 3-5 PMM EP600/EP601/EP602/EP603 with one SB-10

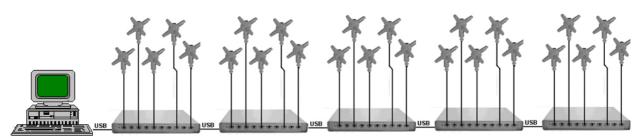


Fig. 3-6 PMM EP600/EP601/EP602/EP603 with five SB-10


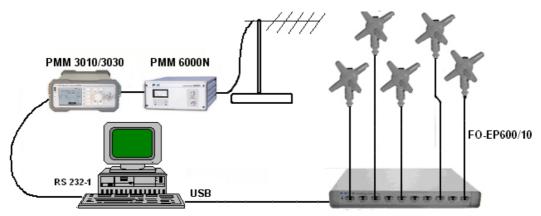


Fig. 3-7 PMM EP600/EP601/EP602/EP603 with SB-10 in open site



The PC software supplied with the PMM SB10 allows for simultaneous displaying of the field strength measured by each single field probe.



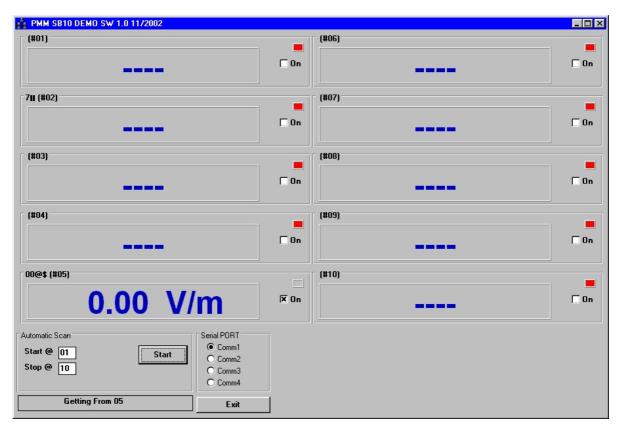

This page has been left blank intentionally



4 – Battery charger EP600 CHARGER

4.1 Foreword

The probe EP600/EP601/EP602/EP603 internal circuitry is supplied by a rechargeable Li-Mn internal battery to recharge by means of the battery charger EP600 CHARGER connected to the mains by means of the supplied adapter.

The EP600 CHARGER is intended for this application only; any other use or application is strictly forbidden.

EP600 CHARGER is intended for operation on desk; its special design allows for keeping the probe under charging in correct and safe position. Inside the EP600 CHARGER a microprocessor controls and checks the recharging operation.

The LED shows the charging status.

The adapter supplied with the EP600 CHARGER works with mains voltages from 100 to 240 VAC, 50/60 Hz. Different socket adapters are supplied with.




Fig. 4-1 AC adapter

Fig. 4-2 EP600 CHARGER

4.2 AC adapter

Always connect the AC adapter to the PMM EP600 CHARGER prior to connect to the mains.



Output: DC, 10 - 15 V, ~ 500 mA

Connector polarity:



4.2.1 AC mains plug

If required to replace the AC mains plug, remove the installed and install the proper one.



4.3 EP600 CHARGER

The following conditions apply to all specifications:

• Operating temperature: -10° to +50 °C.

4.3.1 Specifications

TABLE 4-1 Characteristics and specifications of the battery charger EP600 CHARGER

Characteristics

Charging is stopped when removing the probe

Microprocessor control with autostart

Charging status Led

Self-test

Safety timer

AC adapter supplied

Specifications

Supply voltage 3.8V 5mA (Max)

Supported battery type Panasonic ML621S 3V 5mA/h Li-Mn

Max. recharging time for max. autonomy 48h

Operating temperature $-10^{\circ} \div +50^{\circ}$ Dimensions (LxDxH) 60x60x75mm

Weight 130 g



4.3.2 EP600 CHARGER components

Description:

- 1 Knob and Spring
- 2 Charging connector
- 3A Charging status Led
- 3B DC Supply connector



Fig. 4-3 EP600 CHARGER components


○NOTE	Attempting to charging batteries of different types or dry cells may cause explosion of the same and is strictly forbidden.
NOTE	The internal battery of EP600/EP601/EP602/EP603 can be replaced by the Factory only. In case of failure or incorrect operation please contact the Dealer.
○NOTE	The minimum voltage level for proper operation is of 2,05V; lower voltages do require recharging the battery.
○NOTE	It is recommended to fully recharge the battery before long-term storage of the probe; a full recharge shall be performed every 4 months since then.
✓¬NOTE	The max. battery autonomy is of approx. 80 hours (with Filter 28 Hz and Rate 2.5 sec), according to the filter setting.
○NOTE	When making measurements with PMM EP600/EP601/EP602/EP603 the power supply must be ALWAYS removed.




4.4 Installing EP600/ EP601/EP602/ EP603 on EP600 CHARGER A first complete charging cycle is recommended to achieve the max autonomy.

To install the probe EP600/EP601/EP602/EP603 on the battery charger EP600 CHARGER:

- place the EP600 CHARGER on a flat, stable surface
- hold and lift up the knob as shown in figure



- Insert the EP600/EP601/EP602/EP603 on the EP600 CHARGER in correspondence of the threaded contact pin. Do not spin the probe to avoid damaging the contact pin.



- Release progressively the knob until rubber tip holds the EP600/EP601/EP602/EP603 housing downwards.




- Connect the AC adapter to the EP600 CHARGER first, then to the mains.





- Plug the AC adapter to the mains




- Check the Led status as per the table below:



Fig. 4-4 EP600/EP601/EP602/EP603 on EP600 CHARGER

Table 4-2 EP600 CHARGER Led status - Start up phase						
Fix	Green	The EP600 CHARGER is supplied but without load (battery not present or disconnected).				
Fix	Red	The charging circuit is overloaded (the output is OFF for 30 seconds before attempting a new charging cycle).				

Table 4-3 EP600 CHARGER Led status - Charger phase						
Blinking	Green	The battery is under charge				
Fast Blinking	Red	Charge ended for maximum time limit reached [60 hours]				
Slow Blinking	Orange	Charge ended for maximum time limit reached without 12 hours of stabilisation.				
Fast Blinking	Orange	Charge ended for maximum time limit reached with 12 hours of stabilisation.				



The complete charging cycle is of 48 hours; the charge is completed when the Led of EP600 CHARGER blinks orange.



This page has been left blank intentionally



5 – WinEP600 and SetAddEP600 Operating instructions

5.1 Foreword

This chapter is the installation and operation guide of the PC Softwares WinEP600 and SetAddEP600 Utility supplied with the PMM EP600/EP601/EP602/EP603 field probe.

The SetAddEP600 is a utility that integrates the PMM SB10 Switching Control Box and the PMM EP600/EP601/EP602/EP603.

When several PMM EP600/EP601/EP602/EP603 are connected to the PMM SB-10 each of them need to be set with a different address.

With the SetAddEP600 Utility you can associate an address at each PMM EP600/EP601/EP602/EP603 connected to the PMM SB-10.

5.2 PC minimum requirements

- Processor: Pentium
- 16 Mb RAM
- 10 Mb free space on hard disk;
- Operating system WindowsTM, XP/Vista/Win7.



Software and Utility updates can be downloaded from the web page www.narda-sts.it.



5.3 Installation

To install the WinEP600 and the SetAddEP600 on PC from the supplied CD-ROM proceed as follows:



Do not connect the PMM EP600/EP601/EP602/EP603 to the PC until the installation is completed.

Insert the WinEP600 CD into the PC CD-ROM driver. In Computer Resources double click on the corresponding CD-ROM driver. To start the installation double click on the **WinEP600** icon.




The installation can be aborted by clicking on Cancel:






<**◯**NOTE

In Windows Vista most programs are blocked for computer protection. To start the installation correctly it might be necessary to authorize the operation.

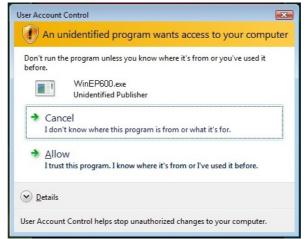


The installation folder must be specified. Click **Next** to confirm the default folder or **Change** to modify.



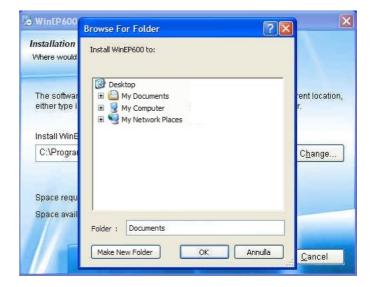



Click **Next** to proceed installing.

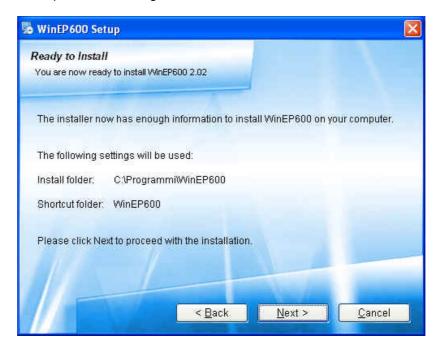

The installing status is displayed then:





Click **Finish** to complete and exit the installer.

The folder **WinEP600** and **SetAddEP600** are created under **Programs** with the icon **WinEP600** on desktop.



Create the **SetAddEP600** shortcut on your desktop.





5.4 COM port settings with 8053-OC

Connect the 8053-OC to the PC first serial port available (for more details see chapter "Installation").

✓ NOTE

In some PC models the power delivered through the DB9 connector may be not enough to supply the optical/serial converter 8053-OC. In such cases, the external power supply adapter mod. 8053-OC-PS must be connected between the PC and the optical/serial converter 8053-OC.

√ NOTE

With the 8053-OC optical/serial converter the software search for the probe PMM EP600/EP601/EP602/EP603 on the first available serial port.

To set a specific serial port:

5.4.1 WinEP600 COM port settings

- Select the icon WinEP600 with the right mouse button;
- · Select Properties;
- Add the command COMM=N preceded by a space (in capital letters) at the end of the Destination field where N indicates the serial port to be used; for example, if the EP600 is connected to port 2, add the command COMM=2.

√ NOTE

The assigned COM port nr. must be between 1 and 9.



√⁄~NOTE

 In some operating system the Destination field is enclosed in double quotation marks ("); in this case, the command COMM=N, preceded by a space must be outside as in the example below;



· then confirm by selecting Apply



5.4.2 SetAddEP600 COM port settings

- Select the icon SetAddEP600 with the right mouse button;
- · Select Properties;
- Add the command COMM=N preceded by a space (in capital letters) at the end of the Destination field where N indicates the serial port to be used; for example, if the EP600 is connected to port 2, add the command COMM=2.



The assigned COM port nr. must be between 1 and 9.



<>>NOTE

• In some operating system the Destination field is enclosed in double quotation marks ("); in this case, the command COMM=N, preceded by a space must be outside as in the example below;



• then confirm by selecting Apply



5.5 COM port setting with adapter USB-RS232

Connect the USB-RS232 adapter to the PC USB port and wait for the "new hardware installation" procedure. Drivers supplied with the adapter can be sued as well.

√ NOTE

After having installed the USB-RS232 adapter, make sure the assigned COM port nr. is comprised between 1 and 9:

Enter in Peripheral management (Start > Settings> Control Panel > System>Hardware> Device Manager).
 The assigned COM can be found in Ports (COM & LPT) – USB Serial Port (COMx).


COMx shows the COM port assigned to the USB-RS232 adapter.




✓™NOTE

If the adapter is set for a COM port nr. Not comprised between 1 and 9, the settings can be changed as follows:

 To change the COMx port, double click the line Ports (COM & LPT) and USB Serial Port (COMx). Enter in Port settings and Advanced.





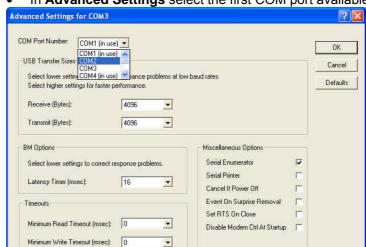


In Advanced Settings select the first COM port available; click OK.

5.5.1 WinEP600 COM port settings

- Select the icon WinEP600 with the right mouse button;
- · Select Properties;
- Add the command COMM=N preceded by a space (in capital letters) at the end of the Destination field where N indicates the serial port to be used; for example, if the EP600 is connected to port 2, add the command COMM=2.




The assigned COM port nr. must be between 1 and 9.

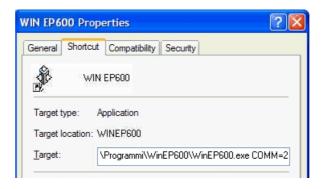

✓ NOTE

 In some operating system the Destination field is enclosed in double quotation marks ("); in this case, the command COMM=N, preceded by a space must be outside as in the example below;



Then confirm by selecting Apply




5.5.2 SetAddEP600 COM port settings

- Select the icon SetAddEP600 with the right mouse button;
- · Select Properties;
- Add the command COMM=N preceded by a space (in capital letters) at the end of the Destination field where N indicates the serial port to be used; for example, if the EP600 is connected to port 2, add the command COMM=2.



The assigned COM port nr. must be between 1 and 9.

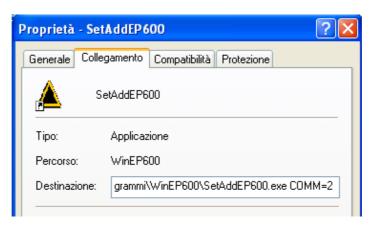



 In some operating system the Destination field is enclosed in double quotation marks ("); in this case, the command COMM=N, preceded by a space must be outside as in the example below;



• Then confirm by selecting Apply



Running WinEP600

<>> NOTA

5.6

Before to start WinEP600, it is recommended to limit the applications running on your computer.

Connect the PMM EP600/EP601/EP602/EP603 to PC an click the icon on desktop.




Alternatively (Windows XP): Start, All Programs, WinEP600, WinEP600. Windows Media Playe Remote Assistance Windows Media Player Windows Messenger Windows Messenger Windows Movie Maker Tour Windows XP Uninstall WinEP600 WinEP600 ▲ WinEP600 Sassafras K2 All Programs Macromedia Log Off Turn Off Compute 🎁 start

Windows Vista or 7: Click Windows (), Programs, WinEP600, WinEP600.

This window is displayed first:



Then, the main window is displayed together with the **WinEP600** - **Connection Incoming** indication of the correct communication with the probe.

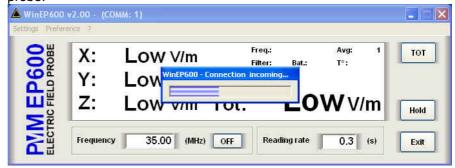


WinEP600 and SetAddEP600 operating instructions

5-11



This message appears when PMM EP600/EP601/EP602/EP603 is not connected or the communication is not established:

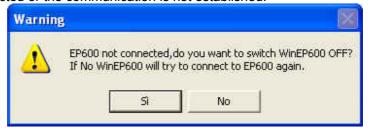


Select **YES** to quit the WinEP600 - the EP600/EP601/EP602/EP603 is switched OFF.

Select **NO** to retry establishing the communication (check the EP600/EP601/EP602/EP603 correct installation before).

5.7 Main window contents

Once connected the main window is displayed:

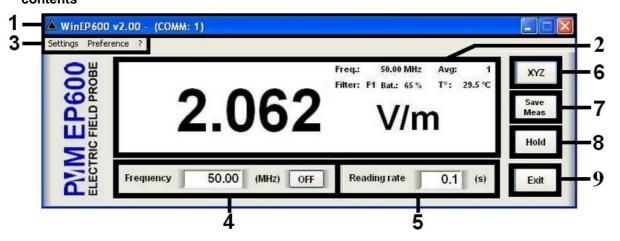

Commands description:

- 1. Title bar
- 2. Measurements and settings
- 3. Settings selection
- 4. Correction frequency setting in MHz
- 5. Reading rate in seconds (s)
- 6. Toggle between total field value or contemporary x y z axis readings
- 7. Button to store the field value (Every time the software starts the button is disabled).
- 8. Hold/run readings
- 9. Exit and quit the program



5.7.1 Title bar

The software release is shown here, together with the serial port as set in the program properties.




The control buttons allow to minimize to icon, enlarge/restore the main window and exit the program:



When minimizing the main window the information is displayed in the Windows application bar at the bottom of screen.



The field measurement remains displayed on desktop meanwhile.



For more information see par. "Setting/Preference/Minimized UI".



5.7.2 Main window displayed measurements

The measurements displayed in the main window are:

- electric field values as x - y - z or total (see par. "XYZ / TOT")

Mode x - y - z

X: 1.855 V/m Freq.: 50.00 MHz Avg: 1 Filter: F1 Bat.: 65 % T°: 27.7 °C Y: 1.739 V/m

Z: 2.105 V/m Tot: 2.279 V/m

Mode Total

2.279 Freq.: 50.00 MHz Avg: 1 Filter: F1 Bat.: 65% T°: 27.7 °C V/m

- **Measuring unit** shows the electric field measuring unit; the value is displayed with three decimals. Min. value displayed: 0.010 V/m.
- **Correction frequency** see par. "Frequency setting" Default: *Freq: 50.00 MHz*
- Average and Filter see par. "Settings" Default: Avg: 1 Filter: F1
- **Battery status** displayed in 5% steps. It shows the residual autonomy during measurements and the achieved autonomy during charging.
- EP600/EP601/EP602/EP603 internal temperature in °C



5.7.3 Frequency correction setting

This setting in MHz recalls the corresponding frequency correction factor stored in the EP600/EP601/EP602/EP603 memory.

<>>NOTE

The graph in chapter 1 shows the correction factor in db as a function of the working frequency.

√ NOTE

The setting displayed at the first run is the default; the last setting will be displayed then.

The frequency is displayed with two decimals, max. resolution of 0.01 MHz. Press the enter key to enter the set frequency value.



To disable the frequency correction, click OFF; the button toggles to ON for enabling the function when required.



<⊅NOTE

When entering the frequency correction value or enabling the function, the "Frequency value" will be updated according to the Reading Time setting.

✓ NOTE

When entering the frequency correction value while in HOLD mode, la the new value will be not displayed until the HOLD is released.

√¬NOTE

The following message will appear when entering frequencies out of the PMM EP600/EP601/EP602/EP603 range:





5.7.4 Reading Rate setting

It shows the time interval (in seconds) between subsequent readings. Setting resolution of $0.1\ s.$

Press the enter key to enter the set frequency value.



✓¬NOTE

The setting displayed at the first run is the default; the last setting will be displayed then.

NOTE

The minimum time interval between readings is in function of the filter setting. The table Filter (Settings/Filter) show the minimum reading rate allowed.

Ĵ™NOTE

The max. time interval between readings is of 30 s regardless of the filter setting.

✓ NOTE

Entering a reading rate not allowed will cause a warning message to appear:






5.7.5 XYZ / TOT

XYZ



Button for selecting the x - y - z or Total mode. Max. display resolution: 0.001 V/m.

2.279





Click on the button to toggle from XYZ to TOT.

X: 1.409 V/m Freq.: 50.00 MHz Avg: 1 Filter: F1 Bat.: 65% T°: 27.7 °C Y: 1.381 V/m Z: 1.607 V/m Tot: 2.279 V/m

If the field value is outside the nominal level range, the following messages are displayed:

Ovr: the field level is higher than 110% of the nominal maximum level (550 V/m for EP601).

!: the field level is between 100% and 110% of the nominal maximum level (from 500 to 550 V/m for EP601). The symbol is close to the value.

- *: the field level is lower than nominal minimum level. The symbol is close to the value.
 - 0.5 V/m per EP601 on the total;
 - 0.5 / $\sqrt{3}$ per EP601 on the single axis.

Low: the field level is lower than 1/15 of the nominal minimum level.

- 0.5 / 15 per EP601 on the total;
- 0.5 / (15 x $\sqrt{3}$) per EP601 on the single axis.



The field value outside the nominal level range could be unreliable.



5.7.6 HOLD / RUN



Press HOLD to freeze the readings. Click on the button to toggle from HOLD to RUN The button XYZ/TOT is active even when in HOLD.



If the program is exit when in HOLD mode, it will restart in RUN mode.

5.7.7 EXIT



Press **EXIT** to end the program. The current settings are saved and will be recalled at the next start.

Message:




Press **YES** to exit and turn the EP600/EP601/EP602/EP603 off. Press **NO** to abort exiting.



5.7.8 Settings menu

Commands:



- Settings: set Average and Filter

- Preference: select program skin and enable the function Minimized UI

-? (Info): software and product information

5.7.8.1 Settings

Settings options:




- **Filter:** the EP600/EP601/EP602/EP603 internal A/D Sigma-Delta converters feature digital filters to improve resolution and sensitivity, as well to reducing interferences.

The filters can be selected according to the application requirements: from the faster (F1) to the slower (F8).

To set the required filter click on the corresponding line, which turns blue. The selected filter will be displayed in the main window.



When selecting a new filter while in HOLD mode, the filter setting indication in the main window will be updated only after toggling to RUN mode.

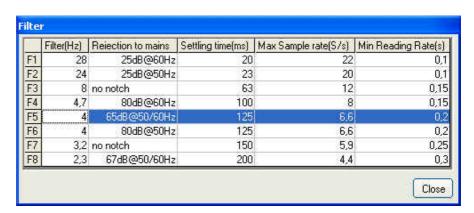

Filter(Hz): indication of the filter characteristics

Rejection to mains: some filters feature notch filtering at mains frequency to reducing interference

Settling time (ms): time required for getting a complete reading

Max Sample rate (S/s): A/D conversion speed

Min Reading Rate (s): min. time interval between readings of electric field



Normally a fast field measurement is required for faster response and better stability when the field probe controls as feedback for a preset field value the radiated power of a system composed by antenna and RF generator.

However, as faster the measurements as higher the noise is, with consequent reduction of sensitivity.

Slower measurements increase sensitivity but increase the response time and the power consumption.

The PMM EP600/EP601/EP602/EP603 features eight different filters to help finding the most suitable combination of the a.m. parameters for each specific application:

F	Settling time	Power consumption	Sensitivity	Rejection @ 50Hz	Rejection @ 60Hz
1	Very fast	Very low	Low		low
2	Very fast	Very low	Average	Low	
3	Fast	Low	Good		
4	Average	Average	High	Good	Very high
5	Average	Average	High	High	High
6	Average	Average	High	Very high	Good
7	Slow	High	Very high	good	Good
8	Slow	Very high	Very high	High	High



In normal operation setting the filters F4 - F5 may offer a good compromise in terms of power consumption, sensitivity, settling time and rejection @ 50Hz.





- **Average:** setting of the number (1, 4, 16, 32 or 64) of readings to calculate the arithmetic average (AVG).







When setting Average = 1, the readings are not averaged and the current measurements are displayed.

In the example, the average value of the last 16 field readings will be displayed. The "Avg" counter shows the progressing of the average calculation, updating according to the "Reading rate" time interval setting.



The message AVG: OK will be displayed shortly after completion of the averaging process, then followed by the indication of the preset averaging Avg: 16.

Then the process continues in moving Average mode: of the 16 readings block, the older is discarded and the latest is added at the speed of the Reading rate setting.

The process is restarted from the beginning when setting a different Average value.



✓ NOTE

When toggling from TOT to XYZ mode the Average is reset to recalculate the field values for each single axis.



✓ NOTE

When in HOLD mode, the new Average value is displayed in the main window and is updated only when the HOLD is released.



5.7.8.2 Preference



Functions of the Settings menu:

- **Display Color:** selection of different color combinations of the main window among:

Background / readings and units

- Blue/Grey
- Grey/White
- Grey/Yellow
- Black/Yellow
- Black/GreenBlack/White



The color of the settings of Freq, Avg, CorFact e Offset will be displayed accordingly.




- **Minimized**: enable the function **Minimized UI (Unit Interface)** to keep the field readings displayed on desktop when minimizing the main window on the tray.



This window can be moved anywhere on the desktop, keeping its final position even at the next minimizing of the main window.



To close this window, restore the main window from the tray and deselect the "Minimized UI" function.



- Measurements Log: enable the function Measurements Log to display the Save Meas button in the main window. The symbol $\sqrt{}$ means that the function is actived.



✓ NOTE


Every time the software starts the function Measurements Log is disabled



Every time the button **Save Meas** is selected, the field value is stored in the file *EP600_Measurements.txt* (at the first run the file is created automatically).



When the file is saved in TXT format and the table is opened, a huge amount of data are available

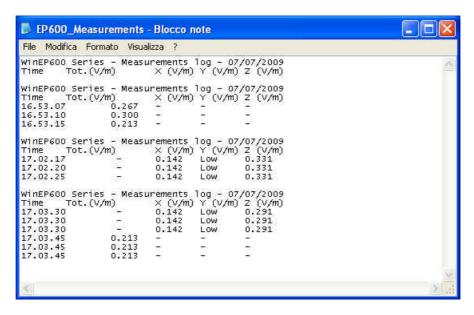

For every working session (from starting to closing the software) the following headline will be created in the txt file:

```
WinEP600 Series - Measurements log - dd/mm/yyyyy 
Time Tot.(V/m) \times (V/m) \times (V/m) Z (V/m)
```

dd/mm/yyyy: working session date.

Time: hour, minute, second of the measurement.

Tot.(V/m): Field value in Total mode.

X(V/m) Y(V/m) Z(V/m): Field value in x, y and z mode.



The recorded data can be viewed either as a graph or as a table. By using Word or Excel application, click the Open file command and select "Type of file": "all files"; then find the file to open starting from the directory and follow the necessary path until the file is found.




5.7.8.3 ? (Info)




Contents:

- **Info:** current EP600/EP601/EP602/EP603 firmware version and date, serial number and battery voltage.

















→ NOTE

Battery voltages below 2.11V (5% of charge) are displayed red.



Info

About

- About: Manufacturer information.






5.8 Running SetAddEP600

Connect the PMM EP600/EP601/EP602/EP603 to PC an click the icon on desktop.




Alternatively (Windows XP): **Start**, **All Programs**, **WinEP600**, **SetAddEP600**.

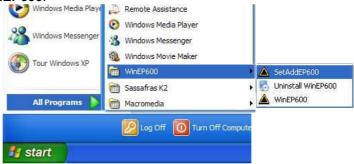


Windows Vista or 7: Click Windows (), Programs, WinEP600, SetAddEP600.

Then, the main window is displayed together with the **SetAddEP600 - Connection Incoming** indication of the correct communication with the probe.

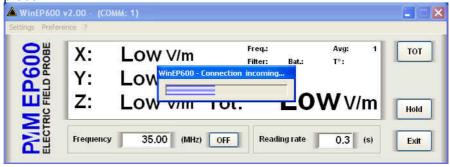

This message appears when PMM EP600/EP601/EP602/EP603 is not connected or the communication is not established:

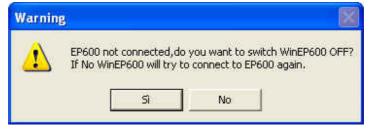

Select **YES** to quit the SetAddEP600 – the EP600/EP601/EP602/EP603 is switched OFF.

Select **NO** to retry establishing the communication (check the EP600/EP601/EP602/EP603 correct installation before).



5.9 Main window contents

Once connected the main window is displayed:



- 1. Title bar
- 2. Probe Data
- 3. New Address
- 4. Exit

5.9.1 Title bar

The title bar displays the name of the program.



The control buttons allow to minimize to icon and exit the program:




When minimizing the main window the information is displayed in the Windows application bar at the bottom of screen.



5.9.2 Probe data

When the communication is established, the probe data displays: probe model, release and data firmware and serial number.





5.9.3 New Address

When the communication is established, the window $\boxed{00}$ displays the current probe address.



Enter new address of and press write to store it.

The software will inform that the address program has been successfully stored:



5.9.4 Exit

Press Exit to close the program.



5.10 Uninstalling WinEP600 and SetAddEP600

Disconnect the USB cable (the procedure of "safe disconnection" is unnecessary).

Windows XP: click Start

in Windows Vista or 7: click Windows



Then All Programs, WinEP600, Uninstall WinEP600.






If the Uninstaller is not available:

Disconnect the USB cable (the procedure of "safe disconnection" is unnecessary).

Click Start, Settings, Control Panel and Add or Remove Programs (Programs and functions for Windows Vista or 7).

Find WinEP600 then click **Remove** and follow the instructions.





When asked if removing the shared files, answer NO to prevent other programs not to run correctly.



Uninstalling the driver of RS232-USB adapter

✓ NOTE

5.11

Apply this method if the driver uninstaller (normally supplied with the hardware) is not available.

Right click My computer to access Properties



Select **Hardware** and **Device Manager**. Click + to expand **Port (COM and LPT)**.

Right click USB Serial Port (COM) then click Uninstall



Click **OK** to end.



Once the uninstall is completed the peripheral **USB Serial Port (COM)** will be removed.





6 - Communication protocol

6.1 Disclaimer

This chapter provides the information required to control the PMM EP600/EP601/EP602/EP603 via the fiber optic connected to a PC and by means of user's own PC software applications. Narda STS S.r.l supports the correctness of the information only, and disclaim for any consequence the use of such information may cause to anybody. The inclusion of Narda's communication protocol into user's or third party software is entirely at the user's risks and responsibility. In no way Narda STS S.r.l shall be liable for damages of any kind consequent to the use of the information provided in this chapter.



All the following examples are indifferently referred to the PMM EP600, EP601, EP602 and EP603.

6.2 Protocol

The serial communication between PC and PMM EP600/EP601/EP602/EP603 is the RS232 standard or USB (via the USB-RS232 converter). Specifications:

- Rate 9600 Baud
- Start 1 bit
- Stop 1 bit
- No Parity

The commands are composed by an ASCII string delimited by "#" (0x23) and "*" (0x2A)

Up to FW 1.02 each command must begin with the address which is made of the string "00".

From FW 1.10 each command starts sending the address which is made of two characters string in the range "00" to "99".

The address "00" is a special one as it is considered Broadcast while all others must match the address stored in the unit (see command "I").

In other words the EP600 will always grant all commands starting with "#00" regardless its own address stored.

Broadcast mode is intended when using the EP600 in a NON-BUS way, typically PC directly linked to EP600, or for setting the new address (see command "I"). In this mode the address can be changed even without knowing the current address.

Careful must be taken, however, when the EP600 works on a BUS (for example via SB10) as using the broadcast address all the device sharing the BUS would answer at the same time creating thus a conflict.

Hereafter all example are made using the broadcast address but, of course, they work also using different address. The only restriction is that the address must be made of two characters and the range is "00" to "99"

The answer can be either in ASCII or Binary, according to the command sent. The first character is always like the character sent, and can be used as control marker or synchronization for the answer.



The available commands are of three categories:

- Query COMMANDs
- Setting COMMANDs
- Operative COMMANDs

The commands have this format: #00Qcommand(parameters)* where:

= command string start
00 = string always present
Q = ? for query commands
 S for setting commands
Command = command string
(parameters) = setting parameters value (where present)
* = command string end



At power ON the EP600/EP601/EP602/EP603 is in Master mode, as required by the communication with the hand-held unit 8053B; the EP600/EP601/EP602/EP603 will continue to send the measurement data independent from receiving the commands. For this might be not useful when interfacing to other software, send the command #00?v* to turn the EP600/EP601/EP602/EP603 in Slave mode to answer only when receiving a query.

To save battery the EP600/EP601/EP602/EP603 automatically turns off 180 seconds after receiving a command; use the operative command #00e n* (see table 6-2) to set the time before the EP600 auto-switches



Table 6-1 Query Commands				
Command	Description			
?v	This query command #00?v* sends back a string containing information about model, release and date of firmware.			
	Example of reply to the command #00?v*: "vEP600:1.02 10/05;"			
? p	This query command #00?p* sends back a string containing information about date of calibration.			
	Example of reply to the command #00?p*: "10/05;"			
?b Battery	This query command #00?b* sends back 3 bytes containing information about the voltage of EP600 battery. The array is made of 3 bytes in which the first is the character 'b' followed by 2 bytes expressing a 16bit unsigned integer (nn) in Big Endian notation.			
	To get the battery voltage use the following formula: V_battery= 3 * (nn / 1024 * 1.6)			
?t Temperature	This query command #00?t* sends back 3 bytes containing information about the temperature of EP600 probe. The array is made of 3 bytes in which the first is the character 't' followed by 2 bytes expressing a 16bit unsigned integer (nn) in Big Endian notation.			
	To get the temperature in degrees Centigrade use the following formula: T_ep600= ((nn / 1024 * 1.6) - 0.986) * 1000 / 3.55			
?s Serial Number	This query command #00?s* sends back a string containing the serial number of the device Example of reply to the command #00?s*: "s123456789AAAA"			
?T Total Field	This query command #00?T* sends back 5 bytes containing information about the total field strength measured by EP600. The array is made of 5 bytes in which the first is the character 'T' followed by 4 bytes expressing a 32bit IEEE floating point number(ff) in Little Endian notation. The figure (ff) represents the square of total field strength (isotropic measure) To get the field strength, the square root must be taken: V/m=√ff			
?A All Field Components	This query command #00?A* sends back 13 bytes containing information about field strength measured by EP600 of every single axis. The array is made of 13 bytes in which the first is the character 'A' followed by 12 bytes expressing 3 (X,Y,Z) 32bit IEEE floating point number(ff) in Little Endian notation. The 3 figures (fx,fy,fz) directly represent the field strength of related axis and are expressed in V/m.			



Table 6-2 Setting Commands			
Command	Description		
k fr	This setting command #00k frq* sets the frequency(frq) to which refer the correction factor.		
	The figure fr is the ASCII string representing the integer frequency multiplied by 100 giving thus the resolution of 10kHz.		
	Once the EP600 has received and granted this command, all measurements will be corrected using the factor stored in factory related to this frequency.		
	Sending a frequency which is out of EP600 range disables frequency correction factor function.		
	The reply is an array made of 5 bytes in which the first is the character 'k' followed by 4 bytes expressing a 32bit IEEE floating point number(ff) in Little Endian notation. The figure (ff) represents the frequency used by the EP600		
	Example of command #00k 10000*: (Set the internal frequency to 100MHz)		
f n	This setting command #00f n* sets the processing filter (n) used for measurements. The index n must be between 0 and 7.		
	For further information on filters please refer to separated document		
	Example of command #00f 2*		
e n	This setting command #00e n* sets the time before the EP600 auto-switches off after receiving a recognized command.		
	Note that this setting is not permanent and it will be kept only while the EP600 is ON. Every time the EP600 is turned off, the default 180 second is taken.		
	The argument n is expressed in second e should be lower than 10800 (3 hours). The replay to this command is 'e' if it has been granted and 'x' if the argument is out of range (in which case the default 180 is taken).		
	Example of command #00e 600*: (sets the switch off time to 10 minutes)		



Table 6-3 Operative Commands		
Command	Description	
@c	This setting command #00@c* temporarily puts the EP600 in "Storing Mode" allowing thus storing a new address. As this permission lasts only for 1 second, the command "I" should be issued closely. This command has not a reply. Example of command #00@c*	
@I addr	This setting command #00@Iaddr* sets the address used for communication protocol. It is made of a 2 character string int range "00" to "99". Neither spaces nor punctuation are allowed between "#@00" and addr. This setting command is executed only if sent within 1 second since the command "c". The reply is the address itself if it has been granted otherwise "ERR" if the EP600 was not in Storing Mode. Example of command #00@0153* which sets the address to "53". Therefore, all following commands starting with #53*, in addition to #00*, will be granted.	





7 - DLL Function reference guide

<->
¬NOTE

All the following examples are indifferently referred to the PMM

EP600, EP601, EP602 and EP603.

✓¬NOTE

The DLL library manages only the broadcast address ("00").

7.1 C language

7.1.1 PMM_CreateProbe()

int PMM_CreateProbe(const char *name, HANDLE *probeHandle, const char *commPort);

Purpose:

Establishes communications with a specified probe.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

const char *name: PMM EP60X model name Ex.: EP601

const char *commPort: Serial communication port name Ex.: COM1, COM3...COM99

Output Parameters:

HANDLE * Handle

<[↑]NOTE

Use #include<windows.h> for the HANDLE type data.

Special value that is used to refer to this probe for subsequent function calls after it is created.

7.1.2 PMM_RemoveProbe()

int PMM_RemoveProbe(const HANDLE probeHandle);

Purpose:

Closes the communications port and releases memory back to the system.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

<u>Input Parameters:</u>

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

None

7.1.3 PMM_Firmware()

int PMM_Firmware(const HANDLE probeHandle, char *firmware, int *arraySize);

Purpose:

Gets the probe's firmware version.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

Pass-by-reference character string: Specifying the length of string



7.1.4 PMM_ProbeName()

int PMM_ProbeName(const HANDLE probeHandle, char *name, int *arraySize);

Purpose.

Return the probe name identification information.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

The name is placed in the user allocated string buffer.

7.1.5 PMM_Model()

int PMM_Model(const HANDLE probeHandle, char *model, int *arraySize);

Purpose:

Return the probe model identification information.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

The model is placed in the user allocated string buffer.

7.1.6 PMM_CalibrationDate()

int PMM_CalibrationDate(const HANDLE probeHandle, char *calibrationDate, int *arraySize);

Purpose:

Returns the probe's the last calibration date. Not available on older probes.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

Pass-by-reference character string: calibrationDate: probe's calibration date

arraySize: the length of the string.



7.1.7 PMM_ReadBattery()

int PMM_ReadBattery(HANDLE probeHandle, float *battery);

Purpose:

This function reads the probe's battery status.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle

Output Parameters:

Pass-by-reference float battery: Is the battery's status in Volt.

7.1.8 PMM_ReadTemperature()

int PMM_ReadTemperature(HANDLE probeHandle, float *temperature);

Purpose:

This function reads the probe's internal temperature.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle

Output Parameters:

Pass-by-reference float temperature. The numeric value of the probe internal temperature in degrees Celsius.

7.1.9 PMM_SerialNumber()

int PMM_SerialNumber(const HANDLE probeHandle, char *serialNumber, int *arraySize);

Purpose:

Returns the probes serial number.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle

Output Parameters:

Pass-by-reference character string serialNumber: probe's serial number. arraySize: the length of the string.



7.1.10 PMM_SetFrequency()

int PMM_SetFrequency(const HANDLE probeHandle, int Frequency);

Purpose.

Sets the frequency to which refer the correction factor. Once the EP600 has received and granted this command, all measurements will be corrected using the factor stored in factory related to this frequency.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle, int Frequency multiplied by 100 giving thus the resolution of 10kHz.

Sending a frequency which is out of EP600 range disables frequency correction factor function.

Output Parameters:

None

7.1.11 PMM_SetFilter()

int PMM_SetFilter(const HANDLE probeHandle, int FILTER);

Purpose:

Sets the processing filter (n) used for measurements.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle, int range Accepts values 0 – 7

Output Parameters:

None

7.1.12 PMM_SetTimeout()

int PMM_SetTimeout(int tout);

Purpose:

Sets the communication timeout with PMM EP600 series.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

int tout in milliseconds. Default value is 500 ms.

Output Parameters:

None



7.1.13 PMM_SetAutoOffTime()

int PMM_SetAutoOffTime(const HANDLE probeHandle, int Time);

Purpose:

Sets the time before the EP600 auto-switches off after having received a recognized command.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle, int time in seconds. Accepts values 180(3 minuts) – 10800(3 hours)

Output Parameters:

None

7.1.14 PMM_ReadTotalField()

int PMM_ReadTotalField (const HANDLE probeHandle, float &XYZField);

Purpose:

Returns the total combined field of the X, Y and Z Axis.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle; as returned from the CreateProbe function

Output Parameters:

Pass-by-reference float. The combined fields of X, Y and Z axis.

7.1.15 PMM_ReadAxisField

PMM_ReadAxisField (const HANDLE probeHandle, float *xField, float *yField, float *zField);

Purpose

To read the field values from the X-axis, Y-axis and Z.

Return Value:

Returns an integer status code. The numeric value of 0 indicates no error occurred. See Status Code chapter for an error code description.

Input Parameters:

HANDLE probeHandle

Output Parameters:

Pass-by-reference float. Returns the X, Y and Z fields.



7.2 Visual Basic

From the Project menu, select References to call up the References dialog box, and then click Browse to find your new type library (PMM_EP60X.tlb). Once you have located it, press OK. Visual Basic will automatically register the library for you the first time you reference it. Make sure that your library ("PMM_EP60X") has been checked in the references List, and then close the dialog box.

7.3 Status Code

TAB	LE 7-1 Status Code
0	OK
1	Bad Handle
2	Unable to open port
3	Not connected
4	Wrong response
5	No response
6	Invalid parameter
7	Commport busy
8	Timeout
9	Commport error
10	Problem writing comport
11	Read comport error
12	Bad connection string
13	Value cannot be set
14	Probe not supported
15	Probe over range
16	Probe under range
17	Error closing commport
18	Error purging commport



The file PMM_EP60X.DLL and PMM_EP60X.TLB are installed automatically by the WinEP600 Setup.exe in the system folder C:\Windows\System32\.



8 - Accessories

8.1 Foreword This chapter explains how to use the accessories of PMM

EP600/EP601/EP602/EP603.

The following general indications apply to all accessories.

8.2 Inspection Check the packing integrity.

If anything is found damaged or missed, immediately contact your Dealer.

Check the accessories with reference to the packing list included in the package.

8.3 Ambient Store the accessories in clean, dry environment free of dust and acid

vapours.

Follow requirements for temperature and humidity:

Operation:

Temperature
 Humidity
 -10° to +40° C
 90% RH

Storage:

Temperature
 Humidity
 -20° to + 70° C
 < 95% RH

8.4 Return for service

Every part of the accessories, included batteries, can only be replaced by NARDA, when the instrument needs repair or is malfunctioning, please contact the NARDA Support center.

When an accessory needs to be sent to NARDA for repairs please complete the questionnaire enclosed with this Operating Manual making sure you fill in all the details relative to the service requested.

In order to minimize repair time, please describe the nature of the failure. If the failure occurs only under certain conditions, please provide details on how we may recreate the same condition in order to identify the fault.

If possible, please reuse the original packaging, making sure the accessory is wrapped in heavy paper or plastic.

Alternatively, use a strong box filled with shockproof material, place enough material all around the equipment so that the unit is stable and firmly blocked inside the box.

Whilst packing, pay special care in protecting the unit's front panel.

Seal the box firmly before shipment.

Mark the box: FRAGILE HANDLE WITH CARE.

8.5 CleaningTo clean the equipment use only dust-free, non-abrasive dry cloths.

WWARNING

To avoid damage never use any kind of solvent, acid, or similar to clean the instrument.





8.6 PMM 8053-OC Optical-Serial converter

This accessory of the field probe PMM EP600/EP601/EP602/EP603 allows the fiber optic to be connected to the PC RS-232 serial port.



Installation

Connect the PMM 8053-OC to a free serial port of PC; connect the fiber optic of the probe respecting the optical connector insertion key. The PMM 8053-OC is powered from the PC serial port directly.

Table 8-1 Specifications of PMM 8053-OC

Max allowed fiber optic length 80 m (see notes below)

9 pin DB9 RS 232 connector

For some PC models the power available at the DB9 connector may be not enough to allow the 8053-OC for driving fiber optics up to 80 m.

NOTE

For some PC models the power available at the DB9 connector may be not enough to guarantee the correct operation of the 8053-OC. In such cases apply the 8053-OC-PS between 8053-OC and PC.

1 – fiber optic connector



Rear panel

Front panel

1 - RS232 DB9 female connector



Fig. 8-1 8053-OC Panels

Power supply

The PMM 8053-OC is powered from the PC serial port directly.





8.7

8053-OC-PS Power Supply



This accessory of the field probe PMM EP600/EP601/EP602/EP603 allows for providing the power supply to the 8053-OC converter whenever the PC serial port power supply is not sufficient or absent.

Installation

Connect the 8053-OC-PS to the PC serial port (or serial cable) and to the 8053-OC. Connect the 8053-OC-PS to the mains by the AC adapter (supplied). Connect the fiber optic to the 8053-OC.



Table 8-2 Specifications of 8053-OC-PS Power Supply

RS 232 Connectors

9 pin DB9



Front panel

DB9 M connector



Rear panel

DB9 F connector



Side

M connector for DC suppli

Fig. 8-2 8053-OC-PS

Power supply

8053-OC-PS is supplied by the 230Vac - 9Vdc Wall Adapter.

Accessories





8.8

PMM TR-02A Tripod



This accessory allows for standing the PMM EP600/EP601/EP602/EP603 field probe or the PMM 8053B hand held unit by means of the fixing screw. The swivel PMM 8053-SN is supplied together with the tripod.

The PMM TR-02A has been specifically designed to prevent influencing the field measurements.

The extensible legs allow for setting the required height; the feet are designed to provide stability on most of the surfaces. The height of the central rod can be set as well.

The PMM TR-02 is supplied in a robust carrying bag.

Table 8-3 Characteristics of PMM TR-02A


• 3 legs of 3 extensible sections

• Transport encumbrance: 76 x 12 x 12 cm

Minimum height: 60 cm
Maximum height: 180 cm
Weight 2,8 kg
Max load: 10 kg
Screw connection 1/4"



Details:

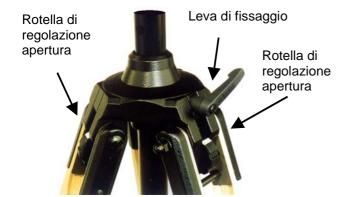

The inclination of each leg can be set in three different positions:

- Fixed 20°: white mark
- Fixed 45°: red mark
- Variable: no marks visible.

The central support can be set and locked by the handle.



Fig. 8-3 TR02A



The swivel **PMM 8053-SN** can be mounted on the PMM TR-02A top.

height: 8 cmweight: 160 gLoad max: 10 kgScrew: ¼ "



Fig. 8-4 adjustable swivel





8.9

PMM TT-01 Telescopic extension

PMM TT-01 allows for extending the distance between field probe and operator or measuring instrument.

The TT-01 top is provided with the screw to fix the conical adapter. The length can be adjusted at any value between minimum and maximum.

The PMM TT-01 is made of fibreglass and has been specifically designed to prevent influencing the field measurements.

Table 8-4 Characteristics of TT-01		
D'a santar	00	
Diameter	32 mm	
Minimum length:	120 cm	
 Maximum extension: 	420 cm	
Weight	500 g	



Fig. 8-5 TT-01 Fiberglass telescopic extension with EP600/EP601/EP602/EP603installed on the top.







8.10 PMM SB-10 Switching Control Box



PLEASE REFER TO THE RELEVANT OPERATION MANUAL





http://www.narda-sts.it

NARDA
Safety
Test
Solutions
S.r.l. Socio Unico

Sales & Support:

Via Leonardo da Vinci, 21/23 20090 Segrate (MI) - ITALY Tel.: +39 02 2699871 Fax: +39 02 26998700 Manufacturing Plant:

Via Benessea, 29/B 17035 Cisano sul Neva (SV) Tel.: +39 0182 58641 Fax: +39 0182 586400



Mod. 18-1

Caro cliente

grazie per aver acquistato un prodotto NARDA! Sei in possesso di uno strumento che per molti anni ti garantirà un'alta qualità di servizio. NARDA riconosce l'importanza del Cliente come ragione di esistenza; ciascun commento e suggerimento, sottoposto all'attenzione della nostra organizzazione, è tenuto in grande considerazione. La nostra qualità è alla ricerca del miglioramento continuo. Se uno dei Suoi strumenti NARDA necessita di riparazione o calibrazione, può aiutarci a servirla più efficacemente compilando questa scheda e accludendola all'apparecchio.

Tuttavia, anche questo prodotto diventerà obsoleto. In questo caso, ti ricordiamo che lo smaltimento dell'apparecchiatura deve essere fatto in conformità con i regolamenti locali. Questo prodotto è conforme alle direttive WEEE dell'Unione Europea (2002/96/EC) ed appartiene alla categoria 9 (strumenti di controllo). Lo smaltimento, in un ambiente adeguato, può avvenire anche attraverso la restituzione del prodotto alla NARDA senza sostenere alcuna spesa. Può ottenere ulteriori informazioni contattando i venditori NARDA o visitando il nostro sito Web www.narda-sts.it.

Dear Customer

thank you for purchasing a NARDA product! You now own a high-quality instrument that will give you many years of reliable service. NARDA recognizes the importance of the Customer as reason of existence; in this view, any comment and suggestion you would like to submit to the attention of our service organization is kept in great consideration. Moreover, we are continuously improving our quality, but we know this is a never ending process. We would be glad if our present efforts are pleasing you. Should one of your pieces of NARDA equipment need servicing you can help us serve you more effectively filling out this card and enclosing it with the product.

Nevertheless, even this product will eventually become obsolete. When that time comes, please remember that electronic equipment must be disposed of in accordance with local regulations. This product conforms to the WEEE Directive of the European Union

(2002/96/EC) and belongs to Category 9 (Monitoring and Control Instruments). You can return the instrument to us free of charge for proper environment friendly disposal. You can obtain further information from your local NARDA Sales Partner or by visiting our website at www.narda-sts.it.

tro: ther:
illei.
tro: Other:
l Altro ∃ Other

<u>Suggerimenti / Commenti / Note:</u> <u>Suggestions / Comments / Note</u> :