


LCR Meter Automation — Measurement Report

CSIR-NPL LCR Automation Software

Report Generated	15 July 2026, 12:39 PM
Instrument	E4980A
Measurement Mode(s)	Cp-D, Cs-Rs, Z-θd
Frequency	1 kHz
Signal Voltage	1.000 V V
Aperture	LONG
Average	16
Number of Readings	15
Source File	LCR_20260715_123814.csv

Measurement Graph

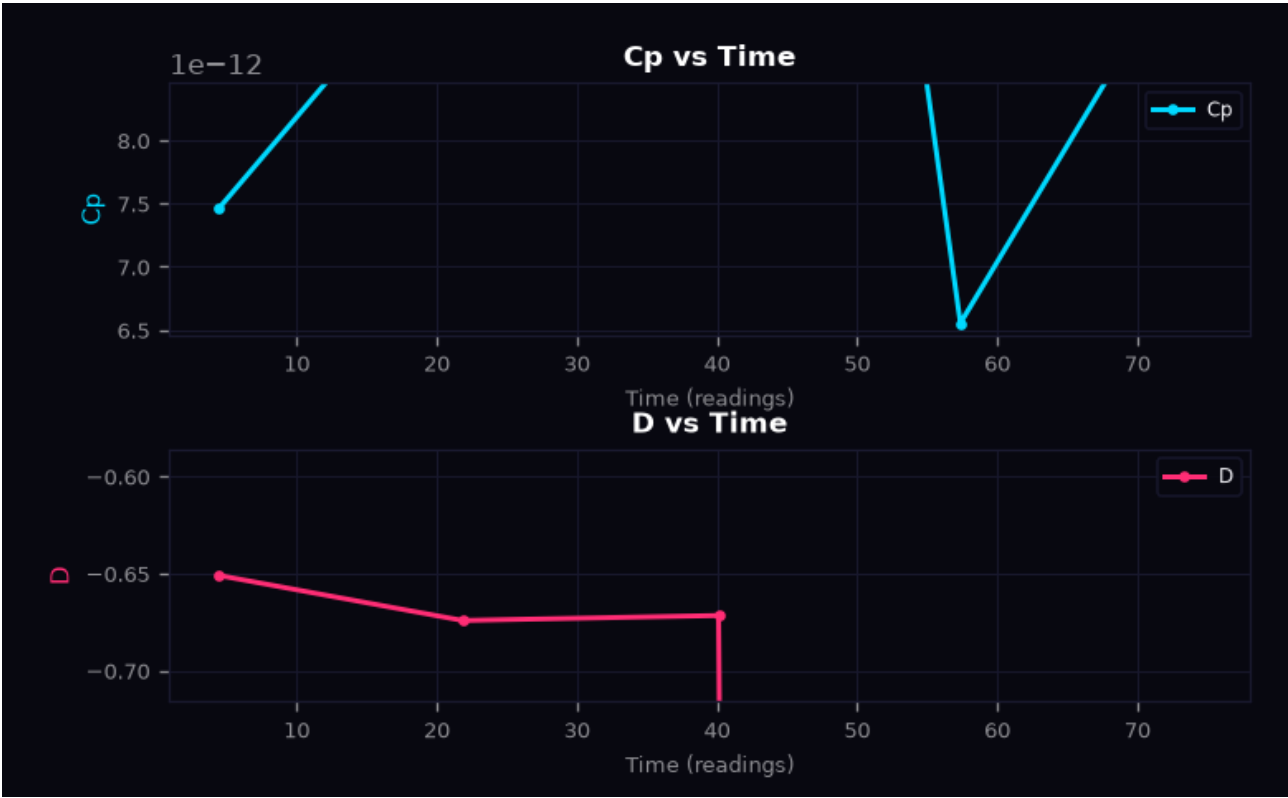

Measurement Data

Reading#	Elapsed(s)	Mode	P1	P2	Status
1	4.419	Cp-D	7.458960 pF	-0.650915	OK
1	8.576	Cs-Rs	16.96130 pF	-7.458180 MOhm	OK
1	12.685	Z-θd	9.533860 MOhm	-108.9420 deg	OK

Reading#	Elapsed(s)	Mode	P1	P2	Status
2	21.837	Cp-D	9.726570 pF	-0.674171	OK
2	26.516	Cs-Rs	19.30890 pF	-17.46540 MOhm	OK
2	30.829	Z-θd	9.450740 MOhm	-143.9820 deg	OK
3	40.105	Cp-D	20.19920 pF	-0.671589	OK
3	44.183	Cs-Rs	19.97240 pF	-1.588720 MOhm	OK
3	48.263	Z-θd	5.797370 MOhm	-152.6840 deg	OK
4	57.365	Cp-D	6.554370 pF	-14.917000	OK
4	61.432	Cs-Rs	21.39780 pF	-6.484450 MOhm	OK
4	65.510	Z-θd	10.44280 MOhm	-123.0470 deg	OK
5	74.574	Cp-D	9.726510 pF	-0.726222	OK
5	78.640	Cs-Rs	9.881400 pF	-21.86320 MOhm	OK
5	82.798	Z-θd	35.78700 MOhm	-90.53580 deg	OK