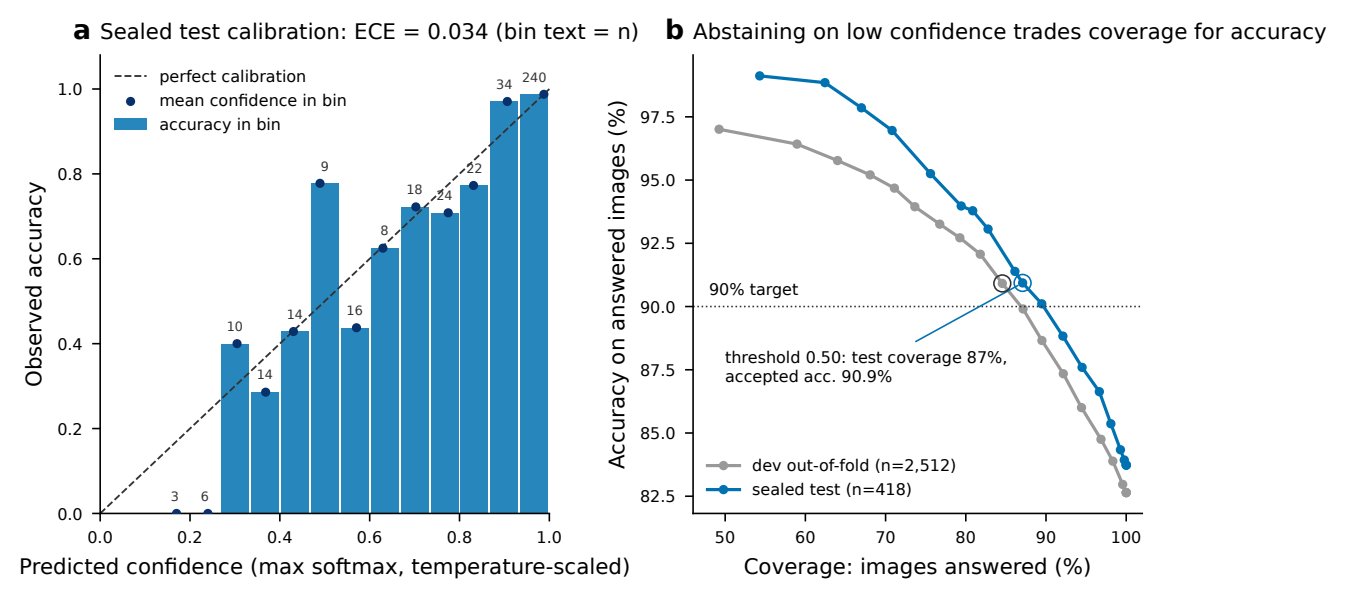
a Sealed test calibration: ECE = 0.034 (bin text = n)
perfect calibration
mean confidence in bin
accuracy in bin
Observed accuracy
Predicted confidence (max softmax, temperature-scaled)
3
6
10
14
14
9
16
8
18
24
22
34
240
b Abstaining on low confidence trades coverage for accuracy
Accuracy on answered images (%)
Coverage: images answered (%)
90% target
threshold 0.50: test coverage 87%,
accepted acc. 90.9%
dev out-of-fold (n=2,512)
sealed test (n=418)