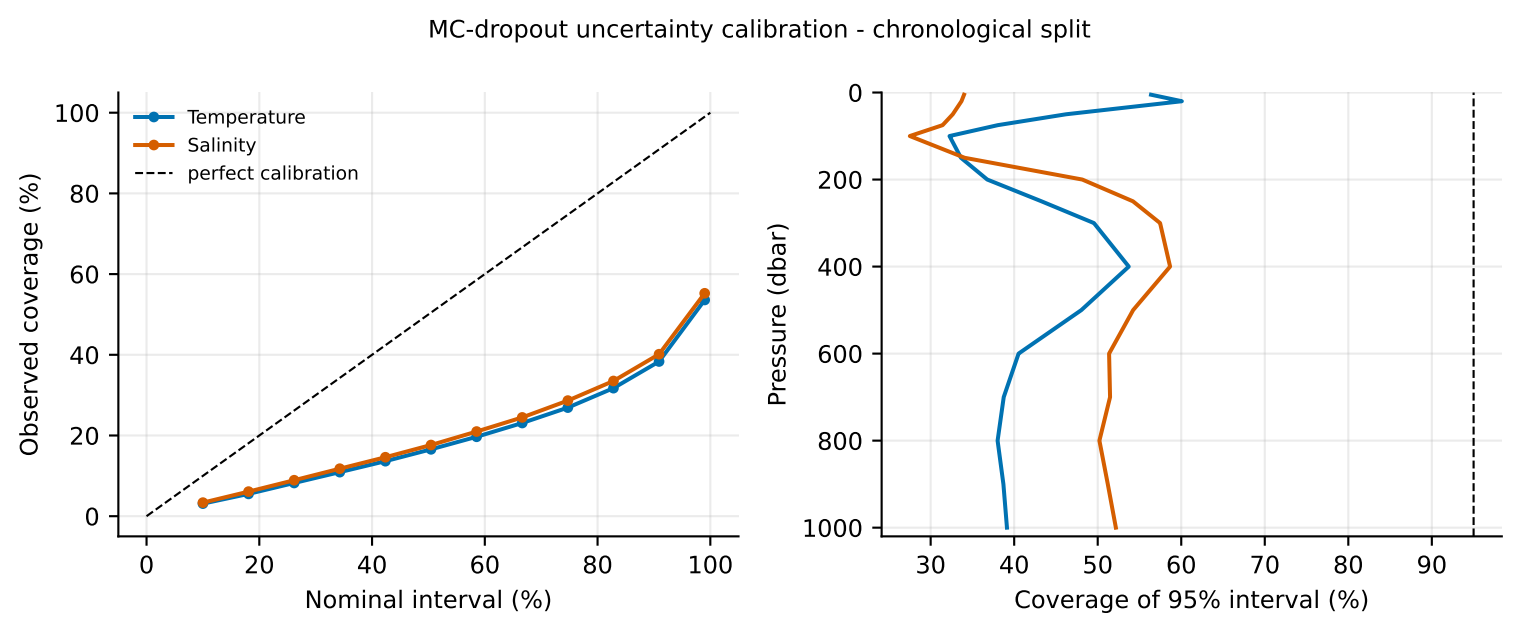
MC-dropout uncertainty calibration - chronological split
Temperature
Salinity
perfect calibration
Observed coverage (%)
Nominal interval (%)
Pressure (dbar)
Coverage of 95% interval (%)