X-Fusion: Tri-Modal Transformer Fusion for Multi-Label Chest X-ray Analysis

K. Vishal Reddy
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
Kasarlavishalreddy@gmail.com

P. Deepesh Reddy
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
deepeshp113@gmail.com

R. Vignesh
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
rvignesh72007@gmail.com

R. Sidhardh Reddy
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
sidhardhramini2007@gmail.com

Saharsh Machendra
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
saharshbatte356@gmail.com

Vura Surya Venkat
Department of Computer Science and Engineering
Keshav Memorial Institute of Technology
Hyderabad, Telangana, India
vuraramesh01@gmail.com

***Abstract*—Chest radiographs frequently exhibit coexisting thoracic findings, motivating multi-label prediction supported by complementary patient information. X-Fusion is a tri-modal framework combining BiomedCLIP visual features, CXR-BERT clinical-note representations, and six demographic and physiological fields in a shared 512-dimensional space. A compact two-layer, eight-head Transformer fuses three modality tokens and a learned classification token to produce fourteen independent finding scores. Asymmetric Loss and an auxiliary contrastive objective support training, while a web application provides visual attention overlays and metadata attribution. A companion study draft reports macro AUROC of 0.9420, micro AUROC of 0.9615, and mean average precision of 0.8840, compared with 0.8162, 0.8740, and 0.7420 for a vision-only baseline. These comparative figures are document-reported rather than independently reproduced. In the available experimental pipeline, generated clinical notes and vital signs depend on target labels, limiting interpretation of the results as evidence of clinical generalization. The work establishes an integrated multimodal research prototype and a basis for subsequent evaluation using independent clinical inputs.**

***Index Terms*—Chest radiography, multimodal learning, Transformer fusion, multi-label classification, explainability**

I. Introduction

Chest radiography is widely used for evaluating thoracic abnormalities. A single image may exhibit several coexisting findings, making multi-label classification more appropriate than mutually exclusive disease prediction. NIH ChestX-ray14 provides a benchmark for this setting [1], [2]. Visual patterns can be ambiguous without clinical context; patient history and physiological measurements may offer complementary information, provided these inputs are collected independently of the reference diagnosis.

X-Fusion integrates three information streams: a radiograph, a clinical note, and six structured patient attributes. Pretrained BiomedCLIP and CXR-BERT representations are projected into a common feature space and combined with an MLP-based metadata representation using Transformer self-attention. The framework predicts fourteen labels and exposes attention and metadata-attribution views through a web interface. The principal contribution is an integrated, inspectable tri-modal prediction workflow, accompanied by a detailed description of its architecture, training objectives, data partitions, and reported comparative experiments.

A. Motivation and Research Objectives

The proposed system addresses a representation-integration problem rather than assuming that any single modality can fully characterize a thoracic finding. A chest radiograph encodes anatomical appearance, a clinical note supplies contextual language, and structured measurements provide numerical context. Each stream has a different representation and measurement scale. A shared latent space makes these streams accessible to a small fusion network without requiring a separate prediction head for every possible combination of modalities.

Three practical objectives guide the design. First, the prediction head must permit multiple simultaneous findings, including the absence of all fourteen findings. Second, the fusion mechanism should expose a compact set of modality representations suitable for attention-based interaction. Third, the prototype should connect the numerical prediction to an interface in which users can inspect visual attention and metadata attribution separately. These are engineering objectives; whether they improve clinical decision making is a separate empirical question.

The distinction between an image-derived finding and contextual information is particularly important for evaluation. A multimodal classifier may exploit correlations between patient context and disease labels. Such correlations are informative only when the context is acquired without access to the target label. Accordingly, the input-generation process is part of the experimental design and not merely a software implementation detail.

II. Related Work

Wang et al. introduced the NIH chest radiograph benchmark [1]; CheXpert subsequently addressed uncertainty labels and expert comparison [3]. Vision Transformers model long-range relationships through attention [4], [5]. BiomedCLIP learns biomedical visual representations from image–text pairs [6], while CXR-BERT specializes language representations for

radiology [7]. DAViT explores domain-adapted Transformer modeling for pneumonia detection [8], a distinct single-disease setting. Asymmetric Loss addresses positive–negative imbalance [9], InfoNCE supports representation alignment [10], and SHAP provides feature-attribution methods [11]. Attention visualization alone should not be interpreted as validated disease localization [12].

A. Positioning Relative to Prior Systems

ChestX-ray14 supports weakly supervised multi-label classification, whereas CheXpert introduces a different dataset and uncertainty-handling setting. These datasets should not be treated as interchangeable evaluation cohorts. The DAViT study investigates domain-adapted vision modeling for pneumonia, while X-Fusion targets fourteen independent findings and incorporates two auxiliary information streams. Therefore, a direct numerical comparison between the two papers would mix different labels, data partitions, and evaluation protocols.

The architectural distinction is also relevant. BiomedCLIP provides a pooled image representation rather than passing every image patch directly into the multimodal encoder. CXR-BERT similarly contributes one contextualized text vector. This reduces the fusion sequence to four tokens, including the learned CLS token. The compact design limits the number of interactions computed at the fusion stage, although it necessarily discards some fine-grained spatial and linguistic structure. Visual attention overlays are obtained separately from the image backbone rather than from a disease-specific spatial decoder.

Asymmetric Loss and contrastive alignment serve different purposes. The former changes the classification gradient assigned to easy negatives in an imbalanced label matrix. The latter encourages matched image and text representations to align within a minibatch. Neither loss alone guarantees calibrated probabilities or robustness to missing modalities; those properties require distinct evaluation.

III. Proposed Architecture and Methodology

A. Modality-Specific Encoders

For an RGB radiograph I, a tokenized note T, and ordered metadata vector $m \in \mathbb{R}^6$, the encoders produce

$$z_v = f_v(I) \in \mathbb{R}^{512}, \tag{1}$$

$$z_t = W_t h_t(T) + b_t \in \mathbb{R}^{512}, \tag{2}$$

$$u = \mathrm{Dropout}_{0.1}(\mathrm{GELU}(W_1 m + b_1)), \tag{3}$$

$$z_m = \mathrm{GELU}(W_2 u + b_2) \in \mathbb{R}^{512}. \tag{4}$$

BiomedCLIP supplies pooled image features. The first CXR-BERT output token is projected from 768 to 512 dimensions, with notes limited to 256 tokens. The metadata encoder maps age, sex, temperature, heart rate, respiratory rate, and oxygen saturation through a 128-unit hidden layer; $W_1 \in \mathbb{R}^{128\times 6}$ and $W_2 \in \mathbb{R}^{512\times 128}$.

B. Transformer Fusion

The learned classification token and three modality vectors form

$$S_0 = [e_{\mathrm{CLS}}; z_v; z_t; z_m] \in \mathbb{R}^{4\times 512}. \tag{5}$$

Two Transformer encoder layers with eight attention heads and feed-forward width 2048 operate on this sequence. For each attention head,

$$\mathrm{Attention}(Q, K, V) = \mathrm{softmax}\left(\frac{QK^\top}{\sqrt{d_k}}\right) V, \quad d_k = 64. \tag{6}$$

The fused CLS vector is classified with dropout probability 0.3:

$$h = \mathrm{Transformer}(S_0)_{\mathrm{CLS}}, \quad p_k = \sigma([W_c\, \mathrm{Dropout}_{0.3}(h) + b_c]_k)\,. \tag{7}$$

Here $W_c \in \mathbb{R}^{14\times 512}$, and $k = 1, \ldots, 14$. The findings are Atelectasis, Cardiomegaly, Effusion, Infiltration, Mass, Nodule, Pneumonia, Pneumothorax, Consolidation, Edema, Emphysema, Fibrosis, Pleural Thickening, and Hernia.

C. Representation Dimensions and Token Interactions

The image, text, and metadata branches produce vectors of identical width, but their internal computations differ. The image representation summarizes visual patches extracted by the pretrained vision backbone. The text representation is derived from the first language-model output token, and its learned projection accommodates the width mismatch between the language encoder and the fusion network. The metadata branch uses two affine mappings separated by GELU and dropout to learn nonlinear interactions among the six structured fields.

Within the fusion encoder, every query token can attend to the classification token and the three modality tokens. With eight heads and model width 512, each attention head operates on a 64-dimensional key space. The two-layer stack permits the learned classification token to aggregate information after intermediate modality-to-modality interactions. Because the sequence has only four tokens, this attention describes interactions among pooled modalities rather than localization among individual anatomical patches. Residual connections and layer normalization support stable information flow through the encoder.

The sigmoid prediction head differs from a softmax classifier. A softmax distribution forces class probabilities to sum to one and is unsuitable when multiple abnormalities can coexist. Independent sigmoid scores instead represent fourteen binary outputs. Their values should be interpreted as model scores until class-specific calibration and an appropriate operating threshold have been established. In particular, selecting the largest score does not imply that the remaining findings are absent.

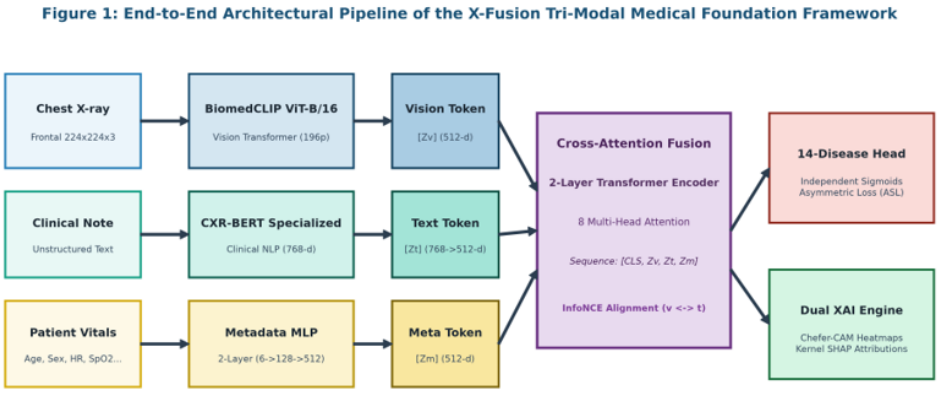


Fig. 1. Overview of the X-Fusion tri-modal architecture. The diagram is schematic; visual attribution is based on attention rather than a validated disease-specific localization method.

D. Optimization Objectives

Let p_{ik} be the predicted probability for finding k in sample i, and $y_{ik} \in \{0, 1\}$ its label. Define $q_{ik} = \min(1-p_{ik}+0.05, 1)$. With $\epsilon = 10^{-8}$, the per-label Asymmetric Loss term is

$$\ell_{ik} = -y_{ik}(1-p_{ik})\log(\max(p_{ik}, \epsilon)) - (1-y_{ik})(1-q_{ik})^4 \log(\max(q_{ik}, \epsilon)). \quad (8)$$

The classification loss is $\mathcal{L}_{\text{ASL}} = B^{-1}\sum_{i=1}^{B}\sum_{k=1}^{14}\ell_{ik}$. For normalized image and text features v_i, t_j, similarity is $C_{ij} = v_i^\top t_j/\tau$, where $\tau = 0.07$. Symmetric contrastive alignment uses

$$\mathcal{L}_{\text{NCE}} = \tfrac{1}{2}[\text{CE}(C, a) + \text{CE}(C^\top, a)], \quad (9)$$

$$\mathcal{L}_{\text{train}} = \mathcal{L}_{\text{ASL}} + 0.1\mathcal{L}_{\text{NCE}}, \quad (10)$$

where a contains matching image–text batch indices.

E. Loss Behavior and Class Imbalance

The positive and negative terms in the classification objective receive different focusing behavior. For positive labels, the factor $(1-p)$ emphasizes positives assigned low predicted probability. For negatives, the clipped complement q and fourth-power focusing term reduce the contribution of easy negative examples. The clipping margin is 0.05, and the numerical floor prevents logarithms from receiving zero-valued arguments. Summing the per-label terms allows each radiograph to contribute multiple positive findings.

Contrastive alignment is computed over paired image and note representations in the current minibatch. The diagonal of the similarity matrix identifies matching samples; off-diagonal entries serve as alternative pairs. The temperature parameter controls the sharpness of the similarity distribution. This objective assumes that the provided note corresponds to its image. Because the current experiment constructs notes from target labels, the resulting alignment must not be interpreted as evidence that the model has learned to align independently collected radiology language with radiographic findings.

The combined objective gives contrastive alignment one tenth of the classification-loss weight. This numerical weighting specifies the optimization objective but does not establish equal influence on gradients, because the losses may have different scales. For this reason, the recorded training and validation losses are discussed separately rather than used as directly comparable estimates of generalization.

TABLE I
DATASET PARTITIONS

Partition	Images	Patients
Training	21,964	9,939
Validation	2,566	1,104
Test	7,100	1,137
Total	31,630	12,180

IV. Dataset and Experimental Setup

A. Data Partitioning

The local study subset contains 31,630 images matched to metadata, drawn from 31,877 available PNG files; the full NIH release includes 112,120 radiographs [2]. Training and validation images are selected from the official train/validation list, with patient IDs shuffled using seed 42 and 10% of patients reserved for validation. Test images follow the official test list. The partitions contain no overlapping patient IDs. Images are resized to 224×224 pixels, converted to RGB, and normalized using channel means $(0.485, 0.456, 0.406)$ and standard deviations $(0.229, 0.224, 0.225)$. Training augmentation includes horizontal flips, rotations up to 10°, and brightness/contrast jitter of 0.15. Validation and test preprocessing is deterministic. The fourteen findings are nonexclusive; "No Finding" is represented by an all-zero target vector.

TABLE II
POSITIVE-LABEL COUNTS BY PARTITION

Finding	Train	Validation	Test
Atelectasis	3237	367	879
Cardiomegaly	723	107	387
Effusion	2687	329	1270
Infiltration	3629	433	1128
Mass	1600	164	476
Nodule	2111	226	476
Pneumonia	42	5	18
Pneumothorax	1148	131	1024
Consolidation	132	11	62
Edema	395	43	262
Emphysema	557	70	335
Fibrosis	558	57	190
Pleural Thickening	787	94	348
Hernia	63	8	49

TABLE III
RECORDED TRAINING-LOSS ENDPOINTS

Quantity	First	Last
Train: ASL + 0.1 InfoNCE	0.1545	0.1190
Validation: ASL	0.0207	0.0007

TABLE IV
COMPARATIVE METRICS REPORTED IN THE ACCOMPANYING STUDY DRAFT

Model	Macro AUROC	Micro AUROC	mAP
Vision only	0.8162	0.8740	0.7420
Vision + text	0.8870	0.9215	0.8250
X-Fusion	**0.9420**	**0.9615**	**0.8840**

B. Auxiliary Inputs and Training

Age and sex come from image metadata. In the available experiment, clinical-note templates and sampled vital signs are conditioned on disease labels. This creates a dependency between auxiliary inputs and the target and is a key consideration when interpreting predictive metrics. Training uses AdamW, cosine annealing, a learning rate of 2×10^{-4}, weight decay of 10^{-4}, batch size 4, gradient accumulation over eight batches, requested 16-bit mixed precision, and a frozen text encoder. The available checkpoint is from epoch 14 of a 15-epoch configuration.

C. Partition Characteristics and Reproducibility

The local matched subset represents only part of the full ChestX-ray14 release. Its 31,630 radiographs are divided into 21,964 training, 2,566 validation, and 7,100 test images. The patient counts are 9,939, 1,104, and 1,137 respectively. These counts matter because multiple images can originate from one patient; image-level random partitioning could otherwise place correlated observations in more than one split. Patient-disjoint partitioning addresses this specific overlap risk.

The positive-label table shows substantial differences in prevalence. For example, the training partition contains 3,629 Infiltration positives but only 42 Pneumonia positives and 63 Hernia positives. A single global accuracy value would obscure these differences. Macro AUROC assigns equal weight to label-specific AUROC values, while micro AUROC pools decisions across labels. Mean average precision summarizes precision–recall ranking behavior and is particularly informative when positive labels are sparse. Hamming loss counts individual label errors, whereas subset accuracy requires the entire fourteen-label prediction vector to match.

The class counts also limit the precision of estimates for rare findings. The test partition contains 18 Pneumonia positives and 49 Hernia positives. Threshold-specific precision and recall can change appreciably when only a few positive cases are reclassified. Confidence intervals and patient-level resampling would therefore be valuable additions to a subsequent evaluation. No such intervals are inferred from the aggregate numbers reported here.

For reproducibility, a complete evaluation package would identify the exact image list, patient partition, checkpoint, preprocessing configuration, auxiliary-input generation procedure, and prediction scores for every label and test sample. The supplied material supports the partition and configuration description, but does not provide the prediction-level evidence needed to reproduce the draft's comparative tables.

V. RESULTS AND DISCUSSION

A. Optimization Records

Fourteen logged epochs show training objective decreasing from 0.1545 to 0.1190 (22.95% relative reduction) and validation ASL from 0.0207 to 0.0007. Training includes ASL and contrastive regularization, while validation records ASL alone; the magnitudes are therefore not directly comparable. These curves document optimization behavior rather than independent clinical discrimination.

B. Comparative Performance

Table IV reproduces aggregate results reported in the accompanying X-Fusion Word draft. Its macro AUROC difference between the vision-only and tri-modal configurations is 0.1258 (12.58 percentage points). The draft does not supply underlying prediction arrays or a reproducible statistical-test record, so these values are presented as reported comparisons rather than independently validated measurements. The draft's ablation study (Table V) attributes incremental improvements to text, metadata, and Transformer fusion. The Pneumonia threshold sweep (Table VI) identifies 0.35 as the highest-F1 threshold among the tabulated settings. These results require independent replication before comparative conclusions can be established.

A separate saved repository evaluation for 7,100 test-list images records macro AUROC 1.0000, macro AUPRC 0.9953, and macro F1 0.9709. These numbers are distinct from the study-draft results and were obtained in the presence of label-conditioned auxiliary inputs; consequently they are not used here to substantiate diagnostic superiority.

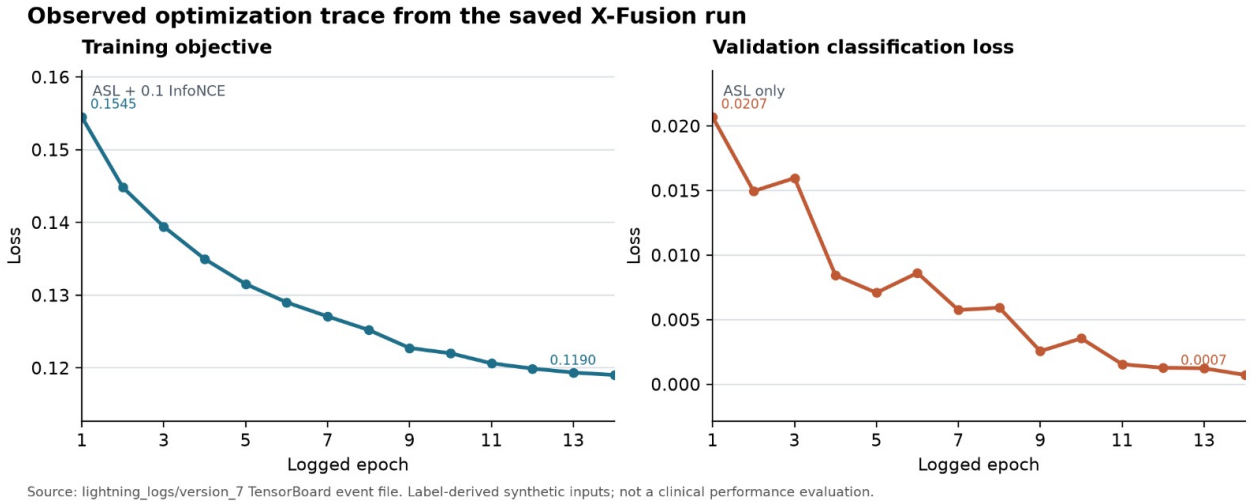


Fig. 2. Saved X-Fusion optimization traces for fourteen logged epochs. Training includes ASL and InfoNCE, while validation includes ASL only; the two scales are not directly comparable.

TABLE V
MODALITY ABLATION REPORTED IN THE ACCOMPANYING STUDY DRAFT

Configuration	Macro AUROC	mAP	Hamming	Subset acc.
Vision only	0.8162	0.7420	0.0840	0.6120
Vision + metadata	0.8540	0.7890	0.0710	0.6780
Vision + text	0.8870	0.8250	0.0580	0.7340
Tri-modal concat.	0.9020	0.8410	0.0490	0.7680
X-Fusion	**0.9420**	**0.8840**	**0.0320**	**0.8420**

TABLE VI
PNEUMONIA THRESHOLD SWEEP REPORTED IN THE STUDY DRAFT

Threshold	Precision	Recall	F1
0.20	0.812	0.978	0.887
0.30	0.885	0.951	0.917
0.35	0.918	0.932	**0.925**
0.40	0.935	0.884	0.909
0.50	0.961	0.810	0.879

C. Reading the Comparative and Threshold Tables

The draft-reported results follow a consistent ordering across its listed configurations. Vision only has the lowest reported macro AUROC and mAP. Adding metadata or text produces higher tabulated values; tri-modal concatenation is higher again, and Transformer fusion is highest. The reported Hamming loss falls from 0.0840 for vision only to 0.0320 for X-Fusion, while subset accuracy rises from 0.6120 to 0.8420. These are descriptive differences within the draft, not a verified causal estimate of the contribution of each component.

The reported macro AUROC gain is 0.1258 in absolute AUROC units, equivalent to 12.58 percentage points. Expressed relative to the vision-only value of 0.8162, the increase is approximately 15.41%. Distinguishing percentage-point change from relative percentage change avoids ambiguity when describing ablations. The same distinction applies to the reported mean average precision increase from 0.7420 to 0.8840.

The Pneumonia threshold table illustrates the usual precision–recall trade-off. At 0.20, the draft reports recall 0.978 and precision 0.812; at 0.50, recall is 0.810 and precision is 0.961. Among the five listed thresholds, 0.35 has the highest reported F1 of 0.925. This does not establish that 0.35 is optimal for every clinical use case. Screening and confirmatory applications may value false negatives and false positives differently, and a clinically selected threshold requires calibration on representative independent data.

D. Explainability and Deployment

The interface overlays attention from the final visual Transformer block: attention from the visual classification token is averaged across twelve heads, arranged into a 14×14 patch grid, and superimposed on the image. This is a visual-attention display, not a validated lesion-localization result. Kernel SHAP evaluates six metadata fields with image and text features fixed; absolute contributions are aggregated across fourteen outputs and normalized. The zero-vector reference used by the current implementation limits clinical interpretation.

A Next.js/React frontend communicates with a FastAPI/PyTorch backend to upload radiographs, enter notes and metadata, return ranked finding scores, and display attribution views. Missing metadata and text are replaced with configured defaults. The interface's leading-finding cutoff of 0.30 is an application setting, not a clinically calibrated threshold.

E. Interpretability and Application Boundaries

The two explanation views answer different questions. The visual overlay indicates which spatial patch locations receive attention in the final visual Transformer block, after averaging over twelve heads. It can help users inspect model behavior, but attention weight is not a direct measure of causal influence



Fig. 3. Illustrative chest radiograph showing the type of input accepted by the prototype. No diagnosis or localization annotation is inferred from this image.

on an individual disease logit. Without a localization benchmark, overlap with a suspected opacity cannot be treated as measured localization accuracy.

Metadata SHAP values quantify changes in model output under the chosen feature-perturbation scheme and reference distribution. Aggregating absolute values across fourteen findings yields a global-looking relative importance display for a single evaluation context, but it discards whether a feature increases or decreases a particular finding score. The current all-zero reference vector is especially difficult to interpret physiologically because zero may be implausible for several vital signs. A clinically meaningful background distribution and finding-specific signed attribution would be preferable in future work.

The web deployment connects a Next.js interface to a FastAPI inference service. Its principal value in the present study is that the same prediction path can be exercised with images, notes, and structured fields and the resulting outputs can be inspected together. The configured default note, fallback metadata values, and leading-finding score cutoff make the prototype usable when fields are missing. They do not constitute a validated missing-data strategy or a clinical triage protocol. Users should therefore interpret the interface as a research demonstration.

F. Study Scope and Limitations

Patient-disjoint splitting protects against patient overlap across image partitions, but does not address target leakage through auxiliary features. Because the current notes and vital signs are generated from diagnosis labels, their predictive contribution cannot be separated from that dependency. The available study also uses a subset of the benchmark, weak image-level labels, and draft-reported comparisons without reproducible prediction-level evidence. Future experiments should use independently collected clinical notes and vitals, release evaluation predictions and threshold-selection procedures, and assess calibration, external generalization, and localization against appropriate reference annotations.

VI. Conclusion and Future Work

X-Fusion demonstrates a compact tri-modal Transformer architecture for fourteen-label chest radiograph analysis, combining pretrained biomedical vision and language encoders, structured metadata, asymmetric classification loss, contrastive alignment, and an explanation-enabled application. The accompanying study draft reports higher aggregate discrimination for tri-modal fusion than for its listed unimodal configurations. Establishing whether these improvements transfer to real clinical inputs requires leakage-free evaluation and external validation. Planned extensions include independent clinical data integration, calibrated class-specific thresholds, and systematic assessment of visual and metadata explanations.

Acknowledgment

The authors thank Keshav Memorial Institute of Technology for its academic support and the NIH Clinical Center for providing the ChestX-ray14 dataset.

References

[1] X. Wang et al., "ChestX-ray8: Hospital-scale chest X-ray database and benchmarks on weakly-supervised classification and localization of common thorax diseases," in *Proc. CVPR*, 2017, pp. 2097–2106.

[2] NIH Clinical Center, "ChestX-ray14 dataset." [Online]. Available: https://nihcc.app.box.com/v/ChestXray-NIHCC

[3] J. Irvin et al., "CheXpert: A large chest radiograph dataset with uncertainty labels and expert comparison," in *Proc. AAAI*, vol. 33, 2019, pp. 590–597.

[4] A. Dosovitskiy et al., "An image is worth 16x16 words: Transformers for image recognition at scale," in *Proc. ICLR*, 2021.

[5] A. Vaswani et al., "Attention is all you need," in *Advances in Neural Information Processing Systems*, vol. 30, 2017.

[6] S. Zhang et al., "BiomedCLIP: A multimodal biomedical foundation model pretrained from fifteen million scientific image-text pairs," arXiv:2303.00915, 2023.

[7] B. Boecking et al., "Making the most of text semantics to improve biomedical vision-language processing," in *Computer Vision–ECCV*, 2022.

[8] M. Fu, C. Tantithamthavorn, and T. Le, "DAViT: A domain-adapted vision transformer for automated pneumonia detection and explanation using chest X-ray images," *IEEE Access*, vol. 13, pp. 103033–103044, 2025.

[9] T. Ridnik et al., "Asymmetric loss for multi-label classification," in *Proc. ICCV*, 2021.

[10] A. van den Oord, Y. Li, and O. Vinyals, "Representation learning with contrastive predictive coding," arXiv:1807.03748, 2018.

[11] S. M. Lundberg and S.-I. Lee, "A unified approach to interpreting model predictions," in *Advances in Neural Information Processing Systems*, vol. 30, 2017.

[12] H. Chefer, S. Gur, and L. Wolf, "Transformer interpretability beyond attention visualization," in *Proc. CVPR*, 2021, pp. 782–791.