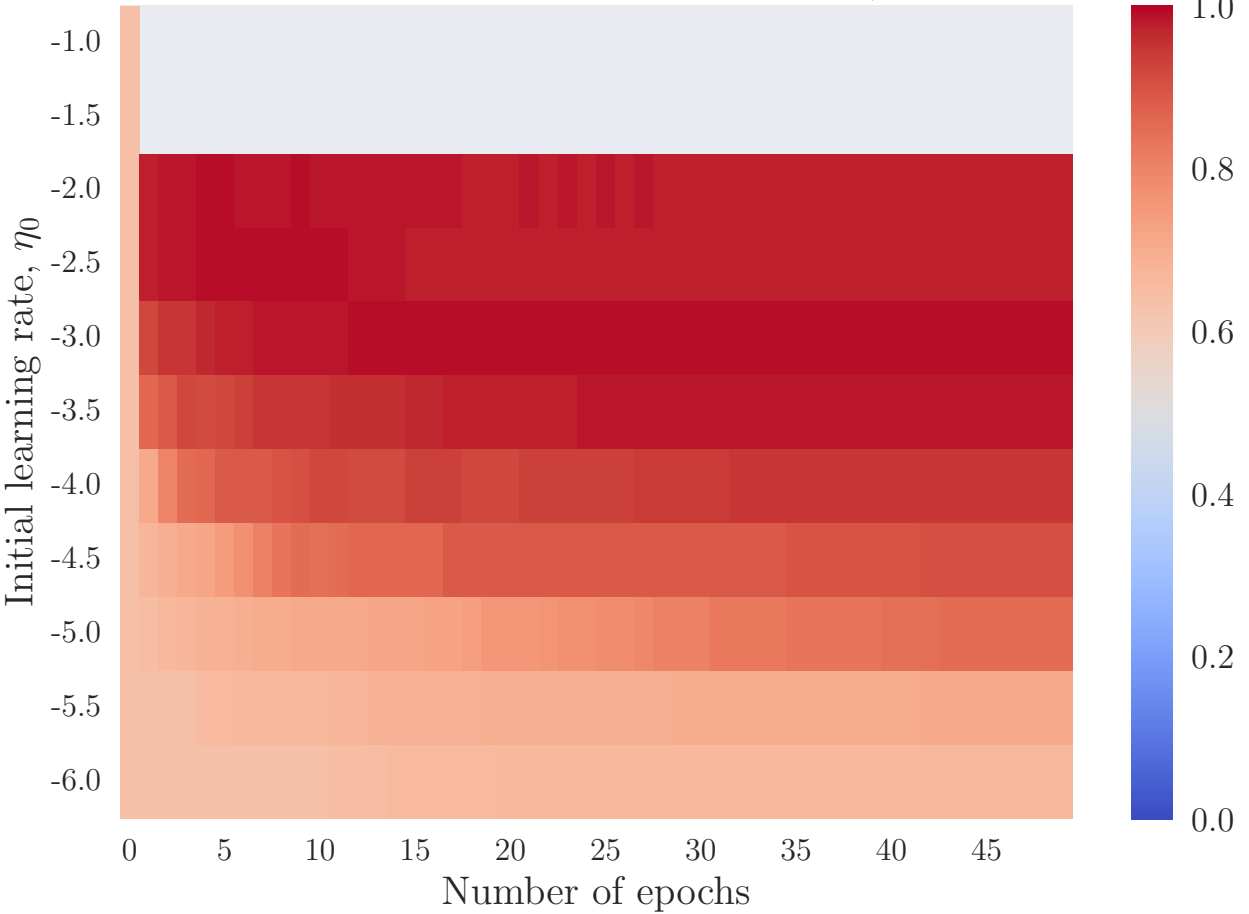test accuracy for Cancer data, using NN with 20 minibatches
Using the Relu activation function
with dynamic learning rate, η