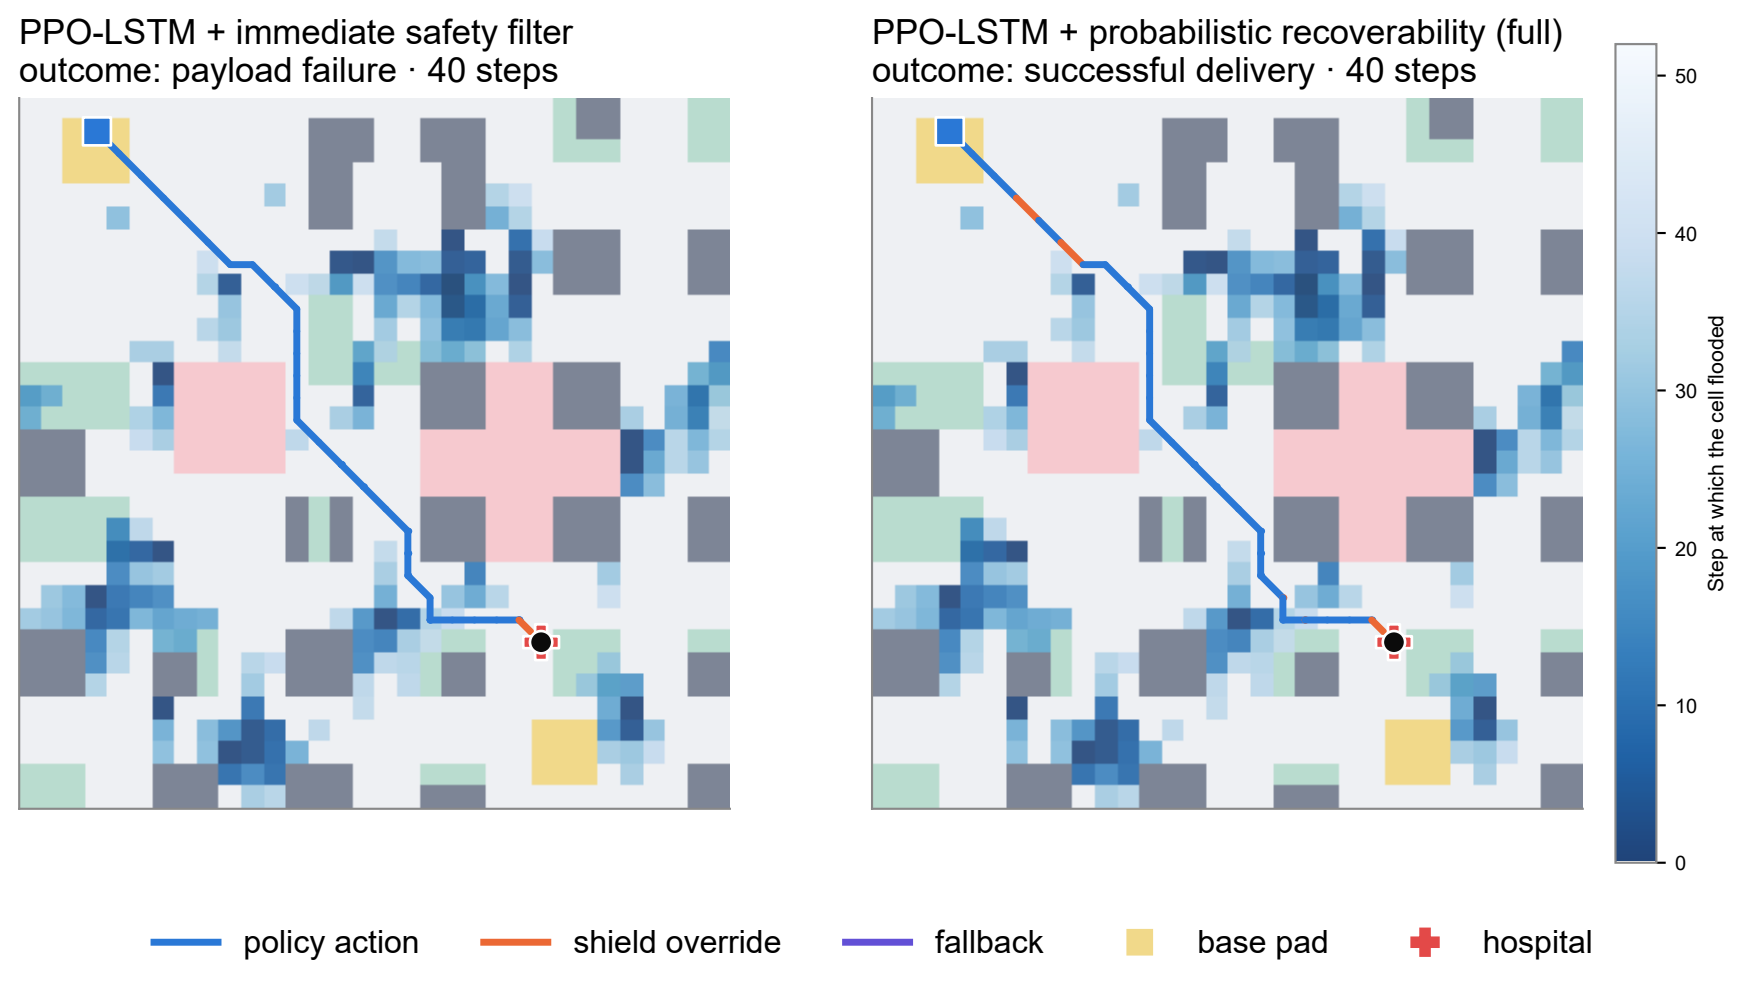
PPO-LSTM + immediate safety filter
outcome: payload failure · 40 steps
PPO-LSTM + probabilistic recoverability (full)
outcome: successful delivery · 40 steps
Step at which the cell flooded
0
10
20
30
40
50
policy action
shield override
fallback
base pad
hospital