



a xylem brand

CALIBRATION CERTIFICATE

Form No 830, March 2021

Certificate no: 4831_466_00237803
Foil batch no: 1206EM

Product: 4831
Calibration date: 03.03.2025

Serial no: 466
Page 1 of 2

Index	Temperature reference(°C)	[O2] Reference(μM)	Temperature raw data(mV)	Phase reading(°)
0	30.379	1.99	-128.780	59.53
1	20.416	1.06	185.967	60.63
2	10.283	0.21	509.740	61.46
3	0.882	-0.95	790.620	62.11
4	0.981	18.90	787.820	59.54
5	1.197	36.81	781.720	57.42
6	1.275	57.65	779.513	55.19
7	1.286	104.54	779.200	50.88
8	1.309	141.87	778.553	48.02
9	1.311	214.51	778.500	43.49
10	1.312	315.42	778.433	38.80
11	1.300	414.74	778.807	35.37
12	1.314	517.33	778.400	32.62
13	10.545	15.21	501.520	58.54
14	10.391	30.95	506.360	56.01
15	10.371	47.56	507.000	53.62
16	10.382	80.28	506.647	49.55
17	10.383	116.34	506.600	45.87
18	10.369	166.07	507.047	41.84
19	10.371	248.97	507.000	36.86
20	10.385	331.20	506.533	33.33
21	10.387	415.59	506.500	30.59
22	20.590	12.59	180.367	57.50
23	20.468	25.50	184.273	54.54
24	20.455	40.04	184.720	51.64
25	20.423	64.81	185.747	47.56
26	20.420	92.30	185.847	43.87
27	20.414	134.06	186.007	39.52
28	20.399	198.57	186.500	34.73
29	20.397	264.58	186.600	31.25
30	20.396	332.62	186.587	28.62
31	30.531	10.58	-133.400	56.45
32	30.547	21.44	-133.907	53.09
33	30.556	32.66	-134.180	50.14
34	30.567	53.79	-134.520	45.59
35	30.574	76.25	-134.713	41.79
36	30.580	110.09	-134.900	37.45
37	30.576	163.10	-134.800	32.72
38	30.582	216.46	-134.980	29.43
39	30.592	273.31	-135.300	26.90

Certificate no: 4831_466_00237803
Foil batch no: 1206EM


Product: 4831
Calibration date: 03.03.2025

Serial no: 466
Page 2 of 2


Giving these coefficients

Index	0	1	2	3	4	5	6
SVUFoilCoef	2.56095E-03	1.06119E-04	2.34867E-06	1.82326E02	-2.13730E-01	-4.21413E01	3.61801E00
TempCoef	2.62343E01	-3.17102E-02	3.10947E-06	-4.49854E-09	0.00000E00	0.00000E00	

Oxygen validation

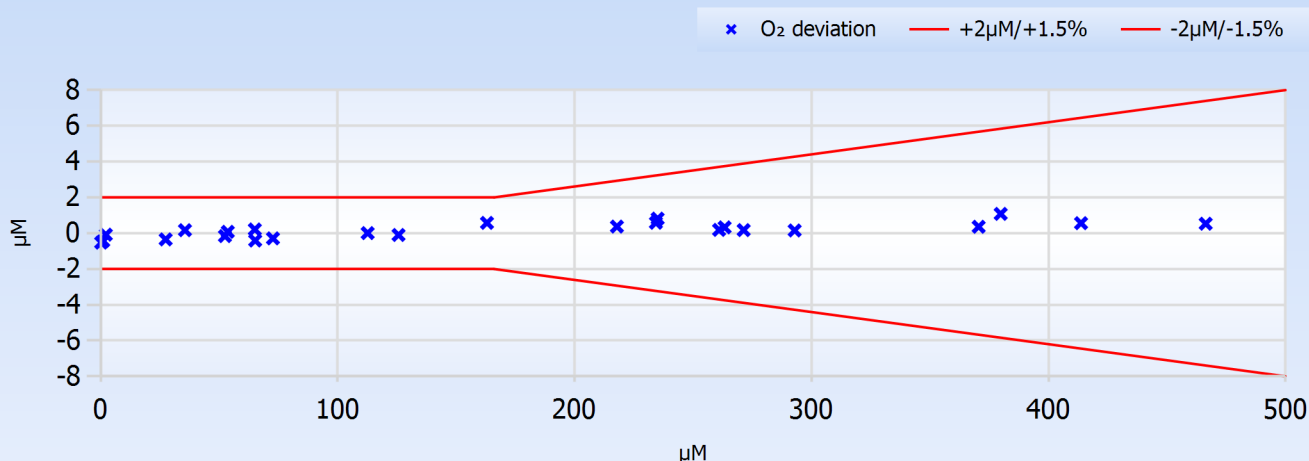

Temperature validation

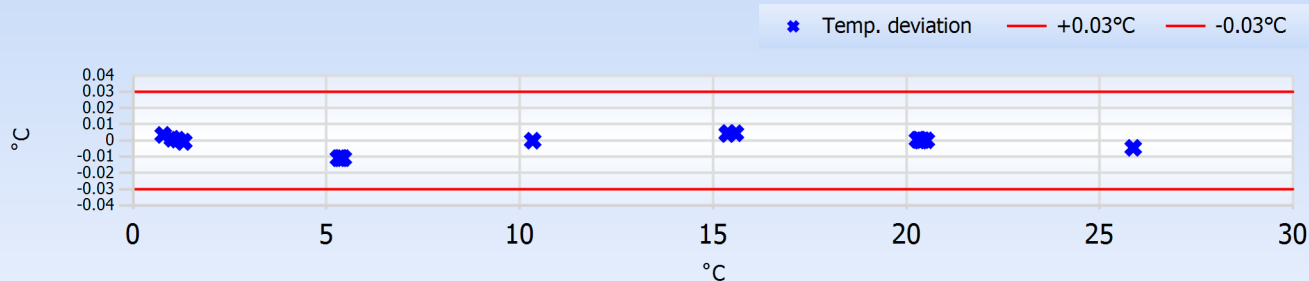

With following settings

Index	0	1	2	3
PhaseCoef	0.00000E00	1.00000E00	0.00000E00	0.00000E00

Index	0 (Offset)	1 (Slope)
ConcCoef	0.00000E00	1.00000E00
Salinity	0.00	

Firmware Version	5.3.1
------------------	-------

Date:03.03.2025

Tor-Ove Kvalvaag
Tor-Ove Kvalvaag, Calibration Engineer