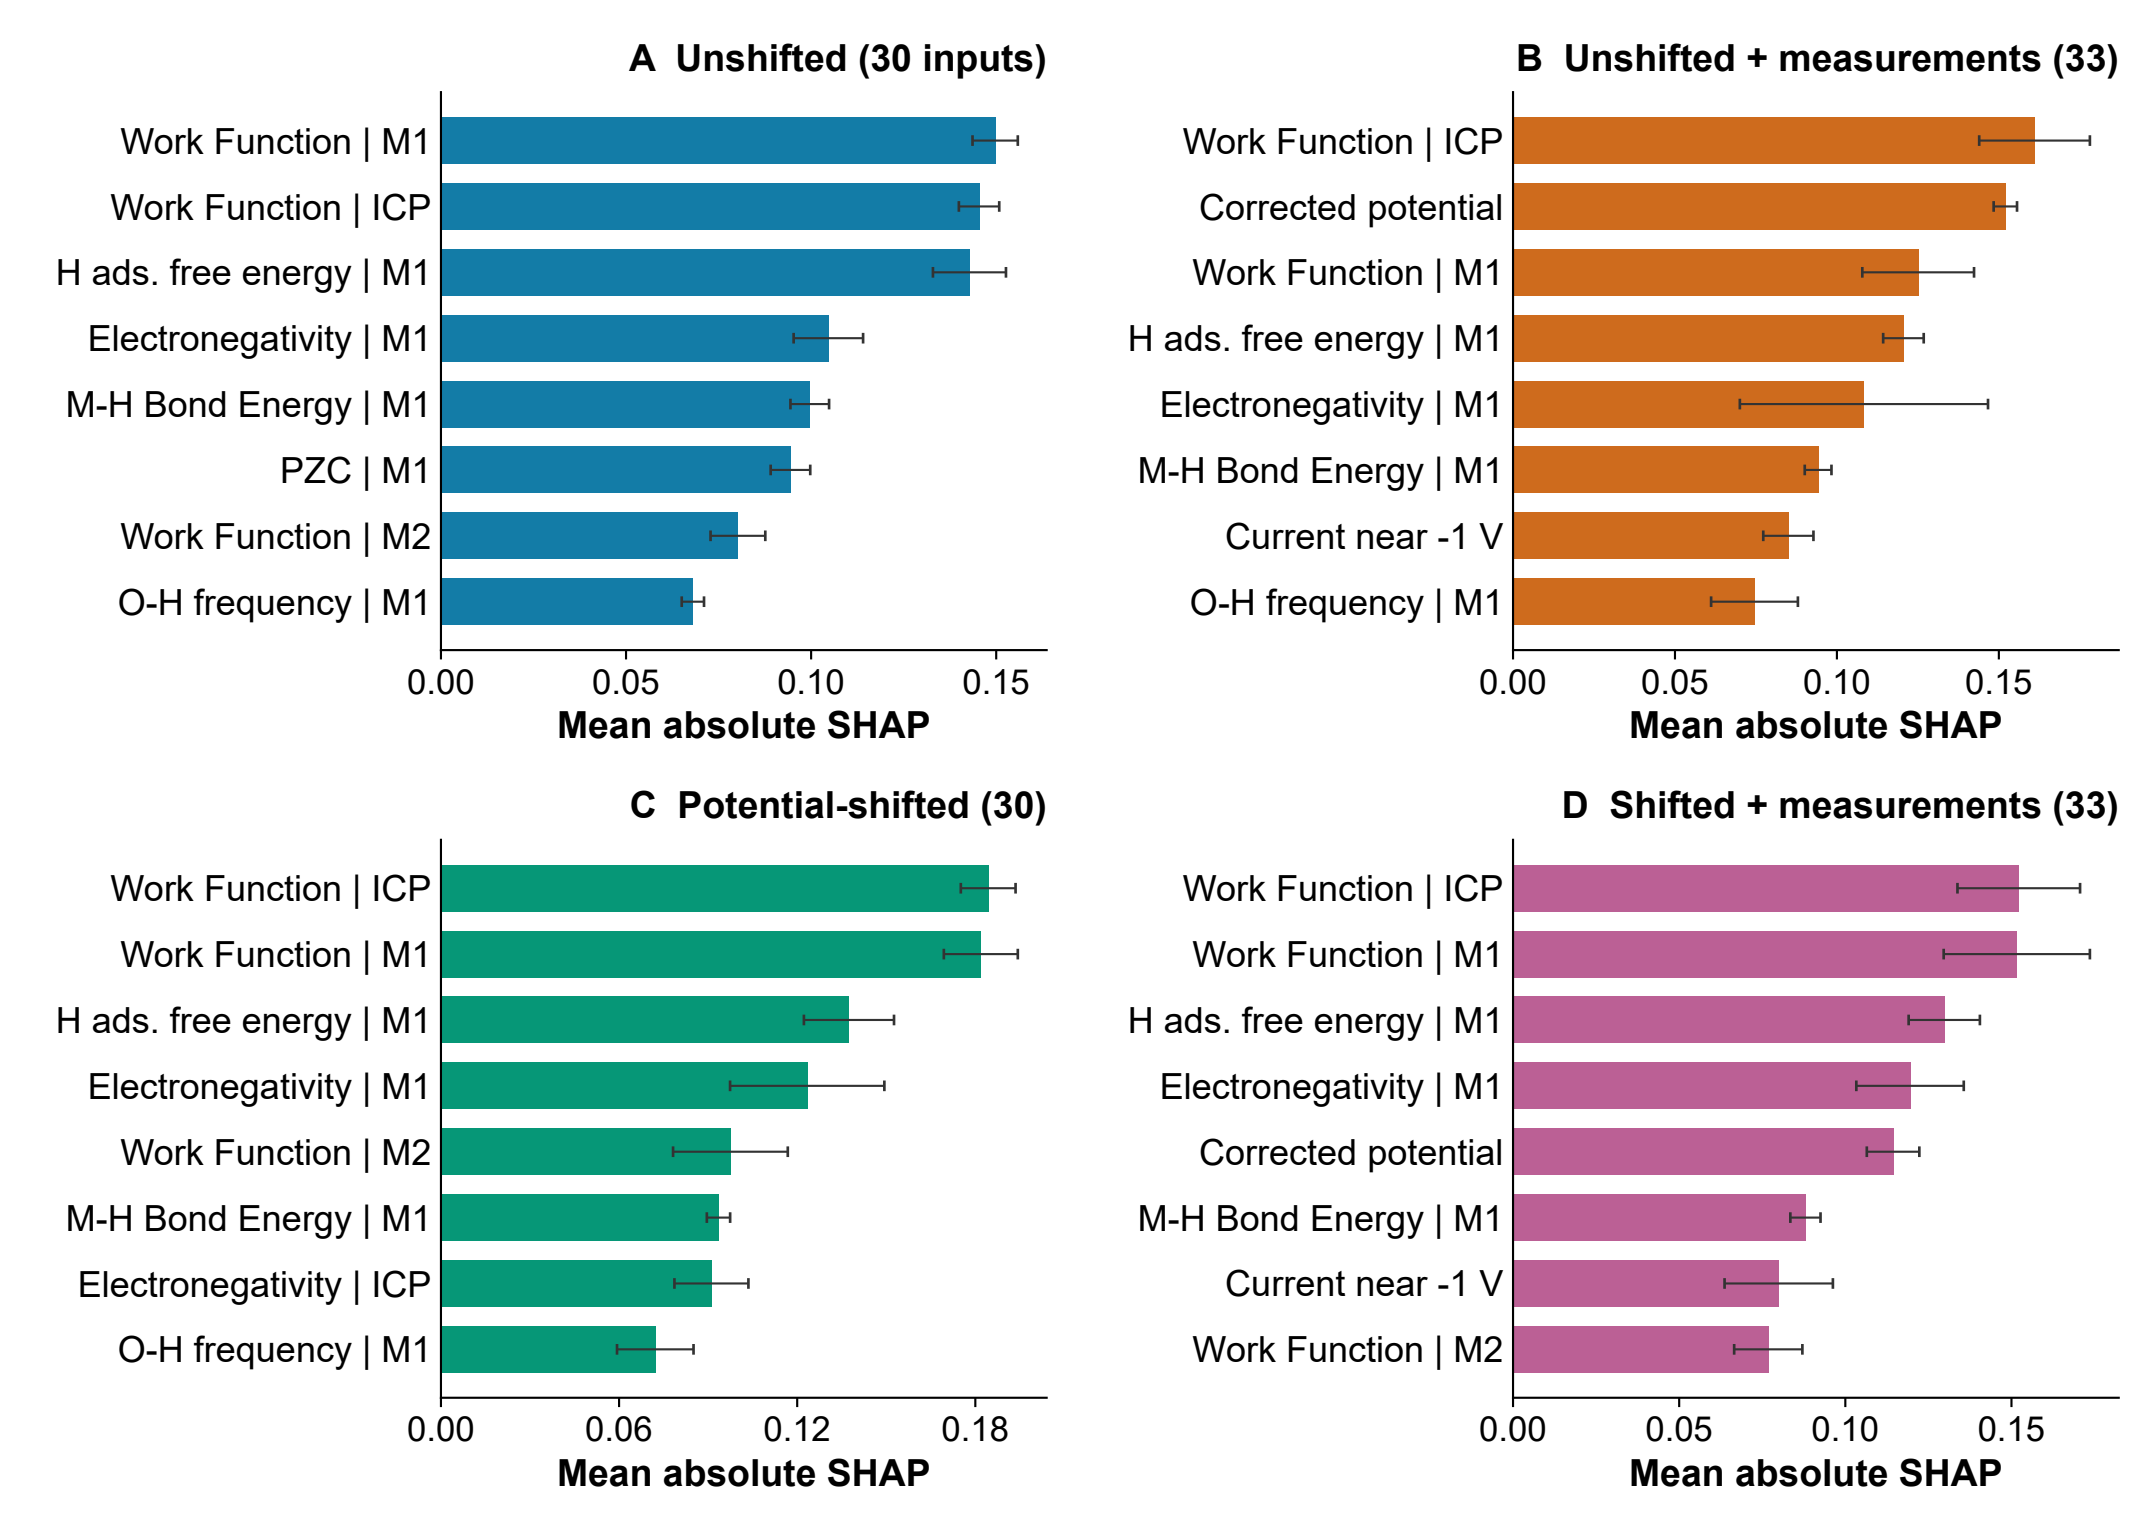
A Unshifted (30 inputs)
Work Function | M1
Work Function | ICP
H ads. free energy | M1
Electronegativity | M1
M-H Bond Energy | M1
PZC | M1
Work Function | M2
O-H frequency | M1
0.00
0.05
0.10
0.15
Mean absolute SHAP
B Unshifted + measurements (33)
Work Function | ICP
Corrected potential
Work Function | M1
H ads. free energy | M1
Electronegativity | M1
M-H Bond Energy | M1
Current near -1 V
O-H frequency | M1
0.00
0.05
0.10
0.15
Mean absolute SHAP
C Potential-shifted (30)
Work Function | ICP
Work Function | M1
H ads. free energy | M1
Electronegativity | M1
Work Function | M2
M-H Bond Energy | M1
Electronegativity | ICP
O-H frequency | M1
0.00
0.06
0.12
0.18
Mean absolute SHAP
D Shifted + measurements (33)
Work Function | ICP
Work Function | M1
H ads. free energy | M1
Electronegativity | M1
Corrected potential
M-H Bond Energy | M1
Current near -1 V
Work Function | M2
0.00
0.05
0.10
0.15
Mean absolute SHAP