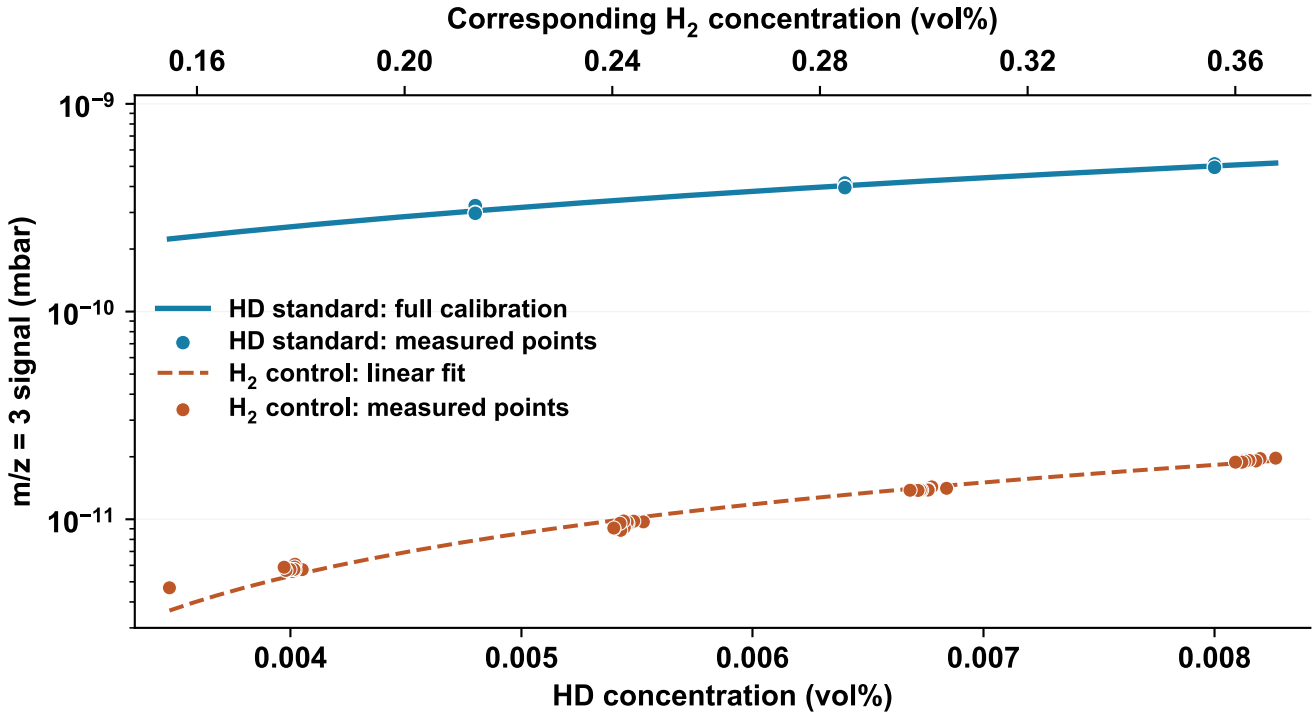

Corresponding H_2 concentration (vol%)
0.16
0.20
0.24
0.28
0.32
0.36
10^{-9}
10^{-10}
10^{-11}
m/z = 3 signal (mbar)
HD standard: full calibration
HD standard: measured points
H_2 control: linear fit
H_2 control: measured points
0.004
0.005
0.006
0.007
0.008
HD concentration (vol%)