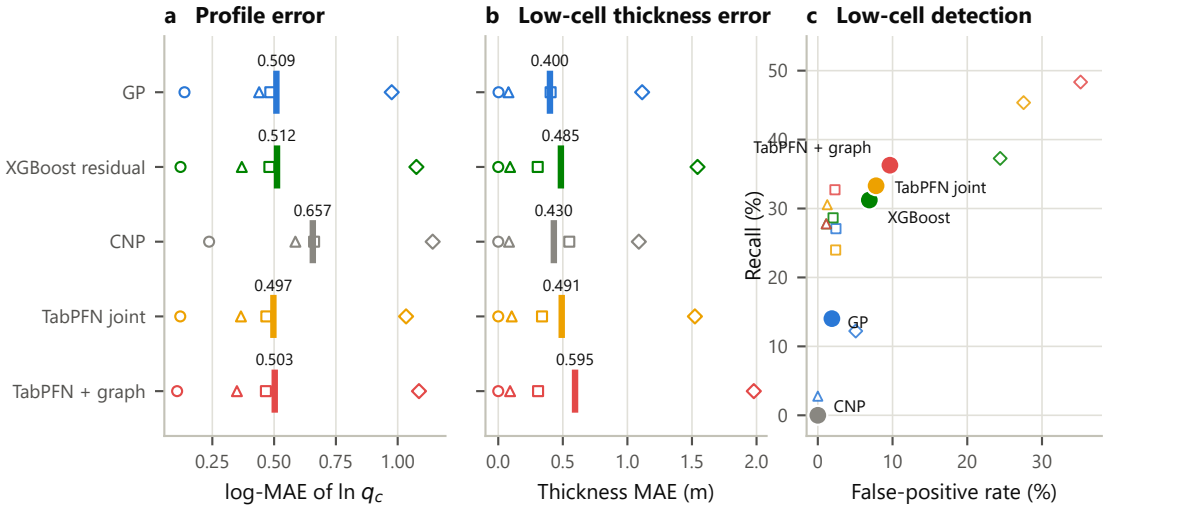
a Profile error
b Low-cell thickness error
c Low-cell detection
GP
XGBoost residual
CNP
TabPFN joint
TabPFN + graph
0.509
0.512
0.657
0.497
0.503
0.400
0.485
0.430
0.491
0.595
0.25
0.50
0.75
1.00
log-MAE of ln q_c
0.0
0.5
1.0
1.5
2.0
Thickness MAE (m)
Recall (%)
False-positive rate (%)
0
10
20
30
40
50
TabPFN + graph
TabPFN joint
XGBoost
GP
CNP
Wellington Airport
Christchurch Stadium
Hollywood
New Lock Terneuzen
Equal-site mean (filled circle in c)