



Parameter sensitivity

Independent test evaluation around the validation-selected setting: $T = 1.3$ and $\alpha = 0.8$.

Semantic-message strength

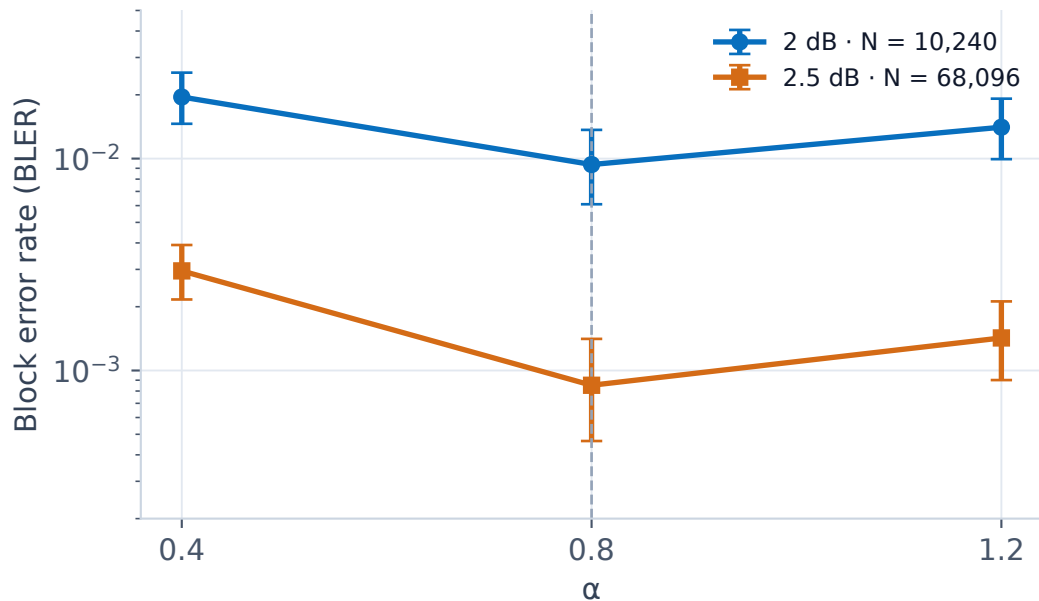

Posterior temperature

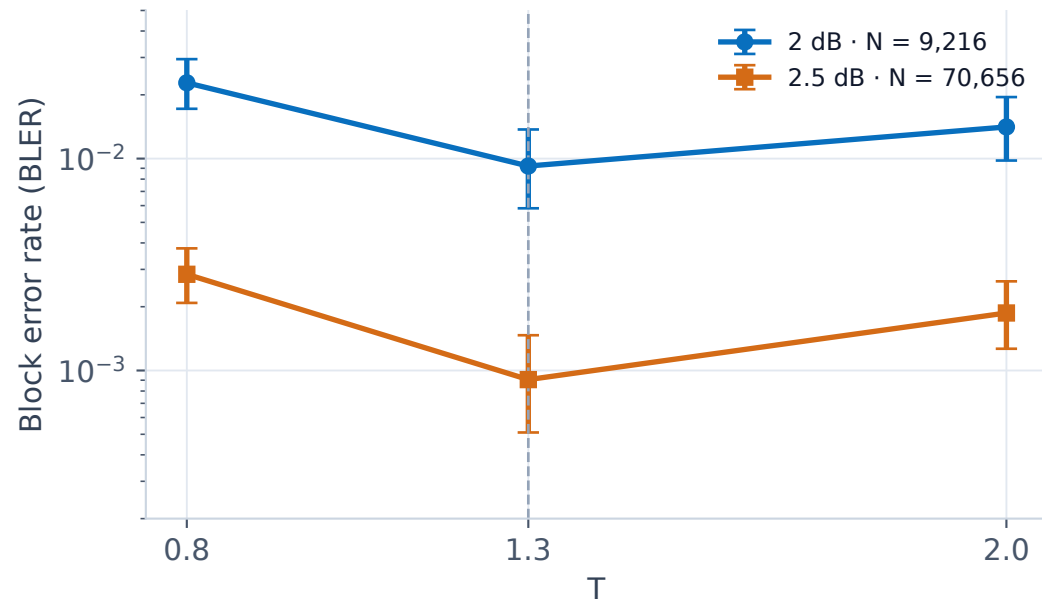

Bars: per-point 95% confidence sequences. Each sweep uses its own common prefix; the reference BLER differs between panels.