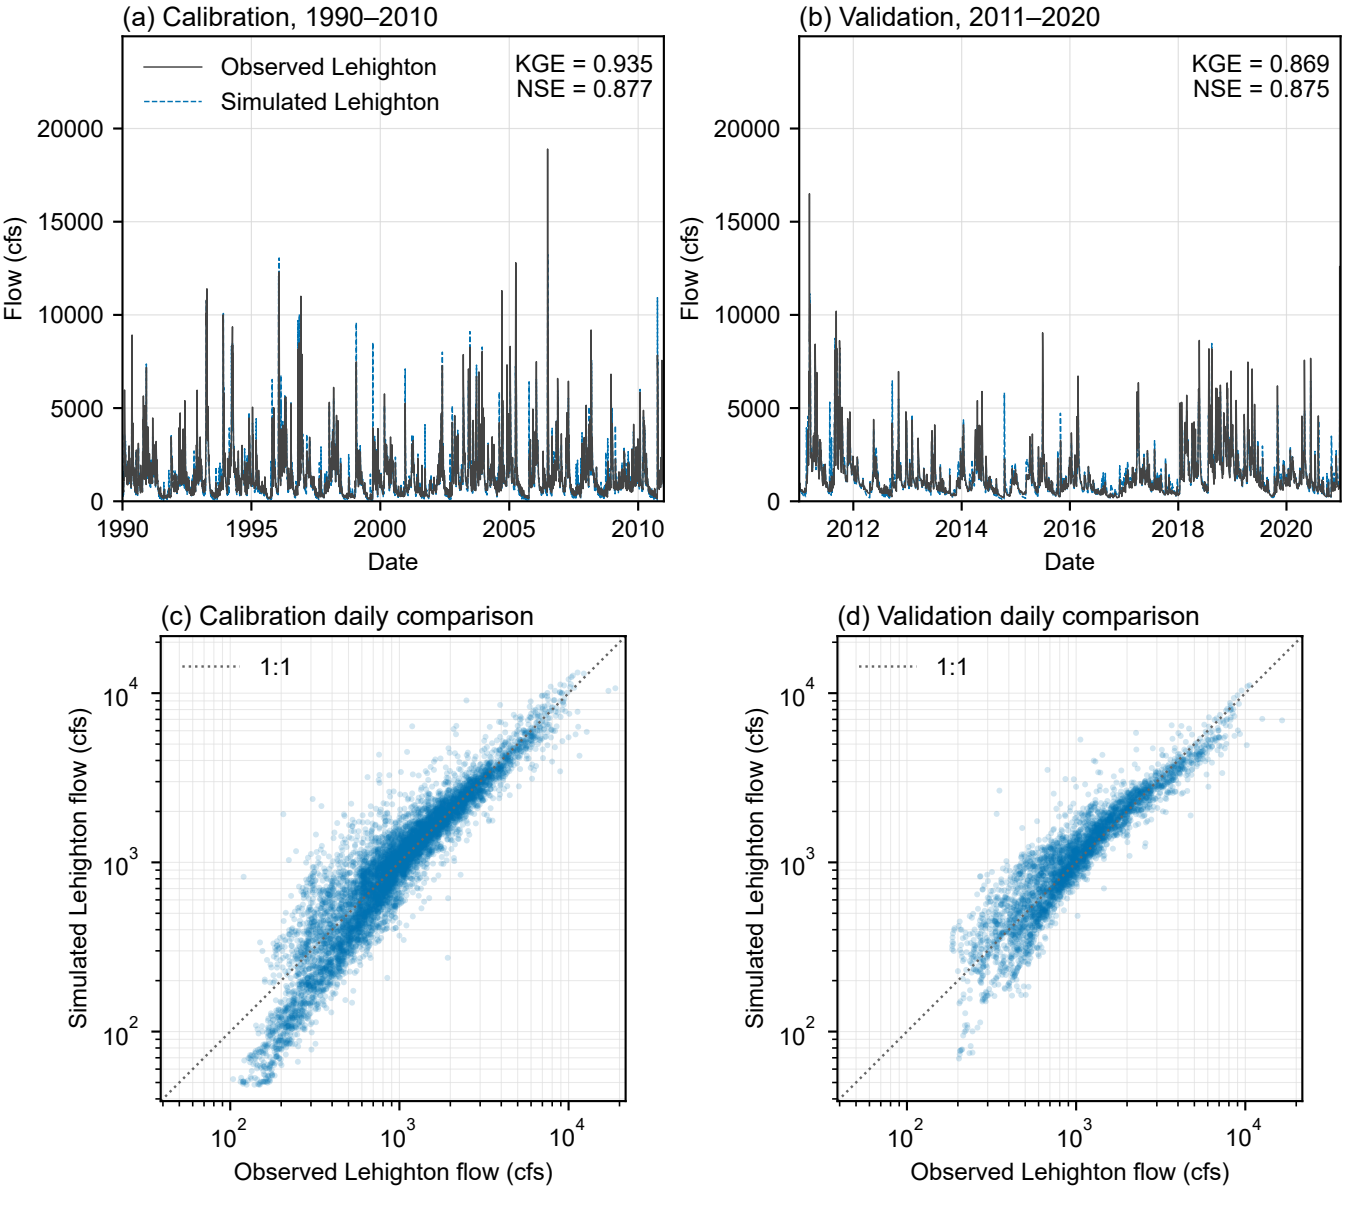

(a) Calibration, 1990–2010
Observed Lehighton
Simulated Lehighton
KGE = 0.935
NSE = 0.877
Flow (cfs)
Date
(b) Validation, 2011–2020
KGE = 0.869
NSE = 0.875
Flow (cfs)
Date
(c) Calibration daily comparison
1:1
Simulated Lehighton flow (cfs)
Observed Lehighton flow (cfs)
(d) Validation daily comparison
1:1
Simulated Lehighton flow (cfs)
Observed Lehighton flow (cfs)