ICONLITE Workshop 2026

From Sample to Species

Amplicon Sequencing Using Oxford Nanopore Technology

Companion Laboratory and Bioinformatics Handbook

Native Barcoding Kit 24 V14 (SQK-NBD114.24) · PromethION · EPI2ME wf-16s

Version 1.0 · 9 November 2026

> **Educational companion.** *The current Oxford Nanopore Technologies protocol remains the controlling reference for any actual laboratory work. For research use only.*

Table of Contents

About This Handbook

How to Use This Handbook
Learning Objectives

Part A – Scientific Foundations

Chapter 1. Introduction and Core Biological Questions
Chapter 2. Scientific Rationale
Chapter 3. Sequencing Strategies
Chapter 4. Marker Selection and Primer Design
4.1 Bacterial and Archaeal Ribosomal Markers (16S rRNA and 16S–23S Operon)
4.2 Fungal Ribosomal Markers (ITS1, 5.8S, ITS2, and 28S)
4.3 Eukaryotic and Microeukaryotic Markers (18S rRNA)
4.4 Animal and Metazoan Markers (Mitochondrial COI)
4.5 Vertebrate and Fish eDNA Markers (Mitochondrial 12S rRNA)
4.6 Plant Metabarcoding Markers (Chloroplast trnL)
Chapter 5. Sequencing Platform Selection
Chapter 6. Nanopore Sequencing Principles and Basecalling
6.1 Biophysical Mechanism of Nanopore Sensing
6.2 Pore Architecture: Evolution from R9.4.1 to R10.4.1 Dual Reader Heads
6.3 Neural Network Basecalling: Decoding Raw Ionic Currents into Nucleotides
Chapter 7. ONT Instrumentation and Experimental Planning

Part B – ONT Laboratory Workflow

Chapter 8. Laboratory Workflow Overview
Chapter 9. Native Barcoding Kit V14 Guided Practical
9.1 Preparing and Evaluating PCR Amplicons
9.2 End-Preparation: Preparing DNA for Ligation
9.3 Native Barcode Ligation and Sample Multiplexing
9.4 Sequencing Adapter Ligation and Final Library Clean-up
9.5 Priming and Loading the PromethION Flow Cell
9.6 MinKNOW Run Configuration and Data Generation
9.7 From FASTQ to Biological Interpretation (`wf-16s` Walkthrough)
9.8 Guided Practical Checkpoint: Five Critical Decisions (H8)

Part C – Bioinformatics

Chapter 10. Nanopore Data Formats and Basecalling
Chapter 11. Quality Control and Taxonomic Assignment
Chapter 12. Community Visualization and Interpretation
Chapter 13. Predictive Functional Profiling (PICRUSt2 and FUNGuild)

Part D – Critical Evaluation and Synthesis

Chapter 14. Limitations and Troubleshooting
Chapter 15. Summary, Synthesis and Further Reading

Appendices

Appendix A. Reagent and Consumables Checklist
Appendix B. Barcode Assignment and Sample-Tracking Template
Appendix C. DNA Mass-to-Molarity Calculation Worksheet
Appendix D. Library Preparation Workflow Checklist
Appendix E. Flow Cell Loading Checklist
Appendix F. FASTQ and Taxonomic Result Interpretation Guide

Appendix G. Glossary
Appendix H. References and Software/Version Register

About This Handbook

This handbook is designed as a practical learning resource and reference guide for long-read amplicon sequencing using Oxford Nanopore Technologies (ONT). It explains the underlying scientific and biophysical mechanisms, detailed laboratory protocols, stoichiometric calculations, quality-control checkpoints, bioinformatic workflows, and ecological data interpretation.

How to Use This Handbook

- Procedural steps and parameters are cross-referenced with official protocol specifications and established molecular literature.
- Crucial warnings highlight failure modes where errors (such as detergent/ethanol carryover or air bubbles) cause irreversible pore loss or library failure.
- Core biological questions structure each stage of experimental design and analysis: **Who is there? What might they be doing? Why is it necessary to know them?**

Table 1. Source-status tags used throughout

Tag	Meaning
`[MFR]`	Procedure or value stated in the manufacturer protocol (ONT `SQK-NBD114.24`, PromethION, rev. NBA_9168_v114_revU_15Jul2026) or in EPI2ME `wf-16s` documentation
`[ADAPT]`	A reasonable adaptation not stated by the manufacturer; confirm before relying on it
`[EX]`	Conceptual or hypothetical worked example; not experimental data
`[LAB]`	Laboratory-specific practice that depends on equipment, workflow preferences, and local optimization

Learning Objectives

1. Distinguish DNA barcoding, metabarcoding, and shotgun metagenomics across experimental aims.
2. Select appropriate molecular markers and primer systems suited to specific taxonomic groups and fragment preservation states.
3. Understand the biophysical principles of nanopore sensing, R10.4.1 dual-reader head pore geometry, and neural network basecalling.
4. Master each operational phase of PCR amplicon verification, end-repair/dA-tailing, native barcode ligation, multiplex pooling, adapter attachment, and PromethION flow cell loading.
5. Trace the computational lifecycle of sequencing data from raw ionic currents (POD5) through basecalling, quality filtering, demultiplexing, and taxonomic assignment.
6. Critically evaluate community composition plots, diversity metrics, and potential artifacts arising from PCR bias, copy number variation, contamination, and reference database limitations.

Part A – Scientific Foundations

Chapter 1. Introduction and Core Biological Questions

A natural or clinical sample contains DNA from every biological entity present in or shed into that environment. Amplicon sequencing selects a phylogenetically informative marker gene, amplifies it through targeted PCR, sequences the amplified copies, and matches each read against curated reference databases.

Rather than treating sequencing as a black-box instrument run, rigorous experimental design addresses three fundamental ecological questions at every stage of the workflow:

7. **Who is there?**

Which organisms, lineages, taxa, or strains constitute the biological community? Amplicon sequencing provides a culture-independent census of community membership, detecting rare, unculturable, fastidious, or cryptic organisms that traditional visual or plating methods overlook.

8. **What might they be doing?**

What ecological roles, physiological capacities, or functional guilds do these taxa represent? While amplicon markers sequence phylogenetic labels rather than metabolic gene suites, high-resolution taxonomic identification (especially at genus and species rank) allows researchers to link detected community members to well-characterized metabolic traits—such as nitrogen fixation, sulfate reduction, organic matter decomposition, secondary metabolite biosynthesis, or pathogenicity.

9. **Why is it necessary to know them?**

Why does understanding community composition matter for environmental monitoring, industry, or public health? Characterizing microbial and macrobial assemblages reveals ecological health, bioindicators of pollution or recovery, shifts triggered by climate stress or anthropogenic disturbance, infectious outbreak dynamics, aquaculture pathogen reservoirs, and invasive species encroachment.

> Think of a molecular marker as a diagnostic barcode sequence naturally carried by every organism. PCR photocopies these barcodes millions of times, the nanopore reader decodes each single molecule in real time, and bioinformatics software classifies the resulting sequence against reference libraries to reveal community structure.

> Every physical and bioinformatic stage functions as a selective filter: cell lysis and DNA extraction recovery, primer annealing efficiency, PCR cycle kinetics, bead cleanup size retention, adapter ligation efficiency, flow cell translocation speed, neural network basecaller calibration, read quality thresholds, and reference database currency. The final taxonomic table reflects the combined product of all these factors; results must always be interpreted critically in light of experimental controls.

Chapter 2. Scientific Rationale

Traditional culture-based microbiology identifies only those organisms capable of growing on chosen synthetic media under specific incubation temperatures, oxygen tensions, and nutrient balances. In natural soil, freshwater, marine, and host-associated microbiomes, fewer than 1% of microbial species are readily culturable in isolation ("the great plate count anomaly"). Similarly, morphological identification of mixed larval, insect, or fungal samples requires rare taxonomic expertise and frequently fails for cryptic life stages or degraded specimens.

Targeted amplicon sequencing overcomes these bottlenecks by bypassing organism cultivation altogether. It recovers DNA directly from complex matrices, scales to multiplex dozens of samples simultaneously, and provides high sensitivity for low-abundance taxa.

Table 2. What each approach can and cannot tell you

Approach	Answers	Misses
Culture-based Plating	What grows under given conditions; yields viable isolates for physiology and antibiotic susceptibility assays	Unculturable, fastidious, slow-growing, or dormant organisms; introduces strong medium-dependent bias
Targeted Molecular ID (Isolates)	Precise species confirmation for a single isolated specimen or colony	Cannot profile mixed communities in a single reaction; blind to taxa outside primer binding sites
Amplicon Metabarcoding	High-throughput community composition across mixed environmental or clinical samples	Does not prove cell viability or metabolic activity; relative sequence abundance does not strictly equal cell count

> Culture reports only organisms capable of growing under specific laboratory conditions and media, whereas amplicon sequencing recovers marker sequences amplified directly from sample DNA regardless of culturability. The two approaches are complementary and often combined in modern microbiology.

Chapter 3. Sequencing Strategies

Table 3. Three related molecular strategies

Feature	DNA Barcoding	DNA Metabarcoding	Shotgun Metagenomics
Primary Question	What is the species identity of this isolated organism?	Who is present across this complex, mixed biological community?	Who is present, and what full metabolic and functional gene repertoire do they carry?
Sample Input	DNA extracted from a single specimen, tissue punch, or pure culture	Mixed environmental DNA (eDNA), soil, stool, water, biofilm, or tissue blend	Total metagenomic DNA extracted directly from mixed environmental or host samples
Target DNA	Single targeted marker amplicon (e.g. full-length 16S, COI, or ITS)	Targeted PCR amplicons generated from mixed templates using universal primers	Untargeted, whole-genome shearing and sequencing of all recoverable DNA fragments
Major Strengths	Highly cost-effective; clean Sanger or long-read consensus; clear taxonomic resolution	Multiplexes dozens to hundreds of samples; highly sensitive to rare taxa at modest sequencing depth	Captures viruses, plasmids, novel lineages lacking primer sites, and complete functional metabolic pathways
Key Limitations	Restricted to one isolated specimen per reaction; fails on mixed community mixtures	Subject to primer binding bias, PCR chimera formation, and marker-length resolution limits	Substantially higher sequencing cost; host DNA often dominates reads; computationally demanding assembly

A practical rule of thumb:

- To identify a single organism, pure isolate, or morphological specimen: **DNA barcoding**.

- To census community membership, monitor biodiversity shifts, or compare hundreds of water, soil, or gut samples: **DNA metabarcoding**.
- To discover novel enzymes, assess antimicrobial resistance gene suites, or reconstruct uncultured metagenome-assembled genomes (MAGs): **Shotgun metagenomics**.

Chapter 4. Marker Selection and Primer Design

Selecting the proper molecular marker dictates the taxonomic breadth and phylogenetic resolution of an amplicon study. An ideal marker gene features two indispensable attributes:

10. **Highly conserved flanking regions** where universal PCR primers can bind across broad taxonomic domains without mismatched dropout.
11. **Internal hypervariable regions** that accumulate sufficient nucleotide divergence to discriminate distinct species or genera.

Table 4. Common amplicon markers across domains

Marker	Target Domain	Typical Amplicon Length	Taxonomic Utility and Caveats
16S rRNA	Bacteria, Archaea	Variable regions (300–450 bp) or full-length (~1,500 bp)	Standard bacterial census; nine variable regions (V1–V9); gene copy number varies between 1 and >15 per genome
16S–23S Operon (rRNA)	Bacteria	~4,500 bp (spans 16S, ITS spacer, 23S)	Unlocks high-confidence species- and strain-level resolution using long reads; requires high-molecular-weight DNA
ITS1 / ITS2 / Full ITS	Fungi	Variable (300–800 bp) or full operon (~2.5 kb)	Primary fungal barcode; multi-copy; high length variability induces PCR size bias; challenging global sequence alignment
18S rRNA	Eukaryotes, Protists	Short variable domains or full-length (~1,800 bp)	Broad eukaryotic surveillance; hypervariable V4 and V9 regions resolve major clades; limited species resolution in some groups
Mitochondrial COI	Animals, Invertebrates	Standard Folmer (~658 bp) or Leray mini-barcode (~313 bp)	Standard animal barcode; high interspecific divergence; primer mismatches common in non-model marine invertebrates
Mitochondrial 12S rRNA	Vertebrates, Fishes	Short fragments (~163–185 bp, e.g. MiFish)	Gold standard for aquatic vertebrate eDNA; recovers degraded DNA; short length limits discrimination of sister species

Marker	Target Domain	Typical Amplicon Length	Taxonomic Utility and Caveats
Chloroplast trnL (UAA)	Plants	P6 loop (~10–143 bp) or c/d intron (~400–600 bp)	Plant metabarcoding and ancient DNA; P6 loop amplifies exceptionally well in degraded herbivore diet and soil samples

4.1 Bacterial and Archaeal Ribosomal Markers (16S rRNA and 16S–23S Operon)

The 16S rRNA gene (~1,542 bp in *E. coli*) consists of nine hypervariable regions (V1 through V9) interspersed between conserved structural stems. Traditional short-read platforms typically sequence isolated sub-regions, such as V3–V4 (primers 341F / 805R, ~464 bp) or V4 (primers 515F / 806R, ~291 bp). While these short segments profile family- and genus-level community dynamics, they frequently lack sufficient nucleotide divergence to differentiate closely related pathogenic and commensal species (e.g. distinguishing *Bacillus anthracis* from *Bacillus cereus*, or *Escherichia coli* from *Shigella* species).

Furthermore, bacterial genomes exhibit substantial 16S rRNA gene copy number variation. As documented in the rrnDB v5 database (Stoddard et al. 2015), bacterial genomes carry between 1 and 21 copies of the 16S gene, with some spore-forming bacilli (such as *Metabacillus*) exhibiting medians up to 19 copies. Additionally, intragenomic 16S divergence—where distinct operons within the same single bacterial chromosome carry divergent nucleotide sequences—can generate multiple distinct sequence variants from a clonal isolate. Researchers must account for copy number heterogeneity when interpreting sequence abundances.

Nanopore sequencing enables full-length 16S sequencing (~1.5 kb) using classical primers 27F (`AGAGTTTGATCMTGGCTCAG`) and 1492R (`GGTTACCTTGTTACGACTT`). By capturing all nine variable regions in individual continuous reads, long-read sequencing significantly refines taxonomic classification to species rank.

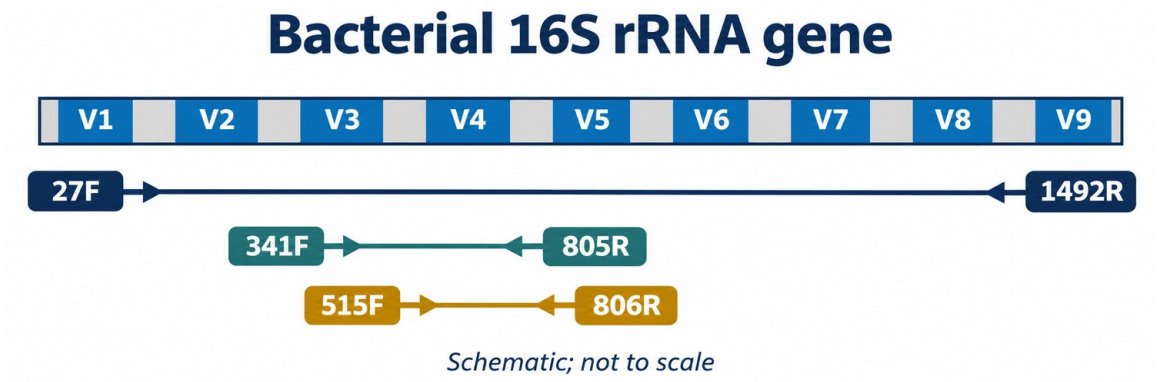


Figure 4.1. Organization of the bacterial 16S rRNA gene showing hypervariable regions V1–V9 and typical primer binding sites for full-length (27F/1492R) and short-read amplicons (341F/805R and 515F/806R).

Where even full-length 16S fails to separate closely related strains, nanopore sequencing can target the entire bacterial ribosomal operon (~4.5 kb), amplifying continuously from the 5′ end of 16S, across the internal transcribed spacer (ITS) containing tRNA genes, and through the 23S rRNA gene using primers 27F and 23SR.

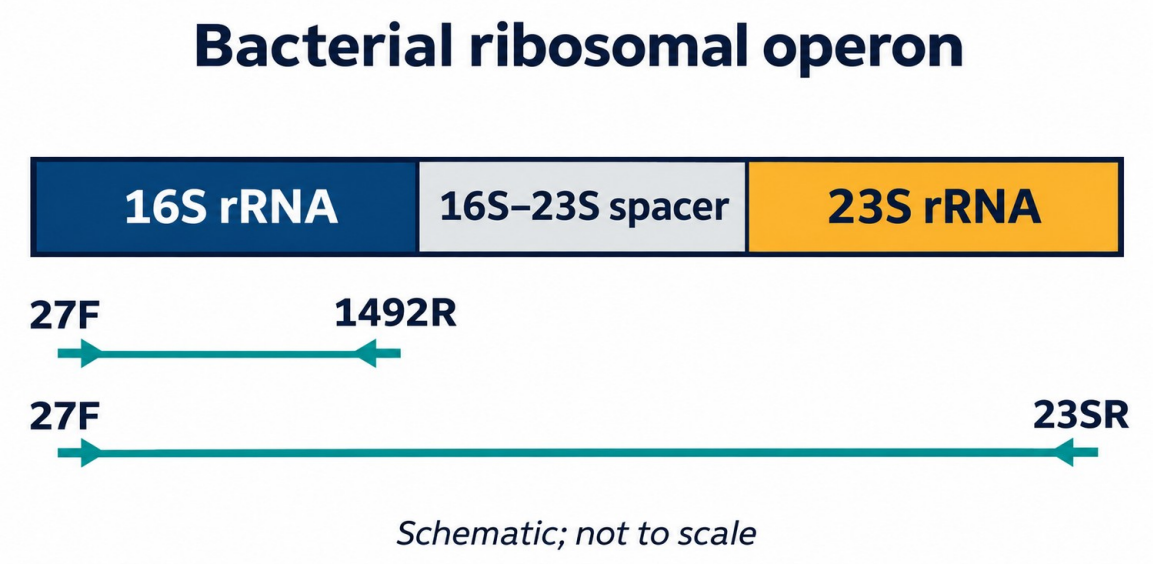


Figure 4.2. Schematic of the full bacterial ribosomal RNA operon (16S–ITS–23S) showing the extended target spanned by long-read amplicons for strain-level discrimination.

4.2 Fungal Ribosomal Markers (ITS1, 5.8S, ITS2, and 28S)

The fungal nuclear ribosomal internal transcribed spacer (ITS) region is the formal universal barcode for Fungi (Schoch et al. 2012). The locus consists of the highly variable ITS1 and ITS2 spacers separated by the conserved 5.8S rRNA gene, flanked upstream by the 18S (SSU) gene and downstream by the 28S (LSU) gene.

Common sub-regional primers include:

- **ITS1F / ITS2:** Targets ITS1 alone (~300 bp).
- **ITS3 / ITS4:** Targets ITS2 alone (~350 bp).
- **ITS1F / ITS4:** Spans the complete ITS region (ITS1–5.8S–ITS2, ~600–800 bp).

Because fungal ITS spacers exhibit pronounced natural insertion/deletion length polymorphisms across taxonomic classes, short-read sequencing often suffers from severe amplification length bias (shorter fragments amplify exponentially faster than longer ones). Long-read nanopore sequencing easily accommodates length-variable amplicons and can extend across the adjacent D1/D2 hypervariable domains of the 28S LSU gene (~1.5–2.5 kb total), providing robust phylogenetic placement for previously unclassified fungi.

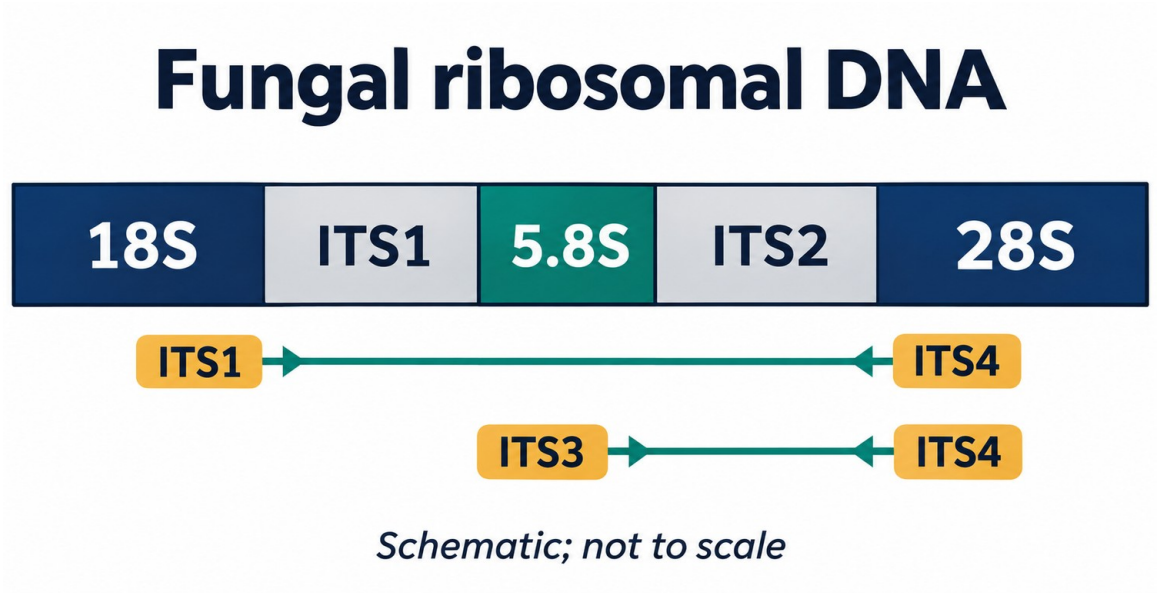


Figure 4.3. Full fungal ribosomal operon schematic showing the positioning of 18S, ITS1, 5.8S, ITS2, and 28S genes alongside universal primer pairs.

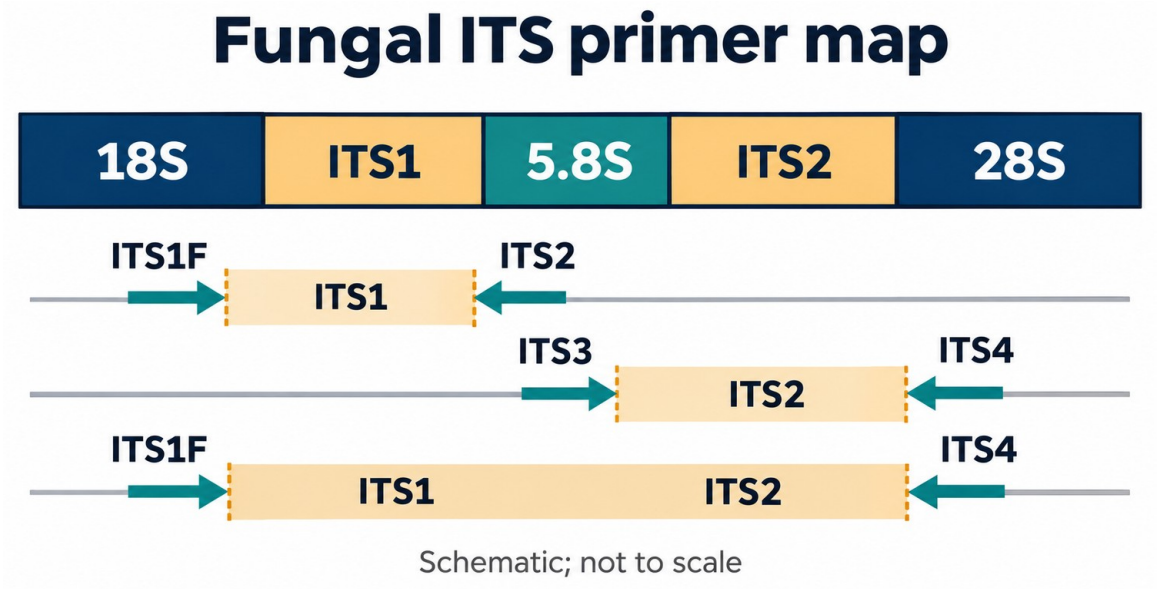


Figure 4.4. Detailed primer map across the fungal ITS region highlighting ITS1F, ITS2, ITS3, and ITS4 primer binding sites.

4.3 Eukaryotic and Microeukaryotic Markers (18S rRNA)

For broad eukaryotic biodiversity surveys—spanning unicellular protists, algae, fungi, and micro-invertebrates—the nuclear small subunit 18S rRNA gene (~1,800 bp) provides deep phylogenetic information. The 18S gene contains nine variable regions (V1–V9).

The V4 region (~380 bp, amplified with primers TAReuk454FWD1 / TAReukREV3) and V9 region (~130 bp, primers 1389F / 1510R) are standard choices for marine and freshwater plankton metabarcoding. Long-read nanopore amplicons spanning the near full-length 18S gene allow researchers to resolve divergent protistan clades that remain unclassified when sequenced over single short variable loops.

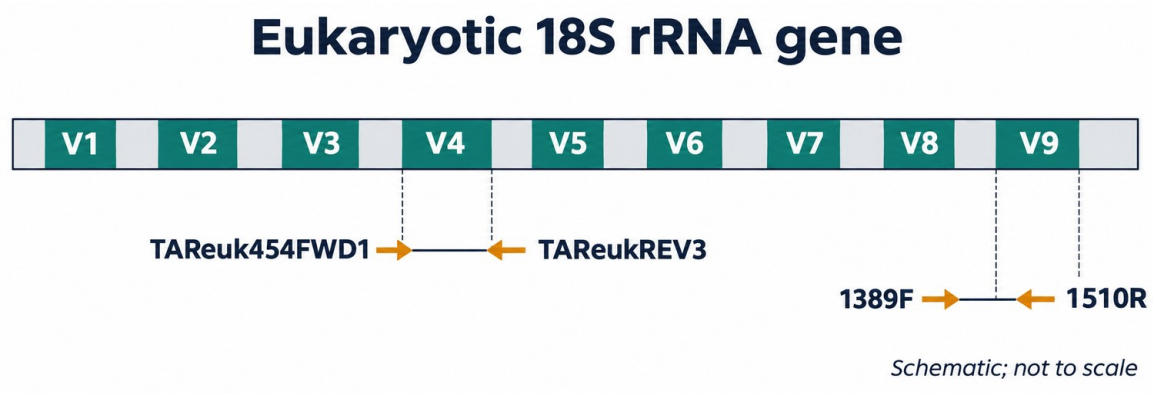


Figure 4.5. Eukaryotic 18S rRNA gene structure illustrating hypervariable regions V1–V9 and targets for universal eukaryotic primers.

4.4 Animal and Metazoan Markers (Mitochondrial COI)

Cytochrome *c* oxidase subunit I (COI) is the primary barcode for the animal kingdom (Hebert et al. 2003). The standard Folmer barcode region (~658 bp) is amplified using primers LCO1490 and HCO2198 (Folmer et al. 1994). Due to the degeneracy of universal primer binding sites across divergent invertebrate phyla, degenerate primer cocktails or internal mini-barcodes—such as the Leray fragment (~313 bp, amplified with mlCOIintF and jgHCO2198; Leray et al. 2013)—are widely deployed for marine benthic biodiversity and gut content metabarcoding.

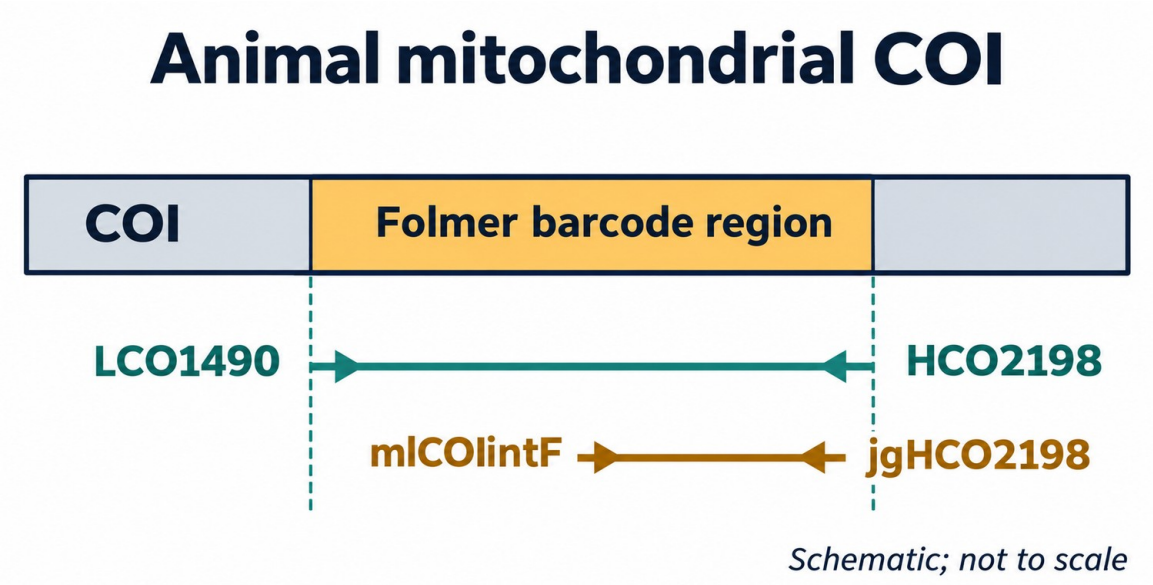


Figure 4.6. Mitochondrial COI gene showing the standard Folmer barcode region and the shorter Leray internal metabarcoding amplicon.

4.5 Vertebrate and Fish eDNA Markers (Mitochondrial 12S rRNA)

Environmental DNA (eDNA) shed into water columns by macro-organisms is typically fragmented into small segments (<300 bp) due to enzymatic, microbial, and photochemical degradation. For aquatic vertebrate and bony fish monitoring, the MiFish primer system (Miya et al. 2015) targets a hypervariable region of the mitochondrial 12S rRNA gene (~163–185 bp) using primers MiFish-U-F and MiFish-U-R.

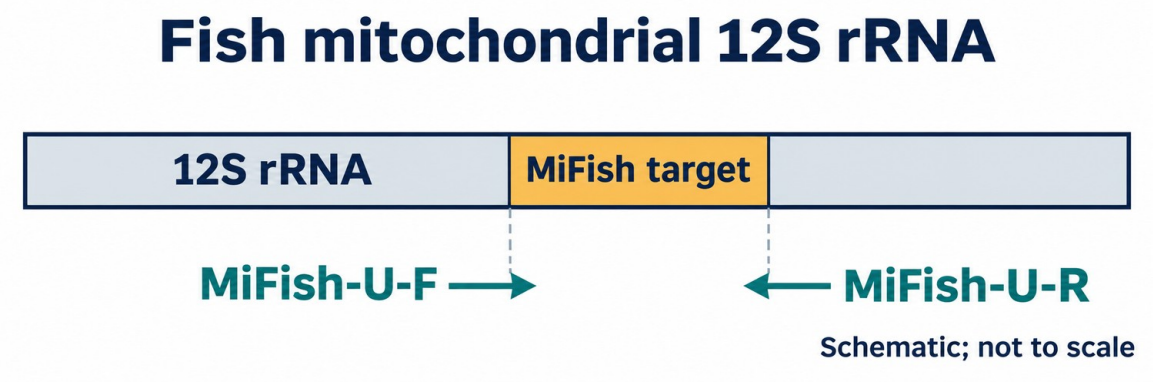


Figure 4.7. Vertebrate mitochondrial 12S rRNA gene schematic highlighting the short MiFish amplicon designed for aquatic eDNA biodiversity surveillance.

4.6 Plant Metabarcoding Markers (Chloroplast trnL)

For botanical community profiling, herbivore dietary analysis, and ancient sedimentary DNA, the chloroplast *trnL* (UAA) intron provides high taxonomic coverage across land plants. Taberlet et al. (2007) developed universal primers targeting the full *trnL* intron (primers c and d, ~400–600 bp) and the ultra-short internal P6 loop (primers g and h, 10–143 bp). The P6 loop's extreme brevity ensures robust amplification from heavily degraded DNA recovered from ancient permafrost cores, fossil faeces, and processed honey.

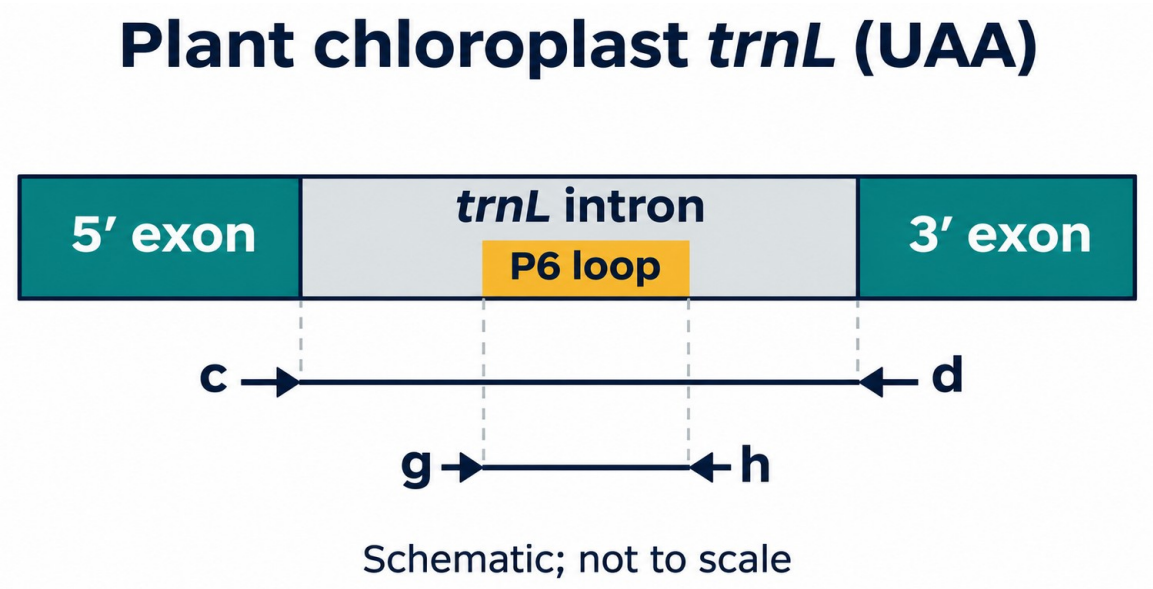


Figure 4.8. Chloroplast trnL gene locus showing the 5' and 3' exons, the full intron (primers c/d), and the ultra-short internal P6 loop (primers g/h).

Chapter 5. Sequencing Platform Selection

Table 5. Methodological trade-offs: short-read vs long-read amplicon sequencing

Analytical Criterion	Short-Read Amplicon Sequencing (e.g. Illumina MiSeq)	Long-Read Nanopore Sequencing (ONT PromethION / MinION)
Typical Target Length	250–500 bp (e.g. V3–V4 or V4 alone)	Full-length markers (1.5 kb 16S, 2.5 kb ITS-LSU, 4.5 kb operons)
Taxonomic Resolution	Often restricted to genus or family level; ambiguous species calls	Discriminates species and specific strains via complete variable suites

Analytical Criterion	Short-Read Amplicon Sequencing (e.g. Illumina MiSeq)	Long-Read Nanopore Sequencing (ONT PromethION / MinION)
Performance on Fragmented eDNA	Highly robust; excels at short degraded amplicons (<200 bp)	Excels on intact amplicons; short amplicons require altered bead ratios
Raw Per-Base Simplex Accuracy	>99.9% (Q30+)	>99% (Q20+) with R10.4.1 chemistry and latest Dorado basecallers
Run Turnaround and Flexibility	Rigid batch runs; hours to days before data access	Continuous real-time streaming; runs can be stopped once target depth is met
Compute & Pipeline	Denoising into Amplicon Sequence Variants (ASVs via DADA2)	Alignment (minimap2) or k-mer classification (Kraken2/Bracken)

Chapter 6. Nanopore Sequencing Principles and Basecalling

6.1 Biophysical Mechanism of Nanopore Sensing

Nanopore sequencing operates on an electro-physical measurement principle rather than sequencing-by-synthesis (SBS). A biological protein nanopore is embedded in a synthetic polymer membrane that exhibits high electrical resistance. The membrane separates two electrolyte-filled chambers (*cis* and *trans*). An applied voltage induces a steady ionic current of potassium (K^+) and chloride (Cl^-) ions through the central pore barrel.

A processive motor protein (derived from a helicase or polymerase), pre-loaded onto the sequencing adapter, docks at the pore opening on the *cis* side. Driven by the trans-membrane potential, the motor protein unwinds double-stranded DNA and steps single-stranded DNA through the pore lumen at a controlled velocity (~400 bases per second).

As nucleotides pass through the narrowest constriction of the pore (the reader head), they partially block the passage of ions. Because each base combination exhibits unique steric volume, spatial geometry, and electrical charge distribution, the electrical current fluctuates characteristically. High-bandwidth Application-Specific Integrated Circuit (ASIC) sensor arrays sample this ionic current thousands of times per second, recording a continuous current-versus-time trace (colloquially termed a "squiggle").

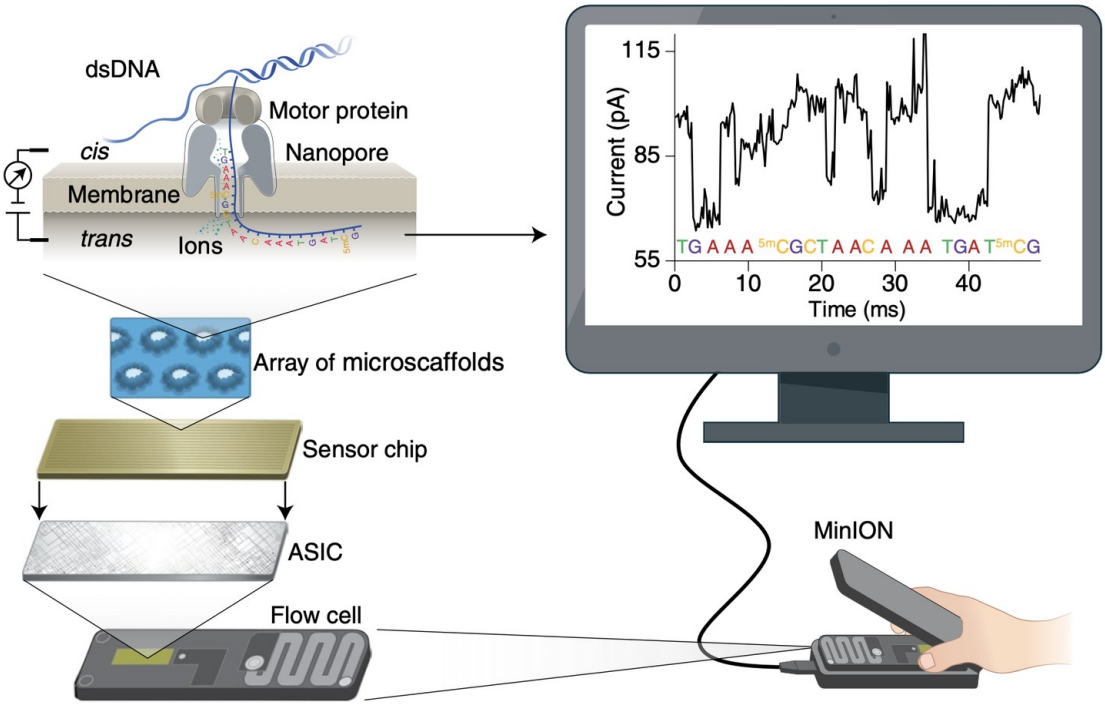


Figure 6.1. Comprehensive overview of nanopore sequencing architecture showing DNA translocation, the motor protein, sensor chip ASIC arrays, flow cell design, and real-time ionic current recording (from Wang et al. 2021).

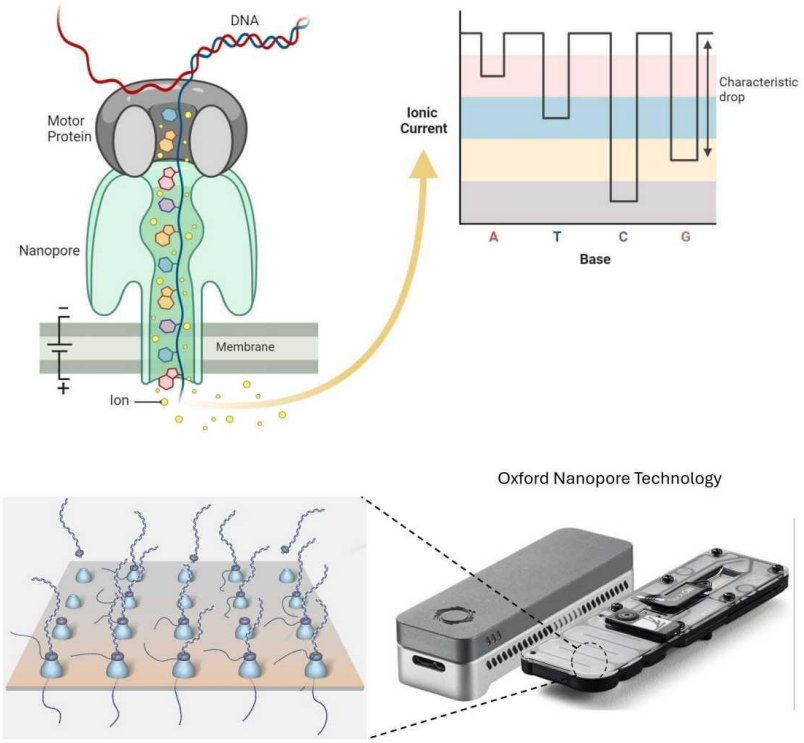


Figure 6.2. Physical schematic of single-molecule strand translocation through a biological nanopore membrane under constant voltage.

6.2 Pore Architecture: Evolution from R9.4.1 to R10.4.1 Dual Reader Heads

The evolution of ONT accuracy from ~90% in early chemistries to >99% (Q20+) today is largely driven by pore engineering and chemistry iterations (Kit 14).

- **R9.4.1 Pores:** Utilized an engineered version of the *E. coli* curli transport protein CsgG, which contains a single reader constriction. Because approximately 4–5 nucleotides occupy this constriction simultaneously, the measured current reflects a compound k-mer. In long homopolymer tracts (e.g. `AAAAAAA`), the current level remains static as the identical bases move through, causing insertion/deletion (indel) errors and homopolymer miscounting.
- **R10.4.1 Pores:** Features an engineered longer barrel with **two distinct reader heads** spaced vertically inside the pore channel. As a DNA strand translocates, nucleotides are read consecutively by both constrictions at slightly shifted intervals. This dual-sensing mechanism breaks the homopolymer degeneracy, vastly improving raw read accuracy and significantly improving homopolymer resolution up to ~9–10 bp. When paired with Kit 14 chemistry and Dorado Super-Accuracy (SUP) neural network basecalling models, modal raw simplex read accuracies reach Q20+ (~99.2%), while duplex sequencing achieves ~Q30 (>99.7%).

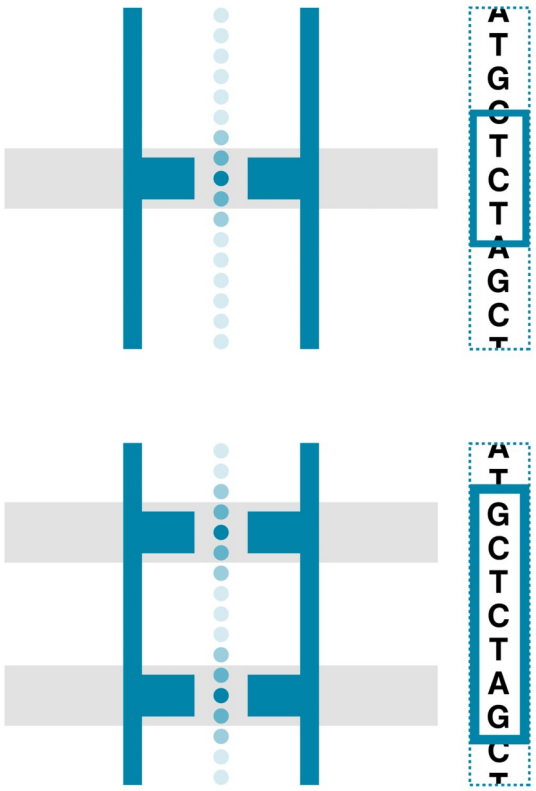


Figure 6.3. Comparison between single-constriction R9.4.1 and dual-constriction R10.4.1 nanopore barrels, illustrating how dual reader heads resolve ambiguous homopolymer current levels.

6.3 Neural Network Basecalling: Decoding Raw Ionic Currents into Nucleotides

Nanopore raw ionic current traces do not exhibit a simplistic one-to-one relationship where a specific current value equals an isolated base. Instead, the signal represents a continuous, noisy time series where each instantaneous measurement is influenced by the 4–6 nucleotides situated within the reader constriction.

ONT's modern basecalling engine—**Dorado**—decodes raw signal stored in `POD5` files using deep neural network architectures built with PyTorch:

12. **Convolutional Neural Networks (CNNs):** Scan raw current samples to extract low-level local signal features, normalizing baseline drifts and transient pore noise.
13. **Transformers / Recurrent Encoders:** Model long-range contextual temporal dependencies across adjacent current shifts.

14. **Connectionist Temporal Classification (CTC) / Modified Beam Search:** Decodes hidden neural layer states into discrete nucleotide calls (`A`, `C`, `G`, `T`) while assigning a probabilistic Phred quality score (Q) to every individual base call.

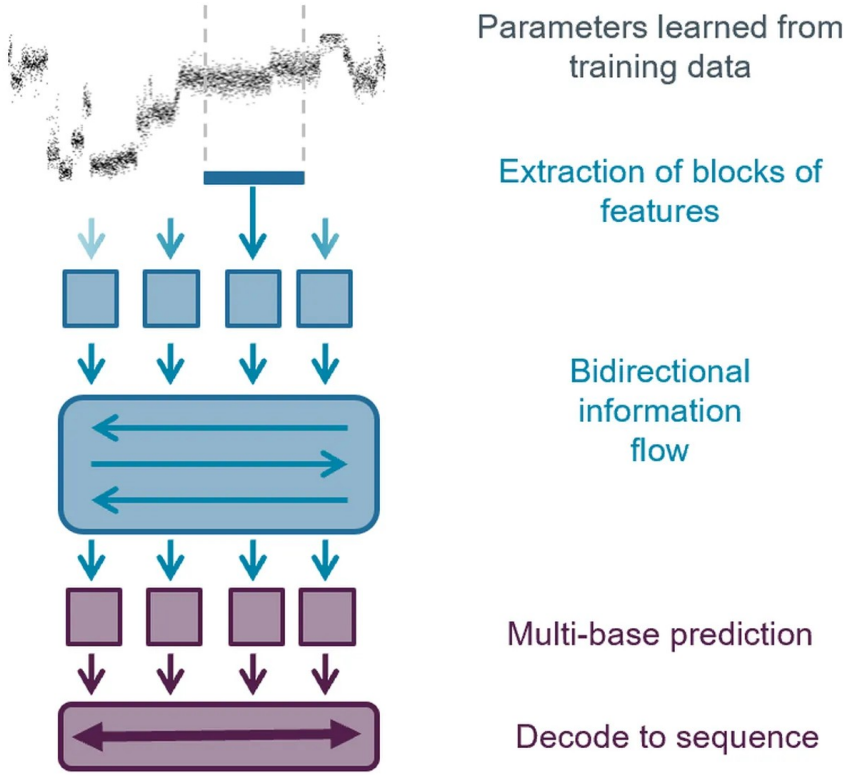


Figure 6.4. Deep neural network basecalling workflow showing raw electrical current processing, feature extraction, neural state probability matrices, and nucleotide sequence decoding.

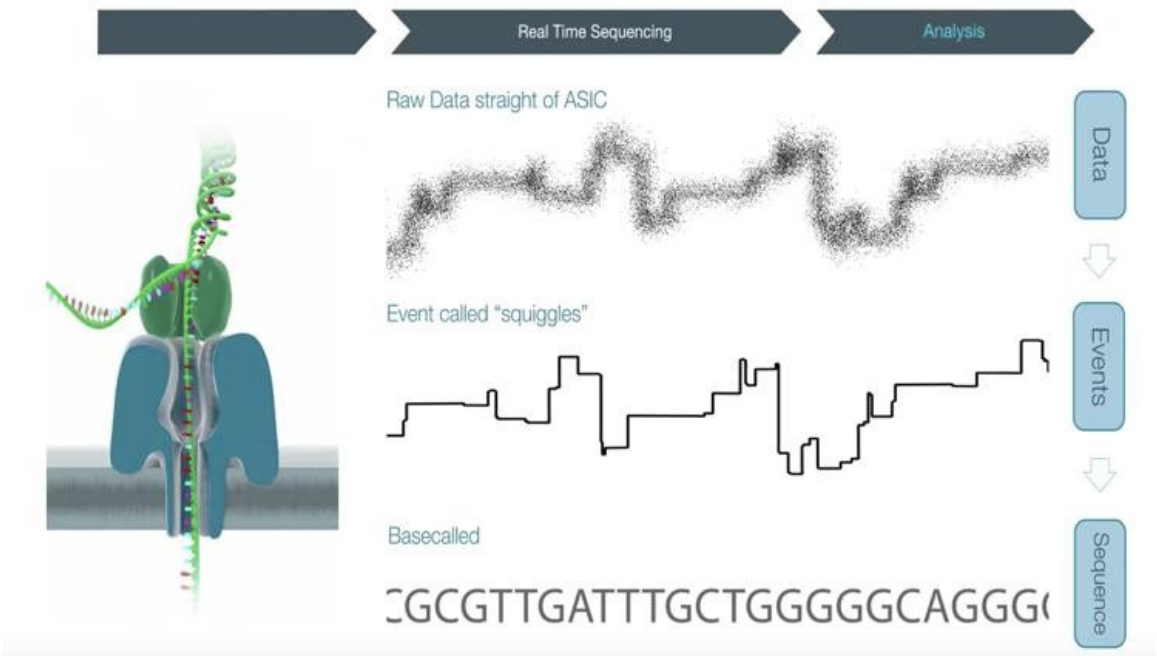


Figure 6.5. Conversion of continuous ionic current traces into basecalled FASTQ sequences with per-base quality metrics. Note: Classic event-segmented schematic view; modern Dorado neural network models decode raw continuous ionic current time series directly without requiring prior discrete event segmentation (Wick et al. 2019).

Chapter 7. ONT Instrumentation and Experimental Planning

Table 6. Oxford Nanopore sequencing platforms

Platform	Form Factor	Flow Cell Capacity	Sensor Architecture & Active Pores	Ideal Amplicon Sequencing Scope
Flongle	Disposable adapter for MinION/GridION	1 Flongle cell	126 channels (up to 504 pores; 50-pore warranty)	Rapid single-sample checks, quality screening, teaching labs
MinION Mk1B / Mk1D	Portable, USB-powered	1 MinION flow cell	512 channels (up to 2,048 pores; 800-pore warranty minimum)	Field sequencing, point-of-care diagnostics, modest multiplex pools
GridION	Benchtop with onboard GPU compute	Up to 5 MinION flow cells	Up to 2,560 channels (5 × 512 channels)	Core facility daily throughput; parallel multi-sample barcoded amplicon runs
PromethION 2 Solo / 24 / 48	High-throughput enterprise instrument	2, 24, or 48 PromethION cells	3,000 channels (addressing 12,000 pores; 5,000-pore warranty minimum)	Large-scale population surveys, massive amplicon multiplexing (thousands of samples)

Oxford Nanopore Library Preparation Kits for Amplicon Sequencing

Selecting the appropriate library preparation chemistry depends on target marker biology, sample throughput, and turnaround requirements.

Table 6b. Comparison of Oxford Nanopore amplicon barcoding kits [MFR / LAB]

Feature / Specification	Native Barcoding Kit 24 V14 (`SQK-NBD114.24`)	16S Barcoding Kit 24 V14 (`SQK-MAB114.24`)	16S Barcoding Kit V14 (`SQK-16S114.24`)
Primary Chemistry	Ligation-based (End-prep dA-tailing + blunt/TA barcode ligation)	PCR-based barcoding with rapid sequencing adapter attachment	PCR-based barcoding (direct preceding generation of MAB)
Target Markers	**Universal / Any amplicon** (16S, 18S, ITS, COI, 12S, custom)	**Bacterial 16S rRNA only** (pre-mixed 27F / 1492R primers)	**Bacterial 16S rRNA only** (pre-mixed 27F / 1492R primers)
Primer Requirement	User provides custom forward/reverse primers	Included in kit (ONT 16S primers with barcode attachment tags)	Included in kit (ONT 16S primers with barcode attachment tags)
PCR in Libprep	None (library construction involves only enzymatic ligation)	Single or two-step barcoding PCR directly incorporates barcodes	Single-step barcoding PCR
Hands-on Time	~3.0–3.5 hours	~2.0–2.5 hours	~2.0–2.5 hours
Multiplexing Scale	24 samples (expandable to 96 with `SQK-NBD114.96`)	24 samples (`SQK-MAB114.24`)	24 samples (`SQK-16S114.24`; legacy `SQK-16S024`)

Feature / Specification	Native Barcoding Kit 24 V14 (SQK-NBD114.24)	16S Barcoding Kit 24 V14 (SQK-MAB114.24)	16S Barcoding Kit V14 (SQK-16S114.24)
wf-16s Compatibility	Fully compatible (accepts demultiplexed FASTQ from any kit) [LAB]	Listed in official wf-16s documentation as primary kit [MFR]	Listed in official wf-16s documentation as primary kit [MFR]
Recommended Use	Multi-domain studies, environmental DNA (eDNA), fungal ITS, fish 12S, or custom targets	Rapid, standardized bacterial 16S surveillance where protocol speed is paramount	Standard bacterial 16S profiling (superseded by SQK-MAB114.24 for Kit 14)

> **Why this workshop focuses on SQK-NBD114.24:** While Oxford Nanopore's wf-16s documentation lists SQK-MAB114.24 and SQK-16S114.24 because they include proprietary 16S PCR primers, this workshop intentionally teaches the **Native Barcoding Kit 24 V14 (SQK-NBD114.24)**. Native barcoding is the foundational, universal ligation chemistry that generalizes across all molecular markers—enabling participants to sequence fungal ITS, eukaryotic 18S, animal COI, and aquatic eDNA 12S amplicons without altering their library preparation protocol. Because EPI2ME wf-16s accepts demultiplexed FASTQ files, libraries constructed with SQK-NBD114.24 run seamlessly through the pipeline.

Experimental Planning Guidelines

- **Sample Multiplexing:** Native Barcoding Kit 24 V14 provides 24 unique barcodes (NB01–NB24), enabling 24 distinct samples per flow cell [MFR].
- **Reserve Barcodes for Quality Controls:** Always allocate barcodes to an extraction blank, a PCR no-template control (NTC), and an optional positive mock community.
- **Target Sequencing Depth [LAB]:** For bacterial 16S community profiling, an empirical target of 20,000 to 50,000 classified reads per sample provides comprehensive coverage of dominant and subdominant taxa, with rarefaction curves typically plateauing past ~20,000 reads in standard communities [LAB]. On a PromethION flow cell yielding millions of reads, 24 samples will reach saturating depth rapidly, allowing the run to be stopped early once saturation is confirmed in MinKNOW or multiplexed at higher barcode tiers (e.g. 96-plex with SQK-NBD114.96).
- **Flow Cell Quality Check:** Always perform an electronic flow cell check via MinKNOW within 12 weeks of purchase. The manufacturer warranty guarantees a minimum of 5,000 active sequencing pores on a new PromethION flow cell [MFR].
- **Consumable Compatibility:** The native barcoding amplicon protocol requires R10.4.1 PromethION flow cells (FLO-PRO114M) [MFR].

Part B – ONT Laboratory Workflow

Chapter 8. Laboratory Workflow Overview

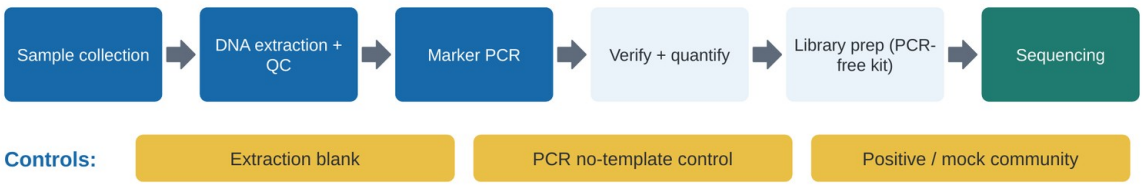


Figure 8.1. High-level laboratory workflow tracing samples from collection through PCR, library construction, PromethION sequencing, and bioinformatic classification.

Sample Collection and DNA Extraction

Samples must be collected using sterile, DNA-free tools and immediately preserved (flash freezing at −80 °C, preservation in 95% molecular ethanol, or stabilization in lysis buffers). Chemical impurities commonly co-extracted from environmental matrices—including humic acids, polyphenols, polysaccharides, residual SDS, phenol, or ethanol—inhibit PCR polymerases and poison nanopores. Spectrophotometric purity guidelines ([MFR]):

- **A_{260} / A_{280} ratio:** 1.8 to 2.0 (lower values indicate protein or phenol contamination).
- **A_{260} / A_{230} ratio:** 2.0 to 2.2 (lower values indicate carbohydrate, humic acid, or salt carryover).

Marker PCR

Amplify marker targets using high-fidelity, proofreading DNA polymerases. Maintain the lowest cycle count that yields a detectable band (typically 25–30 cycles); excessive cycling exponentially increases chimera formation and skewing caused by template exhaustion (Kebschull & Zador 2015).

Table 7. Critical experimental controls

Control Type	Point of Introduction	Diagnostic Value
Extraction Blank (Kitome Control)	DNA Extraction step	Detects background contaminants originating from commercial extraction spin columns and lysis reagents
PCR No-Template Control (NTC)	PCR Amplification step	Identifies cross-contamination, aerosol carryover, or primer-dimer artifacts
Mock Community Positive Control	Extraction or PCR	Calibrates PCR amplification bias, chimera rates, and taxonomic classification accuracy against known standards
DNA Control Sample (DCS)	End-Preparation step	A standard 3.6 kb Lambda DNA fragment confirming that end-repair and ligation chemistries functioned correctly [MFR]

> In ONT terminology, "PCR-free" refers strictly to the library preparation chemistry: no PCR amplification is performed during end-prep, barcoding, or adapter ligation. However, the starting amplicon input material was generated via PCR prior to library entry.

Chapter 9. Native Barcoding Kit V14 Guided Practical

> Protocol specifications follow ONT *Ligation Sequencing Amplicons – Native Barcoding Kit 24 V14 (SQK-NBD114.24), PromethION variant*, rev. NBA_9168_v114_revU_15Jul2026.

Table 8. Reagents and consumables compatibility [MFR]

Reagent / Hardware	Catalog Number
Native Barcoding Kit 24 V14	SQK-NBD114.24
PromethION Flow Cell (R10.4.1)	FLO-PRO114M
Flow Cell Wash Kit	EXP-WSH004
Sequencing Auxiliary Vials V14	EXP-AUX003

Reagent / Hardware	Catalog Number
NEBNext Ultra II End Repair / dA-Tailing Module	NEB `E7546`
NEB Blunt/TA Ligase Master Mix	NEB `M0367`
NEBNext Quick Ligation Module	NEB `E6056`
AMPure XP Magnetic Beads	Beckman Coulter `A63881`

9.1 Preparing and Evaluating PCR Amplicons

Objective: Verify amplicon length, confirm absence of non-specific bands, quantify concentration via fluorometry, and calculate exact molar inputs.

Principle: Enzymatic ligation kinetics depend strictly on the molar concentration of available DNA termini (fmol), not on mass (ng). Equal mass does not mean equal molecules.

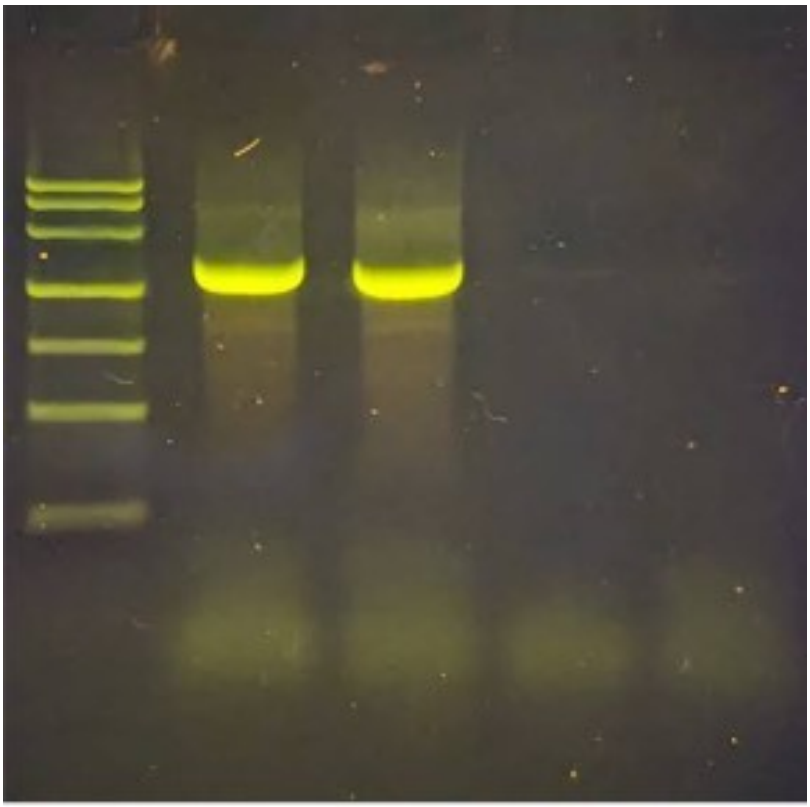


Figure 9.1. Agarose gel electrophoresis verifying full-length 16S rRNA amplicons (~1.5 kb). A clean, distinct single band indicates high amplicon purity suitable for library preparation without non-specific off-target products.

Procedural Steps

15. Load 1–3 µL of PCR product alongside a DNA size ladder on a 1.5% agarose gel. Verify a single discrete band at the expected amplicon length (~1.5 kb for 16S).
16. Quantify amplicon concentration using the Qubit dsDNA High Sensitivity (HS) assay. Do not rely on NanoDrop A_{260} spectrophotometry, which severely overestimates amplicon concentration in the presence of unincorporated dNTPs and primers.
17. Calculate the DNA mass required to deliver **200 fmol** per sample `[MFR]`.

> **Mass-to-Molarity Formula for dsDNA: Mass (ng) ≈ [fmol × Length (bp) × 660] / 1,000,000** For **200 fmol** of a **1,500 bp** full-length 16S amplicon: **Mass ≈ (200 × 1,500 × 660) / 10^6 ≈ 198 ng**

Table 9. Mass vs molarity comparison across amplicon lengths [EX]

Amplicon Fragment Length	Mass Required for 200 fmol	Molar Amount in 130 ng of DNA
500 bp	66.0 ng	394 fmol
800 bp	105.6 ng	246 fmol
1,000 bp	132.0 ng	200 fmol
1,500 bp (Full-length 16S)	198.0 ng	131 fmol

9.2 End-Preparation: Preparing DNA for Ligation

Objective: Repair ragged DNA ends, phosphorylate 5′ termini, and append a single 3′ deoxyadenosine (dA) overhang to facilitate cohesive TA ligation of Native Barcodes.

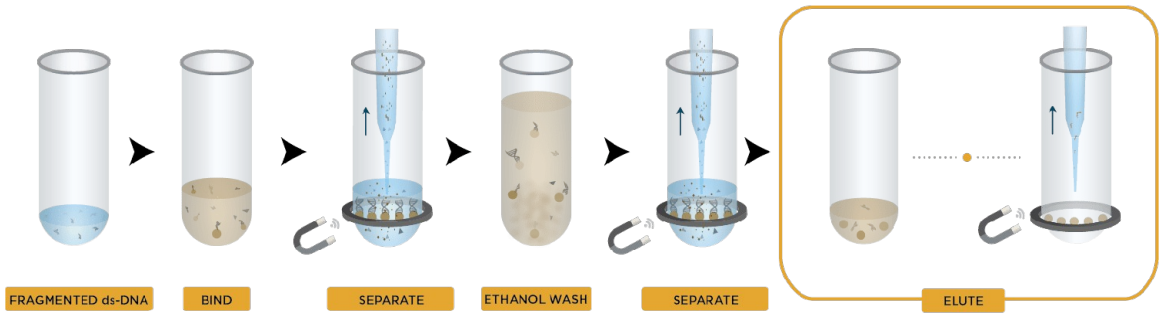


Figure 9.2. Magnetic bead cleanup principle showing DNA binding to carboxylated paramagnetic beads in PEG/NaCl, washing in ethanol, and elution in pure water.

Table 10. End-preparation reaction composition [MFR]

Component	Volume per Reaction
Amplicon DNA (200 fmol)	11.5 µL
Diluted DNA Control Sample (DCS) *[Optional]*	1.0 µL
Ultra II End-prep Reaction Buffer	1.75 µL
Ultra II End-prep Enzyme Mix	0.75 µL
Total Reaction Volume	**15.0 µL**

Incubation and Clean-up Procedure

18. Program a thermal cycler: **20 °C for 5 minutes** (end-repair), followed by **65 °C for 5 minutes** (heat inactivation of enzyme and dA-tailing).
19. Transfer the 15 µL reaction to a clean 1.5 mL DNA LoBind tube.
20. Add **15 µL thoroughly resuspended AMPure XP beads (1.0× ratio)**. Mix gently by flicking or pipetting. Incubate on a rotator for 5 minutes at room temperature.
21. Pellet beads on a magnetic rack until the supernatant clarifies completely (~2 minutes). Discard supernatant.
22. Wash the bead pellet twice with **200 µL freshly prepared 80% ethanol**, taking care not to disturb the bead pellet.
23. Air-dry the pellet briefly (~30 seconds). Avoid over-drying until cracks appear, which significantly impairs elution.

24. Resuspend the pellet in **10 µL nuclease-free water**. Incubate for 2 minutes at room temperature, place on the magnet, and retain the 10 µL clarified eluate.
25. Quantify 1 µL using Qubit dsDNA HS to determine recovery yield.

> Never vortex the Ultra II End Prep Enzyme Mix. Mix reagents by gentle pipetting. Prepare 80% ethanol fresh daily; diluted ethanol below 70% will prematurely elute DNA from the beads.

9.3 Native Barcode Ligation and Sample Multiplexing

Objective: Ligate unique double-stranded native barcode identifiers (`NB01`–`NB24`) to the dA-tailed amplicon ends, allowing up to 24 samples to be pooled and sequenced together.

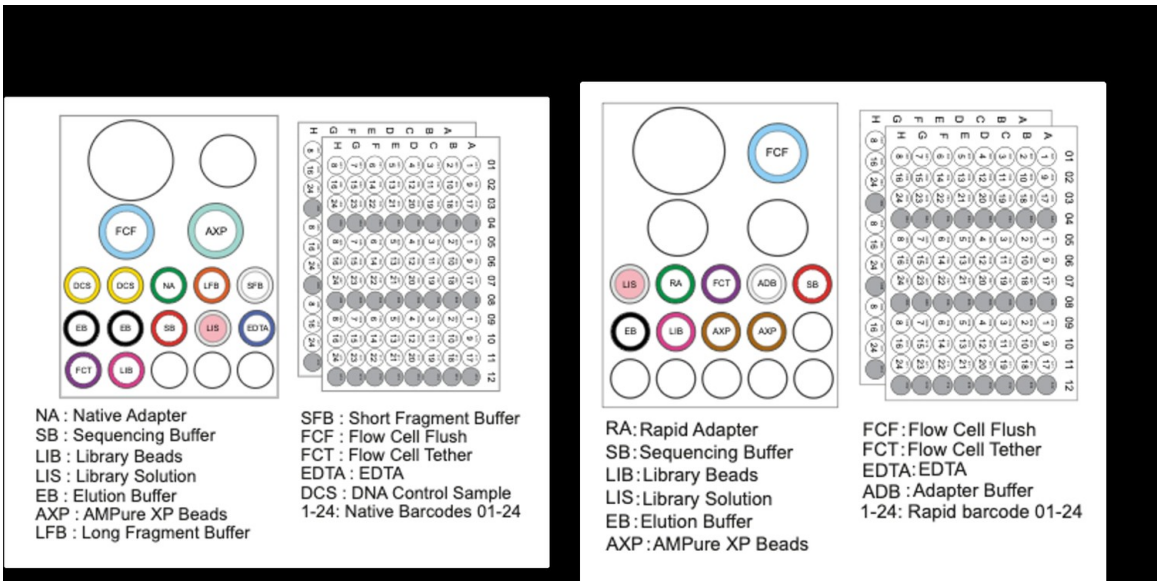


Figure 9.3. Reagent layout and tube formats for Native Barcoding Kit (SQK-NBD114.24) and Rapid Barcoding Kit workflows.

Table 11. Barcode ligation reaction composition [MFR]

Component	Volume per Sample
End-prepped Amplicon DNA	7.5 µL
Native Barcode (`NB01` through `NB24`)	2.5 µL
Blunt/TA Ligase Master Mix	10.0 µL
Total Reaction Volume	**20.0 µL**

Procedural Steps

26. Carefully log barcode assignments in the sample tracking sheet (Appendix B). Native barcode vials are single-use.
27. Combine components in the order listed; mix by pipetting 10–20 times.
28. Incubate at room temperature (**20–25 °C**) for **20 minutes**.
29. Add **4 µL EDTA (blue cap)** to each tube and mix thoroughly to quench ligase activity *(Note: if sourcing EDTA independently, use 0.25 M)*.
30. **Pool all reactions** into a single 1.5 mL LoBind tube (24 µL per sample). Because starting amplicon inputs were normalized to 200 fmol during end-prep, pooling equal volumes achieves an equimolar pool ensuring balanced sequencing depth across all barcodes [MFR].

31. Perform magnetic bead purification using a **0.4× AMPure XP ratio** (see Table 12). *(Note: both this pooling clean-up and the subsequent post-adapter clean-up employ a 0.4× bead ratio, which strongly selects against fragments <1 kb; see Table 25 for short amplicon adaptations)*.
32. Wash the pooled pellet twice using **700 µL Short Fragment Buffer (SFB)**. *Do not use ethanol.*
33. Resuspend pellet in **35 µL nuclease-free water**, incubate at 37 °C for 10 minutes, pellet on magnet, and transfer the 35 µL pooled library eluate to a clean tube.

Table 12. Pooling volumes and 0.4× bead cleanup arithmetic [MFR]

Number of Multiplexed Samples	Pooled Volume (with EDTA)	0.4× AMPure XP Bead Volume
6 Samples	144 µL	58 µL
12 Samples	288 µL	115 µL
24 Samples	576 µL	230 µL

> Always verify sample-to-barcode mappings before pooling. Once tubes are combined, sample identities cannot be recovered if mislabeled.

9.4 Sequencing Adapter Ligation and Final Library Clean-up

Objective: Attach the Native Adapter (NA) to both ends of the pooled, barcoded amplicons. The Native Adapter carries the sequencing motor protein that engages the nanopore reader.

Table 13. Adapter ligation reaction composition [MFR]

Component	Volume
Pooled Barcoded Library	30.0 µL
Native Adapter (NA)	5.0 µL
NEBNext Quick Ligation Reaction Buffer (5×)	10.0 µL
Quick T4 DNA Ligase	5.0 µL
Total Reaction Volume	**50.0 µL**

Incubation and Final Clean-up

34. Incubate the reaction at room temperature for **20 minutes**.
35. Add **20 µL AMPure XP beads** (0.4× ratio), rotate for 10 minutes at room temperature, and pellet on the magnet.
36. Wash the pellet twice with **125 µL Short Fragment Buffer (SFB)**.
37. Resuspend the pellet in **25 µL Elution Buffer (EB)**, incubate for 10 minutes at 37 °C, pellet, and retain the clarified library.
38. Quantify 1 µL via Qubit dsDNA HS. Prepare the final library loading amount in **32 µL Elution Buffer (EB)**.

Table 14. Wash buffer selection criteria [MFR]

Wash Buffer	Fragment Size Retention	Protocol Guidance
Short Fragment Buffer (SFB)	Retains all bead-bound DNA fragments without size stripping	Mandatory for full-length 16S amplicons (~1.5 kb) and shorter targets; size floor is dictated by the bead ratio

Wash Buffer	Fragment Size Retention	Protocol Guidance
Long Fragment Buffer (LFB)	Selectively enriches fragments ≥3 kb	Used strictly for genomic DNA libraries; severely depletes amplicons

> Never use ethanol during post-adapter wash steps! Ethanol denatures the motor protein attached to the Native Adapter, dropping flow cell pore occupancy to near zero.

Table 15. Flow cell loading guidelines by library fragment length [MFR]

Library Insert Size	Recommended Loading Amount (in 32 µL EB)
<1,000 bp (Short amplicons)	100 fmol
1,000–10,000 bp (Full-length 16S)	35–50 fmol
>10,000 bp (Long genomic fragments)	300 ng

9.5 Priming and Loading the PromethION Flow Cell

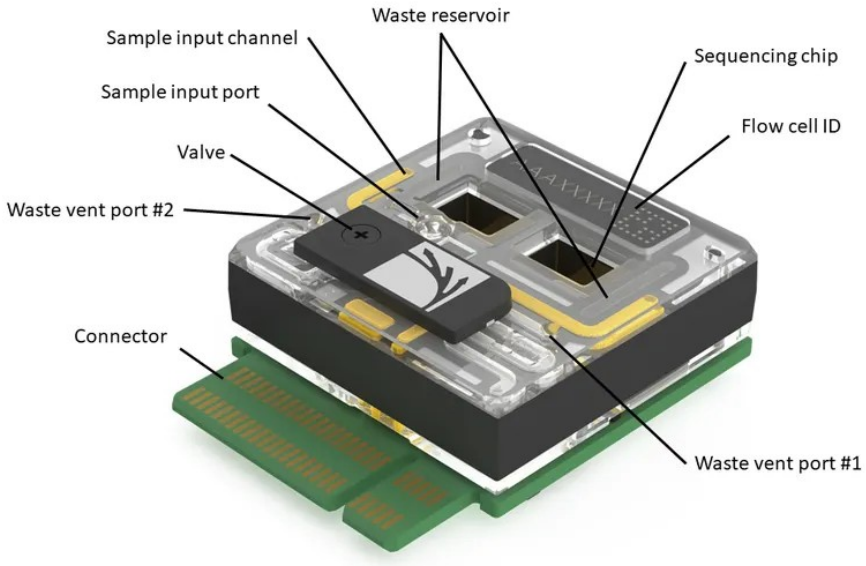


Figure 9.4. PromethION flow cell 3D diagram showing fluidic ports, internal sensor micro-channels, waste ports, and electrical contact pin arrays.

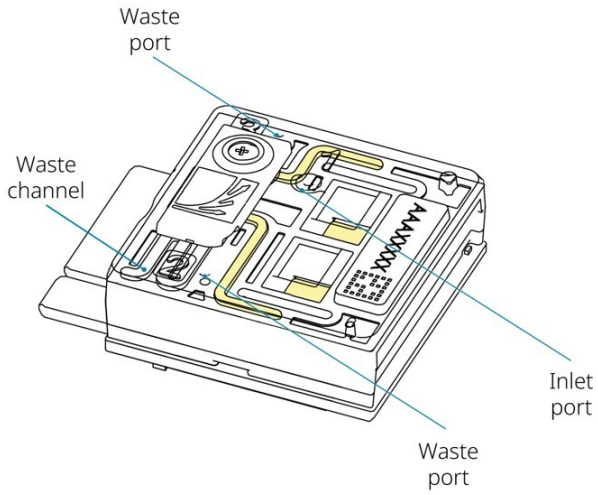


Figure 9.5. Detailed anatomy of the PromethION flow cell fluidic architecture and inlet loading port.

Table 16. Flow cell priming mix [MFR]

Reagent	Volume
Flow Cell Flush (FCF)	1,170 µL
Flow Cell Tether (FCT)	30 µL
Total Volume	**1,200 µL**

Table 17. Final PromethION library loading mix [MFR]

Reagent	Volume
Sequencing Buffer (SB)	100 µL
Library Beads (LIB) *[Thoroughly vortexed]* or Library Solution (LIS)	68 µL
Prepared DNA Library (in EB)	32 µL
Total Loading Volume	**200 µL**

Flow Cell Priming and Loading Steps

39. Equilibrate the flow cell to room temperature for at least 20 minutes before unsealing.
40. Insert the flow cell into the PromethION bay. Ensure smooth horizontal entry; pushing at an awkward angle bends the delicate electrical contact pins.
41. Slide the inlet port cover clockwise to expose the loading port.
42. Set a P1000 pipette to 200 µL. Insert the tip into the inlet port and gently draw back only until a tiny bead of liquid enters the tip (no more than 20–30 µL) to clear any residual air bubbles.
43. Slowly introduce **500 µL of priming mix** through the inlet port. Wait **5 minutes**.
44. Vortex Library Beads (LIB) thoroughly immediately before pipetting; beads settle within seconds. Prepare the 200 µL loading mix.

45. Introduce the second **500 µL of priming mix**.
46. Gently load the **200 µL library loading mix** through the inlet port.
47. Close the inlet port cover. Fit the PromethION Light Shield over the flow cell window and close the instrument lid.
48. Wait at least 10 minutes before starting the sequencing run in MinKNOW; this rest period increases overall sequencing output and pore availability across channels.

Table 18. Physical failure modes and troubleshooting `[MFR]`

Observed Failure	Biological / Physical Cause	Corrective Action
Air bubble introduced into array	Irreversible physical destruction of pores and synthetic polymer membranes	Always draw back a small volume before loading; dispense priming mix smoothly without introducing bubbles
Pore occupancy near 0%	Flow Cell Tether (FCT) omitted, or ethanol used in adapter clean-up	Always add FCT to FCF priming mix; ensure only SFB is used after adapter ligation
Low sequencing pore occupancy (<40%)	Under-loaded library or settled Library Beads	Accurately quantify library via Qubit; vortex LIB vigorously immediately before mixing
Rapid pore degradation during run	Chemical contaminant carryover (phenol, polysaccharides)	Re-purify amplicons with an additional bead wash; execute a Nuclease Flush (`EXP-WSH004`)

9.6 MinKNOW Run Configuration and Data Generation

MinKNOW coordinates real-time data acquisition, voltage control, and neural network basecalling.

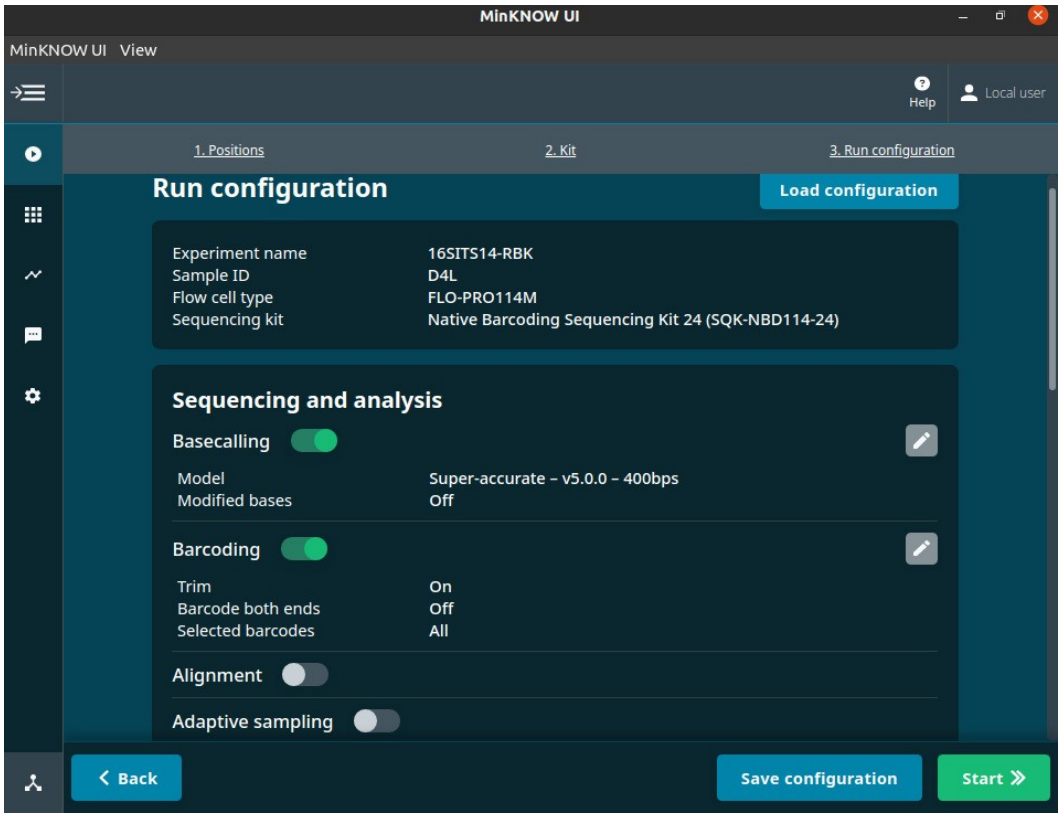


Figure 9.6. MinKNOW sequencing run configuration screen showing flow cell chemistry selection, kit selection (SQK-NBD114.24), and real-time basecalling model configuration.

49. **Start Sequencing:** Navigate to the **Start** tab, select the flow cell position, enter the Experiment Name and Sample ID, and confirm flow cell chemistry (`FLO-PRO114M`).
50. **Kit Selection:** Select **Native Barcoding Kit 24 V14 (`SQK-NBD114.24`)**. Selecting this kit configures MinKNOW to demultiplex reads automatically during acquisition.
51. **Run Options:** Set sequencing duration (typically 24–48 hours, or stop manually when sufficient reads are collected) and minimum read length filter (e.g. 200 bp).
52. **Basecalling Settings:** Enable real-time basecalling. Select High Accuracy (HAC) or Super Accuracy (SUP) models depending on local GPU compute capacity. Enable barcode trimming and mid-read barcode filtering.
53. **Output Formats:** Select `POD5` for raw electrical current storage and `FASTQ` for basecalled reads with per-base quality scores.

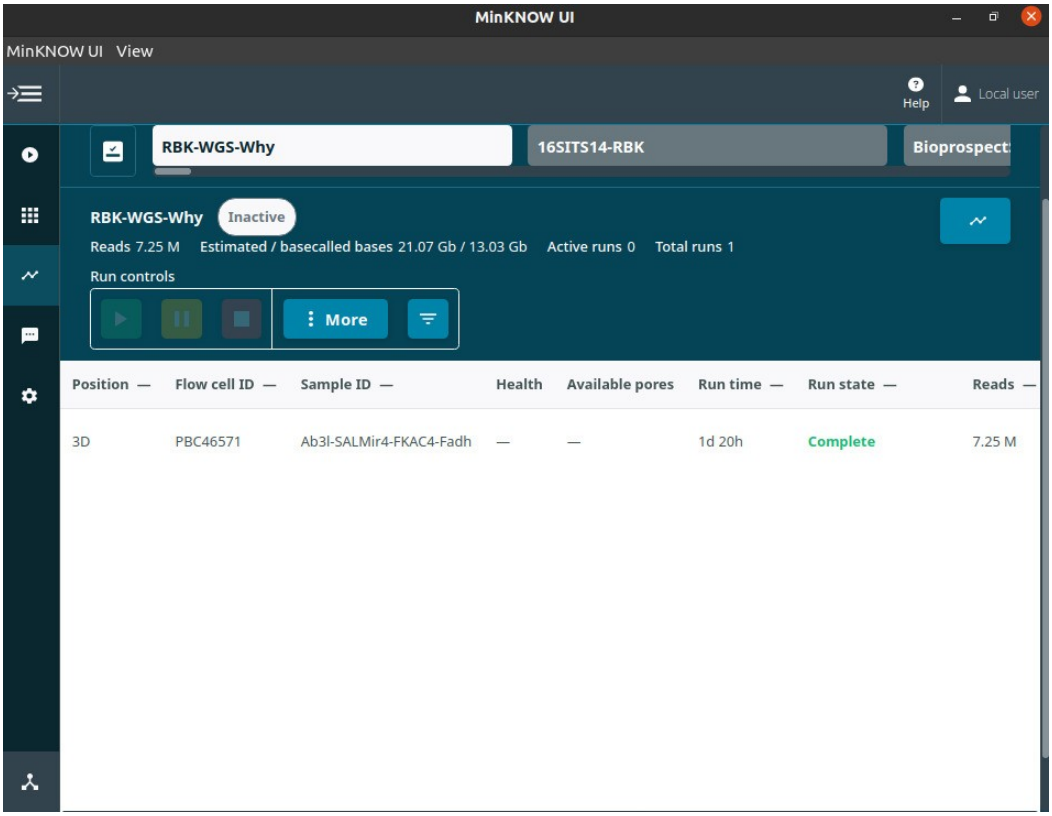


Figure 9.7. MinKNOW active sequencing dashboard displaying real-time pore occupancy, channel activity states, cumulative throughput, and Phred quality score distributions.

9.7 From FASTQ to Biological Interpretation (`wf-16s` Walkthrough)

EPI2ME `wf-16s` is the official Nextflow bioinformatics pipeline developed by Oxford Nanopore for microbial amplicon analysis. It accepts demultiplexed FASTQ files and executes quality filtering, taxonomic assignment, and interactive HTML reporting.

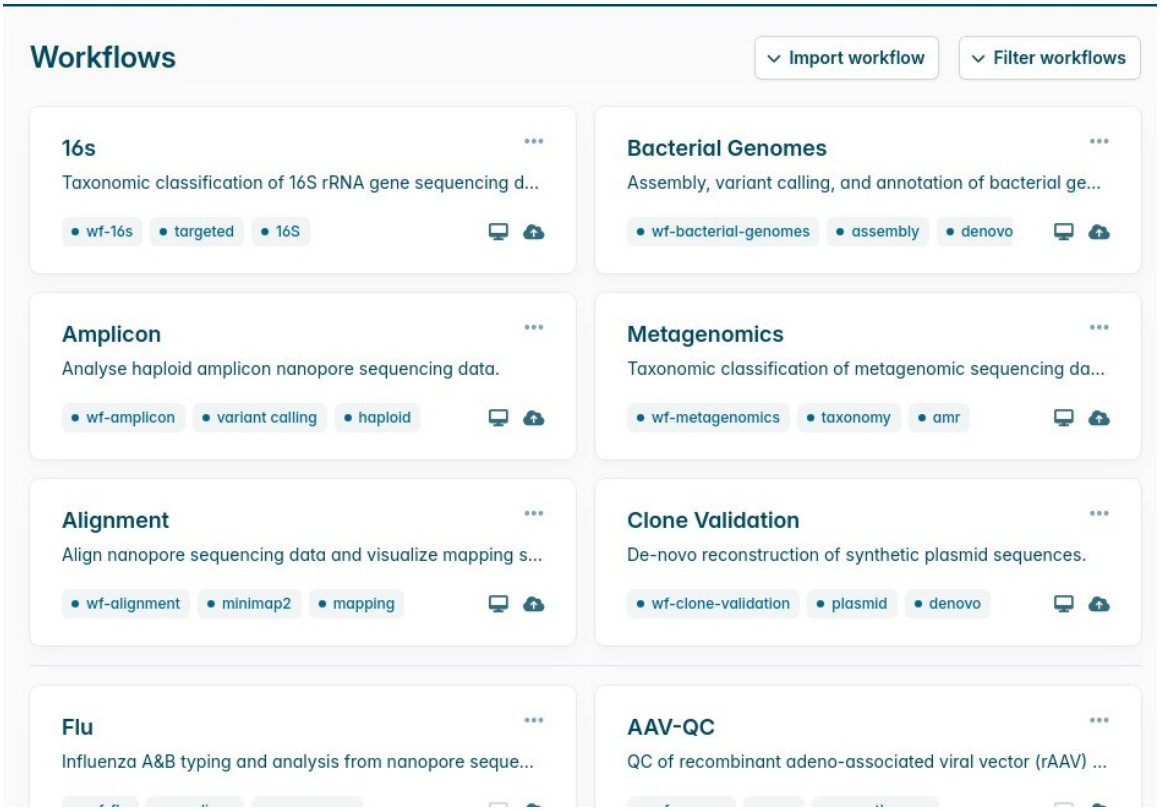


Figure 9.8. EPI2ME desktop application interface showing available automated workflows including 16S/18S amplicon analysis, metagenomics, and quality control pipelines.

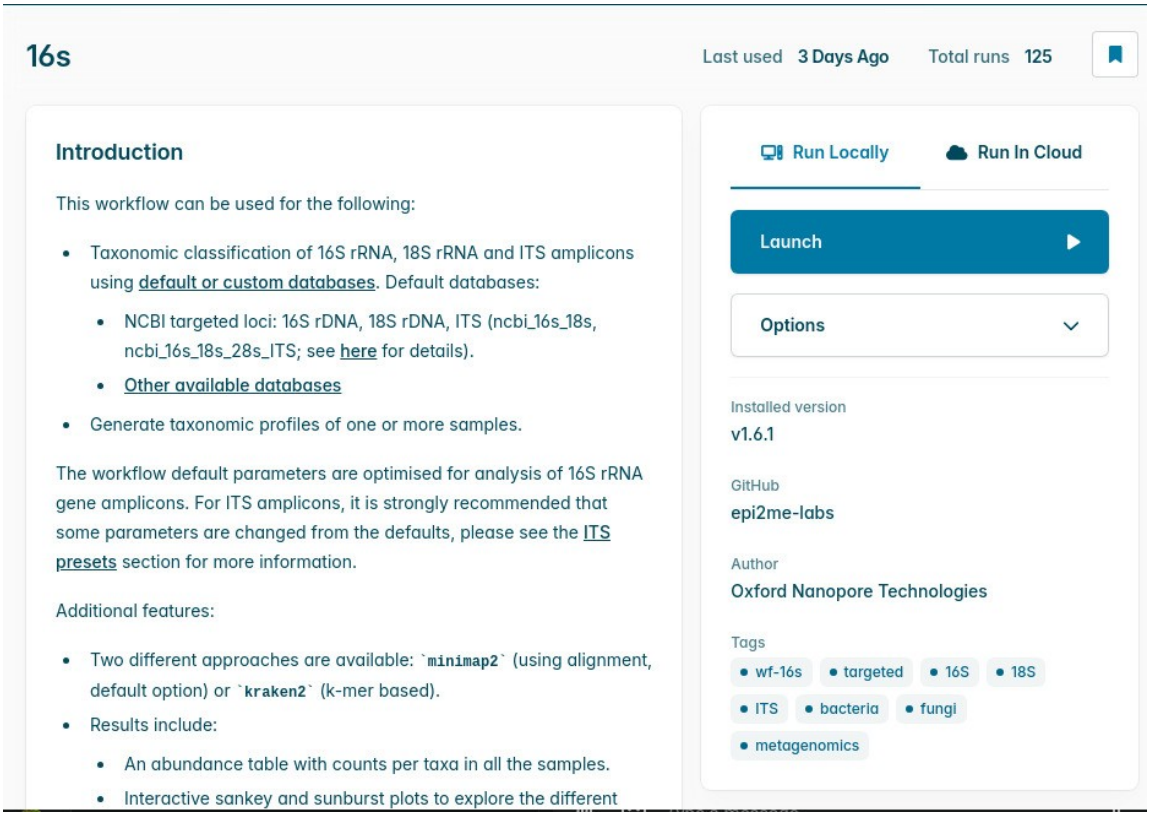


Figure 9.9. Parameter setup screen for wf-16s detailing classifier selection (minimap2 vs. Kraken2), reference database configuration, and read-length filtering windows.

Pipeline Parameters

- **`classifier`:** Choose between `minimap2` (pairwise reference alignment, recommended for fine species resolution) or `kraken2` (exact k-mer matching with Bracken abundance re-estimation, faster execution).
- **Reference Database & Taxonomy Flags:**
- *Minimap2 Mode:* Configured using `--reference` (path to reference FASTA or pre-indexed `.mmi` file; defaults to bundled NCBI 16S/18S targeted loci), `--ref2taxid` (two-column TSV mapping sequence headers to NCBI taxonomy IDs), and `--taxonomy` (directory containing NCBI taxonomy dump files `names.dmp` and `nodes.dmp`).
- *Kraken2 Mode:* Configured using `--database` (directory containing Kraken2 hash index files `hash.k2d`, `opts.k2d`, `taxo.k2d`) and `--taxonomy` (NCBI taxonomy directory for taxonomic lineage roll-up).
- **Read-Length Filtering:** Default `min_len` is 800 bp and `max_len` is 2,000 bp. For short amplicons (e.g. fungal ITS or fish 12S), `min_len` must be adjusted downward (e.g. 100 bp).
- **Alignment Thresholds:** `min_percent_identity: 95` and `min_ref_coverage: 90`. Reads falling below these thresholds remain categorized as "Unclassified".
- **Database Limitation Warning:** The bundled `ncbi_16s_18s` database does **not** contain vertebrate mitochondrial 12S sequences. If analyzing fish 12S eDNA, simply lowering `min_len` will result in 100% unclassified reads. Researchers must supply a custom reference database (e.g. MitoFish FASTA via `--reference`, accompanied by custom `--ref2taxid` and `--taxonomy` parameters). For detailed instructions on running pipelines in air-gapped environments or installing custom databases, refer to Oxford Nanopore Support: *"How to run EPI2ME workflows offline"* (available at https://support.nanoporetech.com/ and https://github.com/epi2me-labs/wf-16s).
- **Kit Compatibility:** While official ONT documentation for `wf-16s` lists `SQK-MAB114.24` and `SQK-16S114.24` as associated protocols because they include proprietary 16S primers, `wf-16s` accepts demultiplexed `FASTQ` files produced by any kit, including `SQK-NBD114.24`.

9.8 Guided Practical Checkpoint: Five Critical Decisions (H8)

This interactive checkpoint reinforces five pivotal laboratory and computational decisions encountered across the workflow:

Table 18b. Guided practical checkpoint questions and decision rationale

Decision #	Scenario / Question	Options & Correct Choice	Scientific Rationale
Q1 · Stoichiometry	You quantify a 1,500 bp amplicon at 30 ng/µL. What mass and volume are needed to deliver 200 fmol into an 11.5 µL reaction?	**A: 198 ng (6.6 µL)** *(Correct)* B: 66 ng (2.2 µL) C: 300 ng (10.0 µL)	Mass = (200 × 1,500 × 660) / 10^6 ≈ 198 ng. At 30 ng/µL: 198 / 30 = 6.6 µL DNA + 4.9 µL water = 11.5 µL.
Q2 · Barcoding & Controls [LAB]	You have 6 biological samples and want to enforce rigorous quality control [LAB good practice]. How many total barcodes should you allocate, and when can you combine the tubes?	A: 6 barcodes; pool immediately **B: 8 barcodes; pool strictly post-EDTA** *(Correct)* C: 8 barcodes; pool pre-ligation	In good laboratory practice, allocate 1 extraction blank and 1 PCR no-template control (NTC) alongside your 6 biological samples (8 barcodes total). Tubes must never be combined before ligase is completely quenched with EDTA; unquenched ligase causes cross-ligation and sample crosstalk.

Decision #	Scenario / Question	Options & Correct Choice	Scientific Rationale
Q3 · Size Selection	You are purifying a 1.5 kb amplicon library post-ligation. Which wash buffer must you use?	**A: Short Fragment Buffer (SFB)** *(Correct)* B: Long Fragment Buffer (LFB) C: 80% Ethanol	SFB retains all bead-bound fragments without stripping. LFB selectively enriches fragments ≥3 kb and severely depletes amplicons.
Q4 · Flow Cell Loading	What is the final PromethION loading mix recipe, and how long should the flow cell rest before starting?	**A: 100 µL SB + 68 µL LIB + 32 µL library; rest ≥10 min** *(Correct)* B: 200 µL pure library; start immediately	SB provides electrolyte balance, LIB provides library beads (which must be vortexed vigorously), and resting ≥10 minutes increases sequencing throughput and pore availability.
Q5 · Lab Troubleshooting	A researcher accidentally washed the final magnetic beads with 80% ethanol after sequencing adapter ligation. What happens upon loading?	A: Yield improves 20% **B: Active pore occupancy drops to near 0%** *(Correct)* C: No observable effect	Ethanol denatures the motor protein pre-attached to the Native Adapter. Without an active motor protein, DNA strands cannot dock and translocate through the pore.

Part C – Bioinformatics

Chapter 10. Nanopore Data Formats and Basecalling

Table 19. File formats in the nanopore computational lifecycle

File Format	Primary Data Content	Long-term Archival Recommendation
`POD5`	Raw ionic current measurements, sampling timestamps, and pore channel telemetry	**Permanent archive.** Allows raw electrical signals to be re-basecalled in future years with improved neural network models
`FASTQ (.fastq.gz)`	Basecalled nucleotide strings with ASCII-encoded per-base Phred quality scores	**Working archive.** Primary input for downstream alignment, taxonomic classification, and variant analysis
`Sample Sheet (.csv)`	Metadata mapping experimental barcodes (`barcode01`–`barcode24`) to biological aliases	**Permanent archive.** Critical for sample traceability and demultiplexing
`HTML Report & Abundance Tables`	Interactive community visualizer, taxonomic abundance matrices, and QC charts	**Final deliverable.** Communicates biological findings

Phred Quality Score: $Q = -10 \cdot \log_{10}(P_error)$

Table 20. Phred quality scores and base accuracy

Phred Q Score	Probability of Incorrect Base Call (P_error)	Base Call Accuracy Percentage
Q10	1 in 10	90.0%
Q20	1 in 100	99.0%
Q30	1 in 1,000	99.9%

Chapter 11. Quality Control and Taxonomic Assignment

Read Quality Control

54. **Length Distribution:** A clean amplicon library produces a sharp unimodal peak centered at the expected marker length (~1,500 bp for 16S). Broad distributions, bimodal profiles, or short tails indicate primer-dimers, chimeras, or degraded input templates.
55. **Quality Score Distribution:** Examine mean Phred scores per barcode; modal quality should exceed Q15–Q20 with modern Dorado models.
56. **Demultiplexing Efficiency:** Confirm that reads are distributed evenly across biological barcodes and that negative control barcodes (`NTC`, `Extraction Blank`) contain negligible read counts.

Table 21. Taxonomic classification algorithms in `wf-16s`

Feature	Alignment Approach (`minimap2`)	k-mer Matching (`Kraken2` + `Bracken`)
Mechanism	Aligns full query read against reference database; requires strict identity and reference coverage thresholds	Breaks query reads into k-mers (e.g. k = 35); finds lowest common ancestor (LCA) in a precomputed taxon tree
Strengths	Superior species-level discrimination; reports actual alignment identity and coverage	Extremely fast processing; modest RAM requirements
Caveats	Slower on large databases; stringent thresholds increase the unclassified fraction	Sensitive to database completeness; may over-classify noisy reads

Chapter 12. Community Visualization and Interpretation

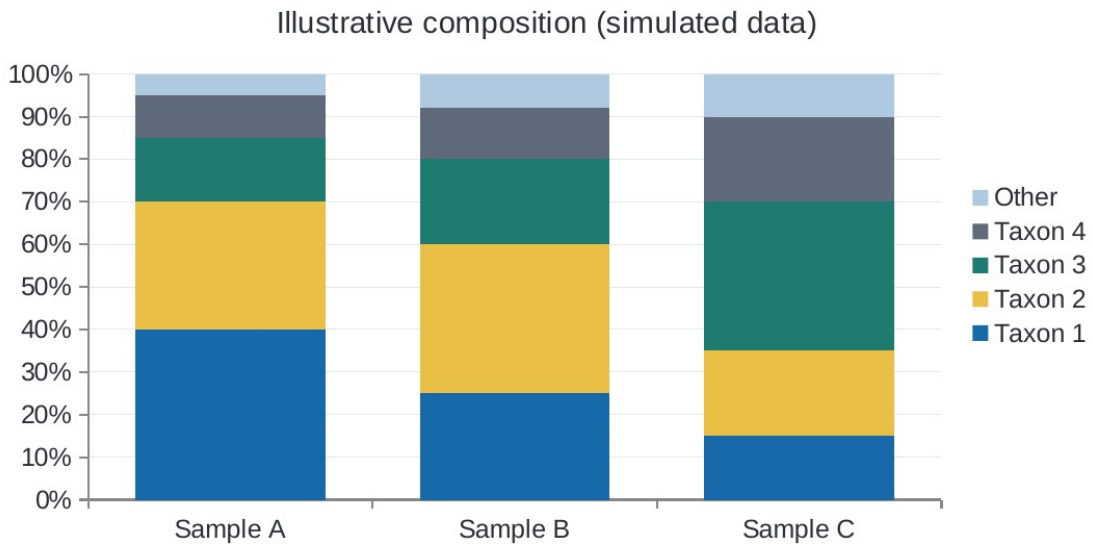


Figure 12.1. Illustrative stacked bar plot displaying relative taxonomic composition across samples. Relative sequence proportions must not be conflated with absolute organism abundance.

Understanding Diversity Metrics

- **Alpha Diversity (Within-sample Diversity):**
- **Species Richness (S):** Total count of unique taxa detected in a sample.
- **Shannon Index ($H = -\Sigma p_i \ln p_i$):** Quantifies both richness and evenness; values decrease when a single taxon dominates.
- **Simpson Index ($D = \Sigma p_i^2$):** Measures the probability that two randomly selected reads belong to the same taxon (dominance index; values approach 1 when a single taxon dominates, and approach 0 in hyperdiverse communities).
- *Practical Note:* Oxford Nanopore documentation describes Simpson as scaling from "0 low to 1 high diversity" while defining $D = \Sigma p_i^2$. Check whether your specific EPI2ME report version prints classical Simpson D (dominance) or the complementary Gini-Simpson index (1 - D), which scales positively with diversity.
- **Pielou's Evenness ($J = H / \ln S$):** Normalizes Shannon diversity on a scale from 0 (complete dominance) to 1 (perfect equitability).
- **Beta Diversity (Between-sample Diversity):** Evaluates compositional turnover between distinct environments using Bray-Curtis dissimilarity, Jaccard distance, or phylogenetic UniFrac metrics visualized via Principal Coordinates Analysis (PCoA).

Rarefaction, Normalization, and Library Depth

EPI2ME `wf-16s` generates an interactive sample rarefaction curve plotting observed taxonomic richness against sequencing read depth per barcode. A curve that approaches an asymptote indicates that additional sequencing would discover few novel taxa, confirming that community richness has been adequately sampled.

To enable fair comparisons across samples with uneven sequencing yields, `wf-16s` exports both the original raw count table and a **rarefied count table**, subsampled down to **95% of the total read count of the smallest sample library** in the run.

Crucially, however, the **alpha diversity indices (Shannon and Simpson) displayed in the summary cards default to the original, non-rarefied counts**. Oxford Nanopore justifies this design by citing McMurdie & Holmes (2014), who demonstrated that rarefying (random subsampling without

replacement) introduces artificial binomial variance, disproportionately discards valid biological reads, and diminishes statistical power in differential abundance testing. For rigorous downstream statistical comparisons, compositional transformations (e.g. centered log-ratio, CLR) or model-based variance-stabilizing methods (e.g. DESeq2 / ANCOM-BC) are recommended over random subsampling.

> **Relative abundance is not population size.** If taxon A yields twice as many reads as taxon B, you cannot conclude that twice as many living cells were present: 1. Ribosomal RNA gene copy numbers vary substantially between microbial genomes: from 1 copy in many oligotrophic taxa up to 21 copies in spore-forming bacilli (medians up to 19 copies in *Metabacillus* and *Bacillus*; rrnDB v5.8; Stoddard et al. 2015). 2. Cell wall structures (Gram-positive peptidoglycan vs. Gram-negative membranes) cause unequal cell lysis efficiencies during DNA extraction. 3. Amplicon sequence data are inherently compositional: percentages sum to 100%, meaning that an expansion in one taxon mathematically depresses the measured relative proportions of all other community members.

Chapter 13. Predictive Functional Profiling: From Taxonomy to Function (PICRUSt2 & FUNGuild)

While amplicon sequencing answers the foundational question **"Who is there?"**, microbial ecologists frequently need to address the consequential follow-up question: **"What are they doing?"** Direct functional profiling requires shotgun metagenomics or metatranscriptomics. However, when working from amplicon data, computational inference tools—most notably **PICRUSt2** (for bacteria and archaea) and **FUNGuild** (for fungi)—can predict the functional potential of microbial communities by leveraging phylogenetic conservation and reference genome databases.

13.1 Bacterial Functional Inference: The PICRUSt2 Pipeline

PICRUSt2 (Phylogenetic Investigation of Communities by Reconstruction of Unobserved States; Douglas et al. 2020) predicts functional metabolic capabilities directly from full-length or short-read 16S rRNA sequence variants.

The pipeline executes four algorithmic steps:

57. **Phylogenetic Sequence Placement:** Full-length 16S amplicon sequences are aligned and placed into a reference phylogenetic tree of ~20,000 sequenced bacterial and archaeal genomes using `EPA-ng` (Barbera et al. 2019) and `GAPPA`. Full-length R10.4.1 reads (~1,500 bp) provide dramatically higher phylogenetic placement precision than short 250–450 bp reads.
58. **Hidden State Prediction (HSP):** Using evolutionary modeling packages (such as `castor`; Louca & Doebeli 2018), PICRUSt2 reconstructs unobserved genomic traits across the tree, predicting 16S rRNA gene copy numbers and genomic abundances of functional gene families (e.g. KEGG Orthology [KO] groups, Enzyme Commission [EC] numbers, and COGs).
59. **16S Copy-Number Normalization:** Observed raw amplicon read abundances are divided by the predicted 16S copy number for each taxon, mitigating the biological bias wherein high-copy-number organisms (e.g. *Bacillus*, *Clostridium*) appear artificially over-represented relative to single-copy oligotrophs.
60. **Metabolic Pathway Inference:** Gene family abundances are mapped to structured metabolic pathways (MetaCyc pathway definitions; Caspi et al. 2018) via `MinPath` (Minimal Pathway Enumeration), yielding pathway abundance and pathway coverage tables.

13.2 Fungal Guild Annotation: FUNGuild

For fungal ITS and 28S amplicon datasets, functional gene prediction from taxonomy is generally unreliable because fungal genomes exhibit massive structural plasticity and evolutionary divergence. Instead, **FUNGuild** (Nguyen et al. 2016) parses taxonomic assignments into ecological guilds based on an expert-curated database of fungal life-history traits:

- **Trophic Modes:** *Pathotroph* (acquiring nutrients by damaging host cells, including animal and plant pathogens), *Saprotroph* (degrading non-living organic matter, such as wood decay fungi), and *Symbiotroph* (exchanging nutrients with living hosts, such as mycorrhizae and lichens).

- **Confidence Rankings:** Each guild assignment is tagged as *Highly Probable*, *Probable*, or *Possible*, allowing researchers to filter out speculative ecological assignments.

13.3 Critical Scientific Evaluation: What Predictions Can and Cannot Claim

Predictive metagenomics provides valuable hypotheses, but researchers must understand its strict methodological boundaries:

Table 21b. Strengths and limitations of predictive functional profiling [LAB]

Analytical Capability	Critical Scientific Limitation & Risk of Over-Interpretation
Formulates testable hypotheses regarding community metabolic shifts (e.g. nitrogen cycling, sulfur reduction, carbohydrate degradation)	**Genomic potential is not expressed activity:** Amplicon-based tools predict the presence of genes in a genome, NOT active gene transcription (mRNA), protein translation, or enzymatic flux (DNA presence ≠ active function)
Normalizes for 16S copy number variation, producing more realistic organismal proportions	**Copy-number normalization is statistically contested:** Operon copy numbers vary even within single species, and ancestral state reconstruction models carry substantial uncertainty for novel lineages
Highly accurate in well-characterized biomes (e.g. human gut, standard lab strains) where reference genome databases are near-complete	**Nearest Sequenced Taxon Index (NSTI) inflation:** Predictions degrade severely in environmental, marine, extreme, or tropical soil biomes with high NSTI (>0.15), where uncharacterized taxa dominate
Cost-effective preliminary screening across hundreds of multiplexed amplicon libraries	**Cannot detect strain-specific genomic islands or plasmids:** Horizontal gene transfer (HGT), phage integrations, and antibiotic resistance plasmids cannot be inferred from a conserved 16S gene

> **Scientific Realism in Reporting:** Never report PICRUSt2 results as "metabolic activities" or "active cellular functions". Always describe them as **"predicted metagenomic potential"**. Significant functional pathways identified by PICRUSt2 should be treated as candidates for validation through direct shotgun metagenomic sequencing, metatranscriptomics (RNA-seq), or metabolomics.

Part D – Critical Evaluation and Synthesis

Chapter 14. Limitations and Troubleshooting

Table 22. Benefits versus methodological limitations in amplicon sequencing

Inherent Strengths	Methodological Limitations & Analytical Pitfalls
Culture-Independent Surveillance	**PCR Amplification Bias:** Universal primers never amplify every lineage with equal thermodynamic efficiency
Full-Length Marker Discrimination	**Reagent Contamination (The "Kitome"):** Low-biomass samples are easily masked by contaminants in extraction columns
Real-Time Data Acquisition	**Barcode Index Switching:** Low-level demultiplexing crosstalk can introduce false-positive read calls

Inherent Strengths	Methodological Limitations & Analytical Pitfalls
High Multiplexing Capacity	**Database Incompleteness:** Unrepresented taxa are forced into incorrect sister clades or labeled "Unclassified"

Table 23. Comprehensive symptom-cause-action troubleshooting guide

Observation / Error	Probable Underlying Cause	Recommended Corrective Action
Low recovery after bead clean-up (<20%)	Ethanol concentration <70%; beads settled; bead-to-sample ratio too low (<0.4×)	Prepare 80% ethanol fresh daily; vortex beads vigorously; verify bead ratio against amplicon fragment length
Pore occupancy <40% at run start	Under-loaded library; library beads settled prior to loading	Re-quantify library with Qubit; vortex LIB beads immediately before mixing; reload additional library
Pore occupancy collapses near 0%	Ethanol wash used after adapter ligation; Flow Cell Tether (FCT) omitted	Strictly wash with SFB/LFB after adapter attachment; ensure FCT is added to FCF priming mix every time
Available pores drop sharply below flow cell check	Air bubble introduced during priming/loading; damaged electrical contact pins	Draw back 20 µL to clear bubbles before dispensing; insert flow cells smoothly at a level horizontal angle
Rapid accumulation of "Inactive" pores	Co-extracted chemical inhibitors (polyphenols, humic acids, protein carryover)	Perform additional 0.4× bead cleanup; execute a flow cell nuclease flush using the Flow Cell Wash Kit (`EXP-WSH004`)
Mean read length substantially shorter than expected	Degraded starting DNA; vortex shearing of amplicons	Check PCR products on an agarose gel; mix libraries by gentle flicking or wide-bore pipetting—never vortex
High read counts in negative controls (NTC/Blank)	Reagent contamination; cross-contamination during pooling; aerosol carryover	Treat taxa present in controls at similar levels as contaminants; clean PCR stations with UV/bleach; use filter tips
Excessive fraction of "Unclassified" reads (>30%)	Reference database lacks target taxa; alignment identity/coverage thresholds too stringent	Inspect unclassified reads via BLAST; test broader databases (e.g. SILVA vs NCBI); verify primer trimming

Chapter 15. Summary, Synthesis and Further Reading

Core Takeaways

61. **Targeted Strategy:** Amplicon sequencing is a marker-directed molecular census. Platform and marker selection determine the taxonomic boundary and biological resolution of the experiment.
62. **Stoichiometric Rigor:** Library chemistry is driven by molar concentration (fmol), not mass (ng). Accurate fluorometric quantification and fragment size conversion are mandatory.
63. **Experimental Quality Controls:** Negative blanks, no-template controls, and mock communities are essential to distinguish true biological signals from kit contaminants and PCR artifacts.

64. **Critical Interpretation:** Sequence read counts represent relative compositional fractions, not absolute cell numbers. High-confidence conclusions require integrating taxonomic results with ecological context.

Review Questions and Answers

Table 24. Conceptual review questions and answers

#	Question	Detailed Scientific Explanation
1	Why do equal masses of two different amplicons contain unequal numbers of DNA molecules?	DNA molecular weight scales linearly with base pair length (M ≈ bp × 660 g/mol). A shorter fragment has fewer grams per mole; consequently, 100 ng of a 500 bp amplicon contains three times as many individual double-stranded molecules as 100 ng of a 1,500 bp amplicon.
2	Which phase makes the Native Barcoding library "PCR-free", and where does PCR occur?	The Native Barcoding Kit (SQK-NBD114.24) is "PCR-free" during library construction because barcodes and adapters are attached via enzymatic end-repair and cohesive TA-ligation without subsequent cycles of PCR amplification. However, the input amplicon DNA was generated by PCR prior to library prep.
3	Why is an extraction negative control mandatory even when multiplexing with native barcodes?	Native barcodes separate multiplexed biological samples from one another during bioinformatic demultiplexing, but they cannot eliminate background DNA present in extraction spin columns, lysis buffers, or enzymes ("the kitome"). Sequencing the extraction blank identifies baseline contaminant taxa that must be filtered out.
4	State three distinct reasons why relative read counts do not directly correspond to living organism cell counts.	(1) Ribosomal RNA gene copy numbers vary from 1 to 21 copies across bacterial genomes (rrnDB v5.x; Stoddard et al. 2015), and intragenomic operon variants exist; (2) Differential cell wall lysis efficiencies cause unequal DNA extraction recovery; (3) DNA sequence counts are compositional proportions that sum to 100%, making read shares interdependent.

#	Question	Detailed Scientific Explanation
5	What parameters must change if applying this workflow to a short 170 bp fish 12S eDNA amplicon instead of 1,500 bp 16S?	(1) Both 0.4× magnetic bead cleanups (post-barcoding pooling and post-adapter ligation) select strongly against DNA <1 kb; recovering ~170 bp fragments requires empirically titrated higher SPRI ratios (~1.5×–1.8×) `[ADAPT]`; (2) The final library loading target must increase to ~100 fmol (<1 kb tier); (3) `wf-16s` read-length filters (`min_len: 800`) must be lowered to ~100 bp; (4) The reference database must be swapped from bacterial 16S to curated vertebrate 12S (e.g. MitoFish), as `ncbi_16s_18s` lacks fish mitochondrial sequences.
6	What implicit assumptions govern the default parameter settings of EPI2ME `wf-16s`?	The workflow assumes intact, full-length bacterial/archaeal 16S amplicons (length window 800–2,000 bp), pairwise alignment with minimap2 requiring ≥95% identity and ≥90% reference coverage, and classification against the NCBI 16S/18S ribosomal targeted loci database.

Synthesis: Adapting Workflows to Environmental DNA (eDNA) Metabarcoding

When transitioning from full-length bacterial 16S sequencing to aquatic eDNA monitoring (such as fish biodiversity surveys using mitochondrial 12S primers), laboratory and bioinformatic parameters must be deliberately adapted rather than blindly copied:

Table 25. Workflow adaptations: Full-length 16S vs Short 12S eDNA `[ADAPT]`

Protocol Parameter	Full-Length 16S Workflow	Short 12S Fish eDNA Workflow
Typical Target Size	~1,500 bp	~163–185 bp (MiFish; Miya et al. 2015)
SPRI Bead Clean-up Ratios (Pooling & Post-Adapter)	0.4× AMPure XP (selects against <1 kb)	Must increase significantly to ~1.5×–1.8× `[ADAPT]`; standard 0.4× cleanups severely deplete ~170 bp fragments. Requires pilot titration.
Final Library Loading Target	35–50 fmol (1–10 kb tier)	100 fmol (<1 kb tier)
`wf-16s` Read-Length Window	800 to 2,000 bp	Must lower `min_len` to 100 bp, or route through dedicated eDNA pipelines
Reference Database	NCBI 16S/18S or SILVA SSU	Curated fish mitochondrial 12S databases (e.g. MitoFish / custom 12S FASTA); `ncbi_16s_18s` contains no vertebrate 12S
Contamination Rigor	Standard extraction blanks and NTCs	Rigorous field sampling blanks, filtration blanks, and DNA-free workspace isolation

Appendices

Appendix A. Reagent and Consumables Checklist

Table 26. Master equipment and reagent inventory `[MFR]`

Check	Category	Item Description	Catalog Number / Specifications
☐	**ONT Kit**	Native Barcoding Kit 24 V14	ONT `SQK-NBD114.24`
☐	**Flow Cell**	PromethION Flow Cell (R10.4.1)	ONT `FLO-PRO114M`
☐	**Enzymes**	NEBNext Ultra II End Repair / dA-Tailing Module	NEB `E7546`
☐	**Enzymes**	NEB Blunt/TA Ligase Master Mix	NEB `M0367`
☐	**Enzymes**	NEBNext Quick Ligation Module	NEB `E6056`
☐	**Clean-up**	AMPure XP Magnetic Beads	Beckman Coulter `A63881`
☐	**Wash Reagents**	Flow Cell Wash Kit	ONT `EXP-WSH004`
☐	**Auxiliary**	Sequencing Auxiliary Vials V14	ONT `EXP-AUX003`
☐	**Quantification**	Qubit dsDNA HS Assay Kit & Assay Tubes	Invitrogen `Q32851` / `Q32856`
☐	**Plastics**	DNA LoBind Tubes (1.5 mL, 2.0 mL) & 96-Well PCR Plates	Eppendorf LoBind
☐	**Reagents**	Nuclease-free water & Freshly prepared 80% Ethanol	Molecular biology grade
☐	**Hardware**	PromethION Instrument with Flow Cell Light Shield	Oxford Nanopore Technologies
☐	**Hardware**	Thermal Cycler, Magnetic Rack, Microcentrifuge, Rotator	Standard molecular biology laboratory

Appendix B. Barcode Assignment and Sample-Tracking Template

Table 27. 24-Sample barcode logging template

Barcode	Sample Identifier	Target Marker	Amplicon Length (bp)	Qubit Concentration (ng/µL)	Calculated Mass for 200 fmol (ng)	Volume Added (µL)
NB01						
NB02						
NB03						
NB04						
NB05						
NB06						
NB07						
NB08						
NB09						
NB10						
NB11						
NB12						
NB13						
NB14						
NB15						
NB16						
NB17						
NB18						
NB19						
NB20						
NB21						
NB22						
NB23	Extraction Blank					
NB24	PCR No-Template Control (NTC)					

Appendix C. DNA Mass-to-Molarity Calculation Worksheet

Mass (ng) = [fmol × Length (bp) × 660] / 1,000,000 fmol = [Mass (ng) × 1,000,000] / [Length (bp) × 660]

Table 28. Amplicon normalisation worksheet

Sample ID	Marker Length (bp)	Qubit (ng/µL)	Target fmol	Required Mass (ng)	Required DNA Volume (µL)	Water Volume to Reach 11.5 µL
Sample 1			200			
Sample 2			200			
Sample 3			200			
Sample 4			200			
Sample 5			200			
Sample 6			200			

Worked calculation: A 1,500 bp amplicon at 35 ng/µL. Required mass for 200 fmol is 198 ng. DNA volume required: 198 ng / 35 ng/µL = 5.66 µL. Volume of nuclease-free water added: 11.50 µL - 5.66 µL = 5.84 µL.

Appendix D. Library Preparation Workflow Checklist

Table 29. Operational workflow verification checklist [MFR]

Step	Verified	Operational Parameter	Mandatory Protocol Specification
1. Input QC	☐	DNA Concentration & Size	200 fmol amplicon per sample in 11.5 µL nuclease-free water
2. End-Prep	☐	Thermal Cycler Program	20 °C for 5 min, then 65 °C for 5 min (15 µL reaction)
3. End-Prep Clean	☐	Bead Purification	1.0× AMPure XP (15 µL); two 200 µL 80% ethanol washes; elute in 10 µL water
4. Barcoding	☐	Native Barcode Ligation	7.5 µL DNA + 2.5 µL NB + 10 µL Blunt/TA mix; 20 min at RT; quench with 4 µL EDTA
5. Pooling	☐	Pooling & Cleanup	Combine 24 µL per sample; add 0.4× AMPure XP; wash 2× with 700 µL SFB; elute in 35 µL water
6. Adapter Ligation	☐	Native Adapter Attachment	30 µL pool + 5 µL NA + 10 µL 5× Buffer + 5 µL Ligase; 20 min at RT

Step	Verified	Operational Parameter	Mandatory Protocol Specification
7. Final Clean-up	☐	Adapter Bead Wash	Add 20 µL AMPure XP; wash 2× with 125 µL SFB (*no ethanol!*); elute in 25 µL EB
8. Library Dilution	☐	Flow Cell Loading Prep	Dilute 35–50 fmol of 1.5 kb library into 32 µL Elution Buffer (EB)

Appendix E. Flow Cell Loading Checklist

Table 30. Flow cell priming and loading checklist `[MFR]`

Step	Verified	Procedural Action
1. Acclimatisation	☐	Equilibrate flow cell to room temperature for 20 minutes before unsealing; inspect gold pins
2. System Check	☐	Run MinKNOW flow cell check; confirm ≥5,000 active pores on PromethION
3. Priming Mix Prep	☐	Combine 1,170 µL Flow Cell Flush (FCF) + 30 µL Flow Cell Tether (FCT) = 1,200 µL
4. Bubble Check	☐	Open inlet port; gently draw back ≤20 –30 µL until fluid enters tip to clear air
5. Prime 1	☐	Slowly dispense 500 µL priming mix into inlet port; wait exactly 5 minutes
6. Loading Mix Prep	☐	Vortex Library Beads (LIB) thoroughly; combine 100 µL SB + 68 µL LIB + 32 µL library = 200 µL
7. Prime 2	☐	Dispense remaining 500 µL priming mix into inlet port
8. Load Library	☐	Gently dispense 200 µL library loading mix into inlet port; close inlet port cover
9. Light Shield	☐	Affix PromethION Light Shield over flow cell window; close instrument lid
10. Incubation	☐	Wait 10 minutes before starting run to facilitate membrane tethering

Appendix F. FASTQ and Taxonomic Result Interpretation Guide

- **Unimodal Read Length:** Does the read length distribution center precisely on the expected marker size? Check for secondary peaks indicating primer-dimers (<200 bp) or chimeric amplicons.

- **Negative Control Validation:** Are read counts in extraction blanks and PCR NTCs near zero? Any taxa present in controls must be benchmarked against biological samples.
- **Unclassified Read Proportion:** Is the unclassified read fraction under 10–15%? High unclassified percentages point to reference database omissions, non-specific amplification, or overly stringent alignment thresholds.
- **Biological Plausibility:** Are dominant taxa consistent with known physiology for the sampled biome?
- **Rank-Appropriate Attribution:** Restrict claims to the taxonomic rank supported by marker variation (e.g. genus level for 16S V3–V4, species level for full-length 16S or ITS).

Appendix G. Glossary

Table 31. Technical glossary

Term	Definition
Amplicon	A specific target DNA fragment generated and exponentially copied through polymerase chain reaction (PCR) amplification
ASIC	Application-Specific Integrated Circuit; the micro-electronic sensor array underlying each flow cell channel that samples ionic currents
Basecalling	The computational process of translating raw continuous ionic current time series into discrete nucleotide strings using neural networks
Chimera	An artificial recombinant PCR artifact formed when an prematurely aborted amplicon primes another template in subsequent cycles
Connectionist Temporal Classification (CTC)	A neural network loss function allowing RNNs to output variable-length character sequences from continuous temporal data without frame alignment
Dorado	Oxford Nanopore's open-source, high-performance basecalling software engine powered by deep learning models
eDNA	Environmental DNA; cellular or extracellular genetic material shed into water, air, or soil by living organisms
Femtomole (fmol)	A unit of molecular quantity equal to 10^{-15} moles; corresponds to approximately 6.022×10^{8} double-stranded DNA molecules
Flow Cell Tether (FCT)	A lipid-conjugated synthetic oligonucleotide anchor present in the priming and loading mix that pre-concentrates DNA/RNA library molecules at the surface of the synthetic polymer membrane adjacent to the nanopores, dramatically improving pore capture rates and sequencing throughput
Homopolymer	A continuous run of identical contiguous bases (e.g. `AAAAAAA`); historically prone to indel errors on single-constriction nanopores
Kitome	The characteristic background microbial DNA profile unintentionally present in commercial extraction spin columns and lysis reagents

Term	Definition
Native Adapter (NA)	An engineered double-stranded sequencing adapter carrying the motor protein that unzips DNA and controls its translocation speed through the pore
Native Barcode (NB)	A defined synthetic double-stranded oligonucleotide identifier ligated to amplicon ends to allow sample multiplexing
Pore Occupancy	The percentage of active nanopores currently occupied and translocating DNA strands during an active sequencing run
POD5	ONT's modern, highly efficient columnar file format for storing raw electrical current measurements and device telemetry
R10.4.1	The current generation of ONT protein nanopores featuring dual-reader constrictions that resolve homopolymers and deliver >Q20 raw read accuracy
Short Fragment Buffer (SFB)	A specialized enzymatic wash buffer that retains DNA fragments across all sizes bound to beads while removing unbound adapters, excess enzymes, and short oligonucleotides

Appendix H. References and Software/Version Register

Primary Authoritative Sources `[MFR]`

- Oxford Nanopore Technologies. *Ligation sequencing amplicons – Native Barcoding Kit 24 V14 (`SQK-NBD114.24`), PromethION*. Document revision NBA_9168_v114_revU_15Jul2026.
- Oxford Nanopore Technologies. *EPI2ME `wf-16s` documentation*: https://epi2me.nanoporetech.com/epi2me-docs/workflows/wf-16s/ (accessed 8 Nov 2026).
- Oxford Nanopore Technologies. *MinKNOW Technical Document* (`MITD_5000_v1_revAK_25Nov2024`).

Literature Citations

- Barbera P, Kozlov AM, Czech L, et al. EPA-ng: massively parallel evolutionary placement of genetic sequences. *Syst Biol*. 2019;68(2):365–369. doi: 10.1093/sysbio/syy054
- Caspi R, Billington R, Ferrer L, et al. The MetaCyc database of metabolic pathways and enzymes and the BioCyc collection of pathway/genome databases. *Nucleic Acids Res*. 2018;46(D1):D633–D639. doi: 10.1093/nar/gkx1072
- Deamer D, Akeson M, Branton D. Three decades of nanopore sequencing. *Nat Biotechnol*. 2016;34(5):518–524. doi: 10.1038/nbt.3423
- Douglas GM, Maffei VJ, Zaneveld JR, et al. PICRUSt2 for prediction of metagenome functions. *Nat Biotechnol*. 2020;38(6):685–688. doi: 10.1038/s41587-020-0548-6
- Folmer O, Black M, Hoeh W, Lutz R, Vrijenhoek R. DNA primers for amplification of mitochondrial cytochrome c oxidase subunit I from diverse metazoan invertebrates. *Mol Mar Biol Biotechnol*. 1994;3(5):294–299.
- Gloor GB, Macklaim JM, Pawlowsky-Glahn V, Egozcue JJ. Microbiome datasets are compositional: and this is not optional. *Front Microbiol*. 2017;8:2224. doi: 10.3389/fmicb.2017.02224

- Hebert PDN, Cywinska A, Ball SL, deWaard JR. Biological identifications through DNA barcodes. *Proc R Soc B*. 2003;270(1512):313–321. doi: 10.1098/rspb.2002.2218
- Jain M, Olsen HE, Paten B, Akeson M. The Oxford Nanopore MinION: delivery of nanopore sequencing to the genomics community. *Genome Biol*. 2016;17:239. doi: 10.1186/s13059-016-1103-0
- Johnson JS, Spakowicz DJ, Hong BY, et al. Evaluation of 16S rRNA gene sequencing for species and strain-level microbiome analysis. *Nat Commun*. 2019;10:5029. doi: 10.1038/s41467-019-13036-1
- Kebschull JM, Zador AM. Sources of PCR-induced distortions in high-throughput sequencing data sets. *Nucleic Acids Res*. 2015;43(21):e143. doi: 10.1093/nar/gkv717
- Leray M, Yang JY, Meyer CP, Mills SC, Agudelo N, Ranwez V, Boehm JT, Machida RJ. A new versatile primer set targeting a short fragment of the mitochondrial COI region for metabarcoding metazoan diversity: application for characterizing coral reef fish gut contents. *Front Zool*. 2013;10:34. doi: 10.1186/1742-9994-10-34
- Li H. Minimap2: pairwise alignment for nucleotide sequences. *Bioinformatics*. 2018;34(18):3094–3100. doi: 10.1093/bioinformatics/bty191
- Louca S, Doebeli M. Efficient comparative phylogenetics on large trees. *Bioinformatics*. 2018;34(6):1053–1055. doi: 10.1093/bioinformatics/bty054
- Lu J, Breitwieser FP, Thielen P, Salzberg SL. Bracken: estimating species abundance in metagenomics data. *PeerJ Comput Sci*. 2017;3:e104. doi: 10.7717/peerj-cs.104
- McMurdie PJ, Holmes S. Waste not, want not: why rarefying microbiome data is inadmissible. *PLoS Comput Biol*. 2014;10(4):e1003531. doi: 10.1371/journal.pcbi.1003531
- Miya M, Sato Y, Fukunaga T, et al. MiFish, a set of universal PCR primers for metabarcoding environmental DNA from fishes: detection of more than 230 subtropical marine species. *R Soc Open Sci*. 2015;2(7):150088. doi: 10.1098/rsos.150088
- Nguyen NH, Song Z, Bates ST, et al. FUNGuild: an open annotation tool for parsing fungal community datasets by ecological guild. *Fungal Ecol*. 2016;20:241–248. doi: 10.1016/j.funeco.2015.06.006
- O'Leary NA, Wright MW, Brister JR, et al. Reference sequence (RefSeq) database at NCBI: current status, taxonomic expansion, and functional annotation. *Nucleic Acids Res*. 2016;44(D1):D733–D745. doi: 10.1093/nar/gkv1189
- Quast C, Pruesse E, Yilmaz P, et al. The SILVA ribosomal RNA gene database project: improved data processing and web-based tools. *Nucleic Acids Res*. 2013;41(D1):D590–D596. doi: 10.1093/nar/gks1219
- Rang FJ, Kloosterman WP, de Ridder J. From squiggle to basepair: computational approaches for improving nanopore sequencing read accuracy. *Genome Biol*. 2018;19:90. doi: 10.1186/s13059-018-1462-9
- Salter SJ, Cox MJ, Turek EM, et al. Reagent and laboratory contamination can critically impact sequence-based microbiome analyses. *BMC Biol*. 2014;12:87. doi: 10.1186/s12915-014-0087-z
- Schoch CL, Seifert KA, Huhndorf S, et al. Nuclear ribosomal internal transcribed spacer (ITS) region as a universal DNA barcode marker for Fungi. *Proc Natl Acad Sci USA*. 2012;109(16):6241–6246. doi: 10.1073/pnas.1117018109
- Stoddard SF, Smith BJ, Hein R, Roller BRK, Schmidt TM. rrnDB: improved tools for interpreting rRNA gene abundance in bacteria and archaea and a new foundation for future development. *Nucleic Acids Res*. 2015;43(Database issue):D593–D598. doi: 10.1093/nar/gku1201
- rrnDB: Ribosomal RNA Operon Copy Number Database. Version 5.8. University of Michigan; 2023. Available from: https://rrndb.umms.med.umich.edu/ (Accessed November 2026; documents 1 to 21 copies per bacterial genome).
- Wick RR, Judd LM, Holt KE. Performance of neural network basecalling tools for Oxford Nanopore sequencing. *Genome Biol*. 2019;20(1):129. doi: 10.1186/s13059-019-1727-y

- Taberlet P, Coissac E, Hajibabaei M, Rieseberg LH. Environmental DNA (Introduction to a special issue). *Mol Ecol*. 2012;21(8):1789–1793. doi: 10.1111/j.1365-294X.2012.05542.x
- Taberlet P, Coissac E, Pompanon F, et al. Power and limitations of the chloroplast trnL (UAA) intron for plant DNA barcoding. *Nucleic Acids Res*. 2007;35(3):e14. doi: 10.1093/nar/gkl938
- Wang Y, Zhao Y, Bollas A, Wang Y, Au KF. Nanopore sequencing technology, bioinformatics and applications. *Nat Biotechnol*. 2021;39(11):1348–1365. doi: 10.1038/s41587-021-01108-x
- Wood DE, Lu J, Langmead B. Improved metagenomic analysis with Kraken 2. *Genome Biol*. 2019;20:257. doi: 10.1186/s13059-019-1891-0

Software and Version Register `[LAB]`

Table 32. Analysis run tracking register

Component	Deployed Version	Execution Parameters / Checksums
MinKNOW Acquisition Software		
Dorado Basecaller & Model		
EPI2ME Desktop / `wf-16s`		
Nextflow & Container Engine		
Taxonomic Reference Database & Snapshot Date		
Downstream Visualization & Ecology Packages		