A60 short-segment recovery versus false alarms

Main · selection

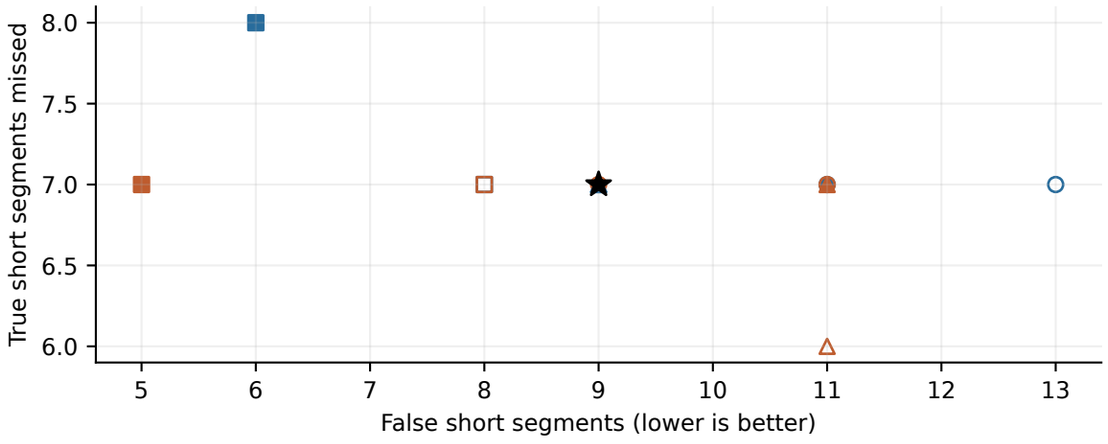

Main · calibration

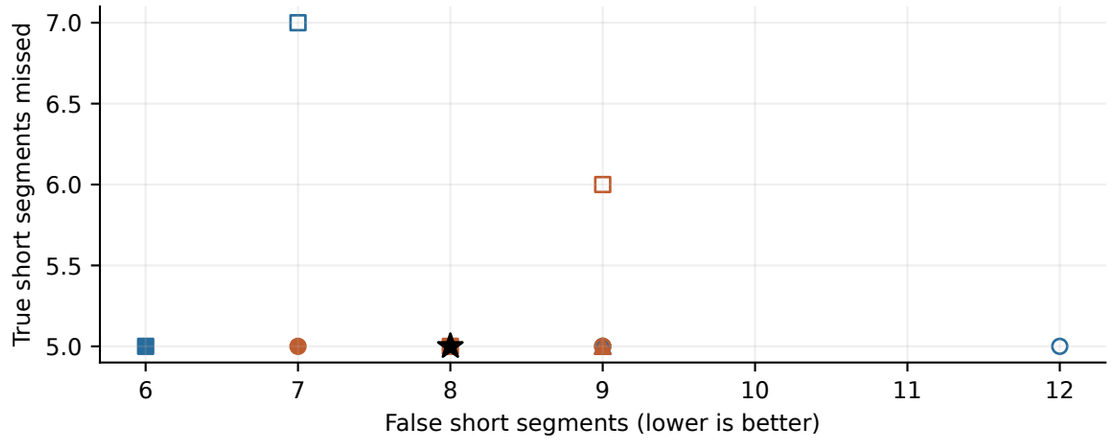

A58 reused stress · selection

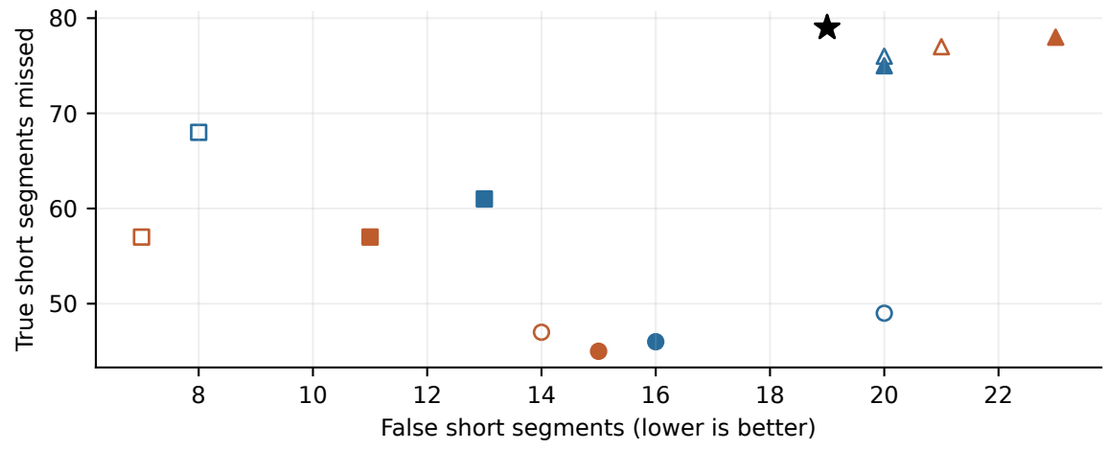

A58 reused stress · calibration

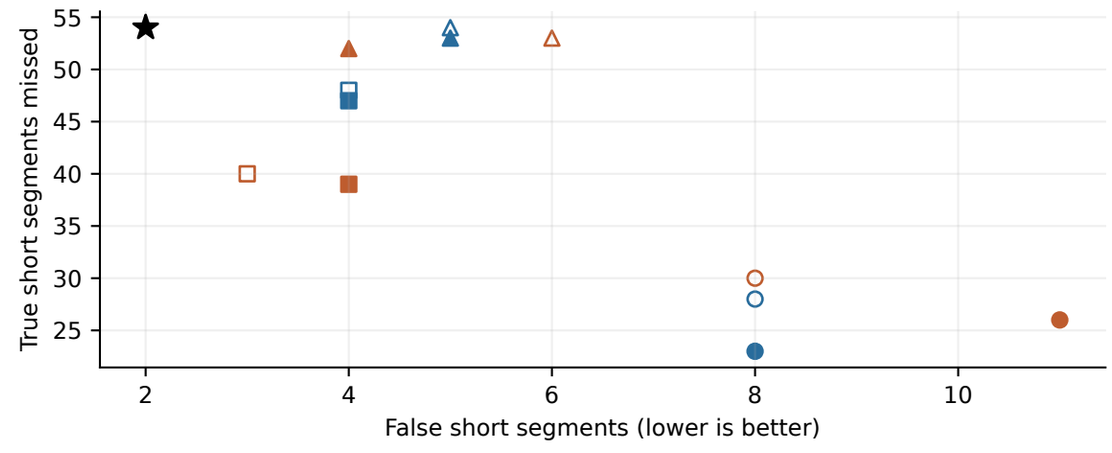

A59 reused bank · selection

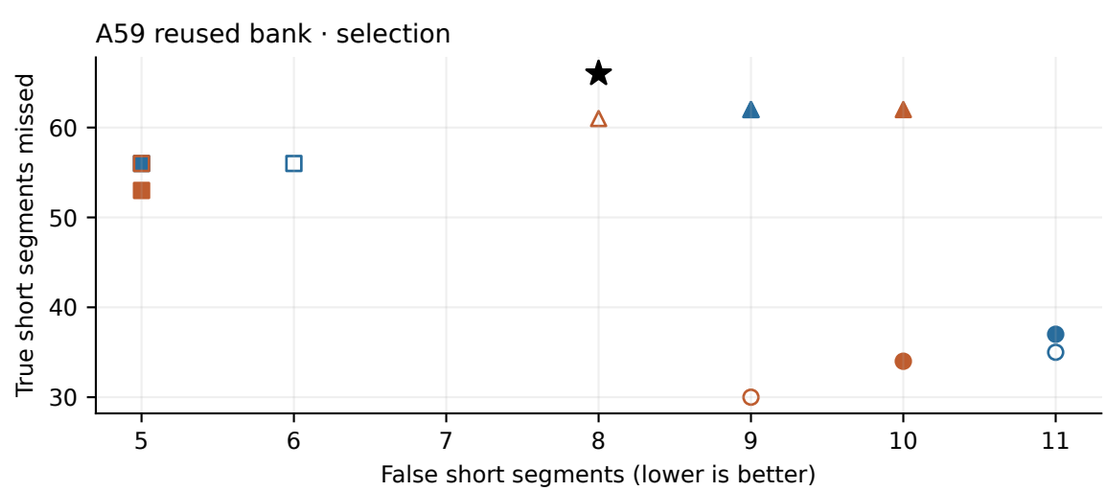

A59 reused bank · calibration

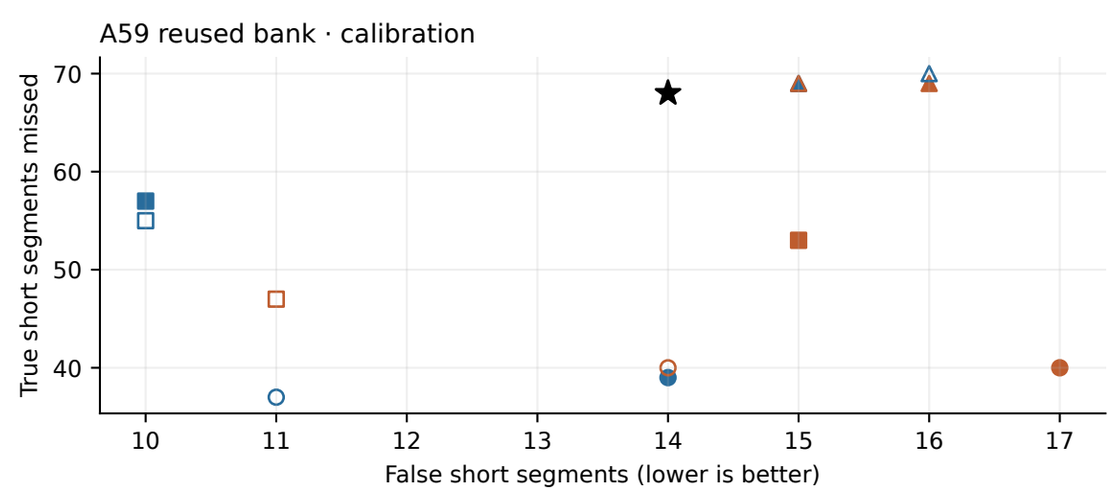

A60 fresh construction · selection

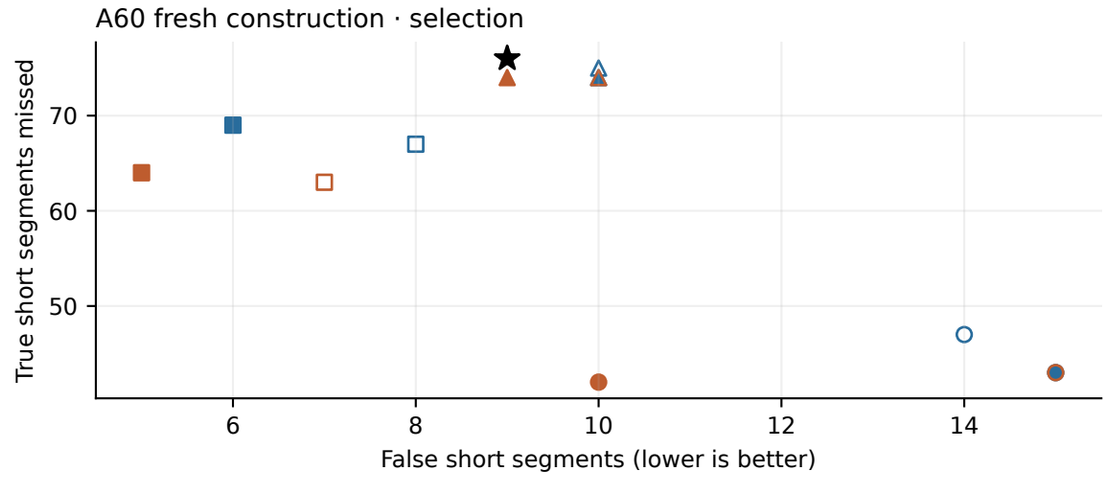

A60 fresh construction · calibration

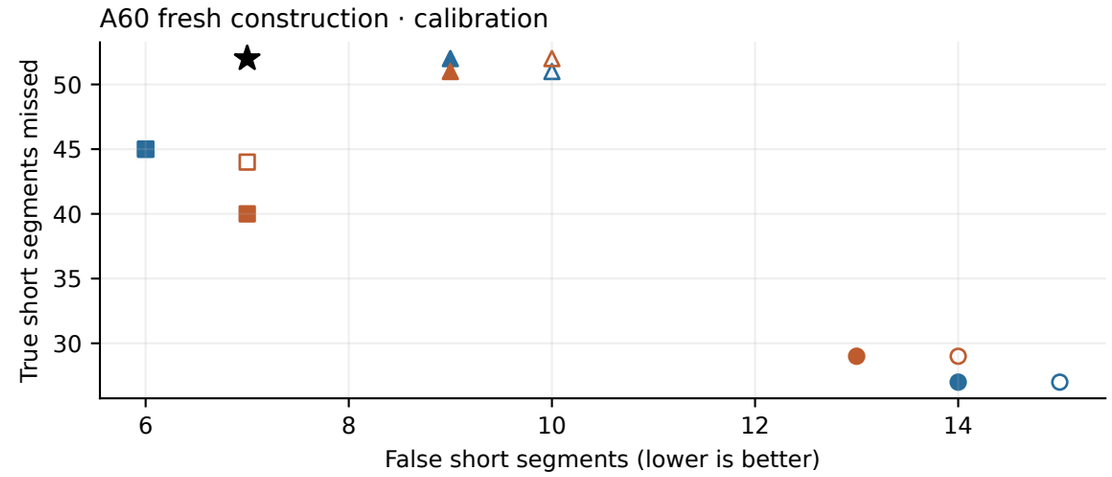

▲ A-O ● A-E ■ A-R ▲ J-O ● J-E ■ J-R ★ A08 anchor

Filled = seed 1; hollow = seed 2. Short ≤16 positions; class-aware IoU50 matching. All 12 fixed policies and the same A08 anchor appear per panel.

Lower left improves both counts. A60 fresh construction reuses OPEN sources; none of these panels establish independent patient or clinical evidence.