# Empirical calibrated veto: coverage and remaining outer false-safe evidence

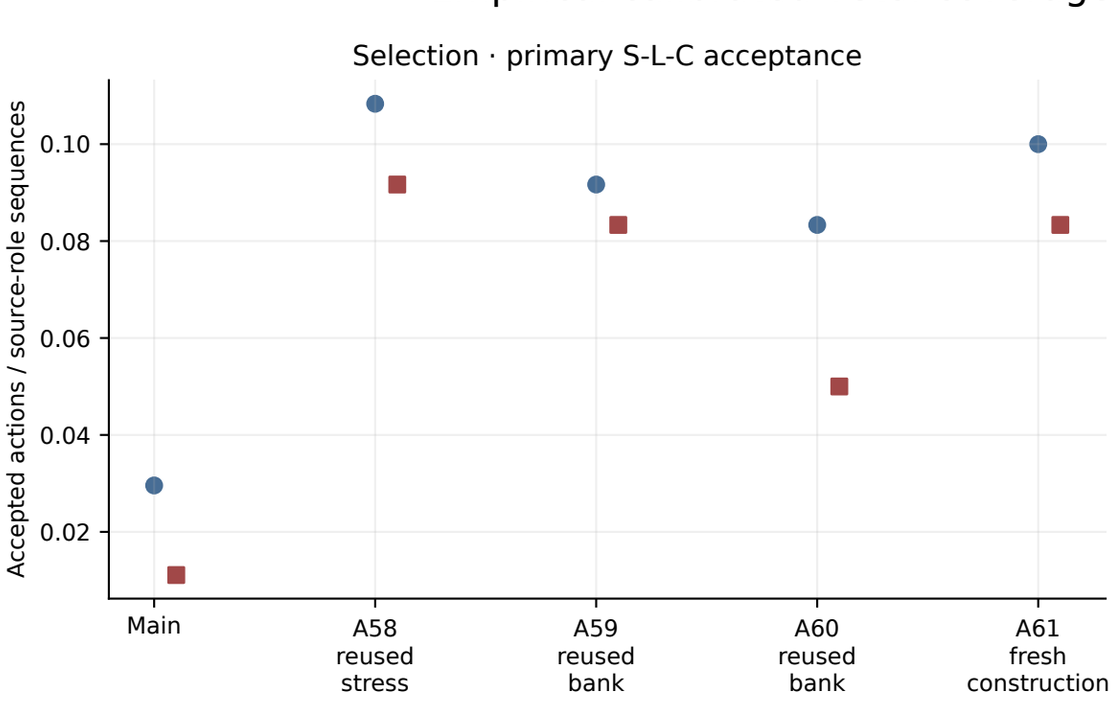


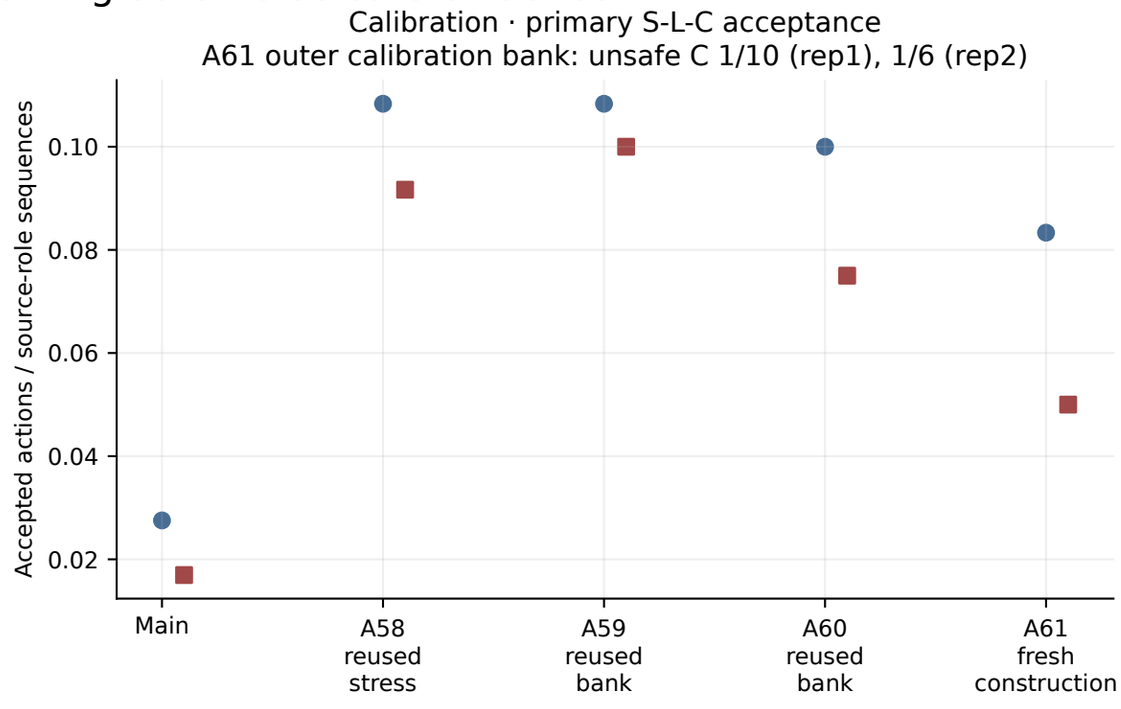


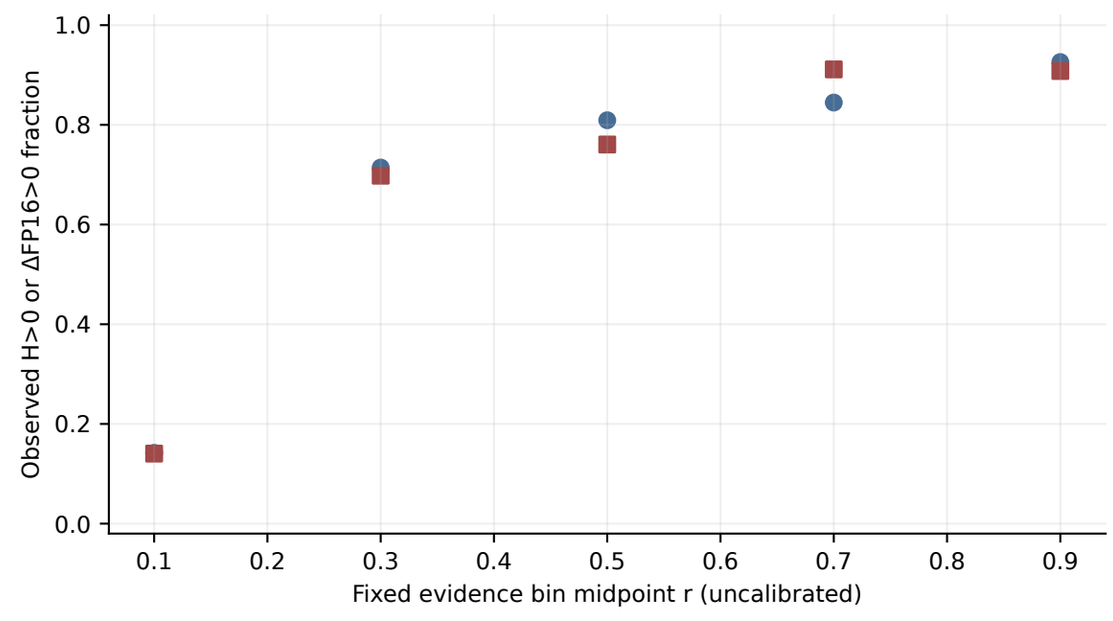


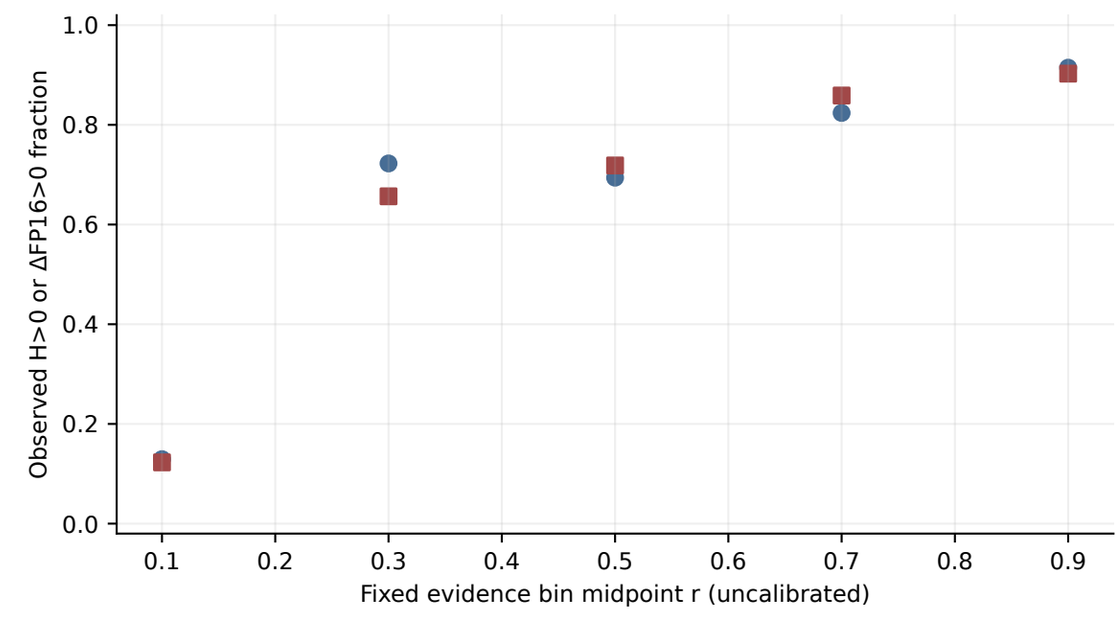


Blue/red=seed1/2. All G candidates, not accepted-only, enter the five fixed risk bins; shared-risk candidate repeats across utility arms are excluded.

C calibration uses all928 inner diagnostic/calibration axes; zero unsafe inner accepts can mean no-op. No finite-sample or clinical guarantee.

Source-role panels use main native/multi/pair once and four separate constructed banks; shared source recordings are not independent observations.