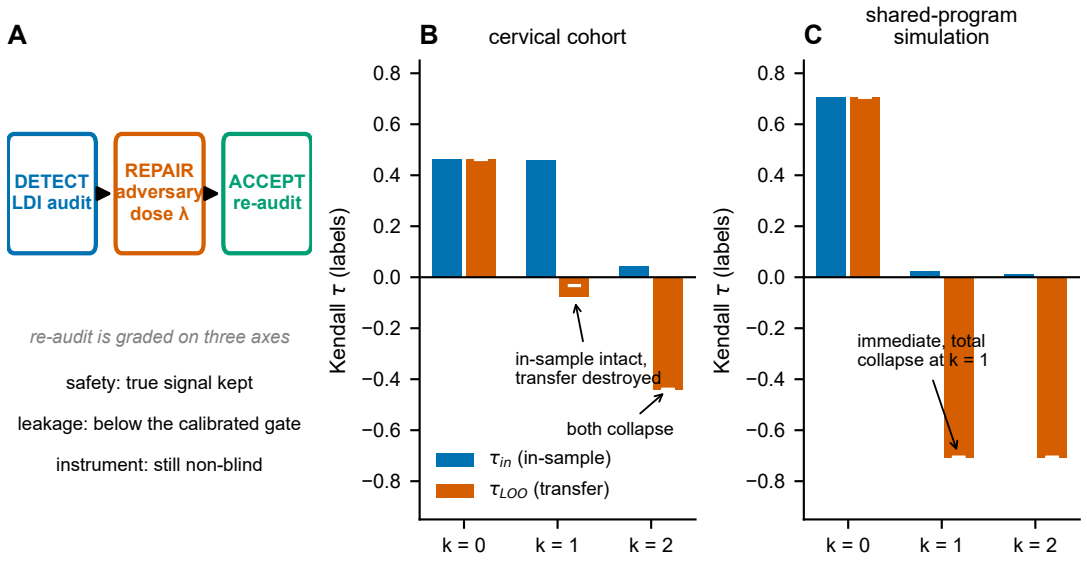

A
DETECT
LDI audit
REPAIR
adversary
dose λ
ACCEPT
re-audit
re-audit is graded on three axes
safety: true signal kept
leakage: below the calibrated gate
instrument: still non-blind
B
cervical cohort
Kendall τ (labels)
0.8
0.6
0.4
0.2
0.0
−0.2
−0.4
−0.6
−0.8
in-sample intact,
transfer destroyed
both collapse
τ_{in} (in-sample)
τ_{LOO} (transfer)
k = 0
k = 1
k = 2
C
shared-program
simulation
Kendall τ (labels)
immediate, total
collapse at k = 1
k = 0
k = 1
k = 2