Example Person

Diagnosis: Essential Tremor

Patient ID: SYN:0002 **Gender:** Male **Date Of Birth:** Nov 2, 1955

Clinician Notes:
Second invented record.

DEVICE

NEUROSTIMULATOR	Serial Number	Implanted
Percept RC	SYN_RC_0002	Feb 3, 2026
Product Application ID:	**Product Version:**	**Model Number**
0000	01.02.03	TEST-RC-02
Core Application ID:	**Core Version:**	**Device Name**
0000	00.01.00	Unit B
Device Application ID:	**Device Version:**	**Components**
0000	00.02.00	Right Chest
Battery Level	**ERI Date**	
64%	Feb 28, 2041	


Feature Information Code
2c3d

STIMULATION SETTINGS

	Initial	Final
STIMULATION	Off	On
CHECK BATTERY REMINDER	Off	Off
CLOSE COMMUNICATION REQUIRED FOR THERAPY OFF	ON	ON


Lead Configuration

Left STN




Contacts: 0–7
Lead Model: B33005
Orientation: 60 °

Right STN




Contacts: 8–15
Lead Model: B33005
Orientation: 300 °

Left STN



Contacts: 0–7
Lead Model: B33005
Orientation: 60 °


Right STN



Contacts: 8–15
Lead Model: B33005
Orientation: 300 °

Group A (Reach)


Left STN



2.9 mA
60 µs
130 Hz

1a: 1.0 mA
1b: 1.0 mA
1c: 1.0 mA

Right STN




3.4 mA
60 µs
130 Hz

8: 1.2 mA
9a: 1.0 mA
9b: 1.0 mA
9c: 1.0 mA

Group A (Reach)


Left STN



3.2 mA
60 µs
130 Hz

1a: 1.0 mA
1b: 1.0 mA
1c: 1.0 mA

Right STN




3.4 mA
60 µs
130 Hz


8: 1.2 mA
9a: 1.0 mA
9b: 1.0 mA
9c: 1.0 mA

Group B (Stand)

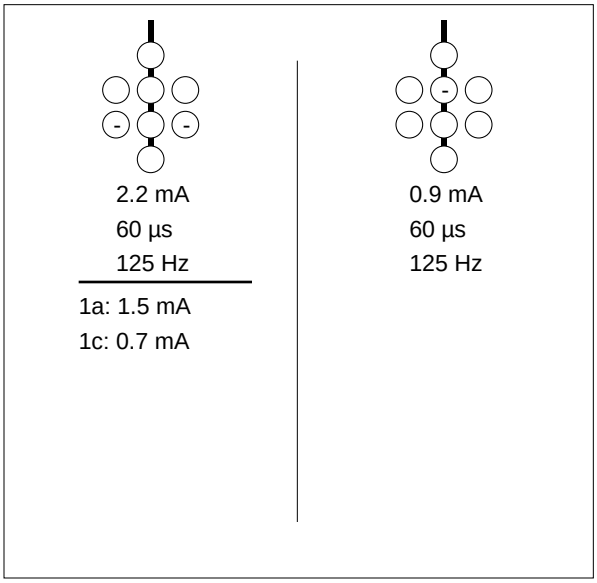Left STN




Right STN

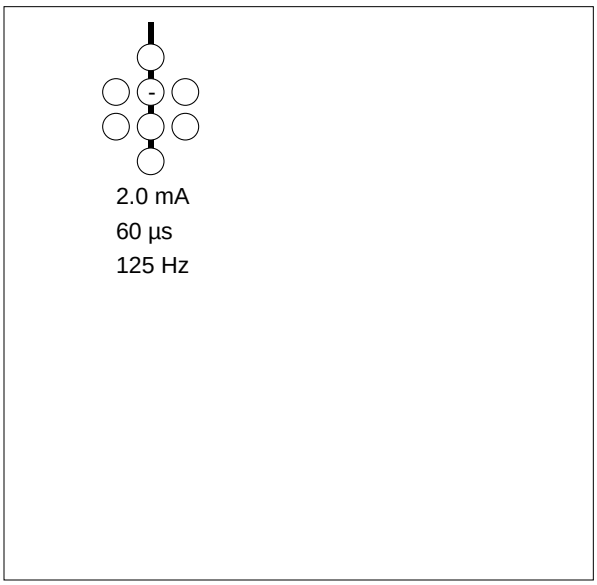


Group B (Stand)

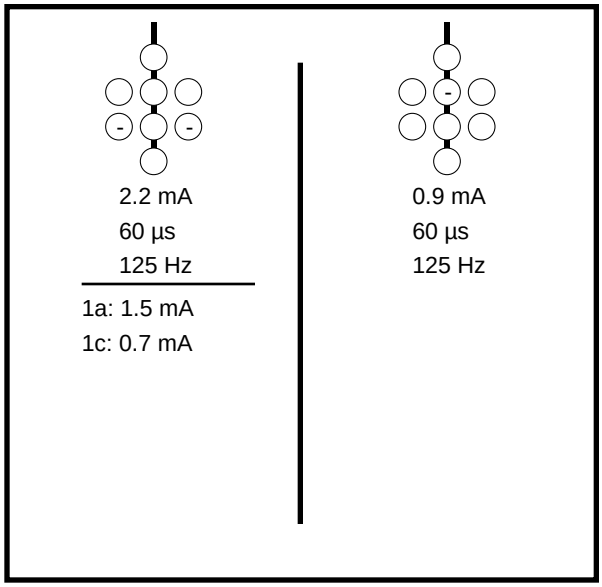Left STN




Right STN

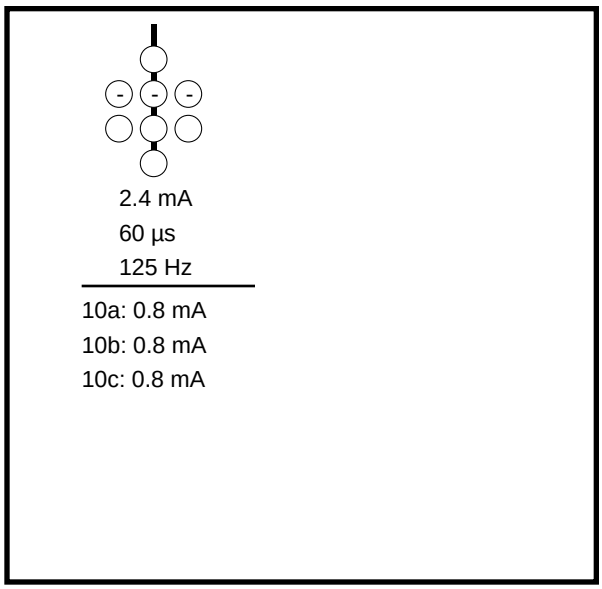

Group C (Imaging)


Left STN



1.3 mA
60 µs
150 Hz

1a: 0.4 mA
1b: 0.4 mA
1c: 0.4 mA

Right STN




1.3 mA
60 µs
100 Hz

10a: 0.4 mA
10b: 0.4 mA
10c: 0.4 mA

Group C (Imaging)


Left STN



1.3 mA
60 µs
150 Hz

1a: 0.4 mA
1b: 0.4 mA
1c: 0.4 mA

Right STN




1.3 mA
60 µs
100 Hz

10a: 0.4 mA
10b: 0.4 mA
10c: 0.4 mA

Group D (Sense)

Left STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.3 mA
60 µs
125 Hz

1a: 1.0 mA
1b: 0.6 mA

SENSING SETUP

LFP Frequency: 24.41 Hz

THRESHOLD MODE

Mode: Dual Threshold

Upper LFP Threshold:	Lower LFP Threshold:
50	20
Captured: 30	Captured: 18

ADAPTIVE SETUP

Maximum Limit:3.2 mA

Paused Amplitude: 2.6 mA

Minimum Limit:2.2 mA


Transition Duration:

Transition Up: 2.3 mins

Transition Down: 5.0 mins

Group D (Sense)

Left STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.6 mA
60 µs
125 Hz

1a: 1.0 mA
1b: 0.6 mA

SENSING SETUP

LFP Frequency: 24.41 Hz

THRESHOLD MODE

Mode: Dual Threshold

Upper LFP Threshold:	Lower LFP Threshold:
50	20
Captured: 30	Captured: 18

ADAPTIVE SETUP

Maximum Limit:3.2 mA

Paused Amplitude: 2.6 mA


Minimum Limit:2.2 mA

Transition Duration:

Transition Up: 2.3 mins

Transition Down: 5.0 mins

Right STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.2 mA
60 µs
125 Hz

10a: 0.9 mA
10c: 0.7 mA

SENSING SETUP

LFP Frequency: 19.53 Hz

THRESHOLD MODE

Mode: Single Threshold

Upper LFP Threshold:	Lower LFP Threshold:
45	15
Captured: 28	Captured: 12

ADAPTIVE SETUP


Maximum Limit:3.0 mA

Paused Amplitude: 2.4 mA

Minimum Limit:2.0 mA

Transition Duration:
Transition Up: 1.5 mins
Transition Down: 4.0 mins

Right STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.2 mA
60 µs
125 Hz

10a: 0.9 mA
10c: 0.7 mA

SENSING SETUP

LFP Frequency: 19.53 Hz

THRESHOLD MODE

Mode: Single Threshold

Upper LFP Threshold:	Lower LFP Threshold:
45	15
Captured: 28	Captured: 12

ADAPTIVE SETUP

Maximum Limit:3.0 mA

Paused Amplitude: 2.4 mA

Minimum Limit:2.0 mA

Transition Duration:
Transition Up: 1.5 mins
Transition Down: 4.0 mins

PATIENT PROGRAMMER SETTINGS

Initial		Final	
Group A (Reach)		**Group A (Reach)**	
Left STN		Left STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 2.5 mA to 3.3 mA Value : 2.9 mA	Advanced Adjust	Program 1: 2.8 mA to 3.6 mA Value : 3.2 mA
Right STN		Right STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 3.0 mA to 3.8 mA Value : 3.4 mA	Advanced Adjust	Program 1: 3.0 mA to 3.8 mA Value : 3.4 mA
Group B (Stand)		**Group B (Stand)**	
Left STN		Left STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 1.8 mA to 2.6 mA Value : 2.2 mA	Advanced Adjust	Program 1: 1.8 mA to 2.6 mA Value : 2.2 mA
Right STN		Right STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust		Advanced Adjust	
Group C (Imaging)		**Group C (Imaging)**	
Left STN		Left STN	
Mode	**Parameter: View Amplitude**	**Mode**	**Parameter: View Amplitude**
Advanced View		Advanced View	
Right STN		Right STN	
Mode	**Parameter: View Amplitude**	**Mode**	**Parameter: View Amplitude**
Advanced View		Advanced View	
Group D (Sense)		**Group D (Sense)**	
Left STN		Left STN	
Mode	Parameter:	**Mode**	Parameter:
Adaptive Therapy Adapting between	Paused Amplitude: 2.6 mA Maximum Limit: 3.2 mA Minimum Limit: 2.2 mA	Adaptive Therapy Adapting between	Paused Amplitude: 2.6 mA Maximum Limit: 3.2 mA Minimum Limit: 2.2 mA
Right STN		Right STN	
Mode	Parameter:	**Mode**	Parameter:
Adaptive Therapy Adapting between	Paused Amplitude: 2.4 mA Maximum Limit: 3.0 mA Minimum Limit: 2.0 mA	Adaptive Therapy Adapting between	Paused Amplitude: 2.4 mA Maximum Limit: 3.0 mA Minimum Limit: 2.0 mA

GROUP SETTINGS

Group A (Reach)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group A (Reach)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group B (Stand)

SoftStart/Stop: Off
Cycling: Off

Group B (Stand)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group C (Imaging)

SoftStart/Stop: Off
Cycling: Off

Group C (Imaging)

SoftStart/Stop: Off
Cycling: Off

Group D (Sense)

SoftStart/Stop: 2 Seconds
Cycling: Off

Group D (Sense)

SoftStart/Stop: 2 Seconds
Cycling: Off

Group D (Sense)

Left STN

High Pass Filter: 1 Hz
Averaging Duration: 1.2 secs
Sensing Blanking Duration: 1.4 ms
Onset Duration:
Upper: 1.2 secs
Lower: 1.2 secs
Detection Blanking Duration: 2.0 secs
Adaptive Startup Delay: 10.0 secs

Right STN

High Pass Filter: 1 Hz
Averaging Duration: 3.0 secs
Sensing Blanking Duration: 1.1 ms
Onset Duration:
Upper: 0.8 secs
Lower: 1.6 secs
Detection Blanking Duration: 2.5 secs
Adaptive Startup Delay: 8.0 secs

Group D (Sense)

Left STN

High Pass Filter: 1 Hz
Averaging Duration: 1.2 secs
Sensing Blanking Duration: 1.4 ms
Onset Duration:
Upper: 1.2 secs
Lower: 1.2 secs
Detection Blanking Duration: 2.0 secs
Adaptive Startup Delay: 10.0 secs

Right STN

High Pass Filter: 1 Hz
Averaging Duration: 3.0 secs
Sensing Blanking Duration: 1.1 ms
Onset Duration:
Upper: 0.8 secs
Lower: 1.6 secs
Detection Blanking Duration: 2.5 secs
Adaptive Startup Delay: 8.0 secs

ELECTRODE IMPEDANCE

Impedance measured at Fixed test current

Left STN

MONOPOLAR

3	1,182
2c	1,393
2b	1,604
2a	>10,000
1c	2,026
1b	2,237
1a	2,448
0	759

BIPOLAR

	0	1a	1b	1c	2a	2b	2c
3	2,030	2,367	2,704	3,041	3,378	1,115	1,452
2c	1,789	2,126	2,463	2,800	3,137	3,474	
2b	1,211	1,548	1,885	2,222	2,559		
2a	2,896	3,233	3,570	1,307			
1c	1,644	1,981	2,318				
1b	2,655	2,992					
1a	3,329						

ELECTRODE IMPEDANCE

Impedance measured at Fixed test current

Right STN

MONOPOLAR










11	1,818
10c	2,029
10b	2,240
10a	2,451
9c	762
9b	973
9a	1,184
8	1,395

BIPOLAR










	8	9a	9b	9c	10a	10b	10c
11	2,882	3,219	3,556	1,293	1,630	1,967	2,304
10c	2,641	2,978	3,315	3,652	1,389	1,726	
10b	2,063	2,400	2,737	3,074	3,411		
10a	1,148	1,485	1,822	2,159			
9c	2,496	2,833	3,170				
9b	3,507	1,244					
9a	1,581						

GROUP HISTORY

Oct 14, 2026










A	 3.2 mA 60 µs 130 Hz	 3.4 mA 60 µs 130 Hz
B	 2.2 mA 60 µs 125 Hz	 0.9 mA 60 µs 125 Hz  2.4 mA 60 µs 125 Hz
C	 1.3 mA 60 µs 150 Hz	 1.3 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.6 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.2 mA 60 µs 125 Hz










Jul 2, 2026

A	 3.1 mA 60 µs 130 Hz	 3.3 mA 60 µs 130 Hz
B	 2.1 mA 60 µs 125 Hz	 0.8 mA 60 µs 125 Hz  2.3 mA 60 µs 125 Hz
C	 1.2 mA 60 µs 150 Hz	 1.2 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.5 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.1 mA 60 µs 125 Hz


Jun 2, 2026

May 3, 2026


A	 3.0 mA 60 µs 130 Hz	 3.2 mA 60 µs 130 Hz
B	 2.0 mA 60 µs 125 Hz	 0.7 mA 60 µs 125 Hz  2.2 mA 60 µs 125 Hz
C	 1.1 mA 60 µs 150 Hz	 1.1 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.4 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.0 mA 60 µs 125 Hz

A	 2.9 mA 60 µs 130 Hz	 3.1 mA 60 µs 130 Hz
B	 1.9 mA 60 µs 125 Hz	 0.6 mA 60 µs 125 Hz  2.1 mA 60 µs 125 Hz
C	 1.0 mA 60 µs 150 Hz	 1.0 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.3 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Adapting 1.9 mA 60 µs 125 Hz

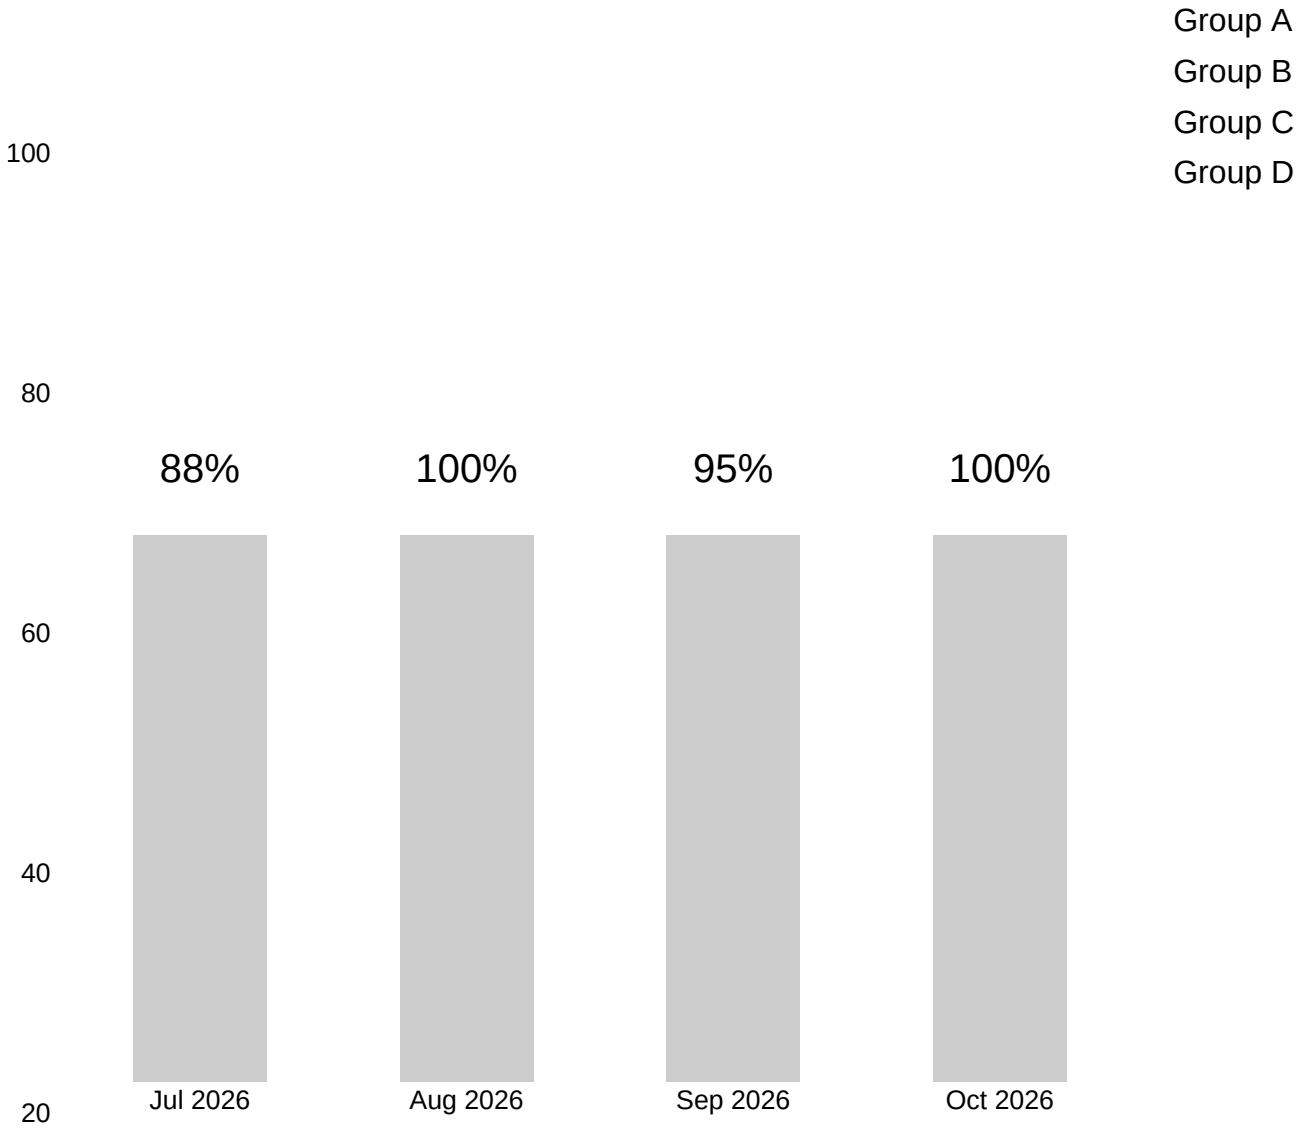GROUP USAGE


Group A
Group B
Group C
Group D
100
80
60
40
20
88%
100%
95%
100%
Jul 2026
Aug 2026
Sep 2026
Oct 2026

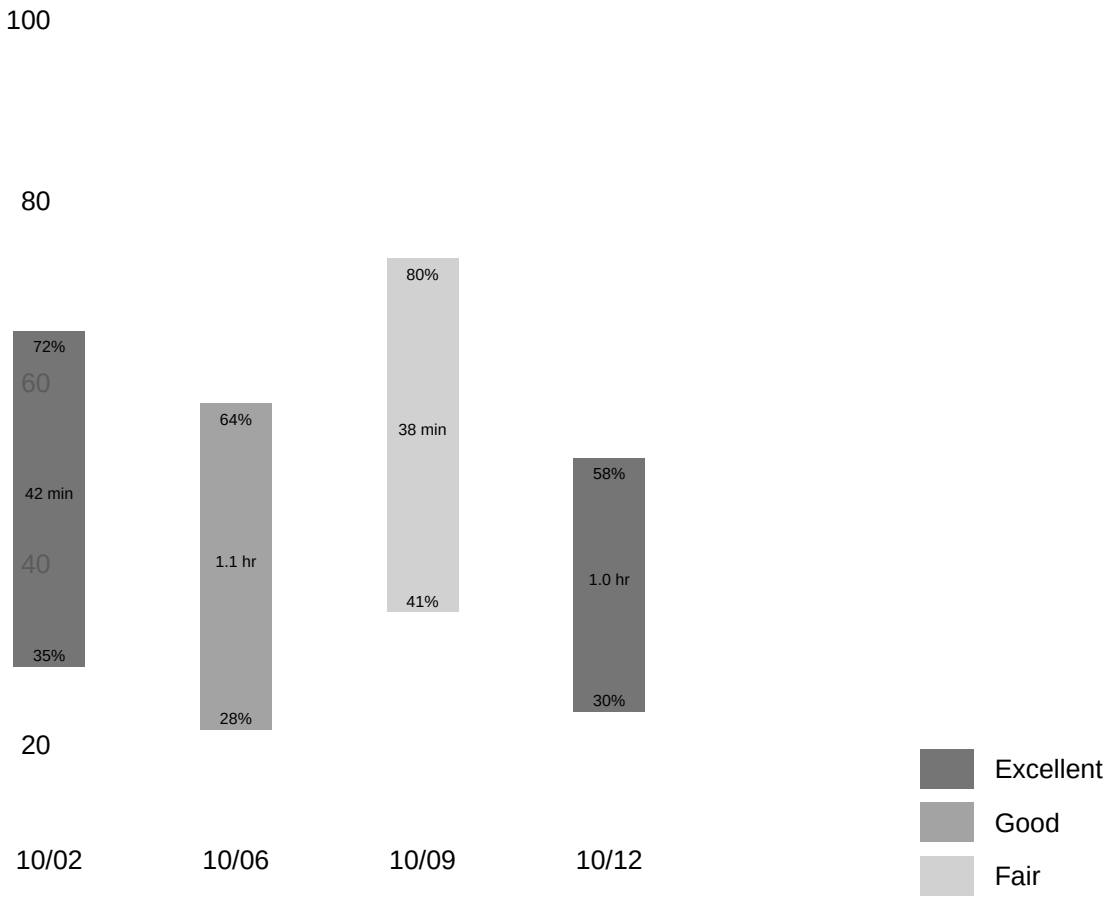BATTERY RECHARGE



Excellent

Recharge Coupling

68%
Avg. Ending

45 min
Avg. Recharge Time

3.4 days
Avg. Recharge Interval

SESSION ANNOTATIONS

	TREMOR	BRADYKINESIA	MOOD ALTERATION	MUSCLE CONTRACTIONS
LEFT HEMISPHERE				
CONFIGURATION				
May 11, 2026 2.40 mA 60 µs 130 Hz	2	1	0	-
Jun 15, 2026 1.95 mA 60 µs 130 Hz	1	-	2	3
RIGHT HEMISPHERE				
CONFIGURATION				
Jul 21, 2026 2.65 mA 60 µs 125 Hz	-	0	1	2

BRAINSENSE SURVEY

No Data Available

ELECTRODE IDENTIFIER

No Data Available

PATIENT EVENTS

Initial	Final
Name: Medication taken Additional Behavior:Early dose	Name: Fall

EVENT SUMMARY

Events	Jul 02 – Oct 14
Medication taken	12
Tremor episode	4
Fall	1

Group D Left STN	Jul 02 – Oct 14
Above Threshold	41%
Between Thresholds	30%
Below Threshold	29%
Average Amplitude	2.62
Adaptive Amplitude Reduction	12%
Time Adaptive Running	87%

Group D Right STN	Jul 02 – Oct 14
Above Threshold	35%
Between Thresholds	40%
Below Threshold	25%
Average Amplitude	2.41
Adaptive Amplitude Reduction	9%
Time Adaptive Running	91%

END OF REPORT