Sample Patient

Diagnosis: Parkinson's Disease

Patient ID: SYN:0001 **Gender:** Female **Date Of Birth:** Mar 17, 1961

Clinician Notes:
Invented test record.
Not a real patient.

DEVICE

NEUROSTIMULATOR	Serial Number	Implanted
Percept PC	SYN_PC_0001	Jan 20, 2026
Product Application ID:	**Product Version:**	**Model Number**
0000	01.02.03	TEST-PC-01
Core Application ID:	**Core Version:**	**Device Name**
0000	00.01.00	--
Device Application ID:	**Device Version:**	**Components**
0000	00.02.00	Left Chest
Battery Level	**Estimated Battery Remaining**	
82%	(based on last 7 days) 3 years, 6 months	


Feature Information Code
0a1b

STIMULATION SETTINGS


	Initial	Final
STIMULATION	On	On
CHECK BATTERY REMINDER	09:30	09:30
CLOSE COMMUNICATION REQUIRED FOR THERAPY OFF	ON	ON

Lead Configuration


Left STN

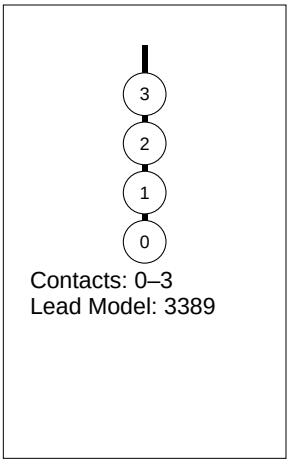


Right STN

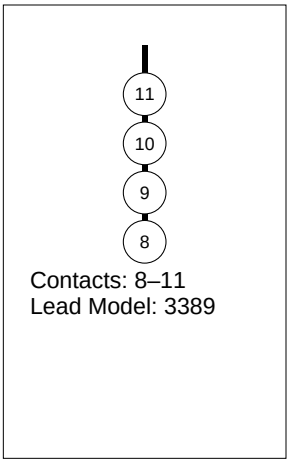

Left STN

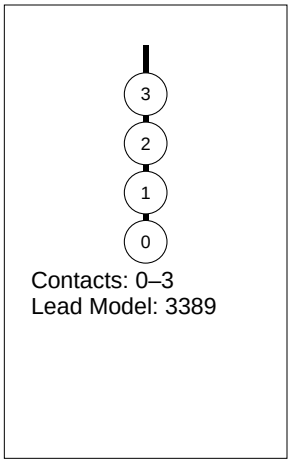


Right STN

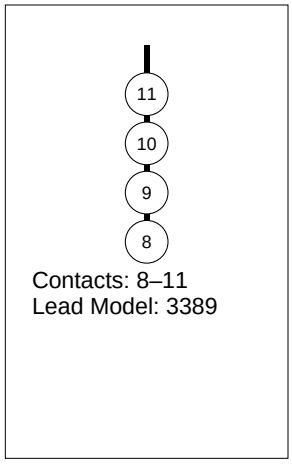


Group A (Gait)

Left STN

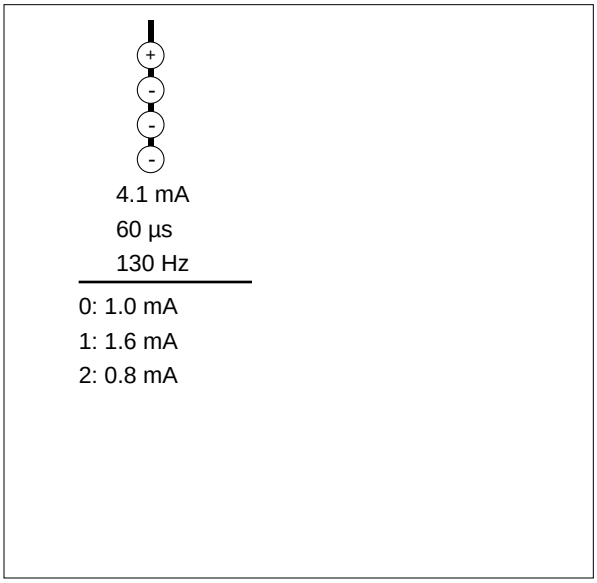


Right STN

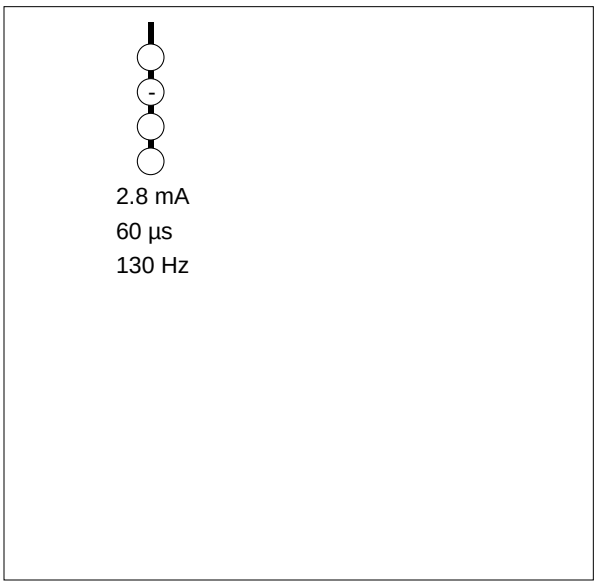


Group A (Gait)

Left STN

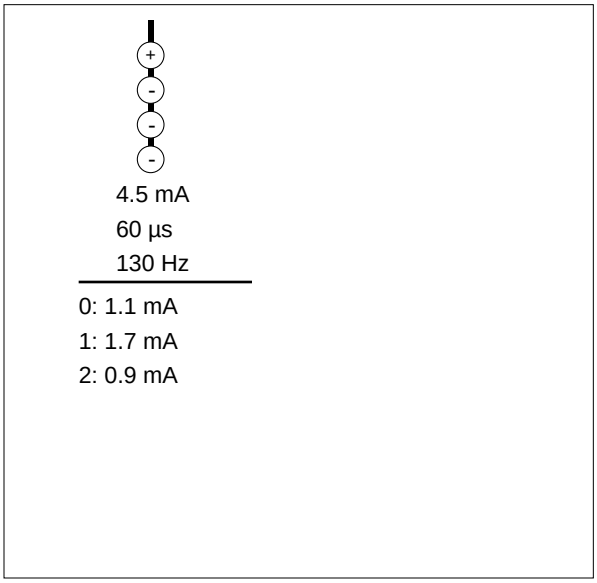


Right STN

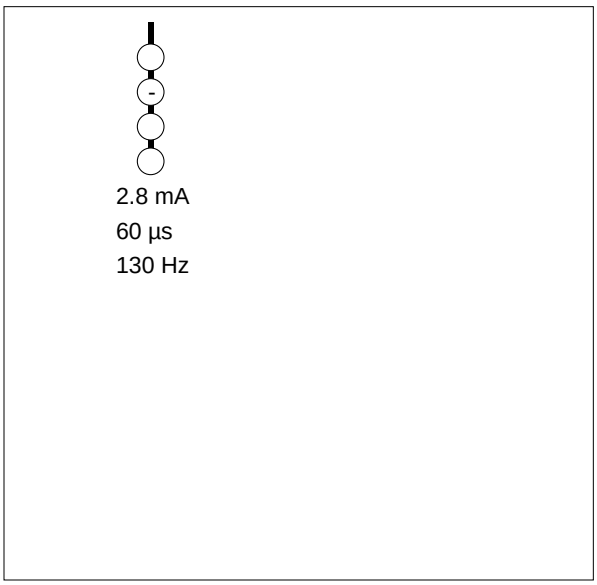


Group B (Speech)

Left STN

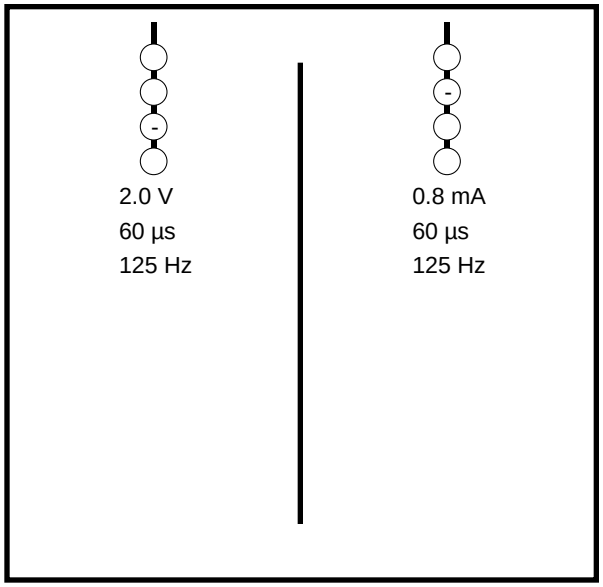


Right STN

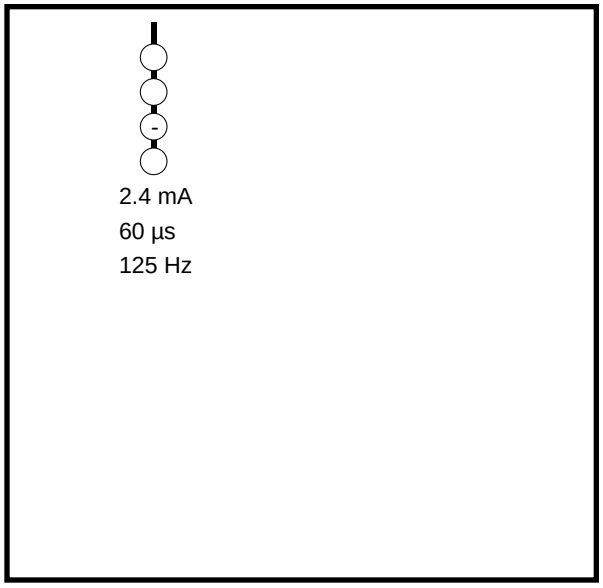


Group B (Speech)

Left STN

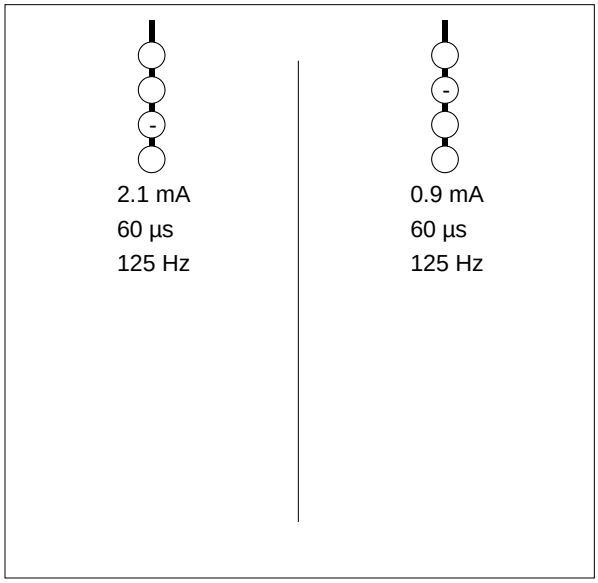


Right STN

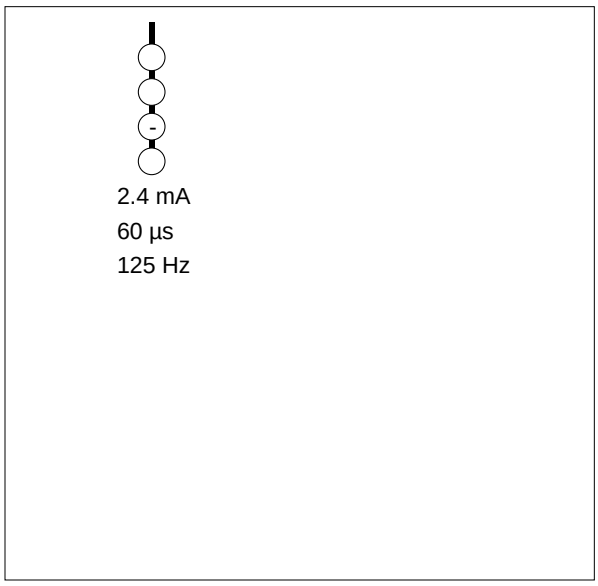


Group C

Left STN

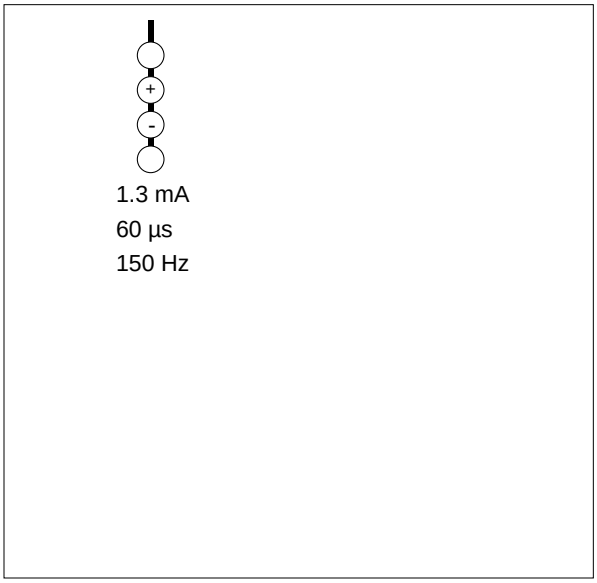


Right STN

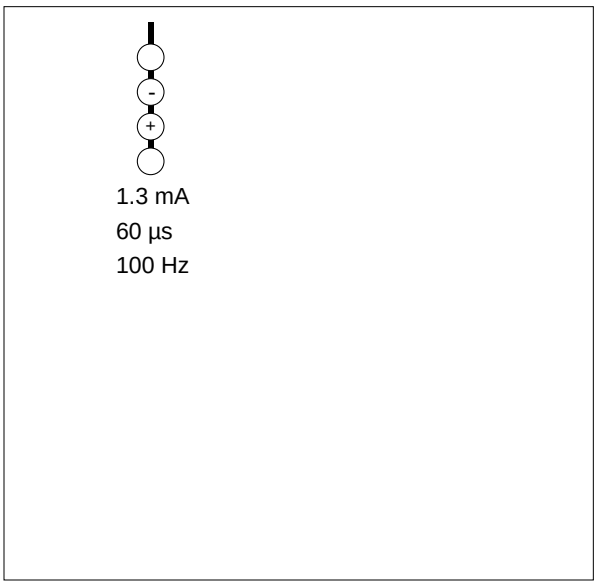


Group C (Scan)

Left STN

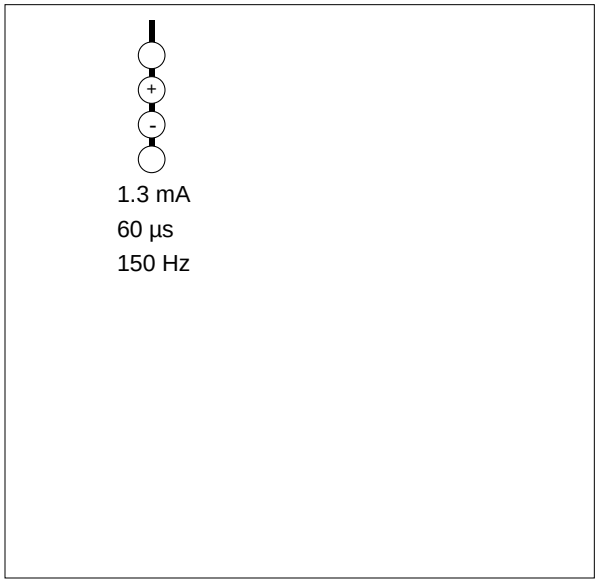

Right STN

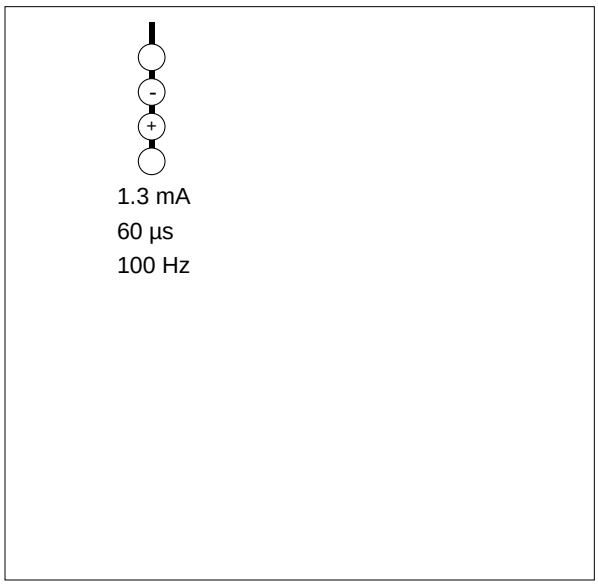

Group D (Adaptive)

Left STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.4 mA
60 µs
125 Hz

SENSING SETUP

LFP Frequency: 24.41 Hz

THRESHOLD MODE

Mode: Dual Threshold

Upper LFP Threshold:	Lower LFP Threshold:
50	20
Captured: 30	Captured: 18

ADAPTIVE SETUP

Maximum Limit:3.2 mA

Paused Amplitude: 2.6 mA

Minimum Limit:2.2 mA

Transition Duration:

Transition Up: 2.3 mins

Transition Down: 5.0 mins

Group D (Adaptive)

Left STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.6 mA
60 µs
125 Hz

SENSING SETUP

LFP Frequency: 24.41 Hz

THRESHOLD MODE

Mode: Dual Threshold

Upper LFP Threshold:	Lower LFP Threshold:
50	20
Captured: 30	Captured: 18

ADAPTIVE SETUP

Maximum Limit:3.2 mA

Paused Amplitude: 2.6 mA

Minimum Limit:2.2 mA

Transition Duration:

Transition Up: 2.3 mins

Transition Down: 5.0 mins

Right STN



BrainSense: Adaptive
Adaptive Therapy: Adapting
2.2 mA
60 µs
125 Hz

9: 1.1 mA
10: 1.1 mA

SENSING SETUP

LFP Frequency: 19.53 Hz

THRESHOLD MODE

Mode: Single Threshold

Upper LFP Threshold:	Lower LFP Threshold:
45	15
Captured: 28	Captured: 12

ADAPTIVE SETUP

Maximum Limit:3.0 mA

Paused Amplitude: 2.4 mA

Minimum Limit:2.0 mA

Transition Duration:
Transition Up: 1.5 mins
Transition Down: 4.0 mins

Right STN



BrainSense: Adaptive
Adaptive Therapy: Paused
2.4 mA
60 µs
125 Hz

9: 1.2 mA
10: 1.2 mA

SENSING SETUP

LFP Frequency: 19.53 Hz

THRESHOLD MODE

Mode: Single Threshold

Upper LFP Threshold:	Lower LFP Threshold:
45	15
Captured: 28	Captured: 12

ADAPTIVE SETUP

Maximum Limit:3.0 mA

Paused Amplitude: 2.4 mA

Minimum Limit:2.0 mA

Transition Duration:
Transition Up: 1.5 mins
Transition Down: 4.0 mins

PATIENT PROGRAMMER SETTINGS

Initial		Final	
Group A (Gait)		**Group A (Gait)**	
Left STN		Left STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 3.7 mA to 4.5 mA Value : 4.1 mA	Advanced Adjust	Program 1: 4.1 mA to 4.9 mA Value : 4.5 mA
Right STN		Right STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 2.4 mA to 3.2 mA Value : 2.8 mA	Advanced Adjust	Program 1: 2.4 mA to 3.2 mA Value : 2.8 mA
Group B (Speech)		**Group B (Speech)**	
Left STN		Left STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust	Program 1: 1.6 mA to 2.4 mA Value : 2.0 mA	Advanced Adjust	Program 1: 1.7 mA to 2.5 mA Value : 2.1 mA
Right STN		Right STN	
Mode	**Parameter: Adjust Amplitude**	**Mode**	**Parameter: Adjust Amplitude**
Advanced Adjust		Advanced Adjust	
Group C		**Group C (Scan)**	
Left STN		Left STN	
Mode	**Parameter: View Amplitude**	**Mode**	**Parameter: View Amplitude**
Advanced View		Advanced View	
Right STN		Right STN	
Mode	**Parameter: View Amplitude**	**Mode**	**Parameter: View Amplitude**
Advanced View		Advanced View	
Group D (Adaptive)		**Group D (Adaptive)**	
Left STN		Left STN	
Mode	Parameter:	**Mode**	Parameter:
Adaptive Therapy Adapting between	Paused Amplitude: 2.6 mA Maximum Limit: 3.2 mA Minimum Limit: 2.2 mA	Adaptive Therapy Adapting between	Paused Amplitude: 2.6 mA Maximum Limit: 3.2 mA Minimum Limit: 2.2 mA
Right STN		Right STN	
Mode	Parameter:	**Mode**	Parameter:
Adaptive Therapy Adapting between	Paused Amplitude: 2.4 mA Maximum Limit: 3.0 mA Minimum Limit: 2.0 mA	Adaptive Therapy Adapting between	Paused Amplitude: 2.4 mA Maximum Limit: 3.0 mA Minimum Limit: 2.0 mA

GROUP SETTINGS

Group A (Gait)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group A (Gait)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group B (Speech)

SoftStart/Stop: Off
Cycling: Off

Group B (Speech)

SoftStart/Stop: 2 Seconds
Cycling: Off

Group C

SoftStart/Stop: Off
Cycling: Off

Group C (Scan)

SoftStart/Stop: Off
Cycling: Off

Group D (Adaptive)

SoftStart/Stop: 3 Seconds
Cycling: Off

Group D (Adaptive)

SoftStart/Stop: 4 Seconds
Cycling: Off

Group D (Adaptive)

Left STN

High Pass Filter: 1 Hz
Averaging Duration: 1.2 secs
Sensing Blanking Duration: 1.4 ms
Onset Duration:
Upper: 1.2 secs
Lower: 1.2 secs
Detection Blanking Duration: 2.0 secs
Adaptive Startup Delay: 10.0 secs

Right STN

High Pass Filter: 1 Hz
Averaging Duration: 3.0 secs
Sensing Blanking Duration: 1.1 ms
Onset Duration:
Upper: 0.8 secs
Lower: 1.6 secs
Detection Blanking Duration: 2.5 secs
Adaptive Startup Delay: 8.0 secs

Group D (Adaptive)

Left STN

High Pass Filter: 1 Hz
Averaging Duration: 1.2 secs
Sensing Blanking Duration: 1.4 ms
Onset Duration:
Upper: 1.2 secs
Lower: 1.2 secs
Detection Blanking Duration: 2.0 secs
Adaptive Startup Delay: 10.0 secs

Right STN

High Pass Filter: 1 Hz
Averaging Duration: 3.0 secs
Sensing Blanking Duration: 1.1 ms
Onset Duration:
Upper: 0.8 secs
Lower: 1.6 secs
Detection Blanking Duration: 2.5 secs
Adaptive Startup Delay: 8.0 secs

ELECTRODE IMPEDANCE

Impedance measured at Fixed test current

Left STN

MONOPOLAR

3	1,182
2	1,393
1	1,604
0	1,815

BIPOLAR

	0	1	2
3	3,282	3,619	1,356
2	1,693	2,030	
1	2,367		

Right STN

MONOPOLAR

11	1,818
10	2,029
9	2,240
8	2,451

BIPOLAR

	8	9	10
11	1,534	1,871	2,208
10	2,545	2,882	
9	3,219		

GROUP HISTORY

Oct 14, 2026

A



4.5 mA
60 µs
130 Hz



2.8 mA
60 µs
130 Hz

B



2.1 mA
60 µs
125 Hz



0.9 mA
60 µs
125 Hz



2.4 mA
60 µs
125 Hz

C



1.3 mA
60 µs
150 Hz



1.3 mA
60 µs
100 Hz

D



BrainSense:
Adaptive
Adaptive Therapy:
Adapting

2.6 mA
60 µs
125 Hz



BrainSense:
Adaptive
Adaptive Therapy:
Paused

2.4 mA
60 µs
125 Hz

Jul 2, 2026

A



4.4 mA
60 µs
130 Hz



2.7 mA
60 µs
130 Hz

B



2.0 mA
60 µs
125 Hz



0.8 mA
60 µs
125 Hz



2.3 mA
60 µs
125 Hz

C



1.2 mA
60 µs
150 Hz



1.2 mA
60 µs
100 Hz

D



BrainSense:
Adaptive
Adaptive Therapy:
Adapting

2.5 mA
60 µs
125 Hz



BrainSense:
Adaptive
Adaptive Therapy:
Paused

2.3 mA
60 µs
125 Hz


Jun 2, 2026

May 3, 2026

A	 4.3 mA 60 µs 130 Hz	 2.6 mA 60 µs 130 Hz
B	 1.9 mA 60 µs 125 Hz	 0.7 mA 60 µs 125 Hz  2.2 mA 60 µs 125 Hz
C	 1.1 mA 60 µs 150 Hz	 1.1 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.4 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Paused 2.2 mA 60 µs 125 Hz

A	 4.2 mA 60 µs 130 Hz	 2.5 mA 60 µs 130 Hz
B	 1.8 mA 60 µs 125 Hz	 0.6 mA 60 µs 125 Hz  2.1 mA 60 µs 125 Hz
C	 1.0 mA 60 µs 150 Hz	 1.0 mA 60 µs 100 Hz
D	 BrainSense: Adaptive Adaptive Therapy: Adapting 2.3 mA 60 µs 125 Hz	 BrainSense: Adaptive Adaptive Therapy: Paused 2.1 mA 60 µs 125 Hz

GROUP USAGE

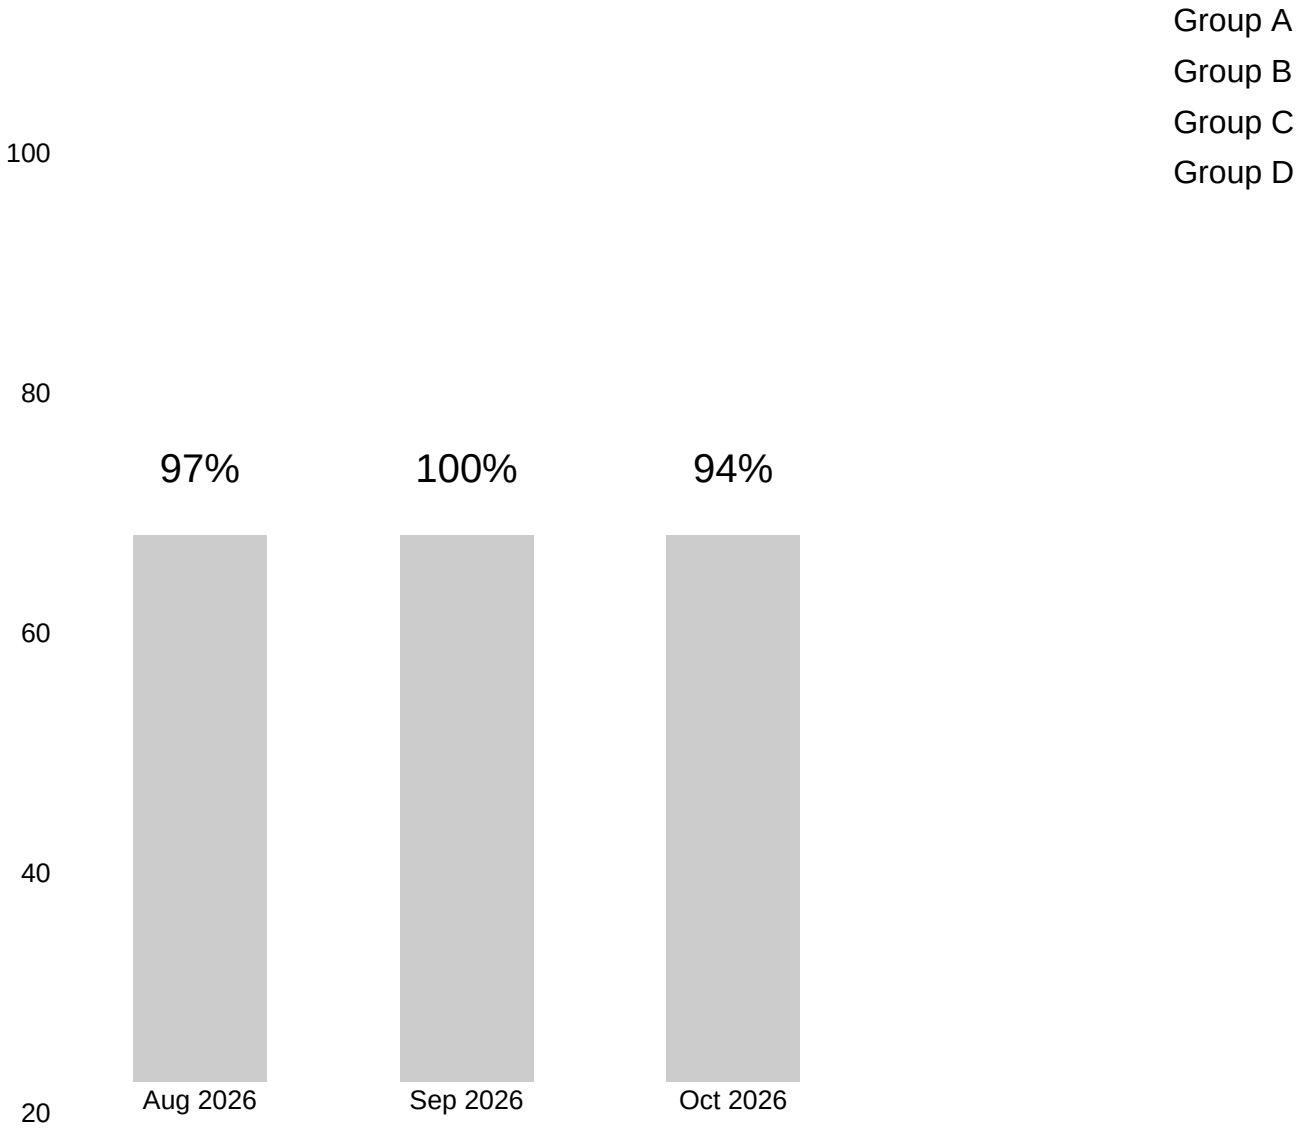
Group A
Group B
Group C
Group D
100
80
60
40
20
97%
100%
94%
Aug 2026
Sep 2026
Oct 2026

SESSION ANNOTATIONS

LEFT HEMISPHERE

CONFIGURATION

	TREMOR	BRADYKINESIA	MOOD ALTERATION	MUSCLE CONTRACTIONS	PARESTHESIA – TRANSIENT
Mar 30, 2026 2.50 mA 60 µs 130 Hz	2	1	-	0	3
Apr 14, 2026 3.10 mA 60 µs 130 Hz	1	1	2	-	-
May 6, 2026 1.80 mA 60 µs 125 Hz	-	0	1	2	1


RIGHT HEMISPHERE

CONFIGURATION


	TREMOR	BRADYKINESIA	MOOD ALTERATION	MUSCLE CONTRACTIONS	PARESTHESIA – TRANSIENT
Apr 2, 2026 2.20 mA 60 µs 130 Hz	3	-	-	1	0
Jun 9, 2026 2.75 mA 60 µs 130 Hz	0	2	1	1	-

BRAINSENSE SURVEY


Right STN

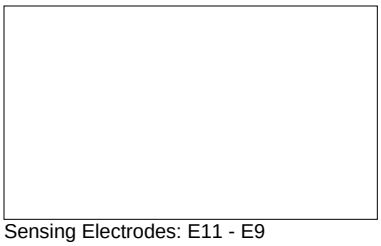

Sensing Electrodes: E11 - E9
Peak Magnitude: 0.512345678 µVp
Peak Frequency: 22.46 Hz

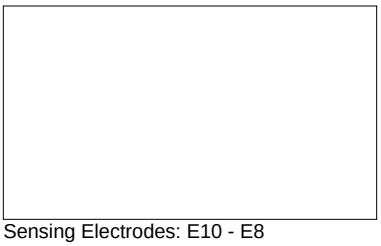

Sensing Electrodes: E10 - E8
Peak Magnitude: 1.250000000 µVp
Peak Frequency: 19.53 Hz

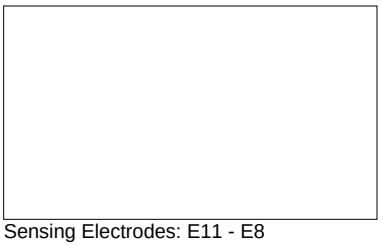

Sensing Electrodes: E11 - E8
Peak Magnitude: 0.073210987 µVp
Peak Frequency: 24.41 Hz

ELECTRODE IDENTIFIER

Right STN

Detected Frequency:

22.46 Hz

Selected Frequency:

22.46 Hz

LFP Magnitude:

11	Most
9	Medium
10	Medium
8	Least

PATIENT EVENTS

Initial	Final
Name: Medication taken	Name: Fall
Name: Tremor episode Additional Behavior: Left arm	Name: Medication taken Additional Behavior: Late dose

EVENT SUMMARY

Events	Jul 02 – Oct 14
Medication taken	12
Tremor episode	4
Fall	1

Group D Left STN	Jul 02 – Oct 14
Above Threshold	41%
Between Thresholds	30%
Below Threshold	29%
Average Amplitude	2.62
Adaptive Amplitude Reduction	12%
Time Adaptive Running	87%

Group D Right STN	Jul 02 – Oct 14
Above Threshold	35%
Between Thresholds	40%
Below Threshold	25%
Average Amplitude	2.41
Adaptive Amplitude Reduction	9%
Time Adaptive Running	91%

END OF REPORT