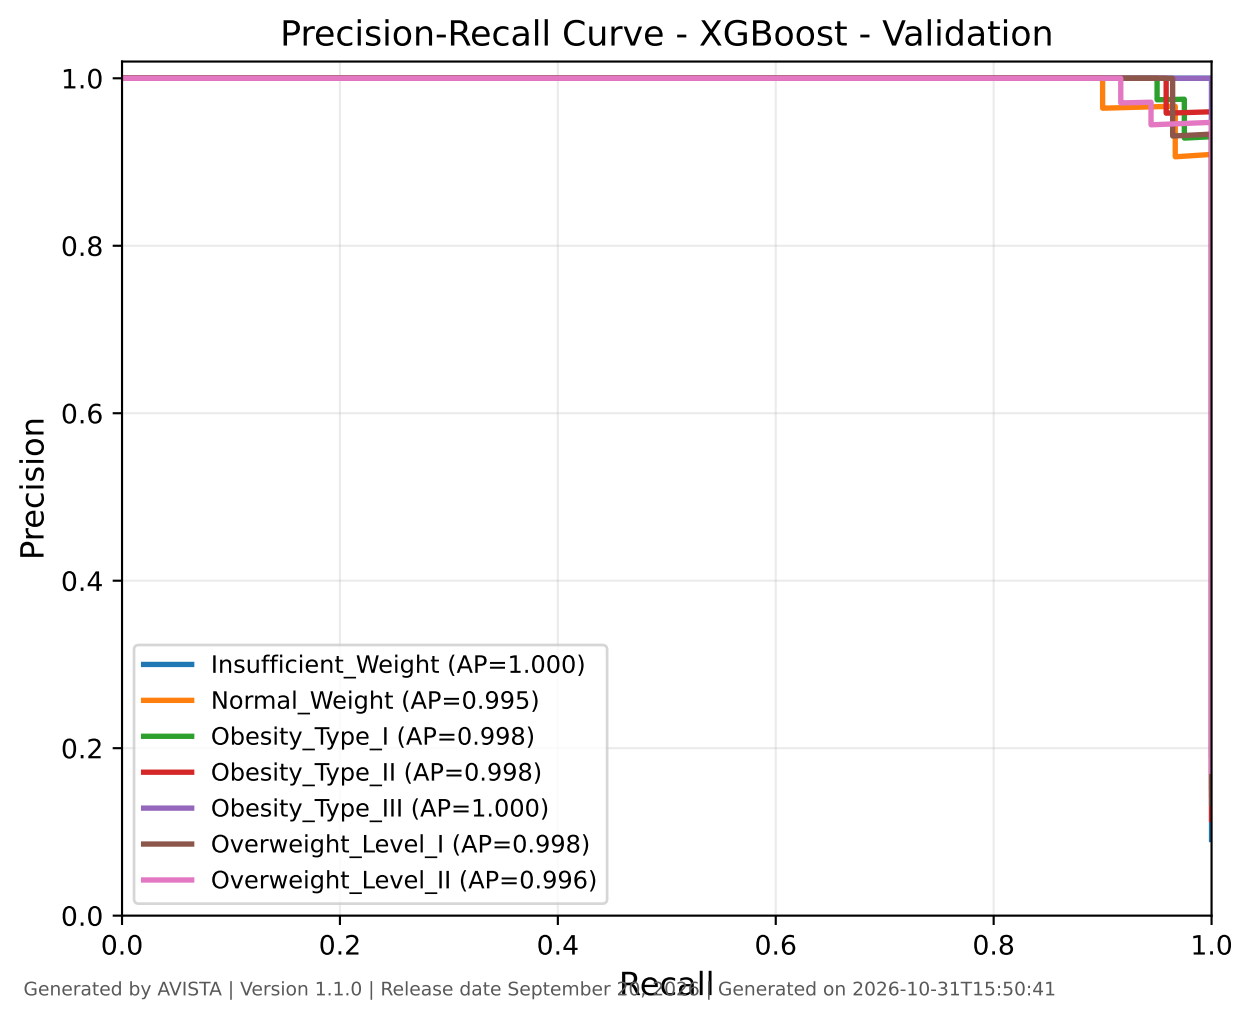
Precision-Recall Curve - XGBoost - Validation
Precision
Recall
1.0
0.8
0.6
0.4
0.2
0.0
0.0
0.2
0.4
0.6
0.8
1.0
Insufficient_Weight (AP=1.000)
Normal_Weight (AP=0.995)
Obesity_Type_I (AP=0.998)
Obesity_Type_II (AP=0.998)
Obesity_Type_III (AP=1.000)
Overweight_Level_I (AP=0.998)
Overweight_Level_II (AP=0.996)