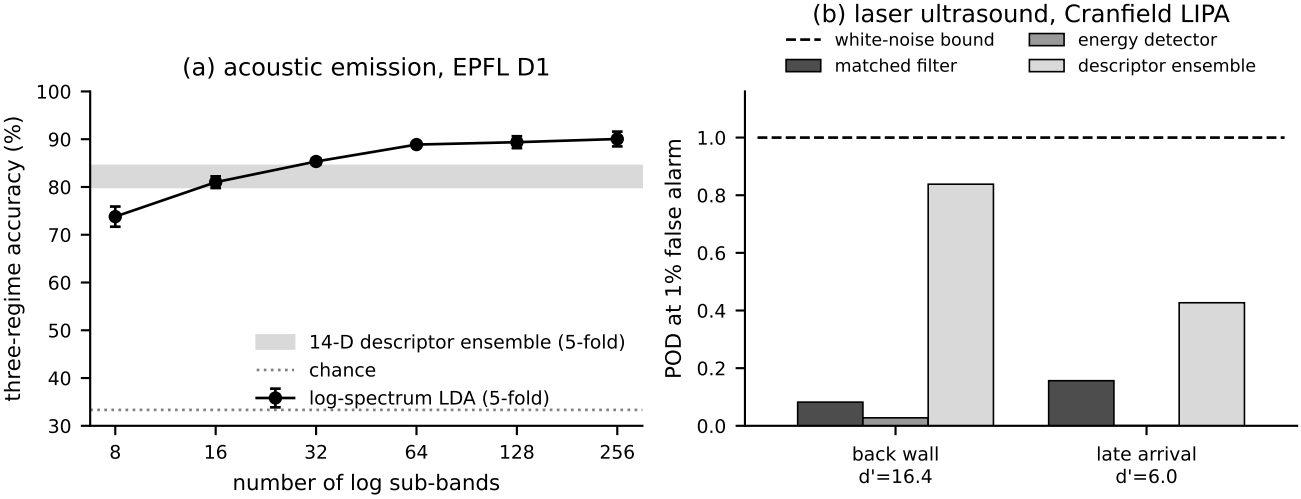
(a) acoustic emission, EPFL D1
three-regime accuracy (%)
100
90
80
70
60
50
40
30
14-D descriptor ensemble (5-fold)
chance
log-spectrum LDA (5-fold)
8
16
32
64
128
256
number of log sub-bands
(b) laser ultrasound, Cranfield LIPA
white-noise bound
energy detector
matched filter
descriptor ensemble
POD at 1% false alarm
1.0
0.8
0.6
0.4
0.2
0.0
back wall
d'=16.4
late arrival
d'=6.0