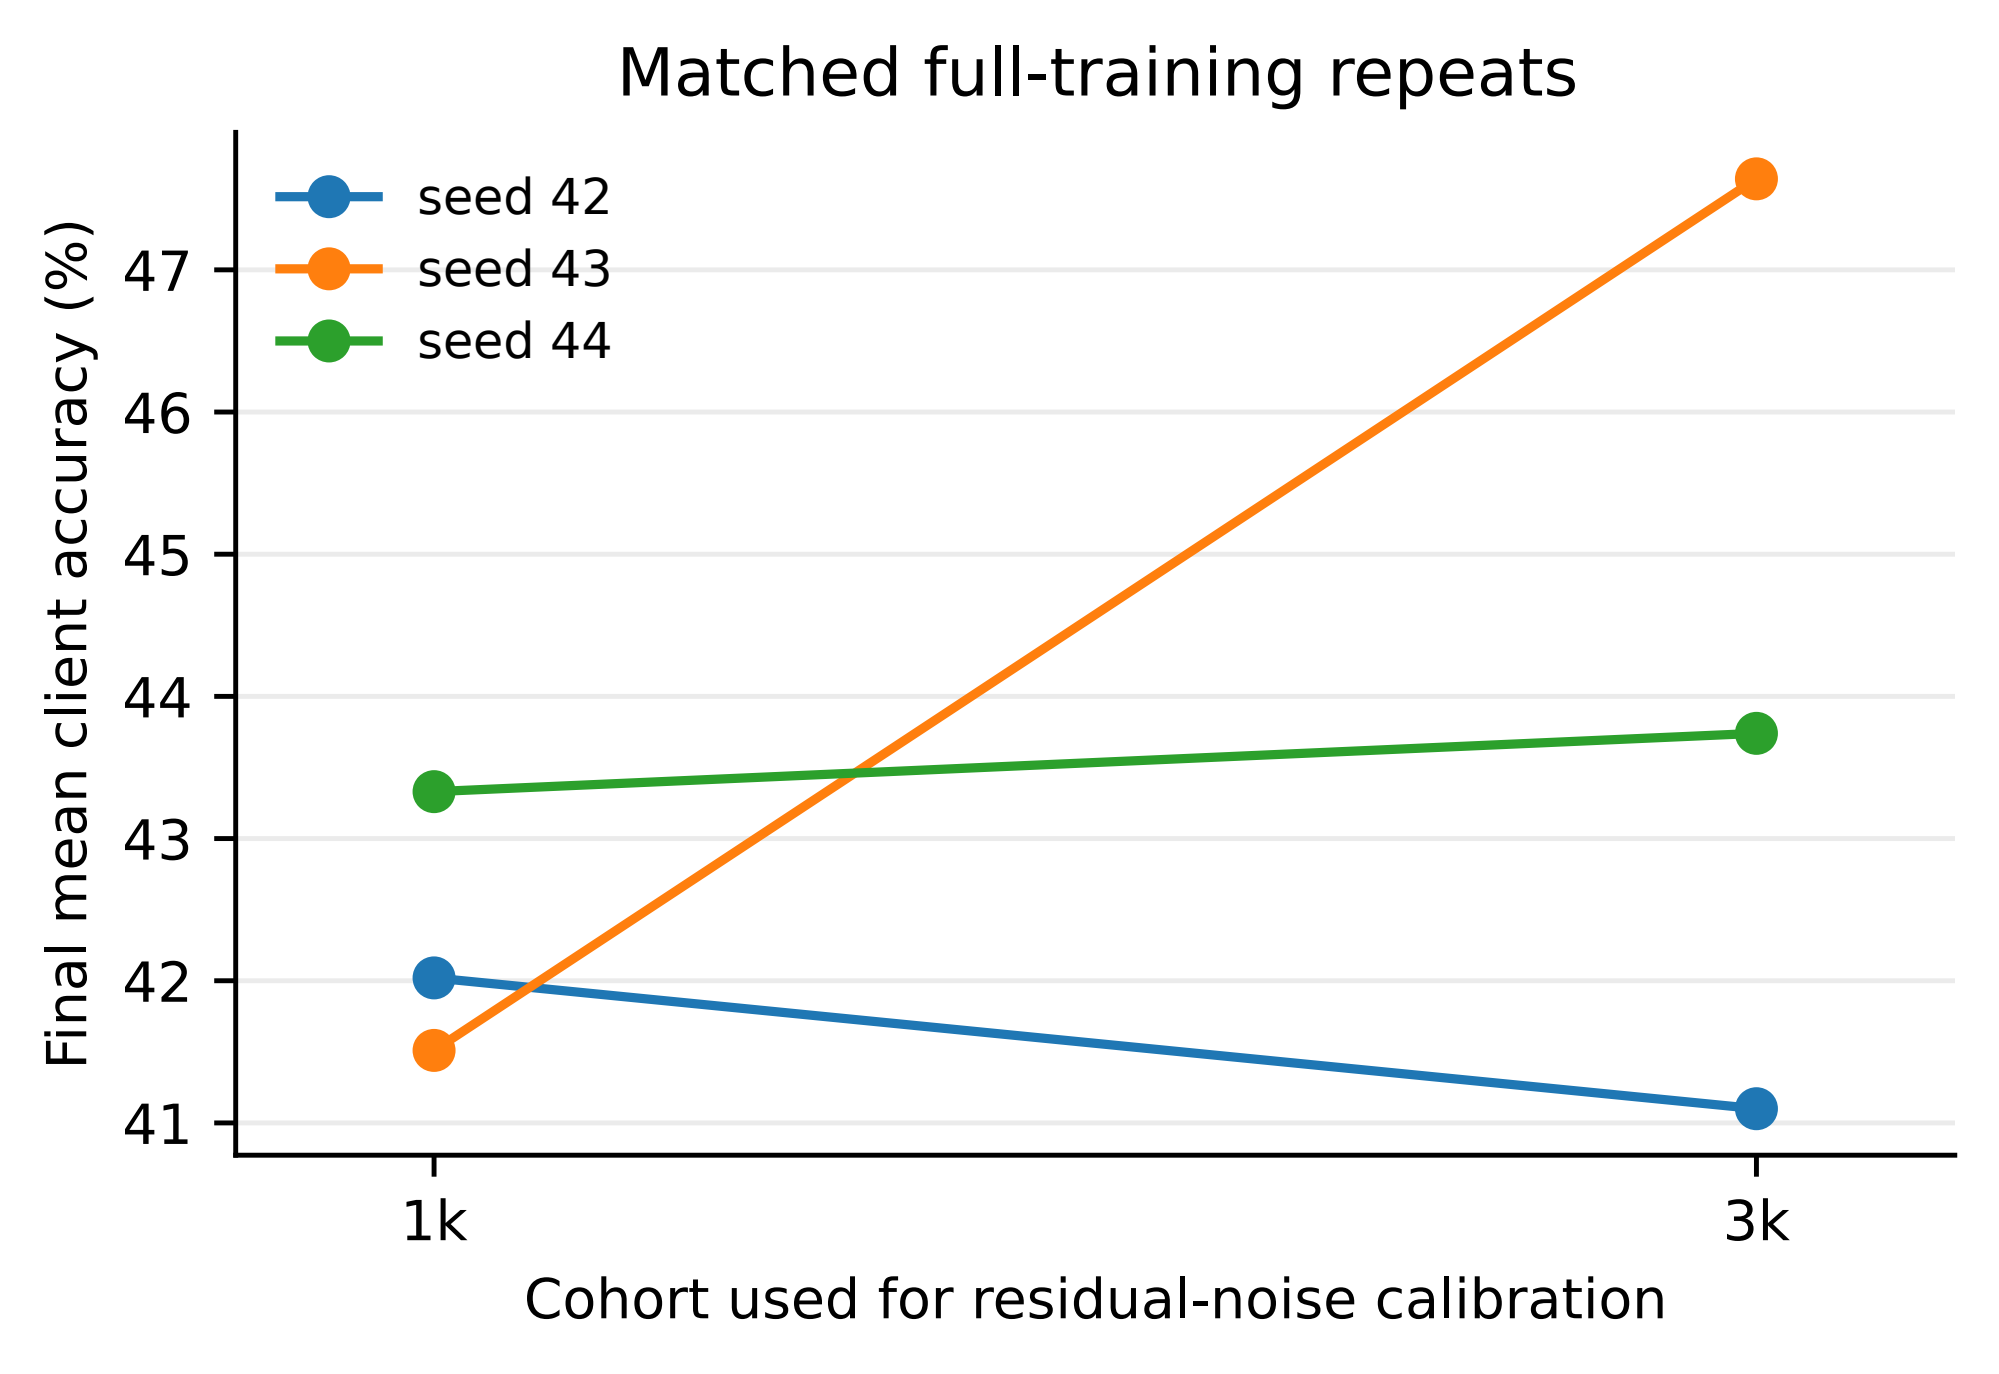
Matched full-training repeats
seed 42
seed 43
seed 44
Final mean client accuracy (%)
47
46
45
44
43
42
41
1k
3k
Cohort used for residual-noise calibration