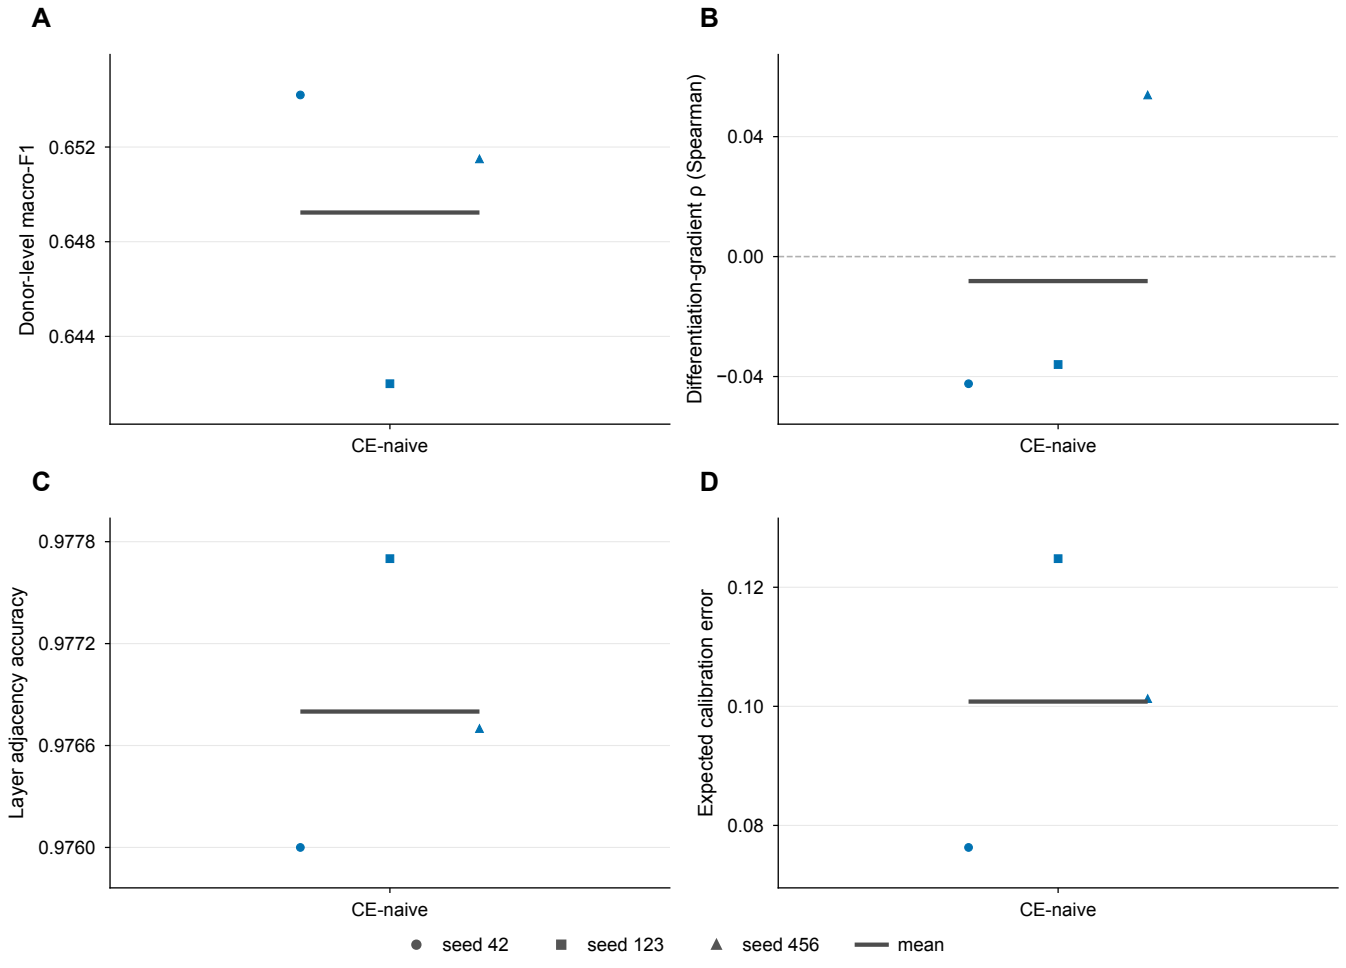
A
Donor-level macro-F1
0.652
0.648
0.644
CE-naive
B
Differentiation-gradient ρ (Spearman)
0.04
0.00
−0.04
CE-naive
C
Layer adjacency accuracy
0.9778
0.9772
0.9766
0.9760
CE-naive
D
Expected calibration error
0.12
0.10
0.08
CE-naive
seed 42
seed 123
seed 456
mean