
37 Oxygen-15 is used in hospitals.

The count rate from a detector placed close to a sample of oxygen-15 was recorded over a period of 15 min. The background count rate is 20 counts / min. The graph shows the total count rate from the detector.

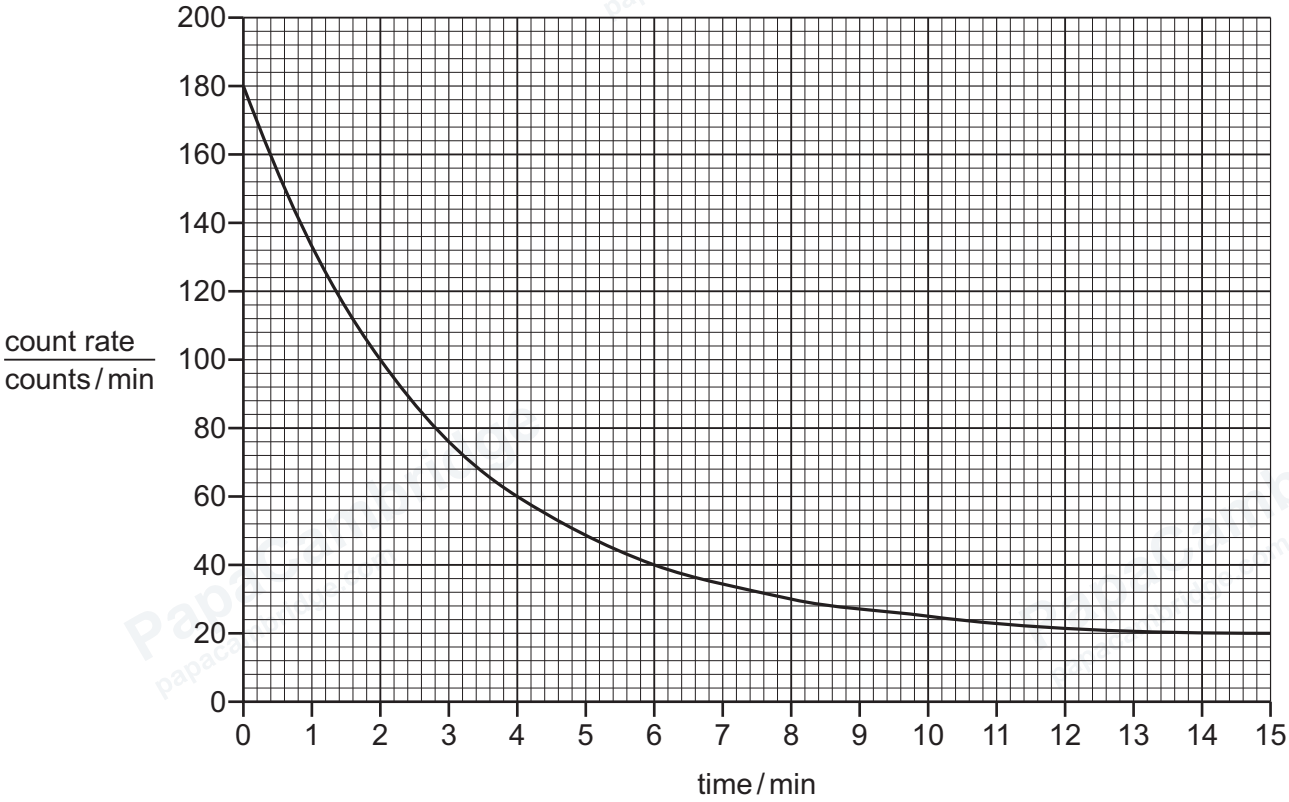

What is the half-life of this sample of oxygen-15?

A 2.0 min **B** 2.4 min **C** 2.8 min **D** 7.5 min