

Universal manuscript template for Optica Publishing Group journals

YASH PATEL,¹ PRAJAKTA BELEKAR,¹ GEORG LADURNER,¹ SYBREN WORM,¹ LUCAS MAY,¹ MARIA VARAKA,¹ THERESA ROHRMOSER,¹ FERNANDO GARCÍA-RAMÍREZ,¹ RENÉ WERKMEISTER,¹ BERNHARD BAUMANN,^{1,2} AND CONRAD W. MERKLE^{1,*}

¹Center for Medical Physics and Biomedical Engineering, Medical University of Vienna, Währinger Gürtel 18-20/4L, 1090 Vienna, Austria

²Institute of Biomedical Physics, Medical University of Innsbruck, Müllerstraße 44, 6020 Innsbruck, Austria

*conrad.merkle@meduniwien.ac.at

Abstract: This template contains important information on submissions to Optica Publishing Group journals. We encourage authors to focus foremost on their content and not on formatting. The template is provided as a guide, but following the visual styling is optional. Each manuscript will be formatted in a consistent way during production. Authors also have the option to [submit articles](#) to the Optica Publishing Group preprint server, [Optica Open](#). You may find it helpful to use our optional [Paperpal manuscript readiness check](#) and [language polishing service](#). Note that copyright and licensing information should not be added to your journal or Optica Open manuscript.

1. Introduction

General structure of intro: Why diameter is an important measurment Brief OCTA Introduction Difficulty of OCTA quantification (different methods yield different results) Artefact contributions and diameter underestimation Proposed solution that we investigate here and evaluation of different methods in a test scenario (vessel dilation)

<https://www.nature.com/articles/s41598-021-84067-2>

Vessel diameter is an important biomarker that provides valuable information regarding local vascular health. Studies have demonstrated statistically significant differences between vessel diameters. Combined with measurements of blood flow, diameter can also be used to investigate local blood pressure [cite]. For this reason, it is imperative that accurate measurements of diameter be used for these extrapolations or when modeling behaviours of flow in digital twins [cite]. Optical imaging techniques are often used to measure vessel diameter due to their high resolution, but accurate measurement of vessel size is more difficult than it first appears.

Optical coherence tomography (OCT) is a non-invasive optical imaging method, which uses interferometry to measure the transit time of light that is backscattered from a sample, thereby producing depth-resolved images of tissue [cite]. Optical coherence tomography angiography (OCTA) is an extension of OCT that visualizes vascular perfusion using the motion contrast from red blood cells (RBCs) [cite]. Over the years, OCTA has demonstrated widespread acceptance and use for clinical evaluations of vascular features in relation to disease [1]. OCT angiograms can be used to evaluate characteristics on the scale of vascular layers by measuring vascular density [cite] or non-perfusion zones [cite], or it can be used to guage vessel size [cite] or tortuosity [cite].

Analysis of OCTA datasets is typically achieved by performing a maximum intensity projection of a 3D vascular network to compress it into 2D before binarising the resulting angiogram. From this binarised angiogram, various vascular metrics can be quantified. That said, there are many methods for performing this binarisation step and the choice of method can significantly affect the reported vascular metrics [cite]. For example, in a simple application of a global threshold,

local intensity fluctuations within an OCTA dataset could result in the underestimation of vessels with low intensity [cite]. To address this problem, there are also a number of dynamically thresholded OCTA algorithms [cite], but these also do not necessarily solve the problem and may risk homogenising the resulting angiogram [cite]. Similarly, there are vascular enhancement algorithms [cite] to highlight structures that resemble vessels before quantification, but these methods also risk affecting the apparent size of the vessels in the network.

Furthermore, OCT is prone to certain artifacts which specifically affect visualization of the vasculature [cite]. When viewed in cross-section, large vessels often demonstrate an hourglass appearance with stronger scattering in the center than at the sides (Figure 1A). This appearance is due to orientation effects of RBCs, which align with the blood flow, causing a reduced scattering cross-section at the sides of the vessels [cite]. We hypothesize that these artifacts may lead to underestimations of measurements of vessel diameter. To compensate for these artifacts, OCT contrast agents such as Intralipid have previously been used to increase intravascular intensity signals, particularly in regions where RBC scattering is diminished [cite].

In this study we examine different methods of measuring vessel size from in vivo OCT scans of mouse retinal vasculature, and we use a contrast agent to obtain ground truth vessel diameter measurements for comparison. In addition to a traditional binarisation-based methods, we also employ model-based methods for quantifying vessel diameter. Traditional Gaussian models have been employed for vessel diameter measurements in techniques such as [insert] and OCT [cite], but we expand this by also investigating the generalized Gaussian model. As part of this study, we measure how much diameter is underestimated from enface projections and evaluate how reliably it can be compensated through calibration. After identifying the best methods for quantifying diameter and compensating for underestimations, we finally evaluated a test scenario using flicker stimulation to induce a measureable change in diameter to evaluate the performance of different methods.

2. Methods and Materials

2.1. Imaging system

All imaging was performed using a custom-built polarisation-sensitive spectral-domain OCT ophthalmoscope, described in detail previously [2]. The system was centred at 840 nm with a spectral bandwidth of 100 nm at full width half maximum (FWHM), providing an axial resolution of approximately 5.1 μm in air and 3.8 μm in tissue (assuming a refractive index of 1.35). A sensitivity of 96 dB was achieved at an A-scan rate of 80 kHz and a beam diameter of 0.5 mm at the pupil plane (power at cornea = 2.85 mW) [3]. This system was employed to acquire volumetric OCT data from mouse retinas before, during, and after an intravascular contrast agent administration, as well as before and after functional stimulation of the mouse retina using a custom 502 nm light-emitting diode (LED) ring flashing at 10 Hz (power at cornea = 26.6 μW). This wavelength was selected to target the peak absorption of mouse rhodopsin (~500 nm), enabling predominantly rod-driven photoreceptor stimulation [4].

2.2. Experimental protocol

Three mouse models were used in this study: VLDLR knockout mice (B6;129S7-Vldlr^{tm1Her}/J, The Jackson Laboratory, Bar Harbor, USA), C57BL/6J mice (C57BL/6J, The Jackson Laboratory, Bar Harbor, USA), and SOD1 non-transgenic mice (strain details), with $n = 1, 1, 2$ mice per VLDLR, SOD1 and C57BL/6J group respectively. All imaging sessions were conducted under general anaesthesia using either isoflurane, medetomidine + midazolam + fentanyl + ketamine (MMFK) combination, or a ketamine + xylazine combination. For the VLDLR knockout and the SOD1 non-transgenic mice, isoflurane was induced at 4% in oxygen for 4 minutes and subsequently maintained at 2% in oxygen at a flow rate of 1.5–2 L/min for the duration of

the imaging session. In cases where isoflurane alone did not provide adequate sedation, an intraperitoneal injection of ketamine + xylazine cocktail (100 mg/kg ketamine, 6 mg/kg xylazine; 10 mL/kg body weight) was administered. For the C57BL/6J mice, isoflurane was induced at 4% in oxygen for 4 minutes and then MMFK (10 mL/kg body weight) was administered. To maintain core body temperature of the mice throughout imaging, they were positioned on a heating pad. Mouse pupils were dilated with one drop of tropicamide (5 mg/mL, Agepha Pharma s.r.o., Senec, Slovakia) per eye, and artificial tear drops (Oculotect, ALCON Pharma GmbH, Freiburg im Breisgau, Germany) were applied at regular intervals to prevent the cornea from drying out.

Intralipid 20% (3 mL/kg body weight) was used as a contrast agent and was administered as a bolus injection via the tail vein. Volumetric angiography data were acquired over a 1 mm × 1 mm field of view centred on the optic nerve head (ONH), with a scan density of 500 A-scans per B-scan and five repeated B-scans at each of 400 slow-axis positions (acquisition time approximately 16 seconds). For this study, pre- and post-injection volumetric datasets were acquired. **This volumetric data was used solely for visualisation purposes.** Additionally, a dynamic-contrast OCT (DyC-OCT) protocol [5] was employed during the contrast injection or during stimulation, consisting of 2000 repeated B-scans over approximately 16 seconds (interscan time 8.2 ms) at the same cross-sectional location over a 1 mm lateral field of view. DyC-OCT scans allow us to track the same vessels over time to precisely measure the effects of the contrast agent or the stimulation with a high degree of spatial coregistration. All quantitative vessel diameter measurements reported in this study were derived from the DyC-OCT data.

Functional flicker stimulation was performed in a C57BL/6 mouse to assess whether the choice of diameter measurement method affects the detection of physiological vascular responses. For this experiment, ketamine/xylazine cocktail was chosen over isoflurane to minimise anaesthesia-induced vasodilation [cite]. During the DyC-OCT acquisition, the retina was unstimulated for approximately 7 seconds, followed by 10 Hz flicker stimulation from the LED ring for the rest of the scan duration. **To compare results before and after stimulation, the data was divided into baseline (pre-stim) and post-stim. Considering the time required for the OCT signal to stabilise after stimulation, four-second time windows at the beginning and end of each scan were selected for the pre- and post-stimulation analyses respectively.**

All animal procedures were approved by the ethics committee of the Medical University of Vienna and the Austrian Federal Ministry of Education, Science, and Research (BMBWF/66.009/0272-V/3b/2019 and GZ 2024-0.802.524).

2.3. Post-processing and analysis

Cross-polarised OCT intensity data from the retinal pigment epithelium (RPE) was used for inter-frame alignment and B-scan flattening [3, 6]. Angiograms were derived by applying the complex subtraction OCT angiography (OCTA) algorithm [7, 8]. We evaluated multiple combinations of methods for quantifying vessel diameter from the OCTA data to determine which combinations of steps work best under different conditions. Specifically, we looked at two types of data projections (maximum intensity and mean intensity) to generate vessel profiles and several different quantifications of those profiles including a traditional binarisation, a Gaussian model approach, and a Generalised-Gaussian (GG) model approach. These methods represent commonly used methods in the literature for OCTA quantification [9–12]. The different methods were evaluated against the ground truth as described in this section. All data processing and analysis was performed in MATLAB (R2019b, MathWorks, Natick, MA, USA).

2.3.1. Ground truth calculation

Ground truth vessel diameters were obtained from contrast-enhanced DyC-OCT B-scan angiograms. The width and height of the vessel were manually measured from the vessel's cross-section. The ground truth diameter was defined as the minimum of the two measurements

141 to account for off-axis cross-sectioning of the vessel, which produces a more elliptical appearance
 142 in the B-scan. For cases where the vessel is perpendicular to the B-scan, the height and width
 143 would therefore be in agreement. Because the lateral diameter is studied here, we defined a
 144 correction factor of *height/width* for cases where the width was larger than the height due
 145 to skewing effect and was equal to 1 otherwise. By multiplying this correction factor against
 146 diameter measured from the ROI projection, we ensured that the measured vessel diameter
 147 reflected the true size of the vessel.

148 2.3.2. Vessel projection calculation

149 For each large vessel in the field of view, a rectangular region of interest (ROI) encompassing
 150 the vessel cross-section, along the lateral (x) and axial (z) dimensions, was selected from the
 151 DyC-OCT B-scan angiograms. En face intensity profiles were then generated by projecting the
 152 A-scans within this ROI along the axial (z) direction. Two projection methods were compared:
 153 maximum intensity projection (MIP), which selects the highest intensity value along the depth
 154 axis of each ROI, and mean intensity projection (MeIP), which averages the values along each
 155 ROI. Each projection resulted in a time-stack of 1-D lateral intensity profiles for each vessel,
 156 which were then used for subsequent diameter quantification. For the model-based approaches,
 157 the profiles were normalised to a range of 0–1 to ensure a good fit.

158 2.3.3. Model-based vessel diameter calculation

159 The two parametric models were fitted (Fig. 1a) to the one-dimensional intensity profiles from
 160 the previous step, using nonlinear least-squares regression in MATLAB.

161 Standard Gaussian function:

$$f(x) = A \exp\left(-\frac{(x - \mu)^2}{2\sigma^2}\right) + C \quad (1)$$

162 where A is the peak amplitude, μ is the centre position, σ is the standard deviation, and C is a
 163 constant baseline offset.

164 Generalised-Gaussian (GG) function:

$$f(x) = A \exp\left(-\left(\frac{|x - \mu|}{\alpha}\right)^\beta\right) + C \quad (2)$$

165 where A is the peak amplitude, μ is the centre position, α is the scale parameter, β is the shape
 166 parameter, and C is a constant baseline offset. Given the imaging system configuration, all vessels
 167 are expected to produce at minimum a Gaussian intensity profile in the B-scan cross-section,
 168 and so profiles sharper than Gaussian profile ($\beta < 2$) are therefore not technically meaningful.
 169 The shape parameter β was hence constrained to $\beta \geq 2$ during fitting. With this constraint, the
 170 GG accommodated to profiles ranging from Gaussian ($\beta = 2$, where $\sigma = \alpha/\sqrt{2}$) to increasingly
 171 flat-topped ($\beta > 2$).

172 Two standard width metrics were calculated from the fitted models: the full width at half
 173 maximum (FWHM) and the $1/e^2$ width. For the standard Gaussian fit, the $1/e^2$ width was
 174 calculated as:

$$w_{1/e^2, G} = 4\sigma \quad (3)$$

175 The FWHM for a Gaussian is related to the $1/e^2$ width by a fixed proportionality:

$$\text{FWHM}_G = 2\sigma\sqrt{2\ln 2} = \frac{\sqrt{2\ln 2}}{2} w_{1/e^2, G} \quad (4)$$

176 and therefore only the $1/e^2$ width was calculated directly from the fit, with the FWHM obtainable
 177 via this known relationship.

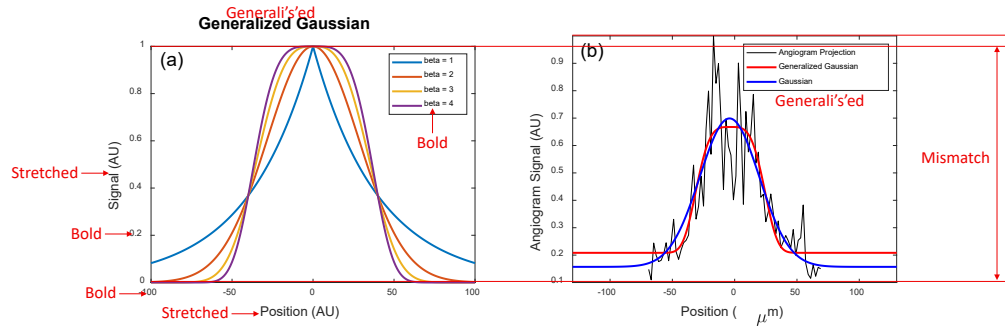


Fig. 1. (a) GG function for shape parameters $\beta = 1, 2, 3$, and 4. (b) Example vessel intensity profile (black) with standard Gaussian (blue) and GG (red) fits.

For the GG fit, no such linear relationship exists between the FWHM and $1/e^2$ width, since both depend on the shape parameter β . Both metrics were therefore calculated independently as:

$$\text{FWHM}_{\text{GG}} = 2\alpha(\ln 2)^{1/\beta} \quad (5)$$

$$w_{1/e^2, \text{GG}} = 2\alpha \cdot 2^{1/\beta} \quad (6)$$

2.3.4. Binary mask based vessel diameter calculation

For comparison with OCTA processing pipelines that rely on image binarisation, vessel diameters were also measured from binary masks generated by global thresholding. A 3D averaging filter with a kernel size of $50 \times 50 \times 10$ voxels (lateral $x \times$ axial $z \times$ temporal t) was applied to the DyC-OCT angiogram volumes to reduce noise and minimize the effects of outliers. To produce a binarised black and white (BW) mask, the maximum angiogram intensity within these smoothed volumes were calculated, and five different threshold values were defined as fixed percentages of these maxima for MIP and MeIP. For MIP, the thresholds were defined as BW-1 = 40%, BW-2 = 50%, BW-3 = 60%, BW-4 = 70%, and BW-5 = 80%. While for MeIP, the thresholds were defined as BW-1 = 07%, BW-2 = 08%, BW-3 = 09%, BW-4 = 10%, and BW-5 = 11%. **These thresholds were selected empirically to cover the usable range of each projection. The upper and lower bounds were selected based on the point at which vessels began to be lost, and at which background noise and tissue signal were increasingly included, respectively.** Each threshold was applied to the unsmoothed en face projection (MIP and MeIP) to generate a binary mask, and the vessel diameter was measured as the number of pixels above the threshold across the lateral vessel cross-section.

2.3.5. Statistical analysis

To evaluate the accuracy and precision of all diameter measurement approaches, the calculated diameter values were plotted against the ground truth for each vessel across three conditions: pre-contrast, peak contrast, and post-contrast. A linear regression was fitted to each condition, yielding the slope (m) and coefficient of determination (R^2). A slope of $m = 1$ indicated perfect agreement with the ground truth, and R^2 quantified the goodness of fit of the linear model. Additionally, the coefficient of variation (CoV) was computed for each method to assess measurement precision (repeatability). For the model-based methods, six combinations were evaluated: two projection methods (MIP and MeIP) by three width metrics ($w_{1/e^2, G}$, FWHM_{GG} , and $w_{1/e^2, \text{GG}}$). For the binary mask based method, diameter was measured at five threshold levels (BW-1 through BW-5) for both MIP and MeIP. For the functional flicker stimulation experiment,

the Pearson correlation coefficient (ρ) between measured diameter values and angiogram intensity was computed for each method and vessel, to assess whether the diameter measurements were affected by changes in angiogram intensity. Measurements with $p < 0.05$ were considered statistically significant.

3. Results

3.1. Qualitative assessment of vessel underestimation

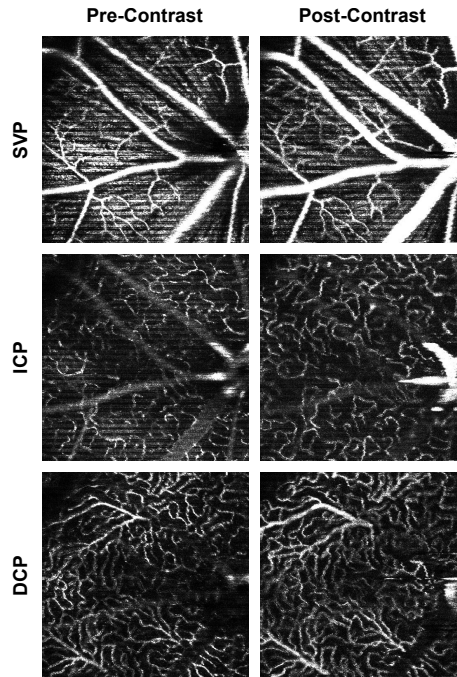


Fig. 2. OCTA MIP en face of the SVP, ICP, and DCP before (left) and after (right) the administration of Intralipid 20%. Vessels appear visibly wider and brighter post-contrast across all layers, most prominently in the larger vessels.

Figure 2 shows OCTA MIP enface images of the superficial vascular plexus (SVP), intermediate capillary plexus (ICP), and deep capillary plexus (DCP) before and after contrast injection. Across all three layers, vessels appeared visibly wider and brighter post-contrast injection, consistent with previous literature showing that OCTA underestimates vessel diameter in the absence of a contrast agent [3]. This effect was most pronounced in the larger vessels, especially in the SVP, where the major retinal arteries and veins appeared noticeably thicker after contrast administration. In the ICP and DCP, the capillary networks also showed improved visibility, though the effect was less dramatic.

DyC OCTA projections helped visualise the temporal changes in vessel diameter pre- and post-contrast injection (Fig. 3). Pre-contrast injection, the vessel cross-sections appeared narrower than their true diameter (Fig. 3a), which could be due to lateral edge signal suppression by the RBC orientation artefact [13]. At peak contrast, the Intralipid filled the vascular lumen uniformly, but the vessels look slightly extended beyond their true extent because of the dynamic range of the image (Fig. 3b). In the post-contrast phase, the signal stabilised as the initial bolus cleared, and the vessel boundaries remained more visible than before injection (Fig. 3c). The MIP and the corresponding binary mask over time (Figs. 3d–e) showed the observed temporal changes in vessel diameter across the three phases. The mean OCTA intensity (Fig. 3f) showed a sharp

231 increase post-contrast injection, followed by a decrease to a new steady state that remained
 232 elevated above the pre-contrast baseline.

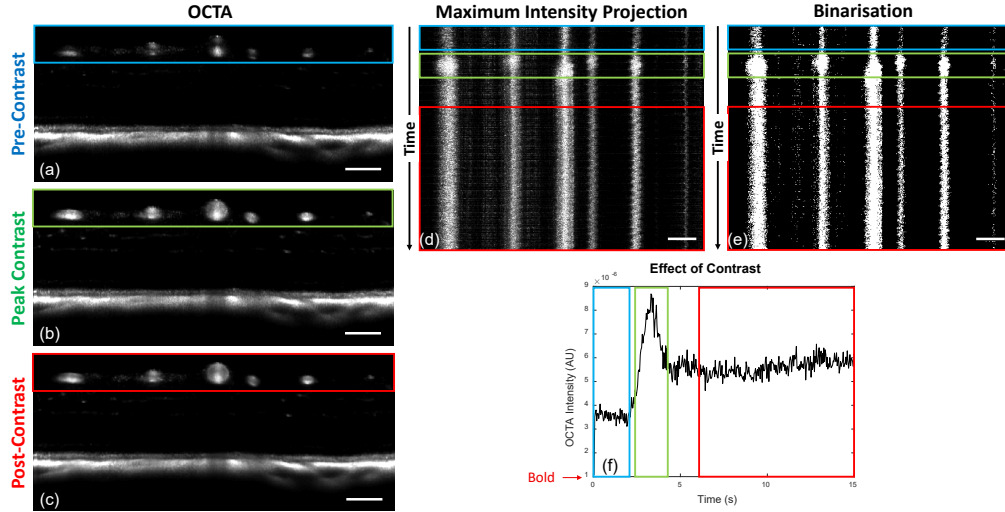


Fig. 3. DyC-OCT B-scan angiograms at (a) pre-contrast, (b) peak contrast, and (c) post-contrast timepoints. (d) MIP and (e) binarisation of the vessel cross-sections over time, with coloured boxes indicating the pre-contrast (blue), peak-contrast (green), and post-contrast (red) windows. (f) Mean OCTA intensity over time, showing the temporal intensity dynamics. All scale bars are 100 μm.

233 3.2. Accuracy and precision of diameter measurements

234 The accuracy (m , R^2) and precision (CoV) of all diameter measurement methods are summarised
 235 in Table 1. All model-based methods underestimated vessel diameter in pre-contrast data, with
 236 slopes ranging from 0.42 to 0.73 (Table 1). Contrast enhancement improved accuracy across
 237 all metrics, though the degree of improvement varied. The FWHM_{GG} metric remained well
 238 below unity even post-contrast. The $w_{1/e^2, \text{G}}$ with MIP slightly overestimated post-contrast
 239 ($m = 1.12$ – 1.15), while MeIP yielded values closer to unity ($m = 1.04$). The $w_{1/e^2, \text{GG}}$ with
 240 MeIP provided the best overall agreement, achieving a slope closest to unity with $m = 1.001$
 241 ($R^2 = 0.97$) post-contrast, which was the closest to the identity line of all tested model-based
 242 methods. Across all metrics, MeIP mostly outperformed MIP in both accuracy and linearity
 243 (Table 1, Fig. 4).

244 For binary mask based methods, the slope decreased with increasing threshold across all
 245 contrast conditions and projections (Table 1). This degradation was steeper for MIP than for
 246 MeIP. MIP slopes dropped from near unity at BW-1 to well below it at BW-5, whereas MeIP
 247 slopes declined more gradually and remained closer to unity across the threshold range. MeIP
 248 slopes were consistently higher than MIP at every threshold and contrast condition, though at
 249 lower thresholds and at peak and post-contrast, MeIP tended to slightly overestimate vessel
 250 diameter. The R^2 values followed a similar pattern. For MIP, pre- and post-contrast R^2 decreased
 251 substantially with increasing threshold, whereas for MeIP, R^2 remained relatively stable. Overall,
 252 MeIP provided more reliable binary mask based diameter measurements than MIP.

253 The precision of each method was assessed via the CoV (Table 1, Fig. 7). For MIP, the
 254 binary mask based CoV increased substantially with threshold, whereas the model-based CoV
 255 remained stable across all contrast conditions. For MeIP, the binary mask based CoV was

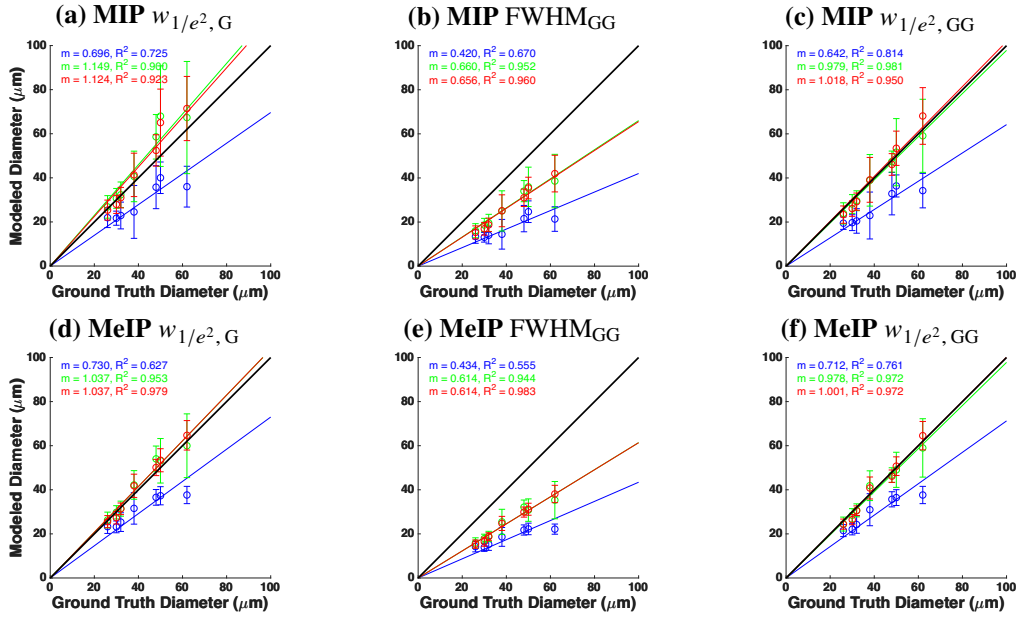


Fig. 4. Modelled versus ground truth vessel diameter using MIP (top row, a–c) and MeIP (bottom row, d–f). Columns correspond to $w_{1/e^2, G}$ (a, d), FWHM_{GG} (b, e), and $w_{1/e^2, GG}$ (c, f). Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions. The black line indicates the identity line ($m = 1$).

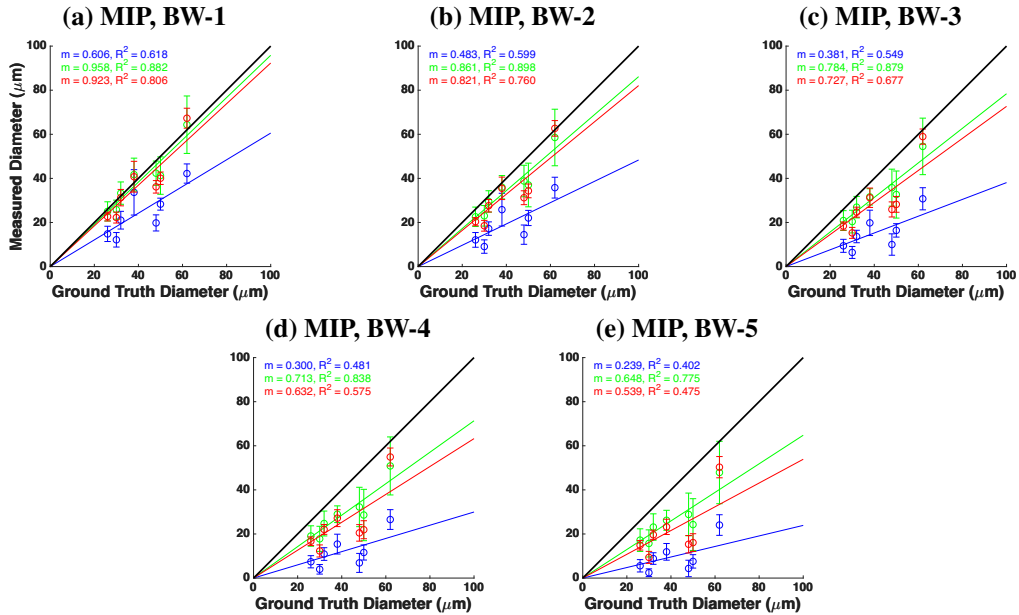


Fig. 5. Vessel diameter measured from binarised masks versus ground truth for MIP at five threshold levels: (a) BW-1 through (e) BW-5. Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions.

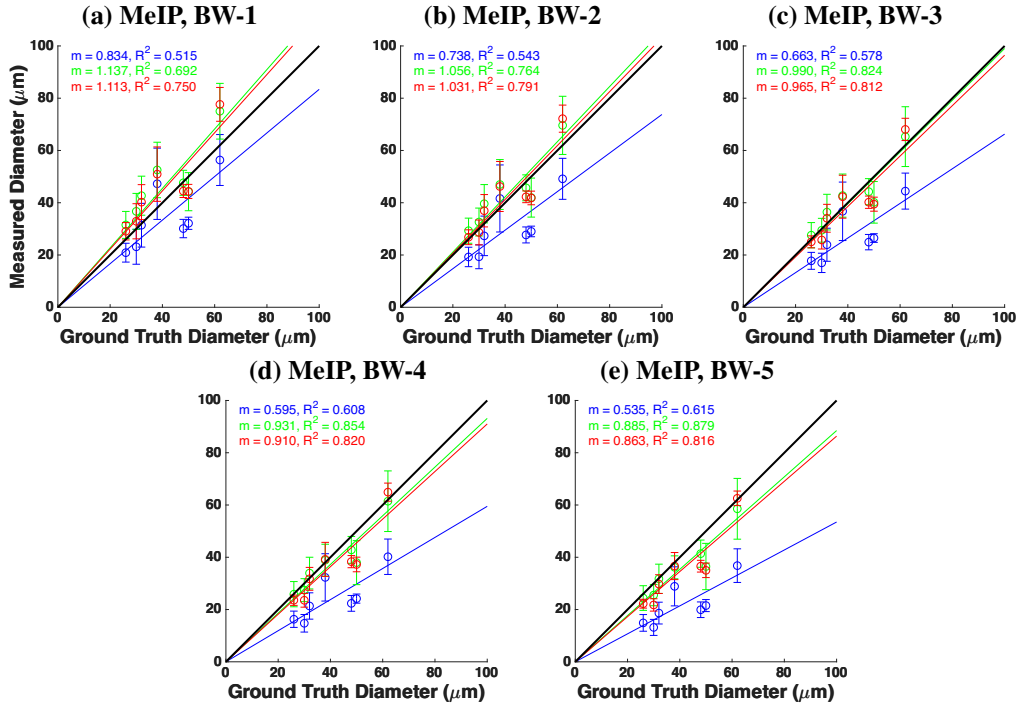


Fig. 6. Vessel diameter measured from binarised masks versus ground truth for MeIP at five threshold levels: (a) BW-1 through (e) BW-5. Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions.

notably more stable across thresholds than for MIP, and the model-based CoV values were lower overall, though they increased slightly at peak contrast before decreasing post-contrast. Across both methods, MeIP yielded lower CoV values than MIP pre-contrast and more stable values post-contrast. Among the model-based metrics, FWHM_{GG} consistently exhibited the weakest accuracy while maintaining comparable precision. Overall, model-based methods consistently outperformed binary mask based methods in both accuracy and precision, and MeIP yielded superior performance compared to MIP across all methods.

3.3. Functional flicker stimulation

The model-based diameter time series (Figs. 8a,b) showed increase in diameter post-stimulation for most of the vessels. The binary mask based diameter time series (BW-3; Fig. 8c) showed a mixed trend, where most vessels showed a decrease in diameter post-stimulation. Bar plots of the mean diameter pre- and post-stimulation (Figs. 8d-f) confirmed this pattern. For the Gaussian model, four of five vessels showed significant diameter increases ($p < 0.01$), and the GG model showed significant increases in three of five vessels (Table 2). In contrast, the binary mask based diameter showed significant decreases in four of five vessels.

The angiogram intensity time series (Fig. 8g) showed a visible decline in angiogram intensity during the duration of the DyC-OCT scan across all five vessels. The mean intensity comparison pre- and post-stimulation (Fig. 8h) confirmed that the decrease was significant for all vessels, ranging from -14.1% to -19.9% (Table 2). The binary mask based method showed uniformly positive per-vessel correlations, with an overall correlation of $\rho = 0.523$ ($p < 0.0005$). The Gaussian and GG models yielded overall correlations of $\rho = -0.101$ and $\rho = -0.098$, respectively.

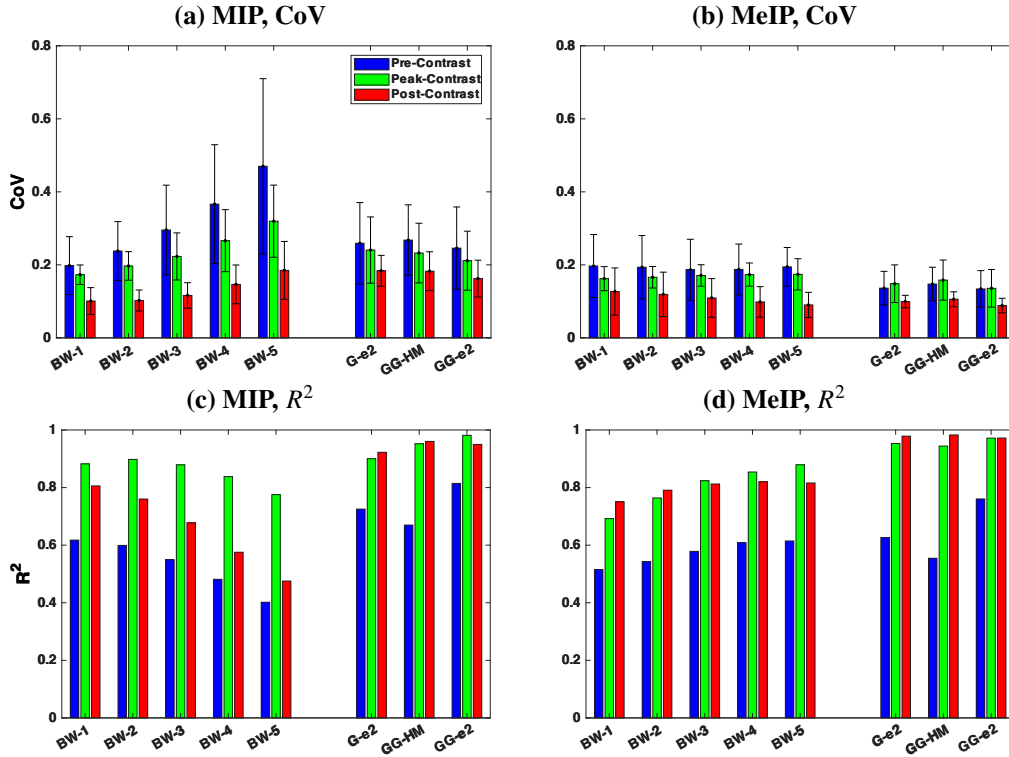


Fig. 7. Summary of accuracy and precision across all diameter measurement methods. (a, b) Coefficient of variation (CoV) and (c, d) coefficient of determination (R^2) for MIP (a, c) and MeIP (b, d), respectively. Bars are grouped by method (BW-1 through BW-5, G- e^2 , GG-HM, GG- e^2) and colour-coded by contrast conditions.

Table 1. Summary of slope (m), coefficient of determination (R^2), and coefficient of variation (CoV) for all diameter measurement methods across pre-contrast, peak contrast, and post-contrast conditions. Methods are grouped as binary mask based and model-based. Bold values indicate slope agreement within 10% of unity ($0.9 \leq m \leq 1.1$), strong linearity ($R^2 \geq 0.90$), or high precision ($\text{CoV} \leq 0.10$).

BW-1			BW-2		BW-3		BW-4		BW-5		$w_{1/e^2, G}$		FWHM _{GG}		$w_{1/e^2, GG}$	
MIP	MeIP		MIP	MeIP	MIP	MeIP	MIP	MeIP	MIP	MeIP	MIP	MeIP	MIP	MeIP	MIP	MeIP
<i>Slope (m)</i>																
Pre	0.61	0.83	0.48	0.74	0.38	0.66	0.30	0.60	0.24	0.54	0.70	0.73	0.42	0.43	0.64	0.71
Peak	0.96	1.14	0.86	1.06	0.78	0.99	0.71	0.93	0.65	0.89	1.15	1.04	0.66	0.61	0.98	0.98
Post	0.92	1.11	0.82	1.03	0.73	0.96	0.63	0.91	0.54	0.86	1.12	1.04	0.66	0.61	1.02	1.00
<i>Coefficient of determination (R^2)</i>																
Pre	0.62	0.51	0.60	0.54	0.55	0.58	0.48	0.61	0.40	0.62	0.73	0.63	0.67	0.55	0.81	0.76
Peak	0.88	0.69	0.90	0.76	0.88	0.82	0.84	0.85	0.78	0.88	0.90	0.95	0.95	0.94	0.98	0.97
Post	0.81	0.75	0.76	0.79	0.68	0.81	0.58	0.82	0.48	0.82	0.92	0.98	0.96	0.98	0.95	0.97
<i>Coefficient of variation (CoV)</i>																
Pre	0.20	0.20	0.24	0.19	0.30	0.19	0.37	0.19	0.47	0.19	0.26	0.14	0.27	0.15	0.25	0.13
Peak	0.17	0.16	0.20	0.17	0.22	0.17	0.27	0.17	0.32	0.17	0.24	0.15	0.23	0.16	0.21	0.14
Post	0.10	0.13	0.10	0.12	0.12	0.11	0.15	0.10	0.18	0.09	0.18	0.10	0.18	0.11	0.16	0.09

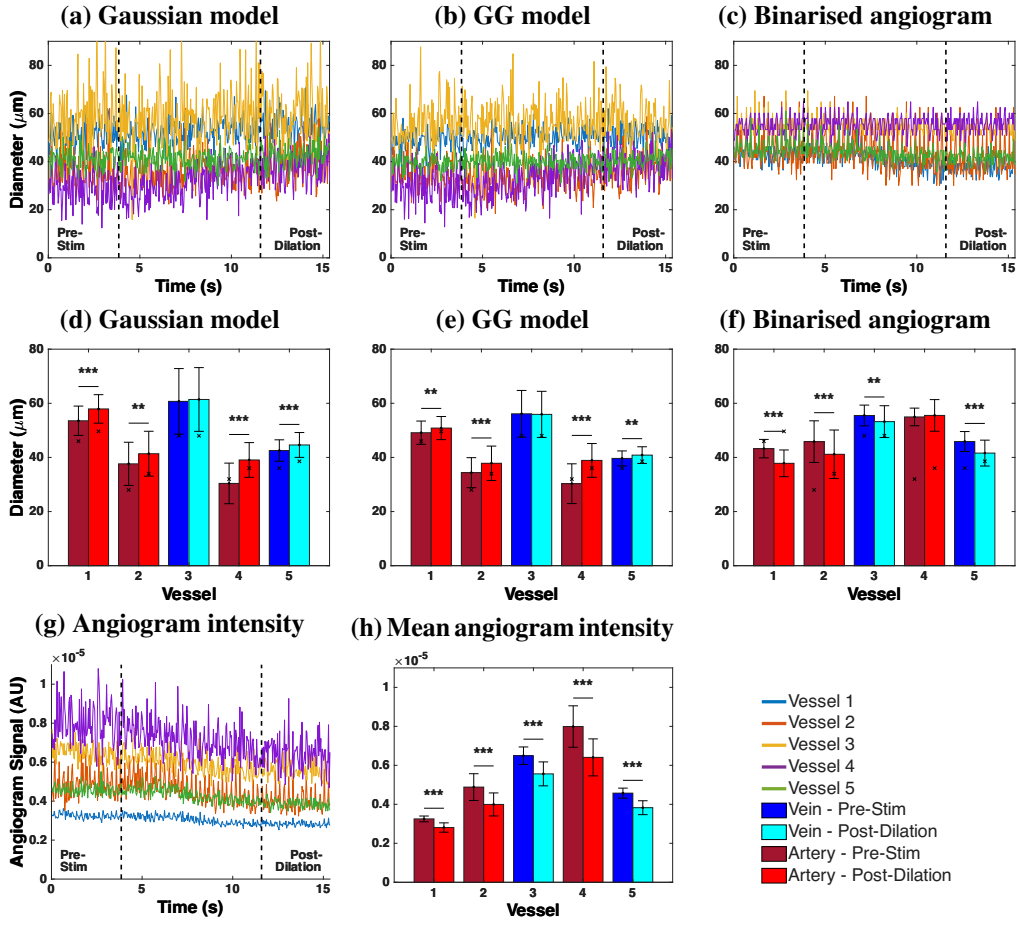


Fig. 8. Functional flicker stimulation results. (a–c) Vessel diameter time series pre- and post-stimulation for (a) Gaussian model, (b) Generalised Gaussian model, and (c) binarised angiogram, across five vessels. Vertical dashed lines indicate stimulation onset and offset. (d–f) Mean diameter per vessel before (dark bars) and after (light bars) stimulation for each method. Veins are shown in blue/cyan and arteries in dark/light red. Significance levels: ** $p < 0.01$, *** $p < 0.001$. (g) Angiogram intensity time series and (h) mean angiogram intensity per vessel pre- and post-stimulation.

277 These results demonstrated that the model-based diameter calculation provided more accurate
 278 and repeatable measurements, and also recovered physiologically meaningful vascular responses
 279 that binary mask based methods misrepresented.

Table 2. Flicker stimulation results. Δd : diameter change (%); ρ : Correlation between diameter and angiogram intensity; ΔI : intensity change (%). Statistically significant values are bold (* $p < 0.05$, ** $p < 0.01$, *** $p < 0.001$).

	Gaussian		GG		Binarised		Intensity
	Δd (%)	ρ	Δd (%)	ρ	Δd (%)	ρ	
Vessel 1	+8.2***	-0.07	+3.5**	0.03	-12.5***	0.59***	-13.6***
Vessel 2	+9.9**	0.23*	+10.1***	0.07	-10.2***	0.80***	-18.2***
Vessel 3	+1.2	-0.28**	-0.4	-0.28**	-4.1**	0.27**	-14.3***
Vessel 4	+28.5***	-0.15	+28.4***	-0.14	+1.0	0.46***	-19.8***
Vessel 5	+4.9***	-0.24*	+3.1**	-0.18	-9.3***	0.52***	-16.3***
Overall ρ		-0.101		-0.098		0.526	

280 4. Discussion

281 4.1. Model-based vs binary mask based diameter measurement

282 The model-based and binary mask based diameter methods define vessel boundary in fundamen-
 283 tally different ways. Binarisation of the en face maps discards the spatial intensity distribution
 284 and reduces each pixel to a binary decision. The measured diameter directly depends on the
 285 chosen threshold value and on angiogram intensity, both of which may vary across imaging
 286 sessions, contrast conditions, and even between vessels within the same scan. Model-based
 287 methods fit a parametric model function to the maximum or mean intensity profiles, and calculate
 288 the diameter from the fitted parameters. As the fit captures the shape of the profile rather than
 289 the absolute intensity, it is inherently less sensitive to changes in angiogram signal and does not
 290 require a varying threshold.

291 This difference explains the trends observed in Fig. 7. Model-based methods maintained
 292 strong linearity with the ground truth across all contrast conditions, whereas the binary mask
 293 based slopes degraded progressively with increasing threshold. Pre-contrast, the hourglass
 294 artefact caused by RBC orientation within vessel lumen suppresses edge signals, causing all
 295 methods to underestimate diameter [13]. However, model-based methods still maintained a linear
 296 relationship with the ground truth, producing systematic, predictable underestimation. Binary
 297 mask based methods on the other hand showed much weaker linearity, potentially because the
 298 suppressed edge signals did not consistently exceed the binarisation threshold, depending on
 299 vessel size and local intensity.

300 The generalised Gaussian (GG) model outperformed the standard Gaussian because the
 301 intensity profiles of the vessels are usually not purely Gaussian (Fig. 1b). The standard Gaussian
 302 cannot capture relatively flat-topped angiogram intensity profiles and tend to fit a narrower
 303 curve, whereas the GG model accommodates through the shape parameter β , which ranges
 304 from Gaussian ($\beta = 2$) to increasingly flat-topped profiles ($\beta > 2$). Among the width metrics,
 305 FWHM_{GG} consistently showed the weakest accuracy. It could be because the half-maximum
 306 determines the vessel boundary where the intensity has already dropped inside the true edge.
 307 The $1/e^2$ width captures more of the transition region and so may have provided a more accurate
 308 measurement of the vessel diameter.

309 4.2. Maximum vs mean intensity projection

310 Across nearly all methods and conditions, MeIP outperformed MIP in both accuracy and
311 precision (Table 1). This finding is noteworthy because MIP has been shown to produce higher
312 signal-to-noise ratio (SNR) and contrast in en face OCTA images [10], and is the default in many
313 commercial OCTA systems and analysis pipelines [9, 11]. However, we observed that higher
314 SNR did not necessarily translate to more accurate diameter measurements. The MIP selects the
315 single highest intensity value along each A-scan within the vessel ROI, which makes it inherently
316 sensitive to outliers. MeIP averages all intensity values along each A-scan, which smooths out
317 intensity fluctuations and provides a more average profile. This averaging could be beneficial for
318 vessel diameter measurement, as the goal is to capture the typical vessel boundary rather than
319 extreme signal events.

320 The difference between MIP and MeIP was especially apparent in the binary mask based results
321 (Table 1). For MeIP, the slope declined more gradually and remained above 0.86 even at BW-5
322 post-contrast. Whereas for MIP, the slope decreased steeply with increasing threshold, dropping
323 from 0.92 at BW-1 to 0.54 at BW-5 post-contrast. These findings suggest that MeIP produces a
324 more uniform intensity distribution across the vessel profile, making the binarisation result less
325 sensitive to the exact threshold value. The CoV data (Table 1) reinforced this as the MIP-based
326 binary mask CoV increased substantially with threshold, whereas the MeIP-based CoV remained
327 relatively stable. This behaviour follows from the shape of the two projected profiles. Because the
328 MIP retains only the brightest pixel along each A-scan, the resulting profile is sharply peaked with
329 steep rises and falls, and the peak intensity could vary considerably between vessels depending
330 on the local signal. Raising the threshold could therefore remove a vessel dependent fraction
331 of the cross-section, and so the measured width scatters more widely about its mean causing
332 increased CoV. Unlike MIP, MeIP averages along each A-scan and produces a broader, smoother
333 profile. As a result, thresholding produces a comparable reduction in measured width across
334 vessels, leading to a largely unchanged CoV despite increasing threshold. For model-based
335 methods, MeIP also showed better performance. The $w_{1/e^2, G}$ using MIP slightly overestimated
336 vessel diameter post-contrast with $m = 1.12$, while MeIP reduced this to $m = 1.04$, a much closer
337 agreement with the ground truth. These results suggest that while MIP may be preferred for
338 visualisation purposes where contrast and SNR are important [10], MeIP should be the preferred
339 projection method for quantitative diameter measurements.

340 4.3. Influence of angiogram intensity on diameter measurements

341 The functional flicker stimulation experiment provided a direct demonstration of how changes in
342 angiogram signal intensity can affect diameter measurements based on the method used. During
343 the DyC-OCT acquisition, the angiogram intensity declined significantly across all five vessels
344 (Fig. 8g,h), with decreases ranging from -14.1% to -19.9% (Table 2). **We are not sure about**
345 **the cause of this decline, but the inspection of the volumetric data ruled out the most important**
346 **confounds. There was no out-of-plane motion or breathing artefact, and the image quality was**
347 **consistent throughout the scan. We suspect a combination of rapid corneal drying and/or cataract**
348 **formation over the course of the scan could have caused the decline in intensity. More importantly,**
349 **the cause of the decline is not essential to our argument for this study, what matters is that the**
350 **intensity decline biases the binary mask-based diameter measurement while the model-based**
351 **diameter remain unaffected.**

352 The model-based methods correctly detected this expected vasodilation, with the Gaussian
353 model showing significant diameter increases in four of five vessels (up to $+28.5\%$) and the
354 GG model showing significant increases in three of five vessels (Table 2). The binary mask
355 based method, however, reported significant diameter decreases in four of five vessels, suggesting
356 vasoconstriction which is a paradoxical result. The reason behind this behaviour could be
357 understood by observing how each method responds to declining signal intensity (Fig. 9). For

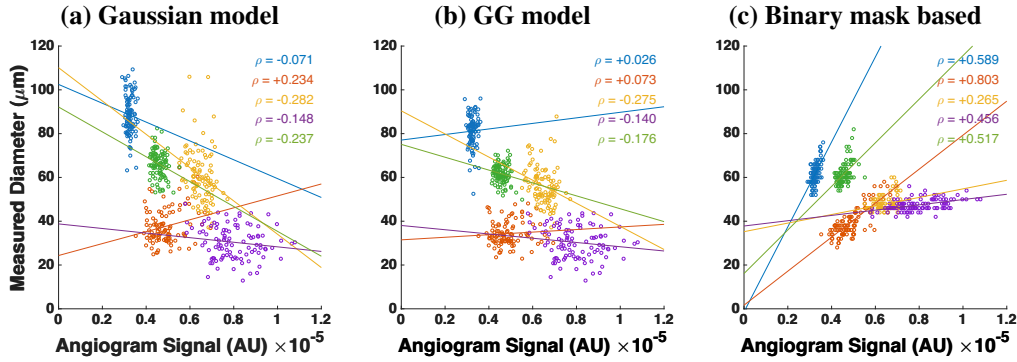


Fig. 9. Measured vessel diameter as a function of angiogram signal intensity during functional flicker stimulation for (a) Gaussian model, (b) Generalised Gaussian model, and (c) binary mask based method. Each colour represents one of five vessels. ρ denotes the Pearson correlation coefficient.

the binary mask based method, the threshold is fixed and diameter is determined by the number of pixels that exceed this threshold. When the overall angiogram intensity drops, fewer pixels at the vessel edges exceed the threshold, and the vessel appears to shrink even if the physical vessel diameter has increased. This is confirmed by the strong positive correlation between measured diameter and angiogram intensity for the binary mask based method ($\rho = 0.523$, $p < 0.0005$). In contrast, the model-based methods showed weak overall correlations with intensity ($\rho = -0.101$ for Gaussian, $\rho = -0.098$ for GG), indicating that the fitted diameter was effectively independent of the signal intensity. Among the methods, the GG model also produced the tightest error bars across the five vessels in the flicker experiment (Fig. 8d–f), consistent with its low CoV post-contrast (Table 1), indicating that it is the most repeatable of the metrics tested.

These findings have important implications for longitudinal studies and any experiment where angiogram intensity may vary between or within imaging sessions. In longitudinal mouse eye imaging, the angiogram signal can vary between and within sessions as anaesthesia alters retinal perfusion and ocular physiology [14, 15], with additional factors such as corneal drying and cataract formation further reducing OCT intensity over time [16, 17] if artificial tear drops are not applied during the imaging. If a binary mask based method is used under such conditions, observed changes in vessel diameter may reflect intensity fluctuations rather than true vascular changes. In contrast, model-based methods may be less sensitive to these intensity variations, as they characterise the shape of the intensity profile rather than relying primarily on absolute intensity values to define vessel boundaries.

4.4. Threshold selection

The results presented here used a basic, global threshold for the binarisation of the angiogram data. There are numerous other approaches for binarising the angiogram, which will most likely each behave differently. For example, angiogram signals can be enhanced with vesselness filters [18] and dynamic thresholds can be used to binarise images with varying SNR. When applying a vesselness filter, it is possible to enhance the shape of the angiogram and omit noise, but it is also possible for such enhancement to overcompensate the signal, leading to larger than expected vessel appearance. Dynamic thresholding can also yield a more uniform angiogram appearance, but similarly risks over- or under-compensating vessels given that threshold level directly affects the measured diameter. Further analysis of these other methods would be required to determine their efficacy in returning accurate and precise diameter values.

The key observation from the present work is that any thresholding approach, regardless of

390 how the threshold is determined, shares the same fundamental limitation that the measured
391 diameter depends on the absolute signal intensity at the vessel edges. As demonstrated by the
392 flicker stimulation experiment, this intensity dependence can introduce artefactual diameter
393 changes when the angiogram signal varies over time or between sessions. A more adaptive
394 thresholding strategy may reduce variability across different regions of a single image, but it
395 would not eliminate the sensitivity to temporal intensity fluctuations that we observed. The
396 model-based approach avoids this limitation entirely by deriving diameter from the shape of the
397 intensity profile rather than from an intensity cut-off, making it a fundamentally different and
398 more robust alternative for quantitative diameter analysis.

399 4.5. *Best choices under different conditions*

400 Under the conditions where a contrast agent is available and accuracy is the primary goal, the
401 $w_{1/e^2, GG}$ metric using MeIP provides the best results post-contrast. This combination achieved
402 a slope of $m = 1.001$ with $R^2 = 0.97$ and a CoV of 0.09, yielding the best accuracy, linearity,
403 and precision of all tested methods. If only pre-contrast data is available, the same metric
404 still provides the best linearity ($R^2 = 0.88$) among all methods, though the slope of $m = 0.71$
405 indicates that diameter could be underestimated by approximately 30%. In this case, a correction
406 factor could be applied if absolute diameter values are needed, though relative comparisons
407 between vessels or timepoints would remain valid without correction.

408 When only MIP data is available, which is the case for many commercial OCTA machines and
409 existing datasets, the $w_{1/e^2, GG}$ still provides good post-contrast accuracy ($m = 1.02$, $R^2 = 0.93$).
410 For binary mask based analysis of MIP data, only the lowest threshold (BW-1) post-contrast
411 achieved a slope near unity ($m = 0.92$), and the slope degraded rapidly with increasing threshold
412 values. This highlights that if binarisation must be used with MIP data, a lower threshold value is
413 essential, though this may come at the cost of increased noise sensitivity.

414 If computation time is a limiting factor and model fitting is not practical, MeIP with a moderate
415 threshold (e.g. BW-3) provides a reasonable alternative. At post-contrast, BW-3 using MeIP
416 achieved $m = 0.97$ and $R^2 = 0.80$, which is acceptable for many applications. MeIP-based
417 binary mask based analysis showed more stable CoV values across all thresholds compared to
418 MIP, making the results less sensitive to the exact threshold choice. This stability makes MeIP
419 the preferred projection for binary mask based OCTA.

420 4.6. *Literature comparison*

421 Hormel et al. [10] showed that MIP produces en face OCTA images with higher SNR and contrast
422 compared to MeIP, and concluded that MIP should be preferred for OCTA visualisation. Our
423 results are consistent with this for image quality purposes, but reveal a different picture when it
424 comes to quantitative vessel diameter measurement. We found that MeIP consistently yielded
425 more accurate and precise diameter values than MIP across both model-based and binary mask
426 based approaches. This suggests that the projection method best suited for visualisation is not
427 necessarily the best suited for quantification, and that the choice of projection should depend on
428 the intended analysis.

429 The challenge of standardising OCTA image analysis has been highlighted by Sampson
430 et al. [11] and Untracht et al. [9], both of whom emphasised the need for transparent, reproducible
431 analysis pipelines. Our findings add to this discussion by showing that the choice of diameter
432 measurement method introduces a source of variability that is at least as significant as the
433 choice of binarisation threshold. The model-based approach presented here offers a path toward
434 more standardised vessel diameter quantification, as it reduces the dependence on selected
435 thresholds and angiogram intensity, and provides measurements that are more robust across
436 imaging conditions.

437 The RBC orientation artefact and its effect on OCTA vessel appearance has been described by

438 Bernucci et al. [13] and Cimalla et al. [19], who used Intralipid contrast to demonstrate that the
439 hourglass pattern in vessel cross-sections is caused by the directional scattering properties of
440 RBCs rather than by true variations in flow. Our work extends this observation by quantifying
441 the degree to which this artefact affects diameter measurements and by proposing model-based
442 fitting as a practical correction strategy. While contrast enhancement with Intralipid is effective
443 for revealing the true vessel diameter, it requires a contrast injection and is not yet applicable in
444 clinical settings. Using a calibrated model-based approach provides a way to partially recover
445 the underestimated diameter from native OCTA data without the need for a contrast agent.

446 Recent work by Son et al. [20] used functional OCT to image flicker-evoked vasodilation in
447 the mouse retina and reported that vasodilation is anisotropic, with larger percent changes in the
448 axial direction ($\sim 18\%$) than the lateral direction ($\sim 11\%$). The authors did not describe how
449 vessel diameters were quantified from their B-scans. It is worth considering whether the lateral
450 diameter measurements may have been affected by the intensity-dependent artefacts observed in
451 the present work. In the lateral direction, the RBC orientation artefact suppresses signal at vessel
452 edges, and depending on how their vessel boundary was defined, this artefact could lead to an
453 underestimation of the lateral diameter. If this were the case, the apparent difference between
454 axial and lateral vasodilation could be influenced by the measurement methodology in addition
455 to the biomechanical anisotropy discussed by the authors. It would be interesting to apply the
456 model-based approach presented here to such data to determine whether their reported anisotropy
457 changes when the lateral diameter is quantified differently.

458 The magnitude of vasodilation detected by our model-based methods ranged from $+1.5\%$
459 to $+28.5\%$ across the five vessels measured (Table 2). The arteries (Vessels 1, 2, and 4)
460 showed the largest diameter increases, with the Gaussian model detecting changes of $+9.2\%$,
461 $+9.6\%$, and $+28.5\%$, respectively, while the veins (Vessels 3 and 5) showed smaller diameter
462 increases of $+1.5\%$ and $+4.9\%$. Table 3 summarises the stimulation protocols and vascular
463 responses reported by previous flicker stimulation studies alongside our own. The listed human
464 studies span several measurement techniques, from fundus photography [21] through retinal
465 vessel analysers [22–24] to Doppler OCT [25] and OCTA [26]. Despite these methodological
466 differences, the reported human arterial responses cluster between $+3\%$ and $+8\%$, and venous
467 responses between $+2\%$ and $+10\%$. Notably, these studies report arterial and venous responses
468 of broadly comparable magnitude, and in some cases the venous response is the larger of the two,
469 for example $+9.8\%$ venous versus $+8.0\%$ arterial in Aschinger et al. [25]. This contrasts with
470 our measurements, in which the arterial response was consistently and substantially larger than
471 the venous response. Whether this asymmetry reflects a genuine feature of the murine flicker
472 response, the small number of vessels sampled, or a greater sensitivity of the model-based fit
473 to the smooth-muscle-driven dilation of arteries remains to be established. Polak et al. [22]
474 additionally showed that the diameter response is relatively stable across flicker frequencies from
475 4 to 40 Hz, suggesting that frequency differences between studies are unlikely to explain the
476 variation.

477 The magnitudes we observed are generally larger than those reported in the human studies,
478 though direct comparison is difficult given the differences in experimental conditions. Species,
479 anaesthesia, stimulation frequency and wavelength, stimulus power and delivery method, stim-
480 ulation duration, dark adaptation period, and imaging modality all vary across the reported
481 studies, and each of these factors could influence the measured vascular response. Among the
482 studies listed, Son et al. [20] used the most similar setup to ours. They used the same mouse
483 strain (C57BL/6J), the same anaesthetic (ketamine/xylazine), a comparable flicker stimulus
484 (10 Hz, 504 nm), however a different stimulation period of 5 s. A systematic comparison of these
485 parameters could help determine which factors are most influential to the results observed in
486 both studies. Importantly, regardless of the absolute magnitude, the fact that we were able to
487 detect vasodilation at all depended on the measurement method, because binary mask based

analysis not only failed to detect vasodilation but reported vasoconstriction which would have led to fundamentally incorrect physiological conclusions.

Previous studies in mice have measured flicker-evoked retinal vessel diameter changes mostly using dynamic vessel analysis (DVA), which is a fundus camera-based technique adapted from human retinal vessel analysers. Albanna et al. [27] demonstrated the feasibility of DVA in the mouse eye using 12.5 Hz flicker at 530 nm but found that quantitative arterial recordings were possible only in a minority of animals, while venous dilation was mostly below 1.5% post-stimulation. Another study by Neumaier et al. [28] used the same setup in wildtype and Cav2.3-deficient mice with overnight dark adaptation and reported median arterial and venous diameter changes of only +1.3% and +1.2%, respectively, in the wildtype group. These values are substantially smaller than those we observed, which could be due to the limited spatial resolution and signal-to-noise ratio of DVA when applied to the smaller mouse eye rather than being a genuine physiological response. The much larger responses we observed may therefore partly result from the higher lateral resolution of OCT combined with the model-based fitting approach, which captures vessel boundary shifts that could fall below the detection limit of DVA. In addition to these diameter-based studies, Rai et al. [29] recently reported that 12 Hz flicker stimulation significantly increased both arterial and venous retinal blood flow in light-adapted C57BL/6J mice, confirming that the mouse retina exhibits a robust neurovascular coupling response. Since blood flow is proportional to the product of vessel cross-sectional area and flow velocity, their findings are consistent with the vasodilation we observed, although a direct quantitative comparison between flow and diameter changes is not straightforward.

Table 3. Comparison of flicker stimulation protocols and reported diameter changes across studies. H = human, M = mouse. DA = dark adaptation. Lat. = lateral, ax. = axial.

Study	Stimulation	Stimulation	Stimulation	DA	Diameter Change (%)	
	Freq. (Hz)	Light Source	Duration (s)	(h)	Artery	Vein
Formaz [21] (H)	10	Xenon arc, 5.4 log Td [§]	60	—	+4.2	+2.7
Polak [22] (H)	8	< 550 nm, ~ 150 μ W, cm ^{-2†}	60	—	+3.5	+1.9
Garhofer [23] (H)	8	< 550 nm, 300 μ W, cm ^{-2†}	60	—	+3.8	+2.8
Nagel [24] (H)	12.5	530 – 600 nm, ~ 196 μ W, cm ^{-2†}	20	—	+6.9	+6.5
Aschinger [25] (H)	12.5	530 – 600 nm, ~ 196 μ W, cm ^{-2†}	120	—	+8.0	+9.8
Kallab [26] (H)	7	White, ~ 450 lux	*	—	+3.7	+4.5
Albanna [27] (M)	12.5	530 nm, 30 lux	20	12	— [#]	< 1.5 [#]
Neumaier [28] (M)	12.5	530 nm, 30 lux	20	12	+1.3	+1.2
Son [20] (M)	10	504 nm, ~ 460 lux	5	1 – 2	lat. +10.8, ax. +18.2	lat. +8.9, ax. +14.3
Present study (M)	10	502 nm, 26.6 μ W [‡]	Cont.	2	+9.2 to +28.5	+1.5 to +4.9

[§]Diameter measured from fundus photographs taken post-stimulation; retinal luminance in trolands.

[#]DVA feasibility study; arterial recordings were not reliably obtainable in the mouse eye.

*Flicker applied during OCTA scan acquisition. [†]Retinal irradiance. [‡]Power at cornea.

4.7. Future direction

A future direction of this work is to move toward fully automated segmentation and calculation of vessel diameters from en face angiogram maps. While ROIs were manually selected in this work, it is also possible to automatically segment angiographic data using traditional skeletonisation methods, which are commonly used for automated OCTA analysis. From a skeletonised image, vessel angle can be computed for further extraction of vascular cross-sections perpendicular to the vessel axis. These cross-sections could then be processed using the model-based methods described here to enable fully automated analysis of 3D OCTA data sets, rather than the semi-

automated approach shown here for 2D OCTA data. This type of model-based approach is particularly important for comparing 3D volumes acquired at different time points in the mouse eye, as there are often intensity losses caused by drying of the eye, cataract formation, etc. As we have shown in this work, even low levels of intensity loss occurring over a short time window can significantly affect the measured vessel diameter when using a binary mask based approach, but not when using the models presented here.

Additionally, this work focused on the larger vessels of the superficial vascular plexus. Extending the model-based approach to the intermediate and deep capillary plexuses, where vessels are smaller and signal levels are lower, would be valuable for studying microvascular changes in diseases. For very small vessels approaching the lateral resolution limit of the imaging system, the measured intensity profile is a convolution of the true vessel profile with the point spread function (PSF) of the incident beam on the retina. Since the lateral resolution of OCT is typically worse than the axial resolution and is determined by the beam optics rather than the source bandwidth, this convolution becomes increasingly significant for smaller vessels. If the PSF were known, a deconvolution approach could be used to recover the true vessel profile before model fitting, potentially improving accuracy for capillary-scale vessels. However, characterising the retinal PSF in vivo remains challenging, as it depends on the ocular optics of each individual eye and may vary with retinal depth and eccentricity.

References

1. A. Javed, A. Khanna, E. Palmer, *et al.*, “Optical coherence tomography angiography: A review of the current literature,” *J. Int. Med. Res.* **51**, 03000605231187933 (2023).
2. S. Fialová, M. Augustin, M. Glösmann, *et al.*, “Polarization properties of single layers in the posterior eyes of mice and rats investigated using high resolution polarization sensitive optical coherence tomography,” *Biomed. Opt. Express* **7**, 1479–1495 (2016).
3. C. W. Merkle, M. Augustin, D. J. Harper, *et al.*, “High-resolution, depth-resolved vascular leakage measurements using contrast-enhanced, correlation-gated optical coherence tomography in mice,” *Biomed. Opt. Express* **12**, 1774–1791 (2021).
4. Y. Fu and K.-W. Yau, “Phototransduction in mouse rods and cones,” *Pflügers Arch. J. Physiol.* **454**, 805–819 (2007).
5. C. W. Merkle and V. J. Srinivasan, “Laminar microvascular transit time distribution in the mouse somatosensory cortex revealed by Dynamic Contrast Optical Coherence Tomography,” *NeuroImage* **125**, 350–362 (2016).
6. M. Augustin, S. Fialová, R. Plasenzotti, *et al.*, “Multi-functional OCT image processing for rodent eyes,” in *Optical Tomography and Spectroscopy*, (OSA - The Optical Society, Center for Medical Physics and Biomedical Engineering, Medical University of Vienna, Waehringer Guertel 18-20, 4L, Vienna, A-1090, Austria, 2016), p. 3.
7. V. J. Srinivasan, J. Y. Jiang, M. A. Yaseen, *et al.*, “Rapid volumetric angiography of cortical microvasculature with optical coherence tomography,” *Opt. Lett.* **35**, 43–45 (2010).
8. D. J. Harper, M. Augustin, A. Lichtenegger, *et al.*, “Retinal analysis of a mouse model of Alzheimer’s disease with multicontrast optical coherence tomography,” *Neurophotonics* **7**, 015006 (2020).
9. G. R. Untracht, M. S. Durkee, M. Zhao, *et al.*, “Towards standardising retinal oct angiography image analysis with open-source toolbox octava,” *Sci. Reports* **14** (2024).
10. T. T. Hormel, J. Wang, S. T. Bailey, *et al.*, “Maximum value projection produces better en face oct angiograms than mean value projection,” *Biomed. Opt. Express* **9**, 6412 (2018).
11. D. M. Sampson, A. M. Dubis, F. K. Chen, *et al.*, “Towards standardizing retinal optical coherence tomography angiography: a review,” *Light. Sci. & Appl.* **11** (2022).
12. C. S. Lee, A. J. Tying, Y. Wu, *et al.*, “Generating retinal flow maps from structural optical coherence tomography with artificial intelligence,” *Sci. Reports* **9** (2019).
13. M. T. Bernucci, C. W. Merkle, and V. J. Srinivasan, “Investigation of artifacts in retinal and choroidal OCT angiography with a contrast agent,” *Biomed. Opt. Express* **9**, 1020–1040 (2018).
14. S. Worm, G. Ladurner, L. May, *et al.*, “Retinal OCT parameters and physiological dynamics as an effect of anesthesia in C57BL/6j mice,” *Investig. Ophthalmol. & Vis. Sci.* **67**, 50 (2026).
15. G. Feng, A. Joseph, K. Dholakia, *et al.*, “High-resolution structural and functional retinal imaging in the awake behaving mouse,” *Commun. Biol.* **6**, 572 (2023).
16. D. M. Stein, G. Wollstein, H. Ishikawa, *et al.*, “Effect of corneal drying on optical coherence tomography,” *Ophthalmology* **113**, 985–991 (2006).
17. G. J. McLellan and C. A. Rasmussen, “Optical coherence tomography for the evaluation of retinal and optic nerve morphology in animal subjects: Practical considerations,” *Vet. Ophthalmol.* **15**, 13–28 (2012).
18. A. F. Frangi, W. J. Niessen, K. L. Vincken, and M. A. Viergever, “Multiscale vessel enhancement filtering,” in *Medical Image Computing and Computer-Assisted Intervention — MICCAI’98*, vol. 1496 of *Lecture Notes in Computer*

- 574 *Science* W. M. Wells, A. Colchester, and S. Delp, eds. (Springer, Berlin, Heidelberg, 1998), pp. 130–137.
- 575 19. P. Cimalla, J. Walther, M. Mittasch, and E. Koch, “Shear flow-induced optical inhomogeneity of blood assessed in
576 vivo and in vitro by spectral domain optical coherence tomography in the 1.3 μm wavelength range,” *J. Biomed. Opt.*
577 **16**, 116020 (2011).
- 578 20. T. Son, G. Ma, and X. Yao, “Functional OCT reveals anisotropic changes of retinal flicker-evoked vasodilation,” *Opt.*
579 *Lett.* **49**, 2121–2124 (2024).
- 580 21. F. Formaz, C. E. Riva, and M. Geiser, “Diffuse luminance flicker increases retinal vessel diameter in humans,” *Curr.*
581 *Eye Res.* **16**, 1252–1257 (1997).
- 582 22. K. Polak, L. Schmetterer, and C. E. Riva, “Influence of flicker frequency on flicker-induced changes of retinal vessel
583 diameter,” *Investig. Ophthalmol. & Vis. Sci.* **43**, 2721–2726 (2002).
- 584 23. G. Garhöfer, C. Zawinka, H. Resch, *et al.*, “Diffuse luminance flicker increases blood flow in major retinal arteries
585 and veins,” *Vis. Res.* **44**, 833–838 (2004).
- 586 24. E. Nagel and W. Vilser, “Flicker observation light induces diameter response in retinal arterioles: A clinical
587 methodological study,” *Der Ophthalmol.* **102**, 305–309 (2005).
- 588 25. G. C. Aschinger, L. Schmetterer, K. Fondi, *et al.*, “Effect of Diffuse Luminance Flicker Light Stimulation on Total
589 Retinal Blood Flow Assessed With Dual-Beam Bidirectional Doppler OCT,” *Investig. Ophthalmol. & Vis. Sci.* **58**,
590 1167–1178 (2017).
- 591 26. M. Kallab, N. Hommer, B. Tan, *et al.*, “Plexus-specific effect of flicker-light stimulation on the retinal microvasculature
592 assessed with optical coherence tomography angiography,” *Am. J. Physiol. Circ. Physiol.* **320**, H23–H28 (2020).
- 593 27. W. Albanna, K. Kotliar, J. N. Lüke, *et al.*, “Non-invasive evaluation of neurovascular coupling in the murine retina by
594 dynamic retinal vessel analysis,” *PLOS ONE* **13**, e0204689 (2018).
- 595 28. F. Neumaier, K. Kotliar, R. H. L. Haeren, *et al.*, “Evaluation of flicker-induced retinal vessel response in cav2.3-deficient
596 mice using dynamic retinal vessel analysis,” *Front. Neurol.* **12**, 659890 (2021).
- 597 29. M. Rai, Y. Lakshmanan, K. Y. Choi, and H. H.-I. Chan, “Effects of flickering light stimulation on retinal blood flow
598 and full-field electroretinogram in mice,” *Documenta Ophthalmol.* **151**, 205–218 (2025).