

# Universal manuscript template for Optica Publishing Group journals

YASH PATEL,<sup>1</sup> PRAJAKTA BELEKAR,<sup>1</sup> GEORG LADURNER,<sup>1</sup> SYBREN WORM,<sup>1</sup> LUCAS MAY,<sup>1</sup> MARIA VARAKA,<sup>1</sup> THERESA ROHRMOSER,<sup>1</sup> FERNANDO GARCÍA-RAMÍREZ,<sup>1</sup> RENÉ WERKMEISTER,<sup>1</sup> BERNHARD BAUMANN,<sup>1,2</sup> AND CONRAD W. MERKLE<sup>1,\*</sup>

<sup>1</sup>Center for Medical Physics and Biomedical Engineering, Medical University of Vienna, Währinger Gürtel 18-20/4L, 1090 Vienna, Austria

<sup>2</sup>Institute of Biomedical Physics, Medical University of Innsbruck, Müllerstraße 44, 6020 Innsbruck, Austria

\*conrad.merkle@meduniwien.ac.at

**Abstract:** This template contains important information on submissions to Optica Publishing Group journals. We encourage authors to focus foremost on their content and not on formatting. The template is provided as a guide, but following the visual styling is optional. Each manuscript will be formatted in a consistent way during production. Authors also have the option to [submit articles](#) to the Optica Publishing Group preprint server, [Optica Open](#). You may find it helpful to use our optional [Paperpal manuscript readiness check](#) and [language polishing service](#). Note that copyright and licensing information should not be added to your journal or Optica Open manuscript.

## 1. Introduction

Optical coherence tomography angiography (OCTA) is an extension of OCT that visualizes vascular perfusion using the motion contrast from red blood cells (RBCs). Over the years, OCTA has demonstrated widespread acceptance and use for clinical evaluations of vascular features in relation to disease [1]. OCT angiograms can be used to evaluate characteristics on the scale of vascular layers by measuring vascular density or non-perfusion zones, or it can be used to examine individual vessels with measurements of diameter or tortuosity. Nevertheless, OCT is prone to certain artifacts which specifically affect visualization of the vasculature. These artifacts may lead to underestimations of measurements of vessel diameter and density. When viewed in cross-section, large vessels often demonstrate an hourglass appearance with stronger scattering in the center than at the sides (Figure 1A). This appearance is due to orientation effects of RBCs, which align with the blood flow, causing a reduced scattering cross-section at the sides of the vessels. To compensate for these artifacts, OCT contrast agents such as Intralipid have previously been used to increase intravascular intensity signals, particularly in regions where RBC scattering is diminished. Here we examine different methods of measuring vessel size from in vivo OCT scans of mouse retinal vasculature, and we use a contrast agent to obtain ground truth vessel diameter measurements for comparison. We finally propose ways of mitigating or correcting for underestimations of vessel diameter related to typical OCT artifacts.

Optical coherence tomography (OCT) is a non-invasive optical imaging method, which uses interferometry to measure the transit time of light that is backscattered from a sample. OCT has found widespread clinical use in ophthalmology with XXX number of systems and XXX OCT scans performed annually around the world. OCT angiography (OCTA) is a functional extension of OCT which highlights motion between repeated OCT scans to generate images of vascular networks. Typically, OCTA signals are first calculated from the OCT intensity and/or phase information, segmented in 3D manually, algorithmically, or using a deep learning approach, and finally compressed into a 2D image using a maximum intensity projection. These 2D vascular maps can then be binarised by using a global or adaptive threshold, and finally vascular metrics

such as vessel density and diameter can be computed. Of these processing stages, the thresholding step is perhaps the most important. There are dozens of different thresholding methods that have been proposed over the years and each of these may produce different results in the binary map, which would in turn influence the quantification of vascular metrics. In this work, we examine an alternate approach for extracting quantitative vessel diameter by fitting a model to the OCTA data before binarisation to avoid thresholding-based effects.

In addition to thresholding-based variability, we hypothesize that OCTA metrics are also affected by OCT artifacts caused by the non-uniform backscattering profiles of red blood cells (RBCs). Because RBCs have a distinct bi-concave disc shape, they more effectively backscatter light when aligned perpendicular to the beam, rather than parallel to it. It has already been observed that in large vessels, a so-called hourglass artifact appears when viewed cross-sectionally. This is caused by the alignment of the RBCs with the vessel walls while under laminar flow, where the RBCs are perpendicular to the beam in the center of the vessels and parallel to the beam at the edges of the vessels. This artifact artificially suppresses the OCT and OCTA signals at the edges of the vessels, making them appear more narrow when projected into an en-face view, which is the preferred way of displaying angiographic data. Here we use contrast enhanced OCT (CE-OCT) to investigate how significant these effects are and how they can be corrected.

## 2. Methods and Materials

### 2.1. Imaging system

All imaging was performed using a custom-built polarisation-sensitive spectral-domain OCT ophthalmoscope, described in detail previously [2]. The system was centred at 840 nm with a spectral bandwidth of 100 nm at full width half maximum (FWHM), providing an axial resolution of approximately 5.1  $\mu\text{m}$  in air and 3.8  $\mu\text{m}$  in tissue (assuming a refractive index of 1.35). A sensitivity of 96 dB was achieved at an A-scan rate of 80 kHz and a beam diameter of 0.5 mm at the pupil plane (power at cornea = 2.85 mW) [3]. This system was employed to acquire volumetric OCT data from mouse retinas before, during, and after an intravascular contrast agent administration, as well as before and after functional stimulation of the mouse retina using a custom 502 nm light-emitting diode (LED) ring flashing at 10 Hz (power at cornea = 26.6  $\mu\text{W}$ ). This wavelength was selected to target the peak absorption of mouse rhodopsin (~500 nm), enabling predominantly rod-driven photoreceptor stimulation [4].

### 2.2. Experimental protocol

Three mouse models were used in this study: VLDLR knockout mice (B6;129S7-Vldlr<sup>tm1Her</sup>/J, The Jackson Laboratory, Bar Harbor, USA), C57BL/6 mice (C57BL/6, The Jackson Laboratory, Bar Harbor, USA), and SOD1 transgenic mice (strain details, The Jackson Laboratory, Bar Harbor, USA), with  $n = XX$  mice per group. All imaging sessions were conducted under general anaesthesia using either isoflurane or a ketamine/xylazine combination. Isoflurane was induced at 4% in oxygen for 4 minutes and subsequently maintained at 2% in oxygen at a flow rate of 1.5–2 L/min. In cases where isoflurane alone did not provide adequate sedation, an intraperitoneal injection of ketamine/xylazine cocktail (100 mg/kg ketamine, 6 mg/kg xylazine; 10 mL/kg body weight) was administered. To maintain core body temperature of the mice throughout imaging, they were positioned on a heating pad. Mouse pupils were dilated with one drop of tropicamide (5 mg/mL, Agepha Pharma s.r.o., Senec, Slovakia) per eye, and artificial tear drops (Oculotect, ALCON Pharma GmbH, Freiburg im Breisgau, Germany) were applied at regular intervals to prevent the cornea from drying out.

Intralipid has been shown to be a highly scattering contrast agent that fills the vascular lumen uniformly, thereby compensating for the artefact caused by the diminished backscattering at vessel peripheries caused by RBC orientation effects [3, 5, 6]. For this study, Intralipid 20%

1 VLDLR KO  
1 SOD1 Ctrl  
2 C57BL/6

Bolus tracking  
used i/o  
stimulation used  
K/X + a/c

simplify

(3 mL/kg body weight) was administered as a bolus injection via the tail vein. Volumetric angiography data were acquired over a 1 mm × 1 mm field of view centred on the optic nerve head (ONH), with a scan density of 500 A-scans per B-scan and five repeated B-scans at each of 400 slow-axis positions (acquisition time approximately 16 seconds). For this study, pre- and post-injection volumetric datasets were acquired. ~~This volumetric data was used solely for qualitative visualisation of the contrast enhancement effect across the retinal vascular plexuses and was not used for quantitative diameter analysis.~~ Additionally, a dynamic-contrast OCT (DyC-OCT) protocol [7] was employed during the contrast injection or during stimulation, consisting of 2000 repeated B-scans over approximately 16 seconds (interscan time 8.2 ms) at the same cross-sectional location over a 1 mm lateral field of view. DyC-OCT scans allow us to track the same vessels over time to precisely measure the effects of the contrast agent or the stimulation with a high degree of spatial coregistration. All quantitative vessel diameter measurements reported in this study were derived from the DyC-OCT data.

for visualization purposes

Functional flicker stimulation was performed in a C57BL/6 mouse to assess whether the choice of diameter measurement method affects the detection of physiological vascular responses. For this experiment, ketamine/xylazine cocktail was chosen over isoflurane to minimise anaesthesia-induced vasodilation. During the DyC-OCT acquisition, the retina was unstimulated for approximately 8 seconds, followed by 10 Hz flicker stimulation from the LED ring for the rest of the scan duration. To compare results before and after stimulation, the data was divided into baseline or pre-stim (4 seconds) and post-stim (4 seconds). ~~(We could maybe get a question about why we chose 4 seconds for pre- and post-stim, and not the full 8 seconds?)~~

Cite  
Here I believe stim started ~ 8s before acquisition and continued through

All animal procedures were approved by the ethics committee of the Medical University of Vienna and the Austrian Federal Ministry of Education, Science, and Research (BMBWF/66.009/0272-V/3b/2019 and GZ 2024-0.802.524).

### 2.3. Post-processing and analysis

Cross-polarised OCT intensity data from the retinal pigment epithelium (RPE) was used for inter-frame alignment and B-scan flattening [3, 8]. Angiograms were derived by applying the complex subtraction OCT angiography (OCTA) algorithm [9, 10]. We evaluated multiple combinations of methods for quantifying vessel diameter from the OCTA data to determine which combinations of steps work best under different conditions. Specifically, we looked at two types of data projections (maximum intensity and mean intensity) to generate vessel profiles and several different quantifications of those profiles including a traditional binarisation, a Gaussian model approach, and a Generalised-Gaussian (GG) model approach. These methods represent commonly used methods in the literature for OCTA quantification [11–14]. The different methods were evaluated against the ground truth as described in this section. All data processing and analysis was performed in MATLAB (R2019b, MathWorks, Natick, MA, USA).

why 10?

model based methods not used. 14?

#### 2.3.1. Ground truth calculation

Ground truth vessel diameters were obtained from contrast-enhanced DyC-OCT B-scan angiograms. The width and height of the vessel were manually measured from the vessel's cross-section. The ground truth diameter was defined as the minimum of the two measurements to account for off-axis cross-sectioning of the vessel, which produces a more elliptical appearance in the B-scan. For cases where the vessel is perpendicular to the B-scan, the height and width would therefore be in agreement. Because the lateral diameter is studied here, we defined a correction factor of  $\text{height}/\text{width}$  for cases where the width was larger than the height due to skewing effect and was equal to 1 otherwise. By multiplying this correction factor against diameter measured from the ROI projection, we ensured that the measured vessel diameter reflected the true size of the vessel.

after arrival of contrast potential

each method

← maybe instead lateral diameter instead of width/height

New Section  
Skew correction  
use Ground truth instead of height for this section

en face  
vs  
en face

large vessel in the field of view

### 2.3.2. Vessel projection calculation

For each vessel of interest, a rectangular region of interest (ROI) encompassing the vessel cross-section, along the lateral ( $x$ ) and axial ( $z$ ) dimensions, was selected from the DyC-OCT B-scan angiograms. En face intensity profiles were then generated by projecting the A-scans within this ROI along the axial ( $z$ ) direction. Two projection methods were compared: maximum intensity projection (MIP), which selects the highest intensity value along the depth axis of each ROI, and mean intensity projection (MeIP), which averages the values along each ROI. Each projection resulted in a time-stack of 1-D lateral intensity profiles for each vessel, which were then used for subsequent diameter quantification. For the model-based approaches, the profiles were normalised to a range of 0–1 to ensure a good fit.

for all time points

angiogram signal

consistent

move to model section

### 2.3.3. Model-based vessel diameter calculation

The two parametric models, the G+GG models, were fitted (Fig. 1a) to the one-dimensional intensity profiles from the previous step, using nonlinear least-squares regression in MATLAB.

Standard Gaussian function:

$$f(x) = A \exp\left(-\frac{(x - \mu)^2}{2\sigma^2}\right) + C \quad (1)$$

where  $A$  is the peak amplitude,  $\mu$  is the centre position,  $\sigma$  is the standard deviation, and  $C$  is a constant baseline offset.

Generalised-Gaussian (GG) function:

$$f(x) = A \exp\left(-\left(\frac{|x - \mu|}{\alpha}\right)^\beta\right) + C \quad (2)$$

where  $A$  is the peak amplitude,  $\mu$  is the centre position,  $\alpha$  is the scale parameter,  $\beta$  is the shape parameter, and  $C$  is a constant baseline offset. Given the imaging system configuration, all vessels are expected to produce at minimum a Gaussian intensity profile in the B-scan cross-section, and so profiles sharper than Gaussian profile ( $\beta < 2$ ) are therefore not technically meaningful. The shape parameter  $\beta$  was hence constrained to  $\beta \geq 2$  during fitting. With this constraint, the GG accommodated to profiles ranging from Gaussian ( $\beta = 2$ , where  $\sigma = \alpha/\sqrt{2}$ ) to increasingly flat-topped ( $\beta > 2$ ).

were not considered here

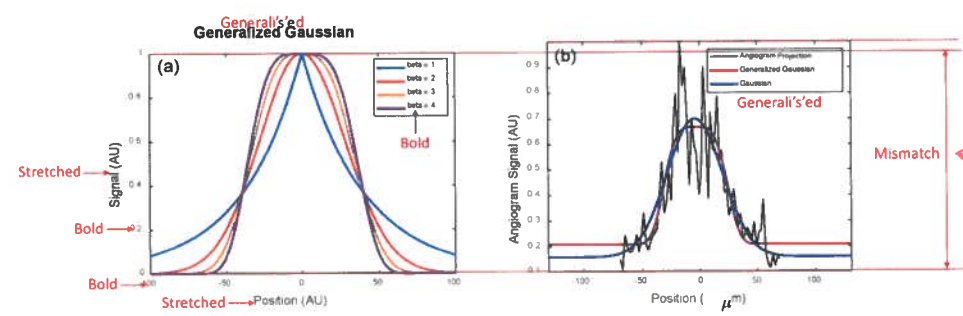


Fig. 1. (a) GG function for shape parameters  $\beta = 1, 2, 3$ , and 4. (b) Example vessel intensity profile (black) with standard Gaussian (blue) and GG (red) fits.

Two standard width metrics were calculated from the fitted models: the full width at half maximum (FWHM) and the  $1/e^2$  width. For the standard Gaussian fit, the  $1/e^2$  width was



166 calculated as:

$$w_{1/e^2, G} = 4\sigma \quad (3)$$

167 The FWHM for a Gaussian is related to the  $1/e^2$  width by a fixed proportionality:

$$\text{FWHM}_G = 2\sigma\sqrt{2\ln 2} = \frac{\sqrt{2\ln 2}}{2} w_{1/e^2, G} \quad (4)$$

168 and therefore only the  $1/e^2$  width was calculated directly from the fit, with the FWHM obtainable  
169 via this known relationship.

170 For the GG fit, no such linear relationship exists between the FWHM and  $1/e^2$  width, since  
171 both depend on the shape parameter  $\beta$ . Both metrics were therefore calculated independently as:

$$w_{\text{FWHM}, \text{GG}} \quad \text{FWHM}_{\text{GG}} = 2\alpha(\ln 2)^{1/\beta} \quad (5)$$

$$w_{1/e^2, \text{GG}} = 2\alpha \cdot 2^{1/\beta} \quad (6)$$

#### 173 2.3.4. Binary mask based vessel diameter calculation

174 For comparison with OCTA processing pipelines that rely on image binarisation, vessel diameters  
175 were also measured from binary masks generated by global thresholding. A 3D averaging  
176 filter with a kernel size of  $50 \times 50 \times 10$  voxels (lateral  $x \times$  axial  $z \times$  temporal  $t$ ) was applied  
177 to the DyC-OCT angiogram volumes to reduce noise and minimize the effects of outliers. To  
178 produce a binarised black and white (BW) mask, the maximum angiogram intensity within  
179 these smoothed volumes were calculated, and five different threshold values were defined as  
180 fixed percentages of these maxima for MIP and MeIP. For MIP, the thresholds were defined as  
181 BW-1 = 40%, BW-2 = 50%, BW-3 = 60%, BW-4 = 70%, and BW-5 = 80%. While for MeIP,  
182 the thresholds were defined as BW-1 = 07%, BW-2 = 08%, BW-3 = 09%, BW-4 = 10%, and  
183 BW-5 = 11% (maybe also explain why these specific thresholds were chosen?). Each threshold  
184 was applied to the unsmoothed en face projection (MIP and MeIP) to generate a binary mask,  
185 and the vessel diameter was measured as the number of pixels above the threshold across the  
186 lateral vessel cross-section.

#### 187 2.3.5. Statistical analysis

188 To evaluate the accuracy and precision of all diameter measurement approaches, the calculated  
189 diameter values were plotted against the ground truth for each vessel across three conditions:  
190 pre-contrast, peak contrast, and post-contrast. A linear regression was fitted to each condition,  
191 yielding the slope ( $m$ ) and coefficient of determination ( $R^2$ ). A slope of  $m = 1$  indicated  
192 perfect agreement with the ground truth, and  $R^2$  quantified the goodness of fit of the linear  
193 model. Additionally, the coefficient of variation (CoV) was computed for each method to assess  
194 measurement precision (repeatability). For the model-based methods, six combinations were  
195 evaluated: two projection methods (MIP and MeIP) by three width metrics ( $w_{1/e^2, G}$ ,  $\text{FWHM}_{\text{GG}}$ ,  
196 and  $w_{1/e^2, \text{GG}}$ ). For the binary mask based method, diameter was measured at five threshold levels  
197 (BW-1 through BW-5) for both MIP and MeIP. For the functional flicker stimulation experiment,  
198 the Pearson correlation coefficient ( $\rho$ ) between measured diameter values and angiogram intensity  
199 was computed for each method and vessel, to assess whether the diameter measurements were  
200 affected by changes in angiogram intensity. Measurements with  $p < 0.05$  were considered  
201 statistically significant.

### 202 3. Results

#### 203 3.1. Qualitative assessment of vessel underestimation

204 Figure 2 shows OCTA MIP enface images of the superficial vascular plexus (SVP), intermediate  
205 capillary plexus (ICP), and deep capillary plexus (DCP) before and after contrast injection. Across

To determine the threshold level, the maximum angiogram intensity was measured after applying...

based on observation to cover a range from borderline too low to borderline too high

a paired t-test was used to evaluate if the flicker stimulation-induced changes were significant, and

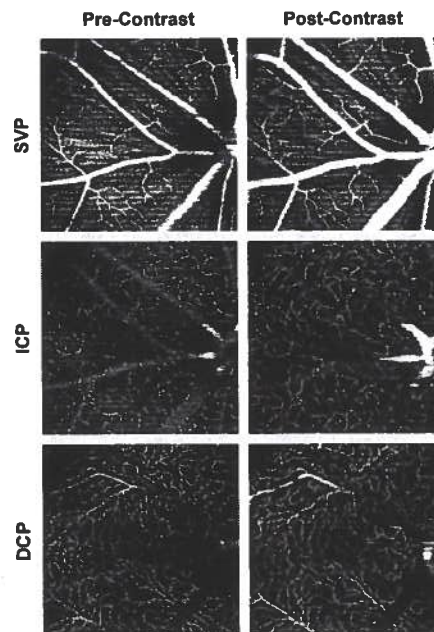


Fig. 2. OCTA MIP en face of the SVP, ICP, and DCP before (left) and after (right) the administration of Intralipid 20%. Vessels appear visibly wider and brighter post-contrast across all layers, most prominently in the larger vessels.

← which mouse and what conditions?  
C57BL/6-5 from 30.06.2023  
Check logs for anaesthesia

all three layers, vessels appeared visibly wider and brighter post-contrast injection, consistent with previous literature showing that OCTA underestimates vessel diameter in the absence of a contrast agent [3]. This effect was most pronounced in the larger vessels, especially in the SVP, where the major retinal arteries and veins appeared noticeably thicker after contrast administration. In the ICP and DCP, the capillary networks also showed improved visibility, though the effect was less dramatic.

DyC OCTA projections helped visualise the temporal changes in vessel diameter pre- and post-contrast injection (Fig. 3). Pre-contrast injection, the vessel cross-sections appeared narrower than their true diameter (Fig. 3a), which could be due to lateral edge signal suppression by the RBC orientation artefact [15]. At peak contrast, the Intralipid filled the vascular lumen uniformly, but the vessels look slightly extended beyond their true extent because of the dynamic range of the image (Fig. 3b). In the post-contrast phase, the signal stabilised as the initial bolus cleared, and the vessel boundaries remained more visible than before injection (Fig. 3c). The MIP and the corresponding binary mask over time (Figs. 3d-e) showed the observed temporal changes in vessel diameter across the three phases. The mean OCTA intensity (Fig. 3f) showed a sharp increase post-contrast injection, followed by a decrease to a new steady state that remained elevated above the pre-contrast baseline.

then with contrast

how are you judging this  
[ ] refit into discussion

### 3.2. Accuracy and precision of diameter measurements

The accuracy ( $m$ ,  $R^2$ ) and precision (CoV) of all diameter measurement methods are summarised in Table 1. All model-based methods underestimated vessel diameter in pre-contrast data, with slopes ranging from 0.42 to 0.73 (Table 1). Contrast enhancement improved accuracy across all metrics, though the degree of improvement varied. The  $FWHM_{GG}$  metric remained well below unity even post-contrast. The  $w_{1/e^2, G}$  with MIP slightly overestimated post-contrast

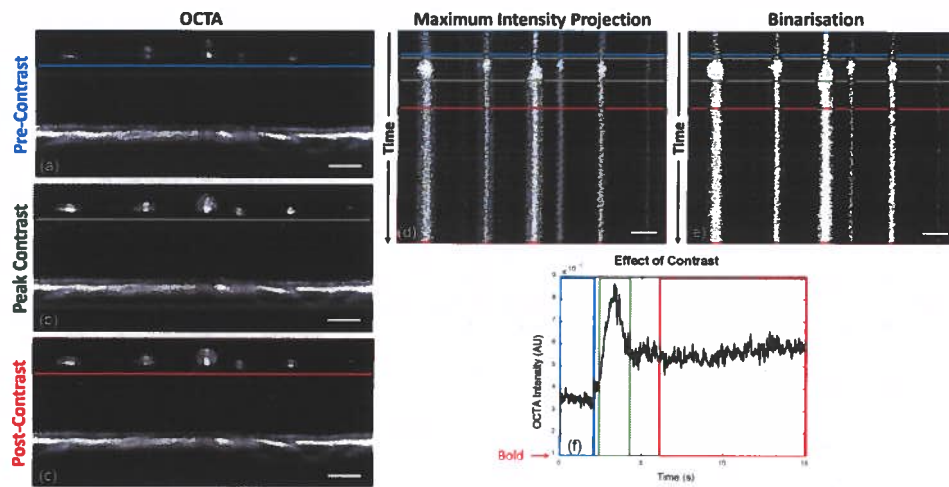


Fig. 3. DyC-OCT B-scan angiograms at (a) pre-contrast, (b) peak contrast, and (c) post-contrast timepoints. (d) MIP and (e) binarisation of the vessel cross-sections over time, with coloured boxes indicating the pre-contrast (blue), peak-contrast (green), and post-contrast (red) windows. (f) Mean OCTA intensity over time, showing the temporal intensity dynamics. All scale bars are 100  $\mu\text{m}$ .

( $m = 1.12-1.15$ ), while MeIP yielded values closer to unity ( $m = 1.04$ ). The  $w_{1/e^2, GG}$  with MeIP provided the best overall agreement, achieving a slope closest to unity with  $m = 1.001$  ( $R^2 = 0.97$ ) post-contrast, which was the closest to the identity line of all tested model-based methods. Across all metrics, MeIP mostly outperformed MIP in both accuracy and linearity (Table 1, Fig. 4).

For binary mask based methods, the slope decreased with increasing threshold across all contrast conditions and projections (Table 1). [This degradation was steeper for MIP than for MeIP. MIP slopes dropped from near unity at BW-1 to well below it at BW-5, whereas MeIP slopes declined more gradually and remained closer to unity across the threshold range.] MeIP slopes were consistently higher than MIP at every threshold and contrast condition, though at lower thresholds and at peak and post-contrast, MeIP tended to slightly overestimate vessel diameter. The  $R^2$  values followed a similar pattern. For MIP, pre- and post-contrast  $R^2$  decreased substantially with increasing threshold, whereas for MeIP,  $R^2$  remained relatively stable. Overall, MeIP provided more reliable binary mask based diameter measurements than MIP.

The precision of each method was assessed via the CoV (Table 1, Fig. 7). For MIP, the binary mask based CoV increased substantially with threshold, whereas the model-based CoV remained stable across all contrast conditions. For MeIP, the binary mask based CoV was notably more stable across thresholds than for MIP, and the model-based CoV values were lower overall, though they increased slightly at peak contrast before decreasing post-contrast. Across both methods, MeIP yielded lower CoV values than MIP pre-contrast and more stable values post-contrast. Among the model-based metrics,  $FWHM_{GG}$  consistently exhibited the weakest accuracy while maintaining comparable precision. Overall, model-based methods consistently outperformed binary mask based methods in both accuracy and precision, and MeIP yielded superior performance compared to MIP across all methods.

maybe remove difficult to compare  
can also discuss fig 7 here

well increased

disagree

with low threshold MIP is more precise but less accurate

Discuss  $R^2$  values for model based methods

MIP could be better for low thresholds.

Need to ~~also~~ include Figs 5+6 in Results.

Model-based showed good agreement between Peak+Post whereas binary (particularly MIP) showed poorer agreement. This gets worse w/ increasing threshold.

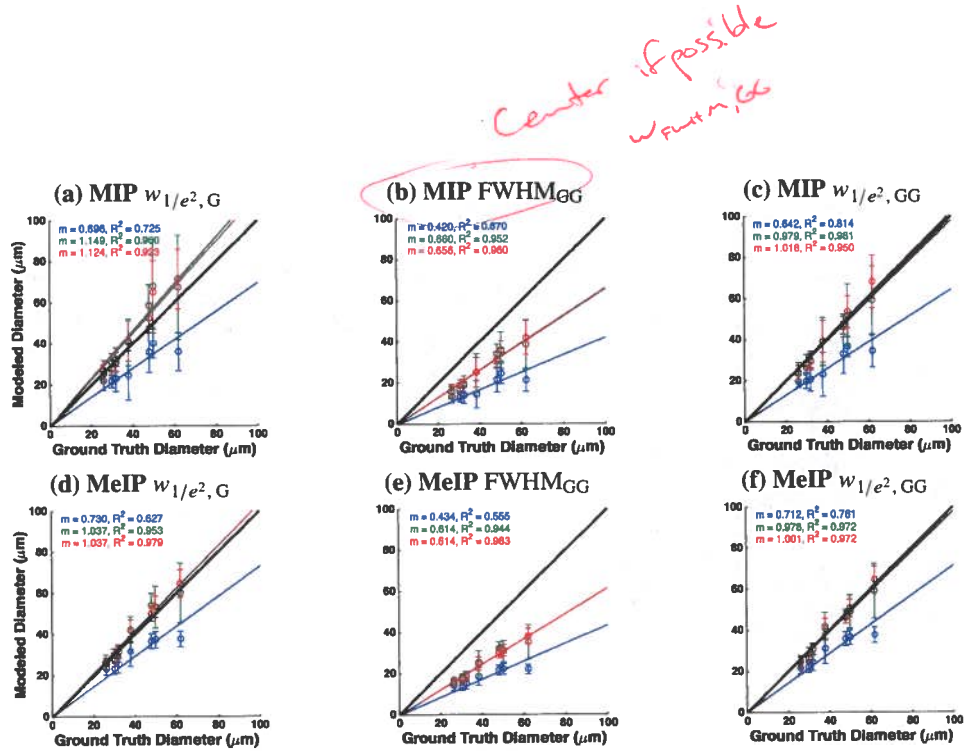


Fig. 4. Modelled versus ground truth vessel diameter using MIP (top row, a–c) and MeIP (bottom row, d–f). Columns correspond to  $w_{1/e^2, G}$  (a, d),  $FWHM_{GG}$  (b, e), and  $w_{1/e^2, GG}$  (c, f). Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions. The black line indicates the identity line ( $m = 1$ ).

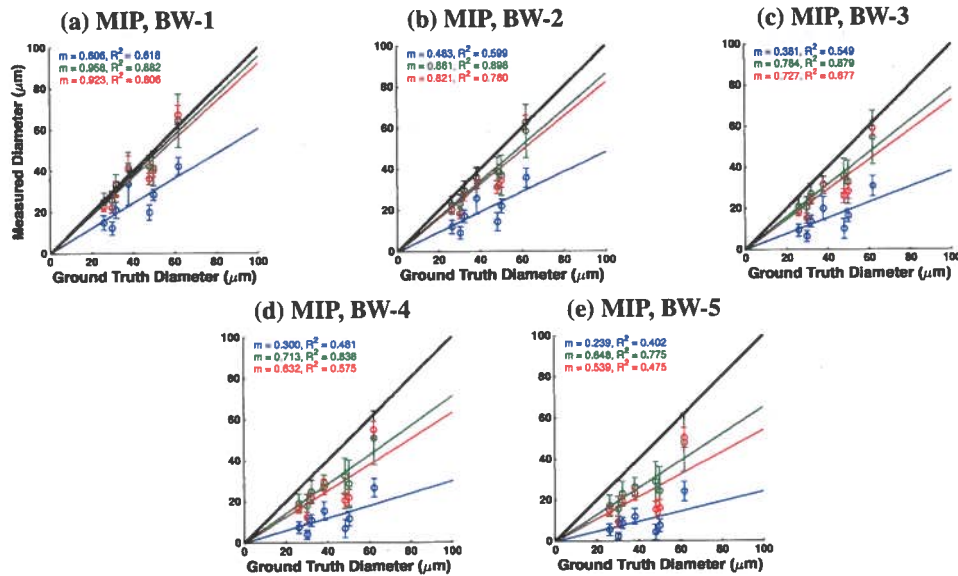


Fig. 5. Vessel diameter measured from binarised masks versus ground truth for MIP at five threshold levels: (a) BW-1 through (e) BW-5. Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions.



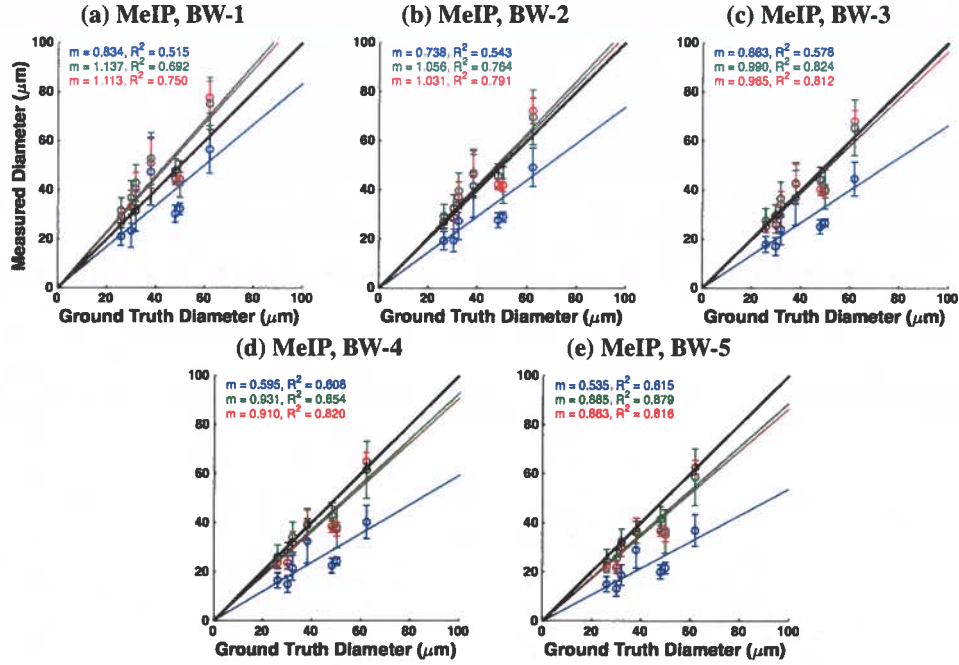


Fig. 6. Vessel diameter measured from binarised masks versus ground truth for MeIP at five threshold levels: (a) BW-1 through (e) BW-5. Linear regression lines and statistics are shown for pre-contrast (blue), peak contrast (green), and post-contrast (red) conditions.

Table 1. Summary of slope ( $m$ ), coefficient of determination ( $R^2$ ), and coefficient of variation (CoV) for all diameter measurement methods across pre-contrast, peak contrast, and post-contrast conditions. Methods are grouped as binary mask based and model-based. Bold values indicate slope agreement within 10% of unity ( $0.9 \leq m \leq 1.1$ ), strong linearity ( $R^2 \geq 0.90$ ), or high precision (CoV  $\leq 0.10$ ). (confirm values with MATLAB.)

|                                                                                       | BW-1        |      | BW-2        |             | BW-3 |             | BW-4 |             | BW-5 |             | $w_{1/\epsilon^2, G}$ |             | FWHM <sub>GG</sub> |             | $w_{1/\epsilon^2, GG}$ |             |
|---------------------------------------------------------------------------------------|-------------|------|-------------|-------------|------|-------------|------|-------------|------|-------------|-----------------------|-------------|--------------------|-------------|------------------------|-------------|
|                                                                                       | MIP         | MeIP | MIP         | MeIP        | MIP  | MeIP        | MIP  | MeIP        | MIP  | MeIP        | MIP                   | MeIP        | MIP                | MeIP        | MIP                    | MeIP        |
| Slope ( $m$ )                                                                         |             |      |             |             |      |             |      |             |      |             |                       |             |                    |             |                        |             |
| Pre                                                                                   | 0.61        | 0.83 | 0.48        | 0.74        | 0.38 | 0.66        | 0.30 | 0.59        | 0.24 | 0.53        | 0.70                  | 0.73        | 0.42               | 0.43        | 0.64                   | 0.71        |
| Peak                                                                                  | <b>0.96</b> | 1.14 | 0.86        | <b>1.06</b> | 0.78 | <b>0.99</b> | 0.71 | <b>0.93</b> | 0.65 | 0.88        | 1.15                  | <b>1.04</b> | 0.66               | 0.61        | <b>0.98</b>            | <b>0.98</b> |
| Post                                                                                  | <b>0.92</b> | 1.11 | 0.82        | <b>1.03</b> | 0.73 | <b>0.97</b> | 0.63 | <b>0.91</b> | 0.54 | 0.86        | 1.12                  | <b>1.04</b> | 0.66               | 0.61        | <b>1.02</b>            | <b>1.00</b> |
| Coefficient of determination ( $R^2$ )                                                |             |      |             |             |      |             |      |             |      |             |                       |             |                    |             |                        |             |
| Pre                                                                                   | 0.58        | 0.59 | 0.54        | 0.62        | 0.45 | 0.64        | 0.34 | 0.65        | 0.24 | 0.65        | 0.83                  | 0.84        | 0.79               | 0.83        | 0.87                   | 0.88        |
| Peak                                                                                  | 0.88        | 0.78 | 0.89        | 0.82        | 0.86 | 0.86        | 0.81 | 0.88        | 0.74 | 0.89        | 0.87                  | <b>0.95</b> | <b>0.95</b>        | <b>0.95</b> | <b>0.98</b>            | <b>0.97</b> |
| Post                                                                                  | 0.76        | 0.77 | 0.69        | 0.79        | 0.57 | 0.80        | 0.45 | 0.80        | 0.34 | 0.78        | 0.89                  | <b>0.97</b> | <b>0.95</b>        | <b>0.98</b> | <b>0.93</b>            | <b>0.97</b> |
| Coefficient of variation (CoV) (values extracted from bar plots, confirm with MATLAB) |             |      |             |             |      |             |      |             |      |             |                       |             |                    |             |                        |             |
| Pre                                                                                   | 0.20        | 0.20 | 0.24        | 0.20        | 0.29 | 0.19        | 0.37 | 0.19        | 0.47 | 0.20        | 0.26                  | 0.14        | 0.26               | 0.15        | 0.25                   | 0.14        |
| Peak                                                                                  | 0.17        | 0.16 | 0.20        | 0.15        | 0.23 | 0.17        | 0.27 | 0.18        | 0.32 | 0.18        | 0.22                  | 0.16        | 0.23               | 0.17        | 0.21                   | 0.15        |
| Post                                                                                  | <b>0.10</b> | 0.12 | <b>0.10</b> | 0.12        | 0.11 | 0.11        | 0.15 | <b>0.10</b> | 0.19 | <b>0.09</b> | 0.19                  | <b>0.10</b> | 0.19               | 0.11        | 0.16                   | <b>0.09</b> |

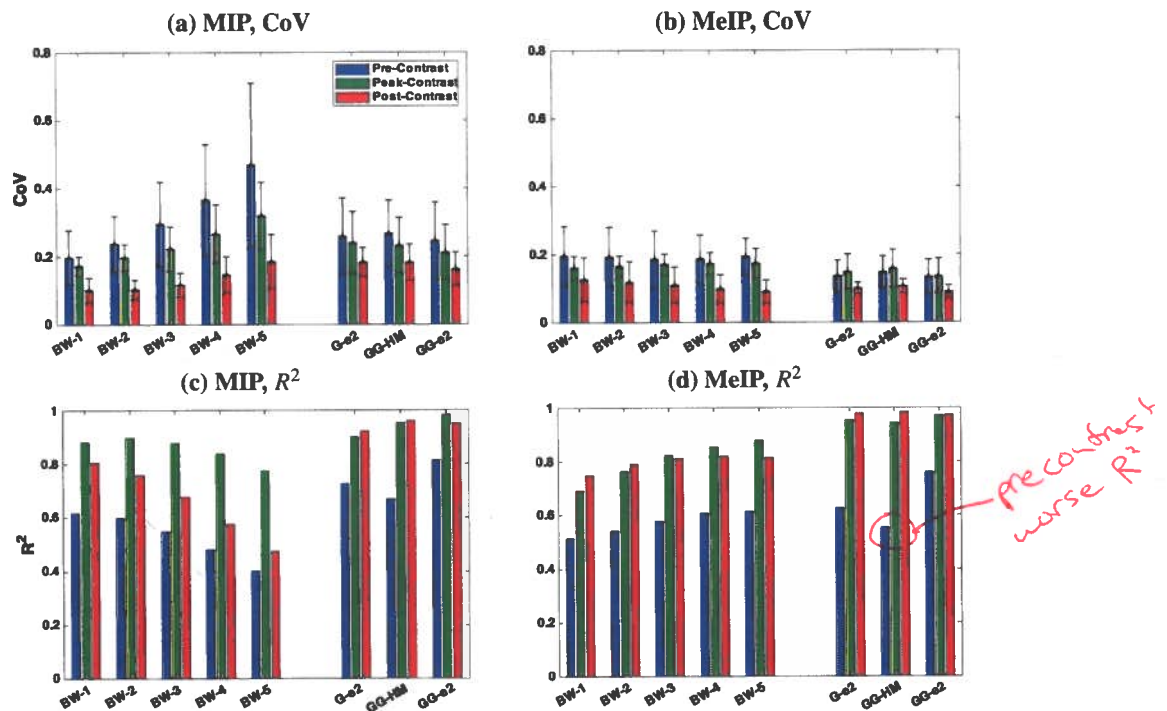


Fig. 7. Summary of accuracy and precision across all diameter measurement methods. (a, b) Coefficient of variation (CoV) and (c, d) coefficient of determination ( $R^2$ ) for MIP (a, c) and MeIP (b, d), respectively. Bars are grouped by method (BW-1 through BW-5, G-e<sup>2</sup>, GG-HM, GG-e<sup>2</sup>) and colour-coded by contrast conditions.

### 3.3. Functional flicker stimulation

The model-based diameter time series (Figs. 8a,b) showed increase in diameter post-stimulation for most of the vessels. The binary mask based diameter time series (BW-3; Fig. 8c) showed a mixed trend, where most vessels showed a decrease in diameter post-stimulation. Bar plots of the mean diameter pre- and post-stimulation (Figs. 8d-f) confirmed this pattern. For the Gaussian model, four of five vessels showed significant diameter increases ( $p < 0.01$ ), and the GG model showed significant increases in three of five vessels (Table 2). In contrast, the binary mask based diameter showed significant decreases in four of five vessels.

The angiogram intensity time series (Fig. 8g) showed a visible decline in angiogram intensity during the duration of the DyC-OCT scan across all five vessels. The mean intensity comparison pre- and post-stimulation (Fig. 8h) confirmed that the decrease was significant for all vessels, ranging from -14.1% to -19.9% (Table 2). The binary mask based method showed uniformly positive per-vessel correlations, with an overall correlation of  $\rho = 0.523$  ( $p < 0.0005$ ). The Gaussian and GG models yielded overall correlations of  $\rho = -0.101$  and  $\rho = -0.098$ , respectively. These results demonstrated that the model-based diameter calculation provided more accurate and repeatable measurements, and also recovered physiologically meaningful vascular responses that binary mask based methods misrepresented.

253 **3.3. Functional flicker stimulation**  
 254 The model-based diameter time series (Figs. 8a,b) showed increase in diameter post-stimulation  
 255 for most of the vessels. The binary mask based diameter time series (BW-3; Fig. 8c) showed a  
 256 mixed trend, where most vessels showed a decrease in diameter post-stimulation. Bar plots of the  
 257 mean diameter pre- and post-stimulation (Figs. 8d-f) confirmed this pattern. For the Gaussian  
 258 model, four of five vessels showed significant diameter increases ( $p < 0.01$ ), and the GG model  
 259 showed significant increases in three of five vessels (Table 2). In contrast, the binary mask based  
 260 diameter showed significant decreases in four of five vessels.  
 261 The angiogram intensity time series (Fig. 8g) showed a visible decline in angiogram intensity  
 262 during the duration of the DyC-OCT scan across all five vessels. The mean intensity comparison  
 263 pre- and post-stimulation (Fig. 8h) confirmed that the decrease was significant for all vessels,  
 264 ranging from -14.1% to -19.9% (Table 2). The binary mask based method showed uniformly  
 265 positive per-vessel correlations, with an overall correlation of  $\rho = 0.523$  ( $p < 0.0005$ ). The  
 266 Gaussian and GG models yielded overall correlations of  $\rho = -0.101$  and  $\rho = -0.098$ , respectively.  
 267 These results demonstrated that the model-based diameter calculation provided more accurate  
 268 and repeatable measurements, and also recovered physiologically meaningful vascular responses  
 269 that binary mask based methods misrepresented.

a significant

double check  
not new numbers

introduce this here

this is discussion

did not accurately capture

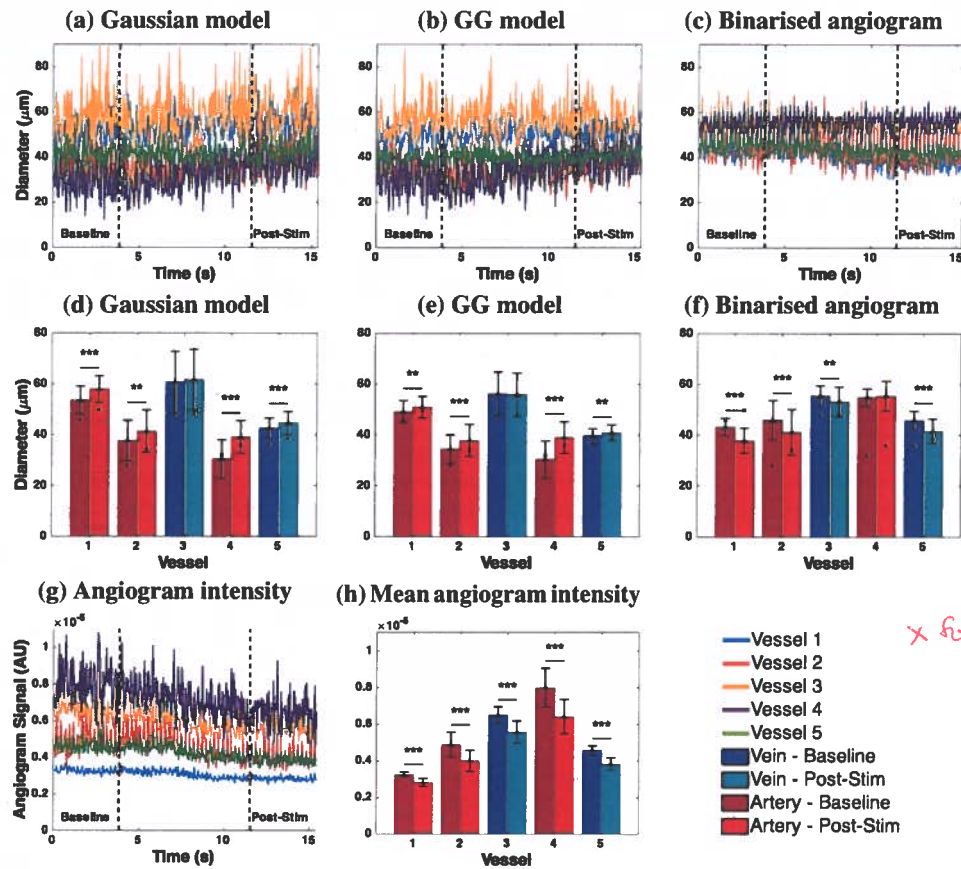


Fig. 8. Functional flicker stimulation results. (a-c) Vessel diameter time series pre- and post-stimulation for (a) Gaussian model, (b) Generalised Gaussian model, and (c) binarised angiogram, across five vessels. Vertical dashed lines indicate stimulation onset and offset. (d-f) Mean diameter per vessel before (dark bars) and after (light bars) stimulation for each method. Veins are shown in blue/cyan and arteries in dark/light red. Significance levels: \*\*  $p < 0.01$ , \*\*\*  $p < 0.001$ . (g) Angiogram intensity time series and (h) mean angiogram intensity per vessel pre- and post-stimulation.

Table 2. Flicker stimulation results.  $\Delta d$ : diameter change (%);  $\rho$ : Correlation between diameter and angiogram intensity;  $\Delta I$ : intensity change (%). Statistically significant values are bold (\*  $p < 0.05$ , \*\*  $p < 0.01$ , \*\*\*  $p < 0.001$ ).

|                | Gaussian       |              | GG             |         | Binarised      |                | Intensity |
|----------------|----------------|--------------|----------------|---------|----------------|----------------|-----------|
|                | $\Delta d$ (%) | $\rho$       | $\Delta d$ (%) | $\rho$  | $\Delta d$ (%) | $\rho$         |           |
| Vessel 1       | +9.2***        | -0.07        | +1.5           | 0.03    | -12.5***       | <b>0.59***</b> | -14.1***  |
| Vessel 2       | +9.6**         | <b>0.23*</b> | +9.9***        | 0.07    | -10.2***       | <b>0.80***</b> | -18.2***  |
| Vessel 3       | +1.5           | -0.28**      | -0.6           | -0.28** | -4.2**         | <b>0.27**</b>  | -14.3***  |
| Vessel 4       | +28.5***       | -0.15        | +28.4***       | -0.14   | +1.0           | <b>0.46***</b> | -19.9***  |
| Vessel 5       | +4.9***        | -0.24*       | +3.1**         | -0.18   | -9.3***        | <b>0.52***</b> | -16.3***  |
| Overall $\rho$ |                | -0.101       |                | -0.098  |                | 0.523          |           |

for what →

overall arterial change  
overall venous change

see updated code

old values?  
Don't match figs

Maybe more fig 9 before  
Table 2 since Table 2 reports  
this info

## 4. Discussion

### 4.1. Model-based vs binary mask based diameter measurement

The model-based and binary mask-based diameter methods define vessel boundary in fundamentally different ways. Binarisation of the en face maps discards the spatial intensity distribution and reduces each pixel to a binary decision. The measured diameter directly depends on the chosen threshold value and on angiogram intensity, both of which may vary across imaging sessions, contrast conditions, and even between vessels within the same scan. Model-based methods fit a parametric model function to the maximum or mean intensity profiles, and calculate the diameter from the fitted parameters. As the fit captures the shape of the profile rather than the absolute intensity, it is inherently less sensitive to changes in angiogram signal and does not require a varying threshold.

This difference explains the trends observed in Fig. 7. Model-based methods maintained strong linearity with the ground truth across all contrast conditions, whereas the binary mask based slopes degraded progressively with increasing threshold. Pre-contrast, the hourglass artefact caused by RBC orientation within vessel lumen suppresses edge signals, causing all methods to underestimate diameter [15]. However, model-based methods still maintained a linear relationship with the ground truth, producing systematic, predictable underestimation. Binary mask based methods on the other hand showed much weaker linearity, potentially because the suppressed edge signals did not consistently exceed the binarisation threshold, depending on vessel size and local intensity.

The generalised Gaussian (GG) model outperformed the standard Gaussian because the intensity profiles of the vessels are usually not purely Gaussian (Fig. 1b). The standard Gaussian cannot capture relatively flat-topped angiogram intensity profiles and tend to fit a narrower curve, whereas the GG model accommodates through the shape parameter  $\beta$ , which ranges from Gaussian ( $\beta = 2$ ) to increasingly flat-topped profiles ( $\beta > 2$ ). Among the width metrics,  $\text{FWHM}_{\text{GG}}$  consistently showed the weakest accuracy. It could be because the half-maximum determines the vessel boundary where the intensity has already dropped inside the true edge. The  $1/e^2$  width captures more of the transition region and so may have provided a more accurate measurement of the vessel diameter.

### 4.2. Maximum vs mean intensity projection

Across nearly all methods and conditions, MeIP outperformed MIP in both accuracy and precision (Table 1). This finding is noteworthy because MIP has been shown to produce higher signal-to-noise ratio (SNR) and contrast in en face OCTA images [12], and is the default in many commercial OCTA systems and analysis pipelines [11, 13]. However, we observed that higher SNR did not necessarily translate to more accurate diameter measurements. The MIP selects the single highest intensity value along each A-scan within the vessel ROI, which makes it inherently sensitive to outliers. MeIP averages all intensity values along each A-scan, which smooths out intensity fluctuations and provides a more average profile. This averaging could be beneficial for vessel diameter measurement, as the goal is to capture the typical vessel boundary rather than extreme signal events.

The difference between MIP and MeIP was especially apparent in the binary mask based results (Table 1). For MeIP, the slope declined more gradually and remained above 0.86 even at BW-5 post-contrast. Whereas for MIP, the slope decreased steeply with increasing threshold, dropping from 0.92 at BW-1 to 0.54 at BW-5 post-contrast. These findings suggest that MeIP produces a more uniform intensity distribution across the vessel profile, making the binarisation result less sensitive to the exact threshold value. The CoV data (Table 1) reinforced this as the MIP-based binary mask CoV increased substantially with threshold, whereas the MeIP-based CoV remained relatively stable. This behaviour follows from the shape of the two projected profiles. Because the

7 should decide and make consistent

on simple binarisation  
how will adaptive methods fare?

discuss peak/post agreement here

linearity was overall lower and depended on threshold

Also because of different vessels have different intensity

Gaussian convolved with a non-reflectable profile

Discuss correcting vessels diameter. Threshold based methods harder to correct

Need to check thresholds



Integrate Fig 3 here?

I think it comes down to variance in the signal we can discuss.

MIP retains only the brightest pixel along each A-scan, the resulting profile is sharply peaked with steep rises and falls, and the peak intensity could vary considerably between vessels depending on the local signal. Raising the threshold could therefore remove a vessel dependent fraction of the cross-section, and so the measured width scatters more widely about its mean causing increased CoV. Unlike MIP, MeIP averages along each A-scan and produces a broader, smoother profile. As a result, thresholding produces a comparable reduction in measured width across vessels, leading to a largely unchanged CoV despite increasing threshold. For model-based methods, MeIP also showed better performance. The  $w_{1/e^2, G}$  using MIP slightly overestimated vessel diameter post-contrast with  $m = 1.12$ , while MeIP reduced this to  $m = 1.04$ , a much closer agreement with the ground truth. These results suggest that while MIP may be preferred for visualisation purposes where contrast and SNR are important [12], MeIP should be the preferred projection method for quantitative diameter measurements.

discuss  $R^2$

#### 4.3. Influence of angiogram intensity on diameter measurements

The functional flicker stimulation experiment provided a direct demonstration of how changes in angiogram signal intensity can affect diameter measurements based on the method used. During the DyC-OCT acquisition, the angiogram intensity declined significantly across all five vessels (Fig. 8g,h), with decreases ranging from -14.1% to -19.9% (Table 2). This decline is expected during prolonged imaging sessions. Because the angiogram signal scales with blood flow [16], and anaesthesia is known to reduce retinal blood flow [17] and to progressively shift murine ocular physiology and superficial vessel parameters over the course of an imaging session [18], a gradual reduction in retinal perfusion would lower the angiogram signal independently of any functional change in vessel diameter. Simultaneously, the physiological response to flicker stimulation produces vasodilation, which has been well established in retinal physiology [19, 20].

Not occurring during long session

Yes and no. would not make this argument just say it's not clear why but measuring location remained stable

Scale is second

More to results

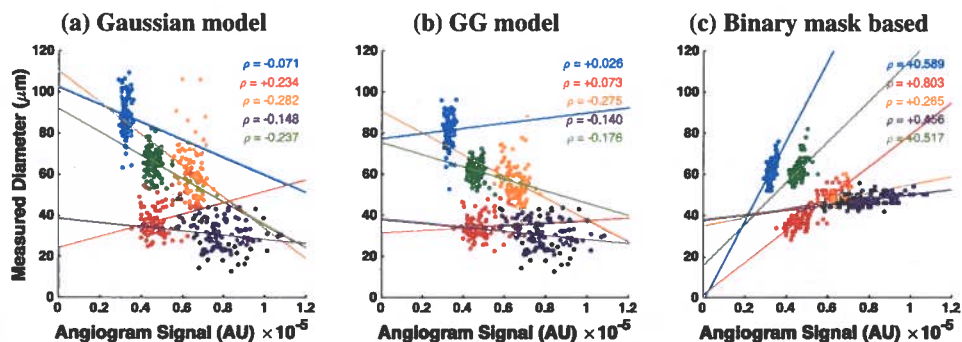


Fig. 9. Measured vessel diameter as a function of angiogram signal intensity during functional flicker stimulation for (a) Gaussian model, (b) Generalised Gaussian model, and (c) binary mask based method. Each colour represents one of five vessels.  $\rho$  denotes the Pearson correlation coefficient.

The model-based methods correctly detected this expected vasodilation, with the Gaussian model showing significant diameter increases in four of five vessels (up to +28.5%) and the GG model showing significant increases in three of five vessels (Table 2). The binary mask based method, however, reported significant diameter decreases in four of five vessels, suggesting vasoconstriction which is a paradoxical result. The reason behind this behaviour could be understood by observing how each method responds to declining signal intensity (Fig. 9). For the binary mask based method, the threshold is fixed and diameter is determined by the number of pixels that exceed this threshold. When the overall angiogram intensity drops, fewer pixels at the vessel edges exceed the threshold, and the vessel appears to shrink even if the physical vessel

would give means for A+V

check new stats

diameter has increased. This is confirmed by the strong positive correlation between measured diameter and angiogram intensity for the binary mask based method ( $\rho = 0.523$ ,  $p < 0.0005$ ). In contrast, the model-based methods showed weak overall correlations with intensity ( $\rho = -0.101$  for Gaussian,  $\rho = -0.098$  for GG), indicating that the fitted diameter was effectively independent of the signal intensity. Among the methods, the GG model also produced the tightest error bars across the five vessels in the flicker experiment (Fig. 8d–f), consistent with its low CoV post-contrast (Table 1), indicating that it is the most repeatable of the metrics tested. *lowest std.*

These findings have important implications for longitudinal studies and any experiment where angiogram intensity may vary between or within imaging sessions. In longitudinal mouse eye imaging, the angiogram signal can vary between and within sessions as anaesthesia alters retinal perfusion and ocular physiology [17, 18], with additional factors such as corneal drying and cataract formation further reducing OCT intensity over time [21, 22] if artificial tear drops are not applied during the imaging. If a binary mask based method is used under such conditions, observed changes in vessel diameter may reflect intensity fluctuations rather than true vascular changes. In contrast, model-based methods may be less sensitive to these intensity variations, as they characterise the shape of the intensity profile rather than relying primarily on absolute intensity values to define vessel boundaries. *can occur even if used*

#### 4.4. Threshold selection

The results presented here used a basic, global threshold for the binarisation of the angiogram data. There are numerous other approaches for binarising the angiogram, which will most likely each behave differently. For example, angiogram signals can be enhanced with vesselness filters [23] and dynamic thresholds can be used to binarise images with varying SNR. When applying a vesselness filter, it is possible to enhance the shape of the angiogram and omit noise, but it is also possible for such enhancement to overcompensate the signal, leading to larger than expected vessel appearance. Dynamic thresholding can also yield a more uniform angiogram appearance, but similarly risks over- or under-compensating vessels given that threshold level directly affects the measured diameter. Further analysis of these other methods would be required to determine their efficacy in returning accurate and precise diameter values.

The key observation from the present work is that any thresholding approach, regardless of how the threshold is determined, shares the same fundamental limitation that the measured diameter depends on the absolute signal intensity at the vessel edges. As demonstrated by the flicker stimulation experiment, this intensity dependence can introduce artefactual diameter changes when the angiogram signal varies over time or between sessions. A more adaptive thresholding strategy may reduce variability across different regions of a single image, but it would not eliminate the sensitivity to temporal intensity fluctuations that we observed. The model-based approach avoids this limitation entirely by deriving diameter from the shape of the intensity profile rather than from an intensity cut-off, making it a fundamentally different and more robust alternative for quantitative diameter analysis. *needs citations*

#### 4.5. Best choices under different conditions

Under the conditions where a contrast agent is available and accuracy is the primary goal, the  $w_{1/e^2, GG}$  metric using MeIP provides the best results post-contrast. This combination achieved a slope of  $m = 1.001$  with  $R^2 = 0.97$  and a CoV of 0.09, yielding the best accuracy, linearity, and precision of all tested methods. If only pre-contrast data is available, the same metric still provides the best linearity ( $R^2 = 0.88$ ) among all methods, though the slope of  $m = 0.71$  indicates that diameter could be underestimated by approximately 30%. In this case, a correction factor could be applied if absolute diameter values are needed, though relative comparisons between vessels or timepoints would remain valid without correction.

When only MIP data is available, which is the case for many commercial OCTA machines and

existing datasets, the  $w_{1/e^2, GG}$  still provides good post-contrast accuracy ( $m = 1.02$ ,  $R^2 = 0.93$ ). For binary mask based analysis of MIP data, only the lowest threshold (BW-1) post-contrast achieved a slope near unity ( $m = 0.92$ ), and the slope degraded rapidly with increasing threshold values. This highlights that if binarisation must be used with MIP data, a lower threshold value is essential, though this may come at the cost of increased noise sensitivity.

If computation time is a limiting factor and model fitting is not practical, MeIP with a moderate threshold (e.g. BW-3) provides a reasonable alternative. At post-contrast, BW-3 using MeIP achieved  $m = 0.97$  and  $R^2 = 0.80$ , which is acceptable for many applications. MeIP-based binary mask based analysis showed more stable CoV values across all thresholds compared to MIP, making the results less sensitive to the exact threshold choice. This stability makes MeIP the preferred projection for binary mask based OCTA.

roughly  
95 is 40% slower  
than 9

#### 4.6. Literature comparison

Hormel et al. [12] showed that MIP produces en face OCTA images with higher SNR and contrast compared to MeIP, and concluded that MIP should be preferred for OCTA visualisation. Our results are consistent with this for image quality purposes, but reveal a different picture when it comes to quantitative vessel diameter measurement. We found that MeIP consistently yielded more accurate and precise diameter values than MIP across both model-based and binary mask based approaches. This suggests that the projection method best suited for visualisation is not necessarily the best suited for quantification, and that the choice of projection should depend on the intended analysis.

We don't show  
this.

The challenge of standardising OCTA image analysis has been highlighted by Sampson et al. [13] and Untracht et al. [11], both of whom emphasised the need for transparent, reproducible analysis pipelines. Our findings add to this discussion by showing that the choice of diameter measurement method introduces a source of variability that is at least as significant as the choice of binarisation threshold. The model-based approach presented here offers a path toward more standardised vessel diameter quantification, as it reduces the dependence on selected thresholds and angiogram intensity, and provides measurements that are more robust across imaging conditions.

The RBC orientation artefact and its effect on OCTA vessel appearance has been described by Bernucci et al. [15] and Cimalla et al. [6], who used Intralipid contrast to demonstrate that the hourglass pattern in vessel cross-sections is caused by the directional scattering properties of RBCs rather than by true variations in flow. Our work extends this observation by quantifying the degree to which this artefact affects diameter measurements and by proposing model-based fitting as a practical correction strategy. While contrast enhancement with Intralipid is effective for revealing the true vessel diameter, it requires a contrast injection and is not yet applicable in clinical settings. Using a calibrated model-based approach provides a way to partially recover the underestimated diameter from native OCTA data without the need for a contrast agent.

Recent work by Son et al. [24] used functional OCT to image flicker-evoked vasodilation in the mouse retina and reported that vasodilation is anisotropic, with larger percent changes in the axial direction ( $\sim 18\%$ ) than the lateral direction ( $\sim 11\%$ ). The authors did not describe how vessel diameters were quantified from their B-scans. It is worth considering whether the lateral diameter measurements may have been affected by the intensity-dependent artefacts observed in the present work. In the lateral direction, the RBC orientation artefact suppresses signal at vessel edges, and depending on how their vessel boundary was defined, this artefact could lead to an underestimation of the lateral diameter. If this were the case, the apparent difference between axial and lateral vasodilation could be influenced by the measurement methodology in addition to the biomechanical anisotropy discussed by the authors. It would be interesting to apply the model-based approach presented here to such data to determine whether their reported anisotropy changes when the lateral diameter is quantified differently.

Conrad needs  
to read this  
paper

The magnitude of vasodilation detected by our model-based methods ranged from +1.5% to

447 +28.5% across the five vessels measured (Table 2). The arteries (Vessels 1, 2, and 4) showed  
448 the largest diameter increases, with the Gaussian model detecting changes of +9.2%, +9.6%,  
449 and +28.5%, respectively, while the veins (Vessels 3 and 5) showed smaller diameter increases  
450 of +1.5% and +4.9%. Table 3 summarises the stimulation protocols and vascular responses  
451 reported by previous flicker stimulation studies alongside our own. The listed human studies  
452 span several measurement techniques, from fundus photography [25] through retinal vessel  
453 analysers [19, 26, 27] to Doppler OCT [28] and OCTA [29]. Despite these methodological  
454 differences, the reported human arterial responses cluster between +3% and +8%, and venous  
455 responses between +2% and +10%. Notably, these studies report arterial and venous responses  
456 of broadly comparable magnitude, and in some cases the venous response is the larger of the two,  
457 for example +9.8% venous versus +8.0% arterial in Aschinger et al. [28]. This contrasts with  
458 our measurements, in which the arterial response was consistently and substantially larger than  
459 the venous response. Whether this asymmetry reflects a genuine feature of the murine flicker  
460 response, the small number of vessels sampled, or a greater sensitivity of the model-based fit  
461 to the smooth-muscle-driven dilation of arteries remains to be established. Polak et al. [26]  
462 additionally showed that the diameter response is relatively stable across flicker frequencies from  
463 4 to 40 Hz, suggesting that frequency differences between studies are unlikely to explain the  
464 variation.

465 The magnitudes we observed are generally larger than those reported in the human studies,  
466 though direct comparison is difficult given the differences in experimental conditions. Species,  
467 anaesthesia, stimulation frequency and wavelength, stimulus power and delivery method, stim-  
468 ulation duration, dark adaptation period, and imaging modality all vary across the reported  
469 studies, and each of these factors could influence the measured vascular response. Among the  
470 studies listed, Son et al. [24] used the most similar setup to ours. They used the same mouse  
471 strain (C57BL/6J), the same anaesthetic (ketamine/xylazine), a comparable flicker stimulus  
472 (10 Hz, 504 nm), however a different stimulation period of 5 s. A systematic comparison of these  
473 parameters could help determine which factors are most influential to the results observed in  
474 both studies. Importantly, regardless of the absolute magnitude, the fact that we were able to  
475 detect vasodilation at all depended on the measurement method, because binary mask based  
476 analysis not only failed to detect vasodilation but reported vasoconstriction which would have led  
477 to fundamentally incorrect physiological conclusions.

478 Previous studies in mice have measured flicker-evoked retinal vessel diameter changes mostly  
479 using dynamic vessel analysis (DVA), which is a fundus camera-based technique adapted from  
480 human retinal vessel analysers. Albanna et al. [30] demonstrated the feasibility of DVA in  
481 the mouse eye using 12.5 Hz flicker at 530 nm but found that quantitative arterial recordings  
482 were possible only in a minority of animals, while venous dilation was mostly below 1.5%  
483 post-stimulation. Another study by Neumaier et al. [31] used the same setup in wildtype and  
484 Cav2.3-deficient mice with overnight dark adaptation and reported median arterial and venous  
485 diameter changes of only +1.3% and +1.2%, respectively, in the wildtype group. These values  
486 are substantially smaller than those we observed, which could be due to the limited spatial  
487 resolution and signal-to-noise ratio of DVA when applied to the smaller mouse eye rather than  
488 being a genuine physiological response. The much larger responses we observed may therefore  
489 partly result from the higher lateral resolution of OCT combined with the model-based fitting  
490 approach, which captures vessel boundary shifts that could fall below the detection limit of DVA.  
491 In addition to these diameter-based studies, Rai et al. [32] recently reported that 12 Hz flicker  
492 stimulation significantly increased both arterial and venous retinal blood flow in light-adapted  
493 C57BL/6J mice, confirming that the mouse retina exhibits a robust neurovascular coupling  
494 response. Since blood flow is proportional to the product of vessel cross-sectional area and  
495 flow velocity, their findings are consistent with the vasodilation we observed, although a direct  
496 quantitative comparison between flow and diameter changes is not straightforward.

Generalized?

← update

→ how do their results compare

← 30 hrs

hard to say



Table 3. Comparison of flicker stimulation protocols and reported diameter changes across studies. H = human, M = mouse. DA = dark adaptation. Lat. = lateral, ax. = axial.

| Study              | Stimulation | Stimulation                                                   | Stimulation  | DA    | Diameter Change (%)   |                      |
|--------------------|-------------|---------------------------------------------------------------|--------------|-------|-----------------------|----------------------|
|                    | Freq. (Hz)  | Light Source                                                  | Duration (s) | (h)   | Artery                | Vein                 |
| Formaz [25] (H)    | 10          | Xenon arc, 5.4 log Td <sup>b</sup>                            | 60           | —     | +4.2                  | +2.7                 |
| Polak [26] (H)     | 8           | < 550 nm, ~ 150 $\mu\text{W}/\text{cm}^{-2}$ <sup>†</sup>     | 60           | —     | +3.5                  | +1.9                 |
| Garhofer [19] (H)  | 8           | < 550 nm, 300 $\mu\text{W}/\text{cm}^{-2}$ <sup>†</sup>       | 60           | —     | +3.8                  | +2.8                 |
| Nagel [27] (H)     | 12.5        | 530 – 600 nm, ~ 196 $\mu\text{W}/\text{cm}^{-2}$ <sup>†</sup> | 20           | —     | +6.9                  | +6.5                 |
| Aschinger [28] (H) | 12.5        | 530 – 600 nm, ~ 196 $\mu\text{W}/\text{cm}^{-2}$ <sup>†</sup> | 120          | —     | +8.0                  | +9.8                 |
| Kallab [29] (H)    | 7           | White, ~ 450 lux                                              | *            | —     | +3.7                  | +4.5                 |
| Albanna [30] (M)   | 12.5        | 530 nm, 30 lux                                                | 20           | 12    | — <sup>#</sup>        | < 1.5 <sup>#</sup>   |
| Neumaier [31] (M)  | 12.5        | 530 nm, 30 lux                                                | 20           | 12    | +1.3                  | +1.2                 |
| Son [24] (M)       | 10          | 504 nm, ~ 460 lux                                             | 5            | 1 – 2 | lat. +10.8, ax. +18.2 | lat. +8.9, ax. +14.3 |
| Present study (M)  | 10          | 502 nm, 26.6 $\mu\text{W}$ <sup>‡</sup>                       | Cont.        | 2     | +9.2 to +28.5         | +1.5 to +4.9         |

<sup>b</sup>Diameter measured from fundus photographs taken post-stimulation; retinal luminance in iolands.

<sup>†</sup>DVA feasibility study; arterial recordings were not reliably obtainable in the mouse eye.

\*Flicker applied during OCTA scan acquisition. <sup>‡</sup>Retinal irradiance. <sup>#</sup>Power at cornea.

Srikrishnan &  
Radha Krishna  
JBO 2013  
RIS  $\alpha$ -dilatation  
arterial increase 11%

#### 4.7. Future direction

A future direction of this work is to move toward fully automated segmentation and calculation of vessel diameters from en face angiogram maps. While ROIs were manually selected in this work, it is also possible to automatically segment angiographic data using traditional skeletonisation methods, which are commonly used for automated OCTA analysis. From a skeletonised image, vessel angle can be computed for further extraction of vascular cross-sections perpendicular to the vessel axis. These cross-sections could then be processed using the model-based methods described here to enable fully automated analysis of 3D OCTA data sets, rather than the semi-automated approach shown here for 2D OCTA data. This type of model-based approach is particularly important for comparing 3D volumes acquired at different time points in the mouse eye, as there are often intensity losses caused by drying of the eye, cataract formation, etc. As we have shown in this work, even low levels of intensity loss occurring over a short time window can significantly affect the measured vessel diameter when using a binary mask based approach, but not when using the models presented here. *model based*

Additionally, this work focused on the larger vessels of the superficial vascular plexus. Extending the model-based approach to the intermediate and deep capillary plexuses, where vessels are smaller and signal levels are lower, would be valuable for studying microvascular changes in diseases. For very small vessels approaching the lateral resolution limit of the imaging system, the measured intensity profile is a convolution of the true vessel profile with the point spread function (PSF) of the incident beam on the retina. Since the lateral resolution of OCT is typically worse than the axial resolution and is determined by the beam optics rather than the source bandwidth, this convolution becomes increasingly significant for smaller vessels. If the PSF were known, a deconvolution approach could be used to recover the true vessel profile before model fitting, potentially improving accuracy for capillary-scale vessels. However, characterising the retinal PSF in vivo remains challenging, as it depends on the ocular optics of each individual eye and may vary with retinal depth and eccentricity.

*cite*

*depends on eye*

*← Conclusion →*

#### References

1. A. Javed, A. Khanna, E. Palmer, *et al.*, "Optical coherence tomography angiography: A review of the current literature," *J. Int. Med. Res.* **51**, 03000605231187933 (2023). Doi: 10.1177/03000605231187933.

2. S. Fialová, M. Augustin, M. Glösmann, *et al.*, "Polarization properties of single layers in the posterior eyes of mice and rats investigated using high resolution polarization sensitive optical coherence tomography," *Biomed. Opt. Express* **7**, 1479–1495 (2016).
3. C. W. Merkle, M. Augustin, D. J. Harper, *et al.*, "High-resolution, depth-resolved vascular leakage measurements using contrast-enhanced, correlation-gated optical coherence tomography in mice," *Biomed. Opt. Express* **12**, 1774–1791 (2021).
4. Y. Fu and K.-W. Yau, "Phototransduction in mouse rods and cones," *Pflügers Arch. J. Physiol.* **454**, 805–819 (2007).
5. Y. Pan, J. You, N. D. Volkow, *et al.*, "Ultrasensitive detection of 3D cerebral microvascular network dynamics in vivo," *NeuroImage* **103**, 492–501 (2014).
6. P. Cimalla, J. Walther, M. Mittasch, and E. Koch, "Shear flow-induced optical inhomogeneity of blood assessed in vivo and in vitro by spectral domain optical coherence tomography in the 1.3  $\mu\text{m}$  wavelength range," *J. Biomed. Opt.* **16**, 116020 (2011).
7. C. W. Merkle and V. J. Srinivasan, "Laminar microvascular transit time distribution in the mouse somatosensory cortex revealed by Dynamic Contrast Optical Coherence Tomography," *NeuroImage* **125**, 350–362 (2016).
8. M. Augustin, S. Fialová, R. Plasenzotti, *et al.*, "Multi-functional OCT image processing for rodent eyes," in *Optical Tomography and Spectroscopy*, (OSA - The Optical Society, Center for Medical Physics and Biomedical Engineering, Medical University of Vienna, Waehringer Guertel 18-20, 4L, Vienna, A-1090, Austria, 2016), p. 3. Export Date: 10 June 2020 Correspondence Address: Augustin, M.; Center for Medical Physics and Biomedical Engineering, Medical University of Vienna, Waehringer Guertel 18-20, 4L, Austria; email: marco.augustin@meduniwien.ac.at.
9. V. J. Srinivasan, J. Y. Jiang, M. A. Yaseen, *et al.*, "Rapid volumetric angiography of cortical microvasculature with optical coherence tomography," *Opt. Lett.* **35**, 43–45 (2010).
10. D. J. Harper, M. Augustin, A. Lichtenegger, *et al.*, "Retinal analysis of a mouse model of Alzheimer's disease with multicontrast optical coherence tomography," *Neurophotonics* **7**, 015006 (2020). Export Date: 4 June 2020 Correspondence Address: Harper, D.J.; Medical University of Vienna, Center for Medical Physics and Biomedical Engineering Austria; email: danielle.harper@meduniwien.ac.at.
11. G. R. Untracht, M. S. Durkee, M. Zhao, *et al.*, "Towards standardising retinal oct angiography image analysis with open-source toolbox octava," *Sci. Reports* **14** (2024).
12. T. T. Hormel, J. Wang, S. T. Bailey, *et al.*, "Maximum value projection produces better en face oct angiograms than mean value projection," *Biomed. Opt. Express* **9**, 6412 (2018).
13. D. M. Sampson, A. M. Dubis, F. K. Chen, *et al.*, "Towards standardizing retinal optical coherence tomography angiography: a review," *Light. Sci. & Appl.* **11** (2022).
14. C. S. Lee, A. J. Tying, Y. Wu, *et al.*, "Generating retinal flow maps from structural optical coherence tomography with artificial intelligence," *Sci. Reports* **9** (2019).
15. M. T. Bernucci, C. W. Merkle, and V. J. Srinivasan, "Investigation of artifacts in retinal and choroidal OCT angiography with a contrast agent," *Biomed. Opt. Express* **9**, 1020–1040 (2018).
16. J. Tokayer, Y. Jia, A.-H. Dhalla, and D. Huang, "Blood flow velocity quantification using split-spectrum amplitude-decorrelation angiography with optical coherence tomography," *Biomed. Opt. Express* **4**, 1909–1924 (2013).
17. G. Feng, A. Joseph, K. Dholakia, *et al.*, "High-resolution structural and functional retinal imaging in the awake behaving mouse," *Commun. Biol.* **6**, 572 (2023).
18. S. Worm, G. Ladurner, L. May, *et al.*, "Retinal OCT parameters and physiological dynamics as an effect of anesthesia in C57BL/6j mice," *Investig. Ophthalmol. & Vis. Sci.* **67**, 50 (2026).
19. G. Garhöfer, C. Zawinka, H. Resch, *et al.*, "Diffuse luminance flicker increases blood flow in major retinal arteries and veins," *Vis. Res.* **44**, 833–838 (2004).
20. M. Sharifzad, K. J. Witkowska, G. C. Aschinger, *et al.*, "Factors determining flicker-induced retinal vasodilation in healthy subjects," *Investig. Ophthalmol. Vis. Sci.* **57**, 3306–3312 (2016). Cited By :12 Export Date: 10 June 2020 CODEN: IOVSD Correspondence Address: Schmetterer, L.; Department of Clinical Pharmacology, Medical University of Vienna, Währinger Gürtel 18-20, Austria; email: Leopold.schmetterer@meduniwien.ac.at.
21. D. M. Stein, G. Wollstein, H. Ishikawa, *et al.*, "Effect of corneal drying on optical coherence tomography," *Ophthalmology* **113**, 985–991 (2006).
22. G. J. McLellan and C. A. Rasmussen, "Optical coherence tomography for the evaluation of retinal and optic nerve morphology in animal subjects: Practical considerations," *Vet. Ophthalmol.* **15**, 13–28 (2012).
23. A. F. Frangi, W. J. Niessen, K. L. Vincken, and M. A. Viergever, "Multiscale vessel enhancement filtering," in *Medical Image Computing and Computer-Assisted Intervention — MICCAI'98*, vol. 1496 of *Lecture Notes in Computer Science* W. M. Wells, A. Colchester, and S. Delp, eds. (Springer, Berlin, Heidelberg, 1998), pp. 130–137.
24. T. Son, G. Ma, and X. Yao, "Functional OCT reveals anisotropic changes of retinal flicker-evoked vasodilation," *Opt. Lett.* **49**, 2121–2124 (2024).
25. F. Formaz, C. E. Riva, and M. Geiser, "Diffuse luminance flicker increases retinal vessel diameter in humans," *Curr. Eye Res.* **16**, 1252–1257 (1997).
26. K. Polak, L. Schmetterer, and C. E. Riva, "Influence of flicker frequency on flicker-induced changes of retinal vessel diameter," *Investig. Ophthalmol. & Vis. Sci.* **43**, 2721–2726 (2002).
27. E. Nagel and W. Vilser, "Flicker observation light induces diameter response in retinal arterioles: A clinical methodological study," *Der Ophthalmol.* **102**, 305–309 (2005).
28. G. C. Aschinger, L. Schmetterer, K. Fondi, *et al.*, "Effect of Diffuse Luminance Flicker Light Stimulation on Total

- 589 Retinal Blood Flow Assessed With Dual-Beam Bidirectional Doppler OCT," *Investig. Ophthalmol. & Vis. Sci.* **58**,  
590 1167–1178 (2017).
- 591 29. M. Kallab, N. Hommer, B. Tan, *et al.*, "Plexus-specific effect of flicker-light stimulation on the retinal microvasculature  
592 assessed with optical coherence tomography angiography," *Am. J. Physiol. Circ. Physiol.* **320**, H23–H28 (2020). Doi:  
593 10.1152/ajpheart.00495.2020  
594 Export Date: 17 June 2021 CODEN: AJPPD Correspondence Address: Garhöfer, G.; Department of Clinical  
595 Pharmacology, Austria; email: gerhard.garhoefer@meduniwien.ac.at.
- 596 30. W. Albanna, K. Kotliar, J. N. Lüke, *et al.*, "Non-invasive evaluation of neurovascular coupling in the murine retina by  
597 dynamic retinal vessel analysis," *PLOS ONE* **13**, e0204689 (2018).
- 598 31. F. Neumaier, K. Kotliar, R. H. L. Haeren, *et al.*, "Evaluation of flicker-induced retinal vessel response in cav2.3-deficient  
599 mice using dynamic retinal vessel analysis," *Front. Neurol.* **12**, 659890 (2021).
- 600 32. M. Rai, Y. Lakshmanan, K. Y. Choi, and H. H.-I. Chan, "Effects of flickering light stimulation on retinal blood flow  
601 and full-field electroretinogram in mice," *Documenta Ophthalmol.* **151**, 205–218 (2025).

} Don't  
export  
notes

