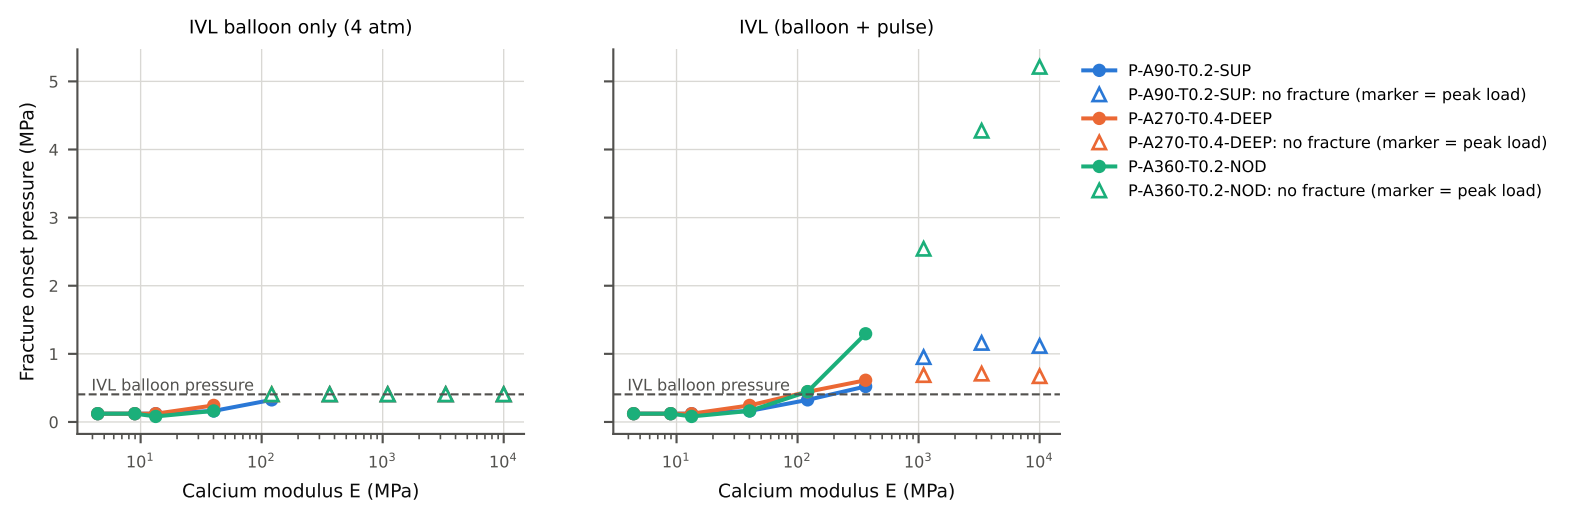
IVL balloon only (4 atm)
IVL (balloon + pulse)
Fracture onset pressure (MPa)
IVL balloon pressure
IVL balloon pressure
Calcium modulus E (MPa)
Calcium modulus E (MPa)
P-A90-T0.2-SUP
P-A90-T0.2-SUP: no fracture (marker = peak load)
P-A270-T0.4-DEEP
P-A270-T0.4-DEEP: no fracture (marker = peak load)
P-A360-T0.2-NOD
P-A360-T0.2-NOD: no fracture (marker = peak load)