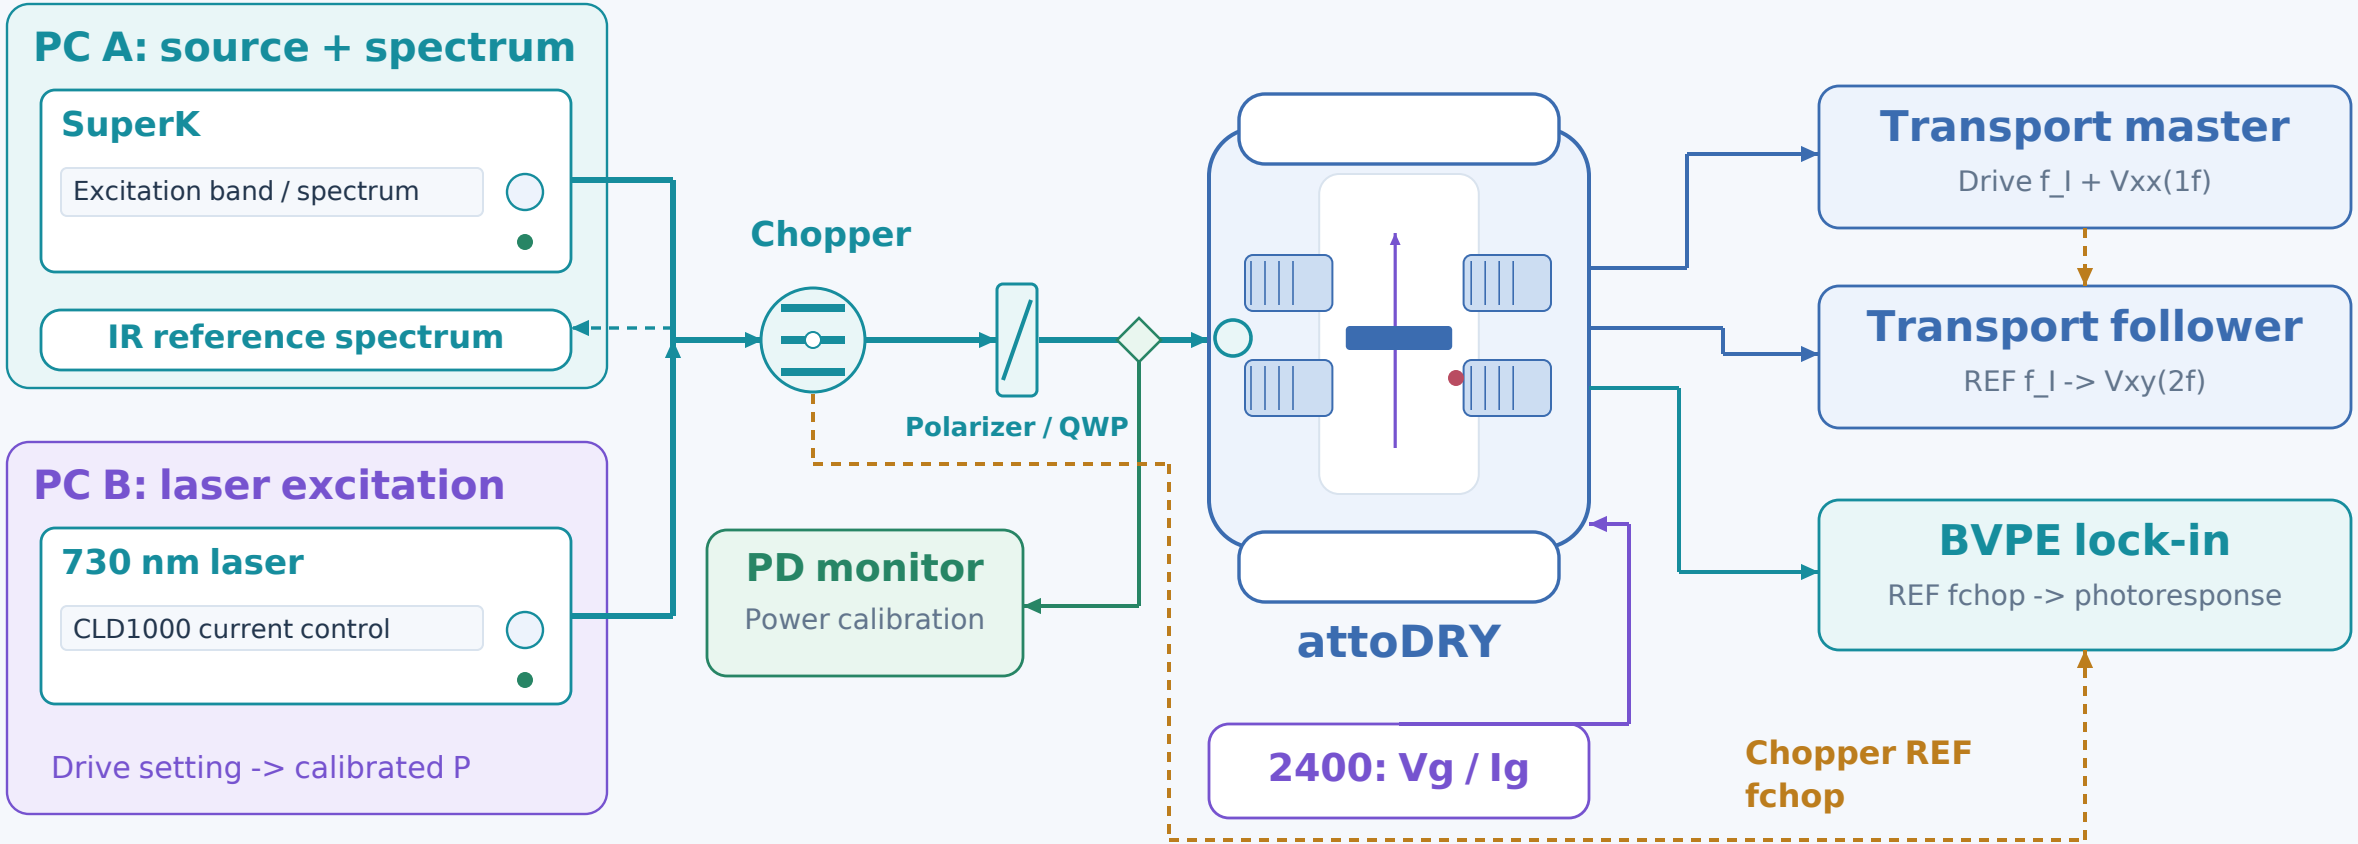
PC A: source + spectrum
SuperK
Excitation band / spectrum
IR reference spectrum
PC B: laser excitation
730 nm laser
CLD1000 current control
Drive setting -> calibrated P
Chopper
Polarizer / QWP
PD monitor
Power calibration
attoDRY
2400: Vg / Ig
Transport master
Drive f_I + Vxx(1f)
Transport follower
REF f_I -> Vxy(2f)
BVPE lock-in
REF fchop -> photoresponse
Chopper REF
fchop