



Test ECG JS36402 (first 5 s): d clean, e the four augmentations, f real artifacts

Good-quality ECG (lead I)


d

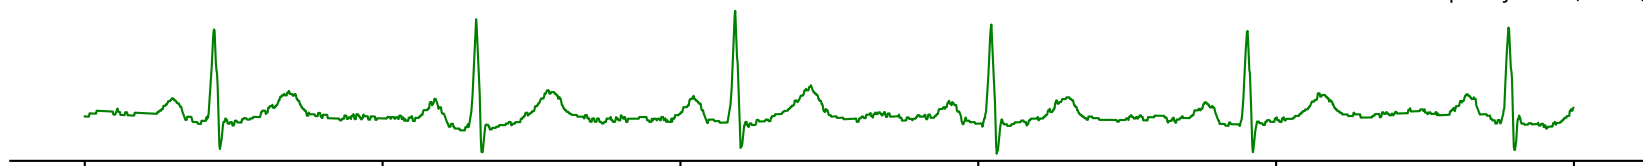


e

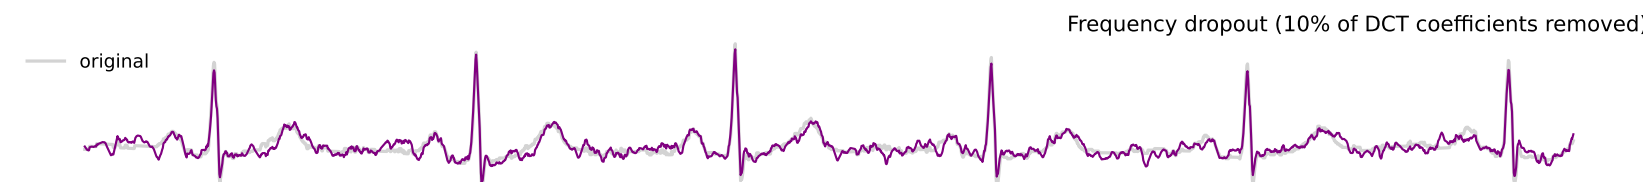


Crop resize (85% of the record stretched to full length)

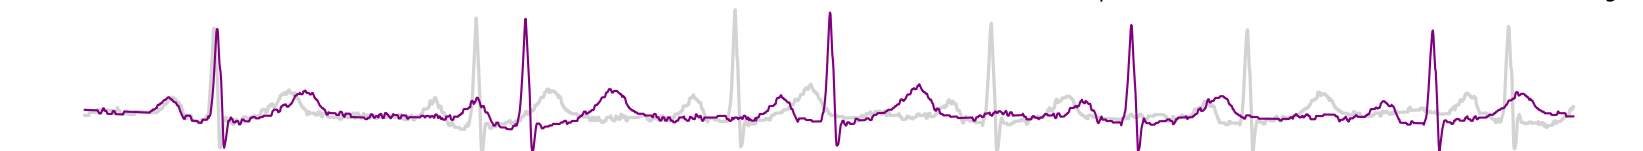


Cycle mask (40-160 ms after every R peak set to zero)

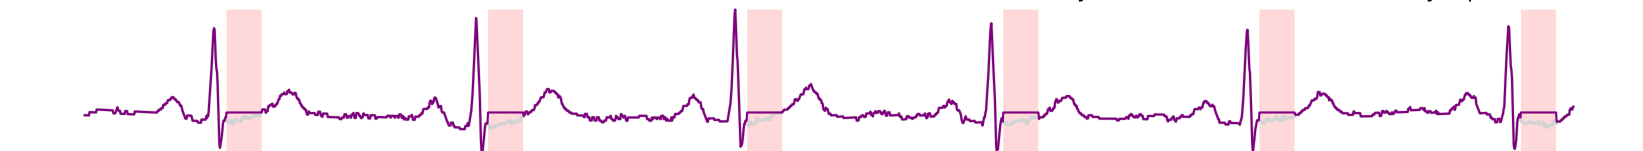

Channel mask (lead I set to zero)

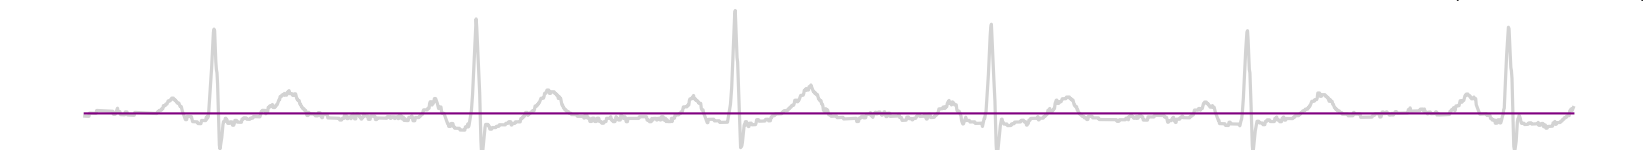

f

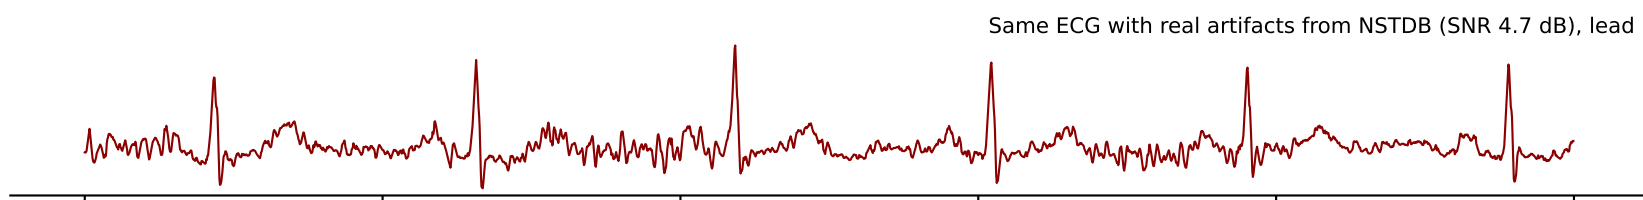

Same ECG with real artifacts from NSTDB, lead V2



0 1 2 3 4 5

Time (s)