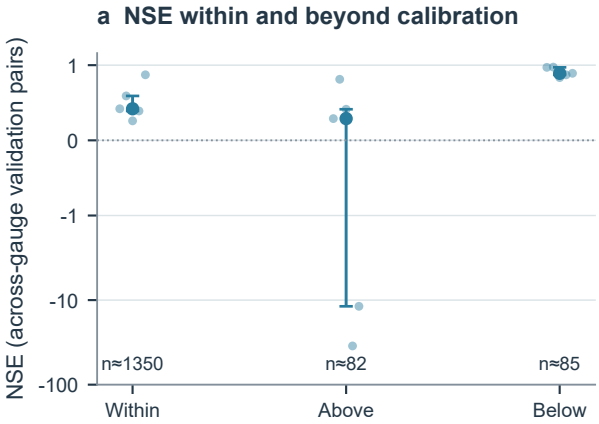
a NSE within and beyond calibration
NSE (across-gauge validation pairs)
1
0
-1
-10
-100
n≈1350
n≈82
n≈85
Within
Above
Below

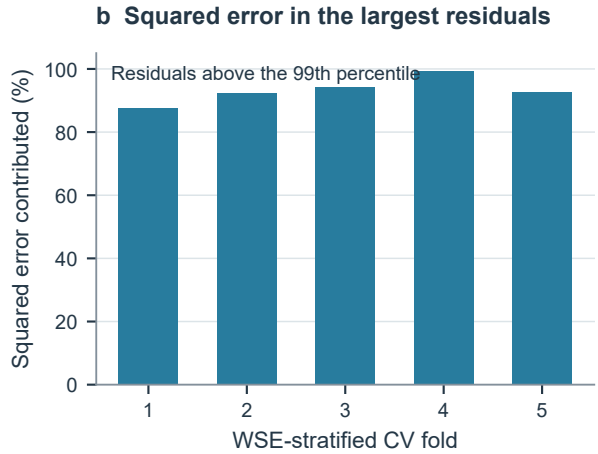
b Squared error in the largest residuals
Residuals above the 99th percentile
Squared error contributed (%)
100
80
60
40
20
0
1
2
3
4
5
WSE-stratified CV fold

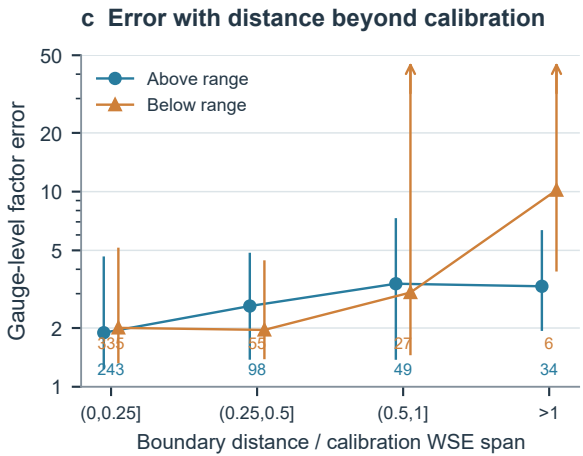
c Error with distance beyond calibration
Above range
Below range
Gauge-level factor error
50
20
10
5
2
1
335
243
55
98
27
49
6
34
(0,0.25]
(0.25,0.5]
(0.5,1]
>1
Boundary distance / calibration WSE span

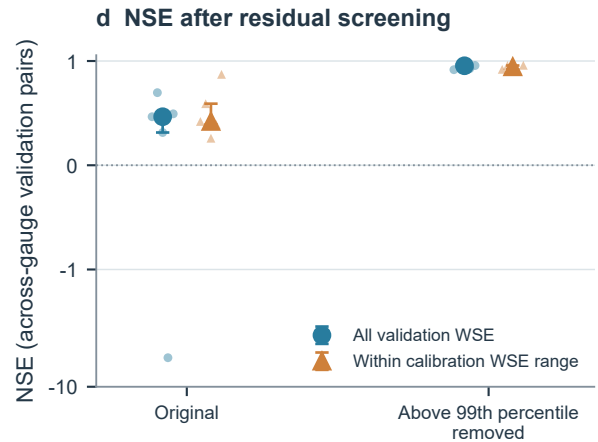
d NSE after residual screening
NSE (across-gauge validation pairs)
1
0
-1
-10
All validation WSE
Within calibration WSE range
Original
Above 99th percentile removed