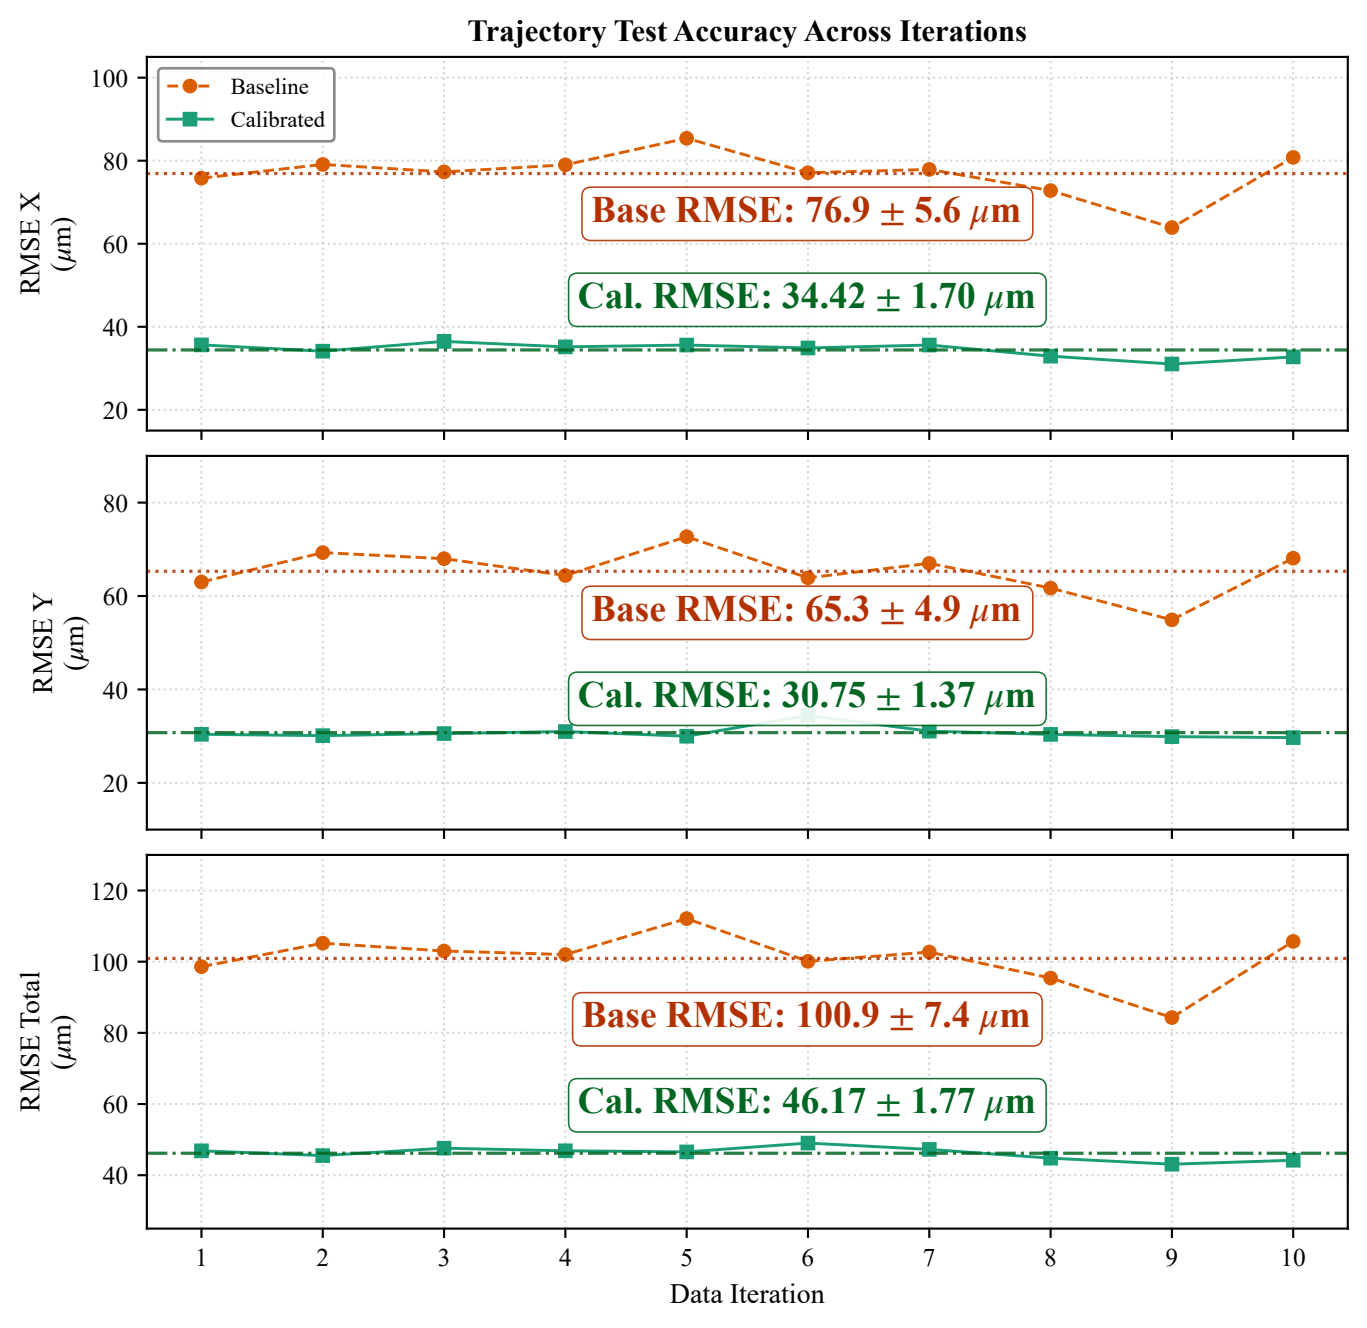

Trajectory Test Accuracy Across Iterations
Baseline
Calibrated
RMSE X (μm)
Base RMSE: 76.9 ± 5.6 μm
Cal. RMSE: 34.42 ± 1.70 μm
RMSE Y (μm)
Base RMSE: 65.3 ± 4.9 μm
Cal. RMSE: 30.75 ± 1.37 μm
RMSE Total (μm)
Base RMSE: 100.9 ± 7.4 μm
Cal. RMSE: 46.17 ± 1.77 μm
Data Iteration