

INCIDENT REPORT



ALTAIR 5X - A5X-00014922

Start Date: Fri, Dec 05, 2025, 09:57:15 AM GMT+11
End Date: Fri, Dec 05, 2025, 05:12:15 PM GMT+11
Duration: 7 hours 15 minutes

Was Assigned To

Company **ERO Station**
Department **ERO**

CALIBRATION

Instrument Calibration Status **✓ Compliant**

Last Calibration Test **Passed**
Mon, Dec 1, 2025, 1:10:45 AM GMT+11

Last Bump Test **Expired**
Thu, Dec 4, 2025, 9:10:24 AM GMT+11

Sensors Calibration

Status	Gas Type	Calibration Status	Bump Status
 Bump Due	Combustible	Passed Dec 1, 2025, 1:10:45 AM GMT+11	Expired Dec 4, 2025, 9:10:24 AM GMT+11
 Bump Due	O ₂	Passed Dec 1, 2025, 1:10:45 AM GMT+11	Expired Dec 4, 2025, 9:10:24 AM GMT+11
 Bump Due	CO	Passed Dec 1, 2025, 1:10:45 AM GMT+11	Expired Dec 4, 2025, 9:10:24 AM GMT+11
 Bump Due	H ₂ S	Passed Dec 1, 2025, 1:10:45 AM GMT+11	Expired Dec 4, 2025, 9:10:24 AM GMT+11
 Bump Due	CO ₂	Passed Nov 30, 2025, 1:00:00 PM GMT+11	Expired Dec 4, 2025, 9:10:24 AM GMT+11

INSTRUMENT CONFIGURATION

Alert Behaviors

Alarms LEDs, Horn, Vibrate

Instrument Alerts

Man Down Alarm	Enabled
----------------	---------

Instrument Configuration

Firmware Version	2.20.0
Language	English
Calibration Interval	Disabled
Bump Test Interval	Disabled
Session Logging Status	Enabled
Periodic Logging Status	Peak Readings Only

INSTRUMENT ALARM SETPOINTS

Combustible

Serial Number	00221101894
Manufactured	11/2022
Deadband Enabled	Disabled
Exposure Warning	5 %LEL
Exposure Alarm	10 %LEL
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

O₂

Serial Number	01221288859
Manufactured	12/2022
Deficiency Alarm	19.5 %VOL
Exposure Alarm	23 %VOL
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

CO

Serial Number	04221202633
Manufactured	12/2022
Exposure Warning	30 PPM
Exposure Alarm	100 PPM
STEL Alarm Alarm	200 PPM
TWA Alarm Alarm	30 PPM
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

H₂S


Serial Number	04221202633
Manufactured	12/2022
Exposure Warning	10 PPM
Exposure Alarm	15 PPM
STEL Alarm Alarm	15 PPM
TWA Alarm Alarm	10 PPM
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

CO₂


Serial Number	
Manufactured	
Exposure Warning	0.5 %VOL
Exposure Alarm	1.5 %VOL
STEL Alarm Alarm	0.5 %VOL
TWA Alarm Alarm	1 %VOL
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

GAS READINGS


COMB %LEL Avg: 0.00 Peak: 0.00 Min: 0.00

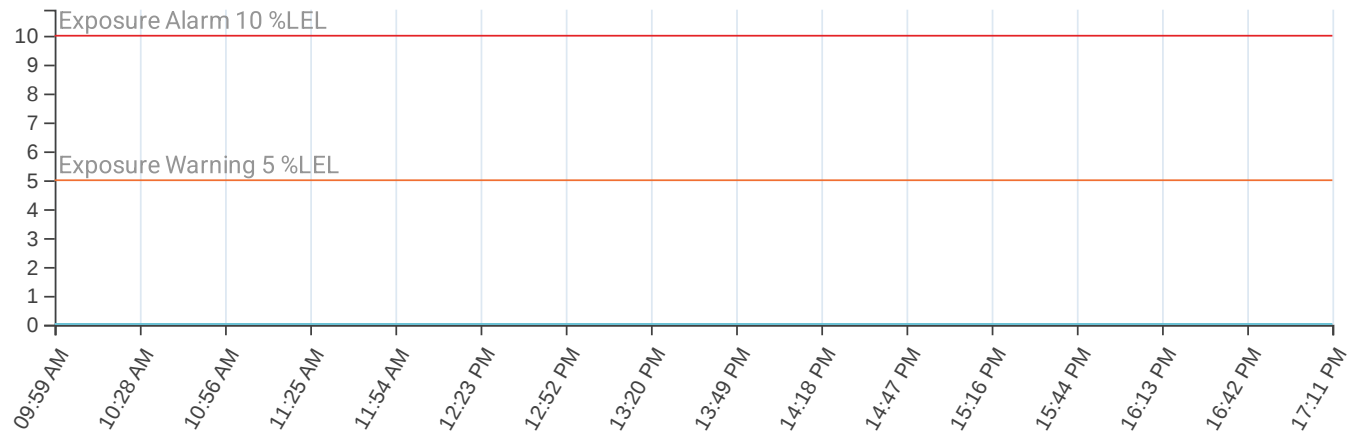

CO PPM Avg: 0.00 Peak: 1.00 Min: 0.00

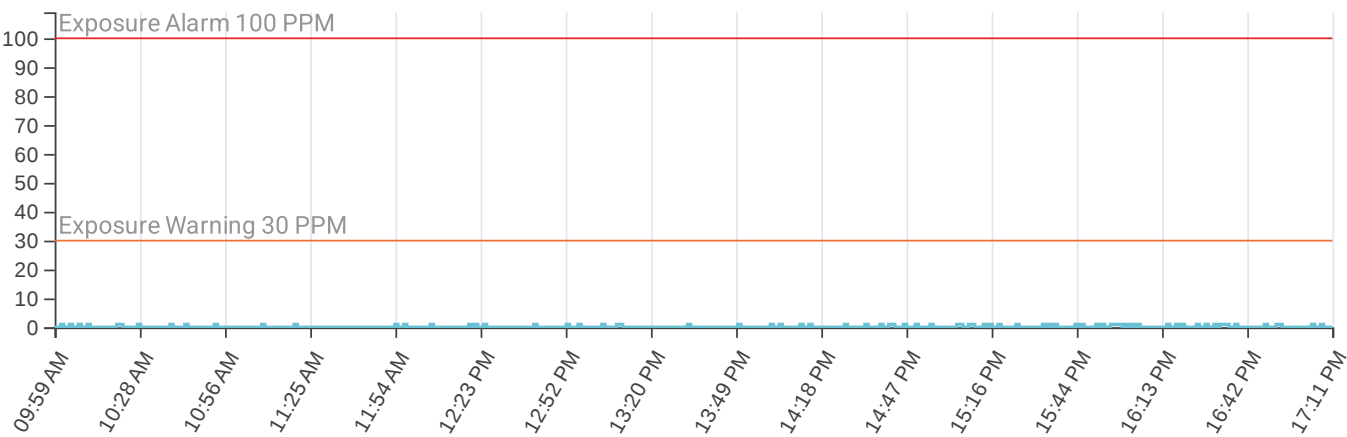


H₂S PPM Avg: 0.00 Peak: 1.00 Min: 0.00

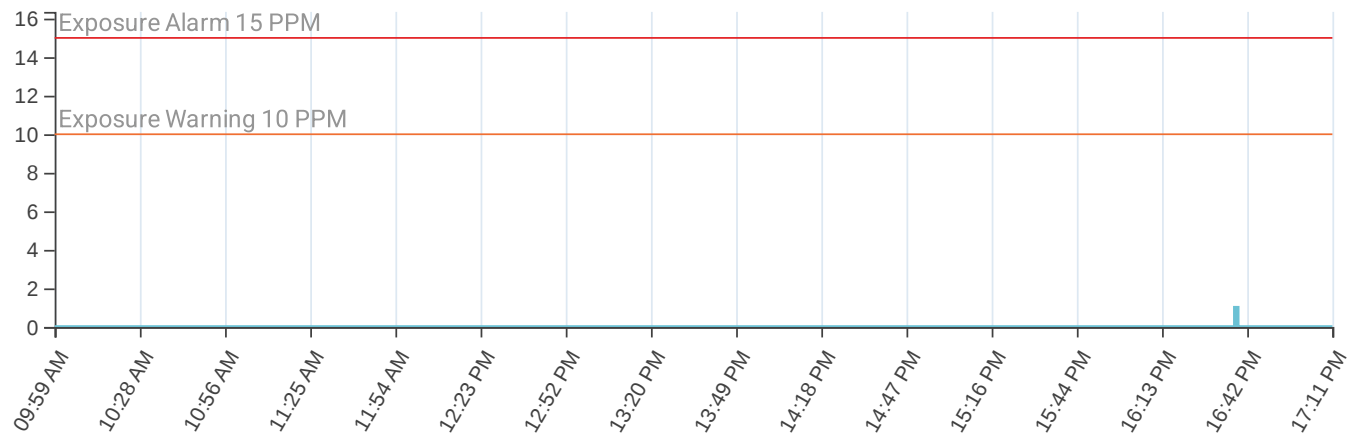


CO₂ %VOL

Avg: 0.00 Peak: 0.22 Min: 0.00

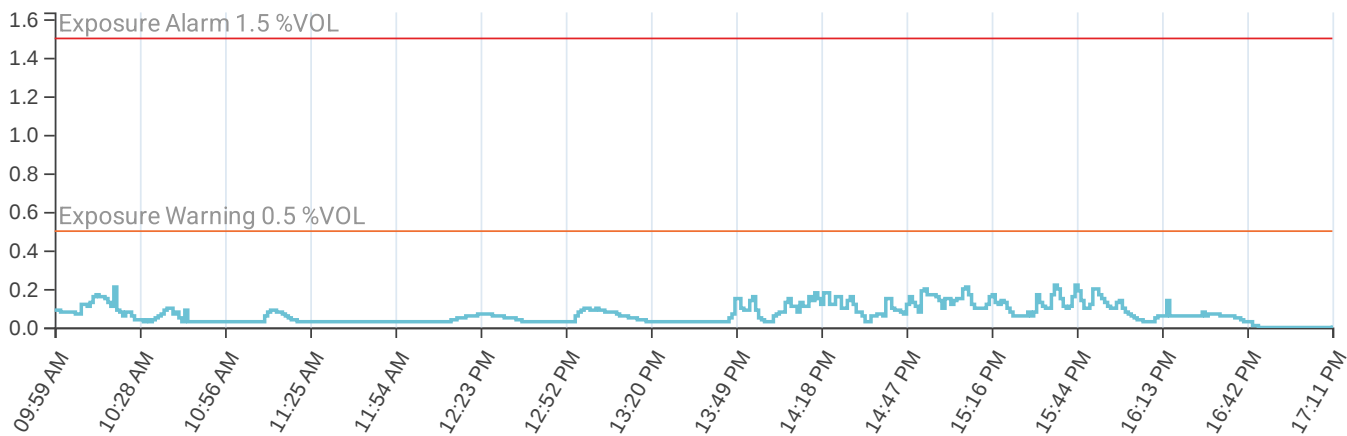

O₂ %VOL

Avg: 20.80 Peak: 23.20 Min: 20.80

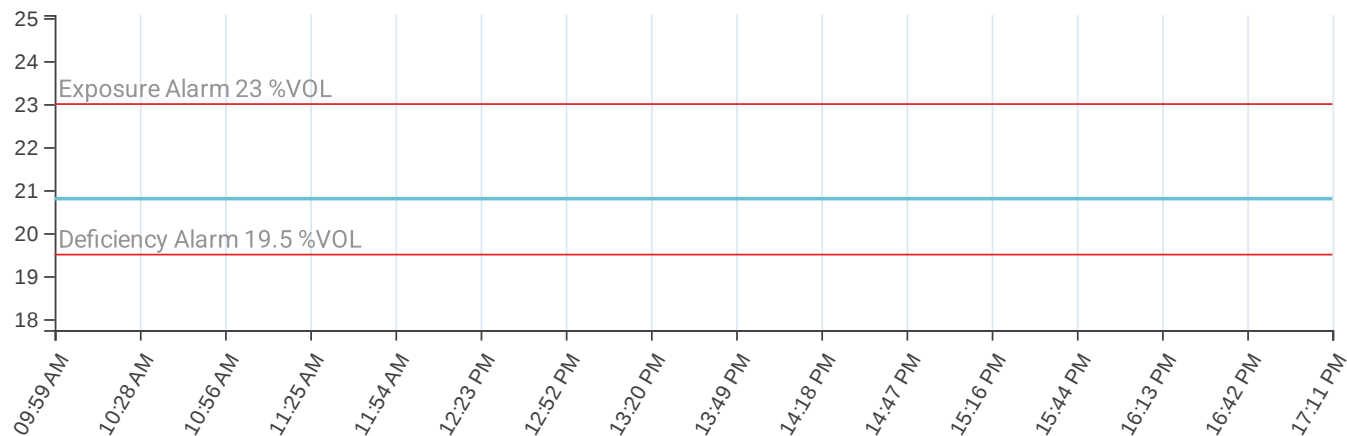

USAGE EVENTS

Dec 5, 2025, 9:57:15 AM	Instrument Powered On	Received by Grid Dec 8, 2025, 11:00:57 AM
Dec 5, 2025, 4:49:00 PM	O ₂ Exposure Alarm Active	Received by Grid Dec 8, 2025, 11:00:57 AM
Dec 5, 2025, 4:49:00 PM	O ₂ Exposure Alarm Cleared	Received by Grid Dec 8, 2025, 11:00:57 AM
Dec 5, 2025, 5:12:15 PM	Instrument Powered Off	Received by Grid Dec 8, 2025, 11:00:57 AM

NOTES

No notes present.