

USAGE REPORT



The Safety Company

ALTAIR 5X - A5X-00229002

Start Date: Fri, Dec 05, 2025, 09:55:00 AM GMT+11
End Date: Fri, Dec 05, 2025, 04:46:45 PM GMT+11
Duration: 6 hours 51 minutes

Was Assigned To

Company

CE Production

Department

Production

CALIBRATION

Instrument Calibration Status

✓ Compliant

Last Calibration Test

Passed

Sat, Nov 15, 2025, 4:58:35 AM GMT+11

Last Bump Test

Expired

Sun, Nov 16, 2025, 4:07:52 AM GMT+11

Sensors Calibration

Status	Gas Type	Calibration Status	Bump Status
 Bump Due	Combustible	Passed Nov 15, 2025, 4:58:35 AM GMT+11	Expired Nov 16, 2025, 4:07:52 AM GMT+11
 Bump Due	O ₂	Passed Nov 15, 2025, 4:58:35 AM GMT+11	Expired Nov 16, 2025, 4:07:52 AM GMT+11
 Bump Due	CO	Passed Nov 15, 2025, 4:58:35 AM GMT+11	Expired Nov 16, 2025, 4:07:52 AM GMT+11
 Bump Due	NO ₂	Passed Nov 15, 2025, 4:58:35 AM GMT+11	Expired Nov 16, 2025, 4:07:52 AM GMT+11
 Bump Due	NH ₃	Passed Nov 15, 2025, 4:58:35 AM GMT+11	Expired Nov 16, 2025, 4:07:52 AM GMT+11

INSTRUMENT CONFIGURATION

Alert Behaviors

Alarms

LEDs, Horn, Vibrate

Instrument Alerts

Calibration Due Alarm	Enabled
-----------------------	---------

Instrument Configuration

Firmware Version	2.20.0
Language	English
Calibration Interval	30 days
Bump Test Interval	Disabled
Session Logging Status	Enabled
Periodic Logging Status	Peak Readings Only

INSTRUMENT ALARM SETPOINTS

Combustible

Serial Number	08231001048
Manufactured	10/2023
Deadband Enabled	Disabled
Exposure Warning	10 %LEL
Exposure Alarm	20 %LEL
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

O₂

Serial Number	01220581776
Manufactured	05/2022
Deficiency Alarm	19.5 %VOL
Exposure Alarm	23 %VOL
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

CO

Serial Number	11240780309
Manufactured	07/2024
Exposure Warning	25 PPM
Exposure Alarm	100 PPM
STEL Alarm Alarm	100 PPM
TWA Alarm Alarm	25 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

NO₂


Serial Number	11240780309
Manufactured	07/2024
Exposure Warning	2.5 PPM
Exposure Alarm	5 PPM
STEL Alarm Alarm	5 PPM
TWA Alarm Alarm	2.5 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

NH₃


Serial Number	06241100103
Manufactured	11/2024
Exposure Warning	25 PPM
Exposure Alarm	50 PPM
STEL Alarm Alarm	35 PPM
TWA Alarm Alarm	25 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

GAS READINGS


COMB %LEL Avg: 0.00 Peak: 3.00 Min: 0.00

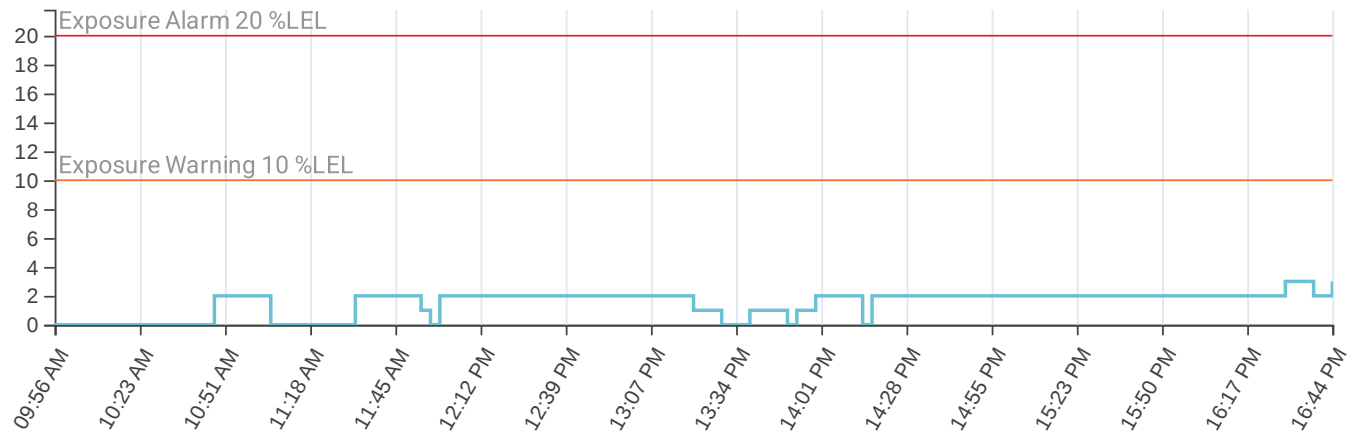

CO PPM Avg: 0.00 Peak: 1.00 Min: 0.00

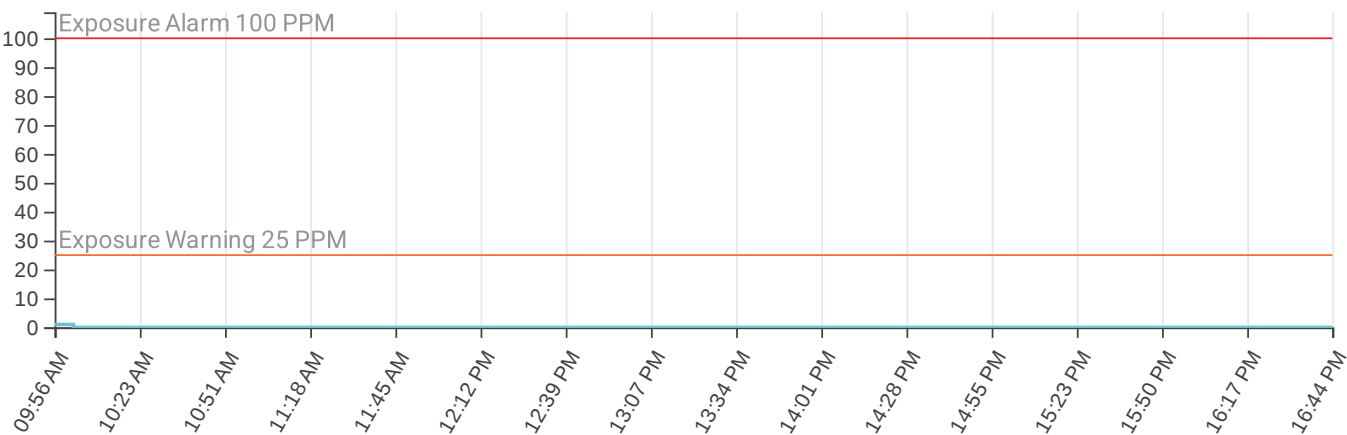


NO₂ PPM Avg: 0.00 Peak: 0.90 Min: 0.00

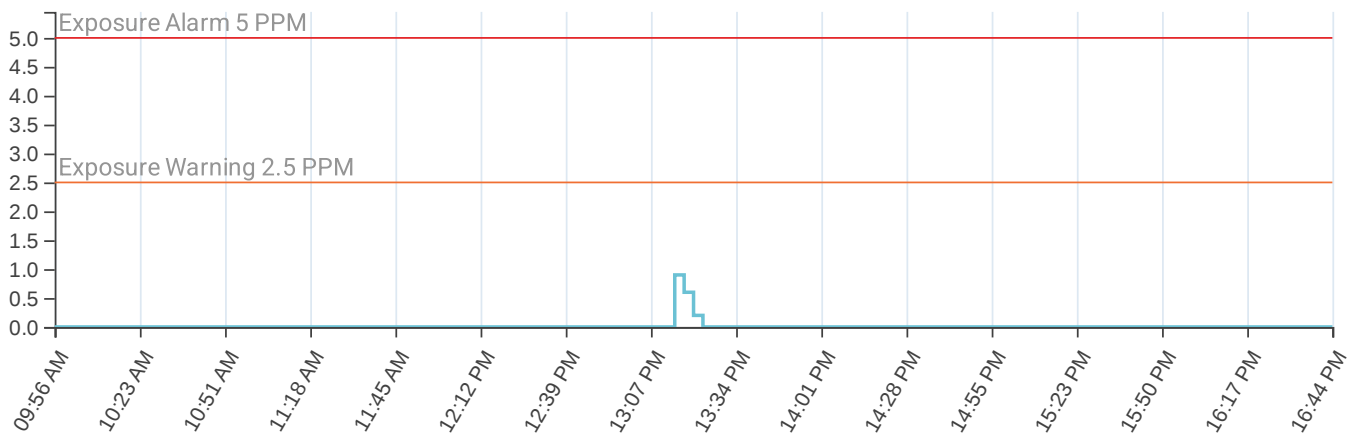


NH₃ PPM

Avg: 0.00 Peak: 7.00 Min: 0.00

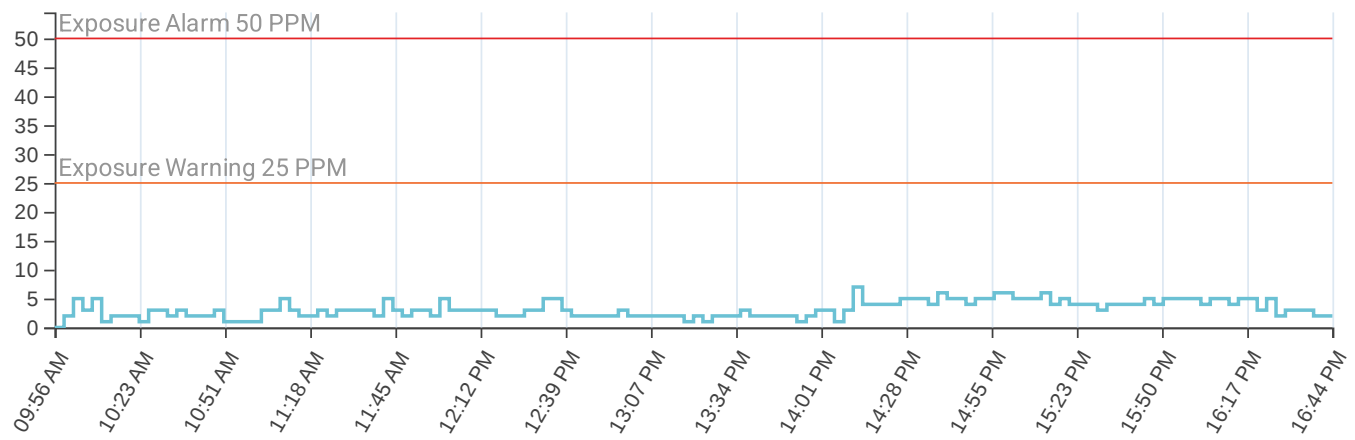

O₂ %VOL

Avg: 20.80 Peak: 20.80 Min: 20.80

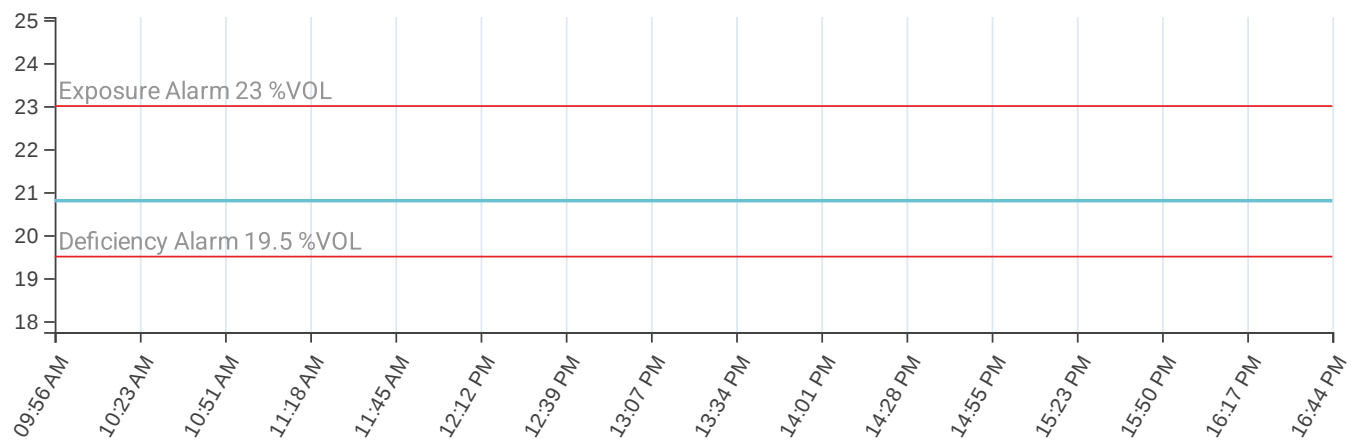

USAGE EVENTS

Dec 5, 2025, 9:55:00 AM	Instrument Powered On
Received by Grid Dec 5, 2025, 9:26:07 PM	
Dec 5, 2025, 9:56:45 AM	Fresh Air Baseline: Passed
Received by Grid Dec 5, 2025, 9:26:07 PM	
Dec 5, 2025, 4:46:45 PM	Instrument Powered Off
Received by Grid Dec 5, 2025, 9:26:07 PM	

NOTES

No notes present.