

USAGE REPORT



ALTAIR 5X - A5X-00033288

Start Date: Fri, Dec 05, 2025, 09:59:00 AM GMT+11
End Date: Fri, Dec 05, 2025, 05:13:15 PM GMT+11
Duration: 7 hours 14 minutes

Was Assigned To

Worker: AL84
Company: Ore Processing
Department: Surface Fixet Plant Toolstore

CALIBRATION

Instrument Calibration Status ✓ Compliant

Last Calibration Test Passed
Thu, Dec 4, 2025, 10:54:13 AM GMT+11

Last Bump Test Expired
Thu, Dec 4, 2025, 10:54:13 AM GMT+11

Sensors Calibration

Status	Gas Type	Calibration Status	Bump Status
 Bump Due	Combustible	Passed Dec 4, 2025, 10:54:13 AM GMT+11	Expired Dec 4, 2025, 10:54:13 AM GMT+11
 Bump Due	O ₂	Passed Dec 4, 2025, 10:54:13 AM GMT+11	Expired Dec 4, 2025, 10:54:13 AM GMT+11
 Bump Due	CO	Passed Dec 4, 2025, 10:54:13 AM GMT+11	Expired Dec 4, 2025, 10:54:13 AM GMT+11
 Bump Due	H ₂ S	Passed Dec 4, 2025, 10:54:13 AM GMT+11	Expired Dec 4, 2025, 10:54:13 AM GMT+11
 Bump Due	SO ₂	Passed Dec 4, 2025, 10:54:13 AM GMT+11	Expired Dec 4, 2025, 10:54:13 AM GMT+11

INSTRUMENT CONFIGURATION

Alert Behaviors

Alarms	LEDs, Horn, Vibrate
--------	---------------------

Instrument Alerts

Man Down Alarm	Enabled
----------------	---------

Instrument Configuration

Firmware Version	2.24.0
Language	English
Calibration Interval	Disabled
Bump Test Interval	Disabled
Session Logging Status	Enabled
Periodic Logging Status	Enabled

INSTRUMENT ALARM SETPOINTS

Combustible

Serial Number	00130302935
Manufactured	03/2013
Deadband Enabled	Disabled
Exposure Warning	5 %LEL
Exposure Alarm	10 %LEL
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

O₂

Serial Number	01180500189
Manufactured	05/2018
Deficiency Alarm	19.5 %VOL
Exposure Alarm	23 %VOL
Ovrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

CO

Serial Number	04130304753
Manufactured	03/2013
Exposure Warning	25 PPM
Exposure Alarm	60 PPM
STEL Alarm Alarm	60 PPM
TWA Alarm Alarm	25 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

H₂S


Serial Number	04130304753
Manufactured	03/2013
Exposure Warning	10 PPM
Exposure Alarm	15 PPM
STEL Alarm Alarm	15 PPM
TWA Alarm Alarm	10 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

SO₂


Serial Number	07180100432
Manufactured	01/2018
Exposure Warning	2 PPM
Exposure Alarm	5 PPM
STEL Alarm Alarm	5 PPM
TWA Alarm Alarm	2 PPM
Overrange Alarm	
Underrange Warning	
Replace soon Notification	
Replace now Notification	

GAS READINGS


COMB %LEL Avg: 0.00 Peak: 0.00 Min: 0.00

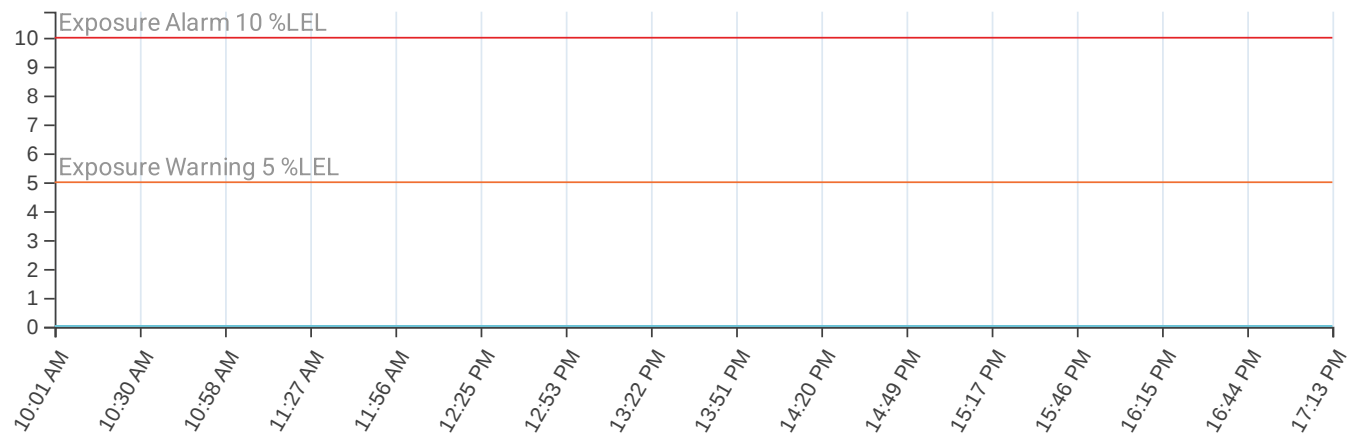

CO PPM Avg: 0.00 Peak: 1.00 Min: 0.00

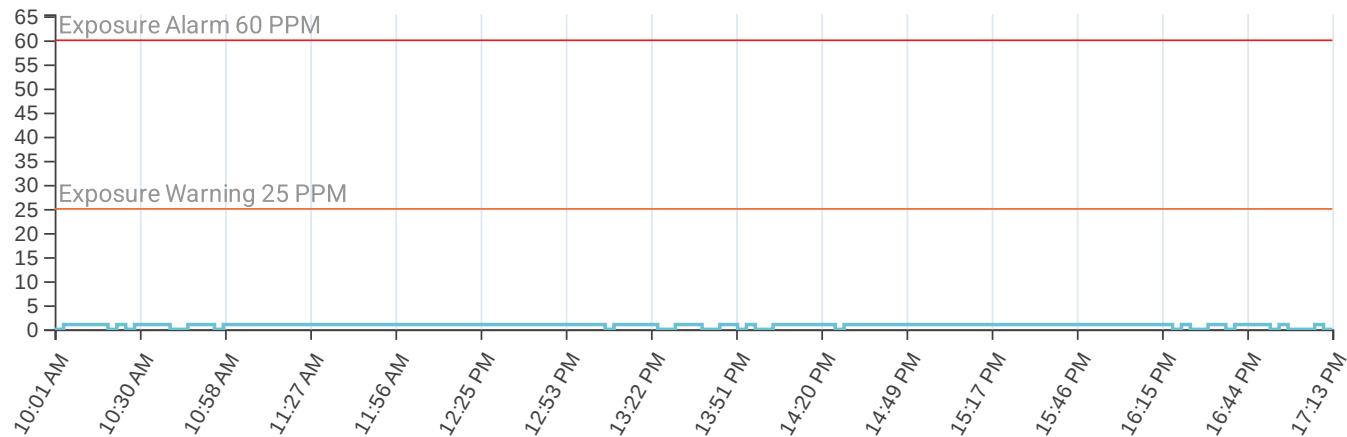


H₂S PPM Avg: 0.00 Peak: 1.00 Min: 0.00

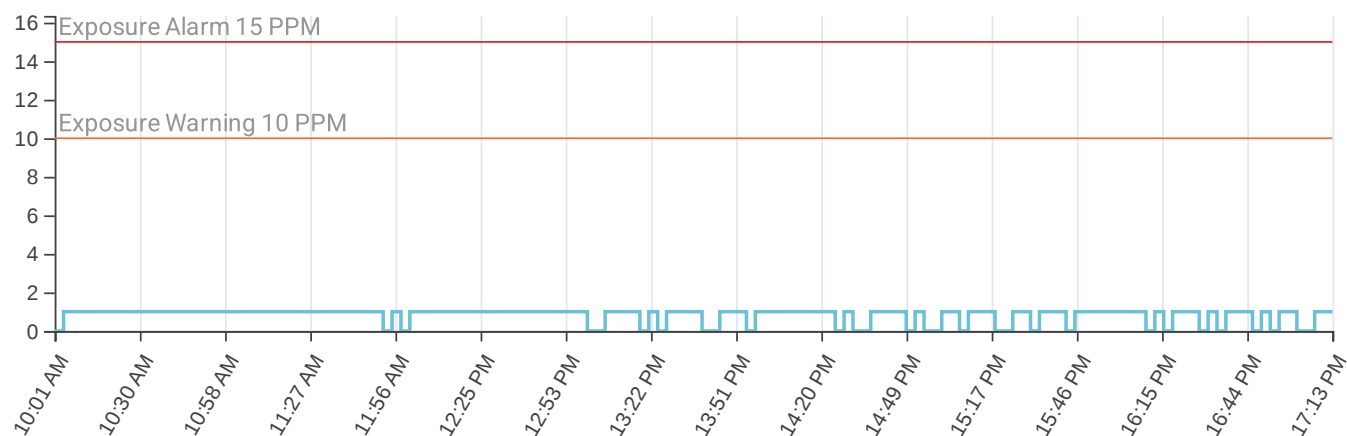


SO₂ PPM

Avg: 0.00 Peak: 0.60 Min: 0.00

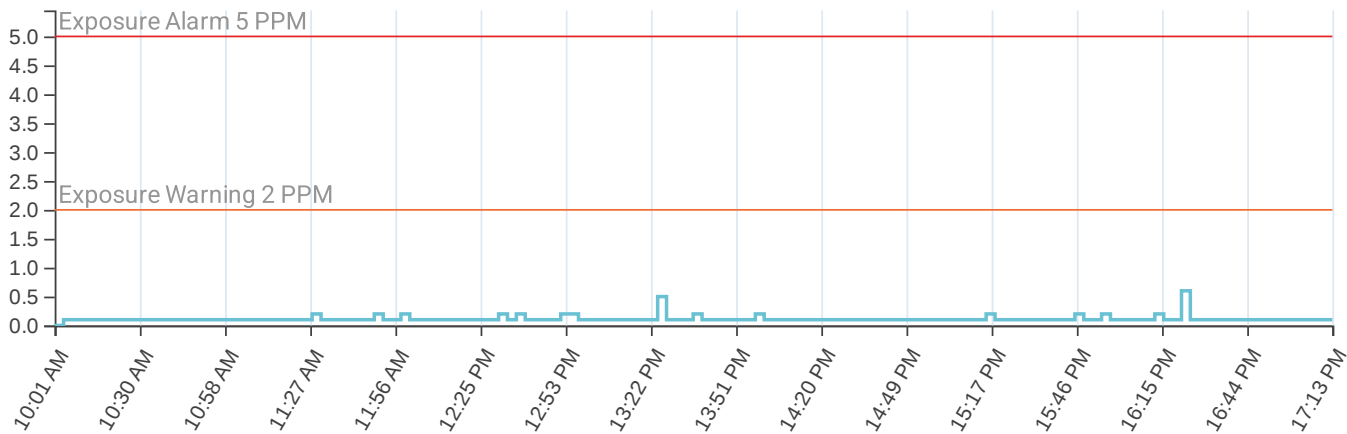

O₂ %VOL

Avg: 20.80 Peak: 20.80 Min: 20.80

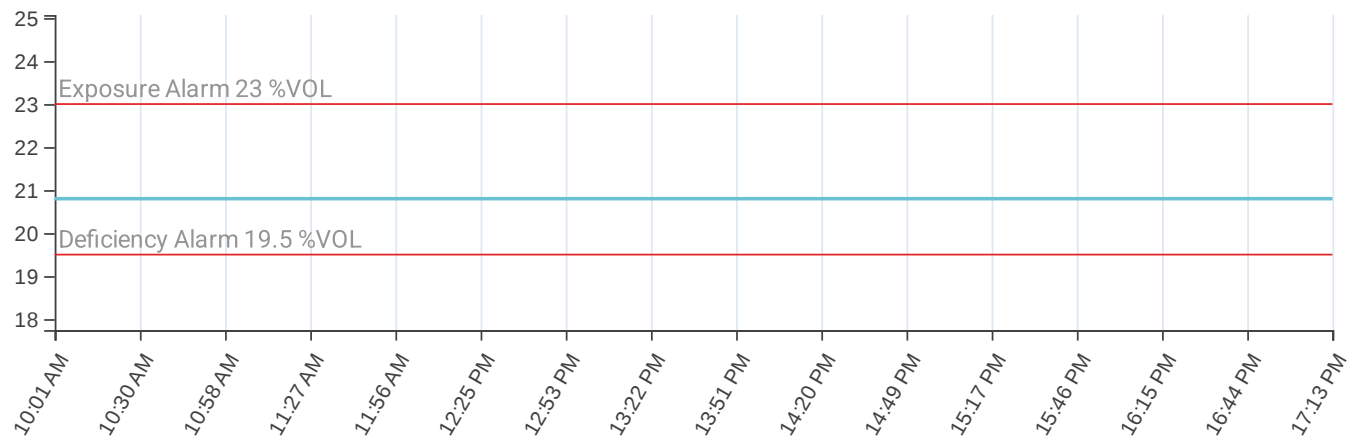

USAGE EVENTS

Dec 5, 2025, 9:59:00 AM	Instrument Powered On
Received by Grid Dec 8, 2025, 11:00:28 AM	
Dec 5, 2025, 5:13:15 PM	Instrument Powered Off
Received by Grid Dec 8, 2025, 11:00:28 AM	

NOTES

No notes present.